
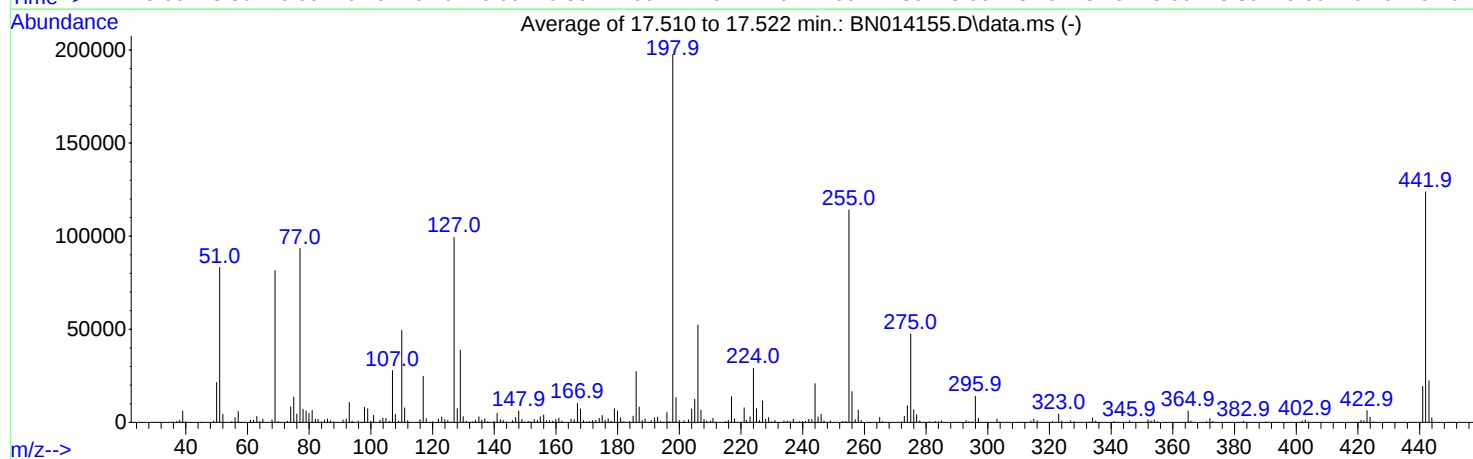


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033121\
 Data File : BN014155.D
 Acq On : 01 Apr 2021 00:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 31 12:15:38 2021

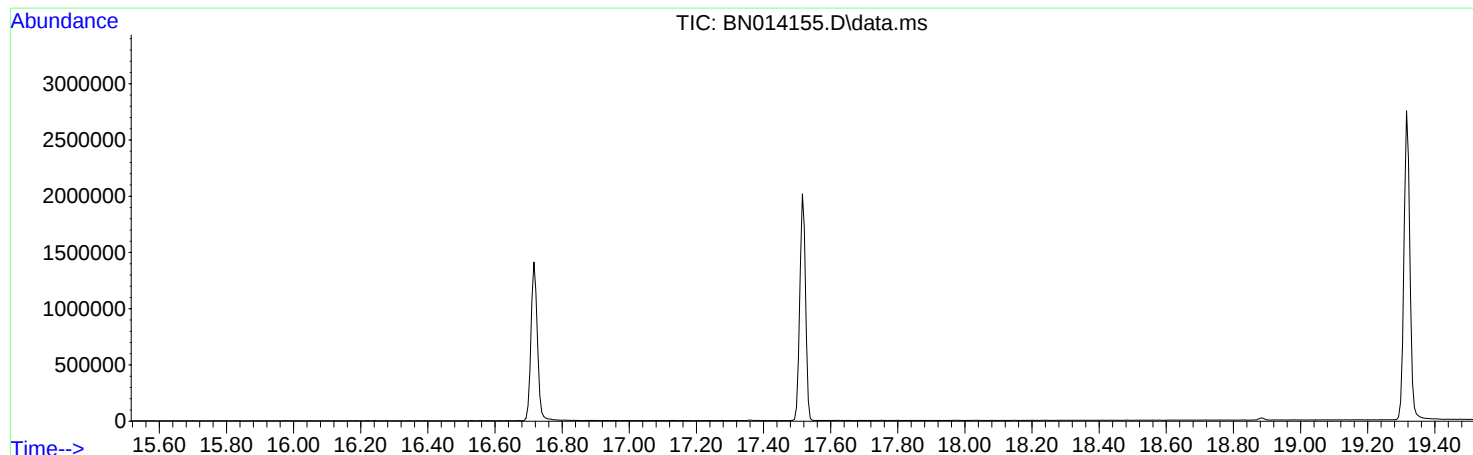




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	83229	PASS
68	69	0.00	2	1.7	1399	PASS
69	198	0.00	100	41.3	81592	PASS
70	69	0.00	2	0.5	422	PASS
127	198	10	80	50.3	99365	PASS
197	198	0.00	2	0.2	435	PASS
198	198	100	100	100.0	197568	PASS
199	198	5	9	6.8	13363	PASS
275	198	10	60	24.1	47520	PASS
365	198	1	100	3.1	6145	PASS
441	198	0.01	100	9.8	19370	PASS
442	442	50	100	100.0	123792	PASS
443	442	15	24	18.0	22291	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033121\
 Data File : BN014155.D
 Acq On : 01 Apr 2021 00:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 01 08:31:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 25 09:00:06 2021
 Response via : Initial Calibration

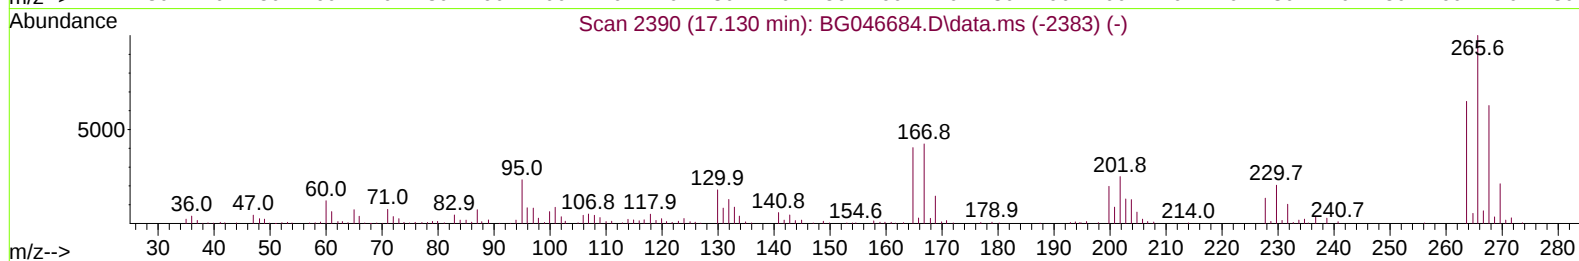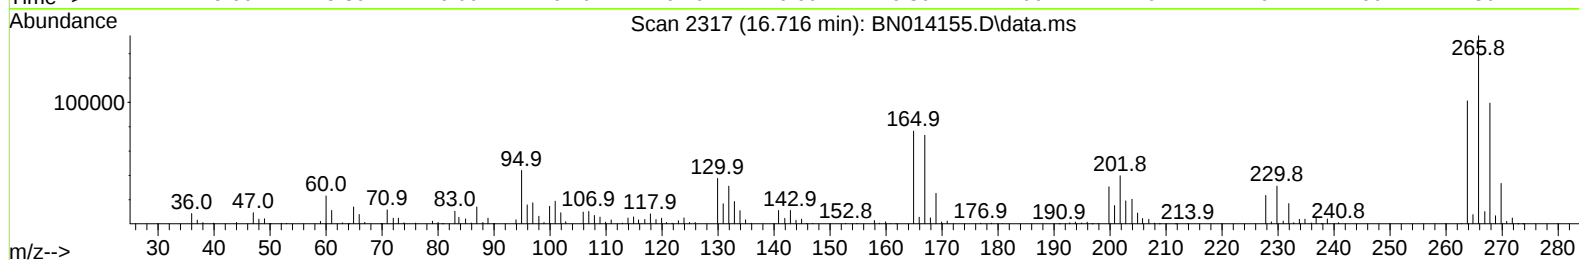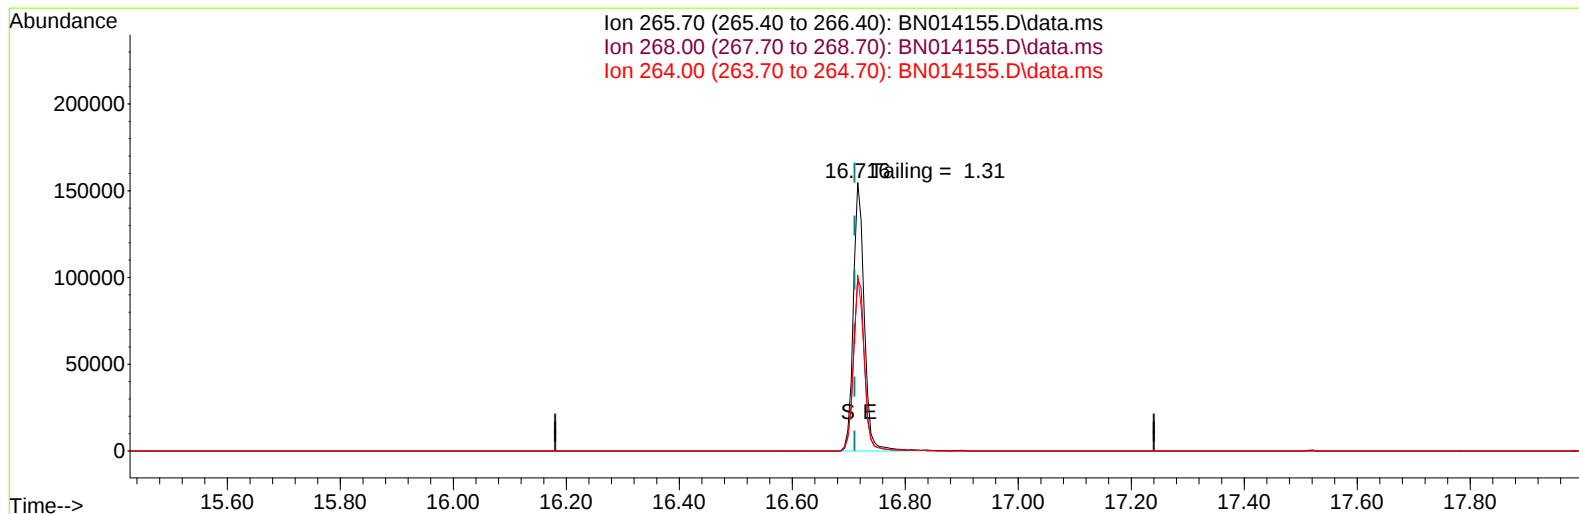

TIC: BN014155.D\data.ms

(70) Pentachlorophenol (C)

16.716min (+ 0.006) 18093.49 ng




response 208162

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.22
264.00	61.60	65.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033121\
Data File : BN014155.D
Acq On : 01 Apr 2021 00:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 01 08:31:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 09:00:06 2021
Response via : Initial Calibration

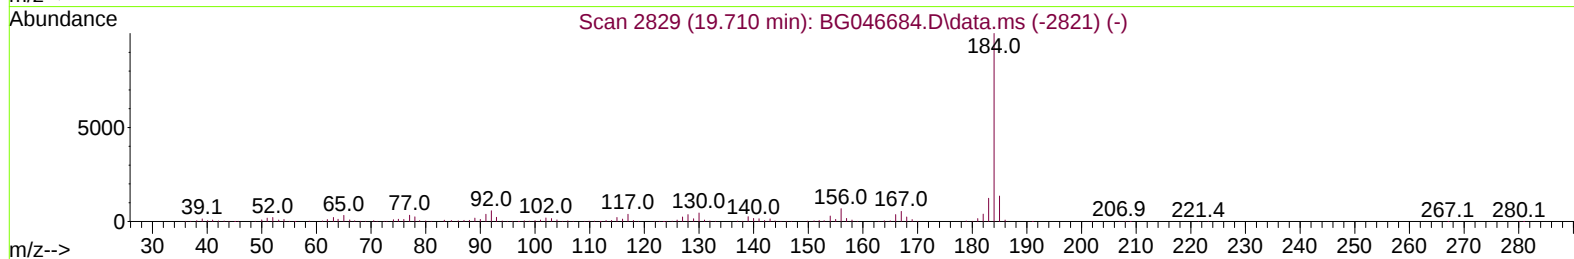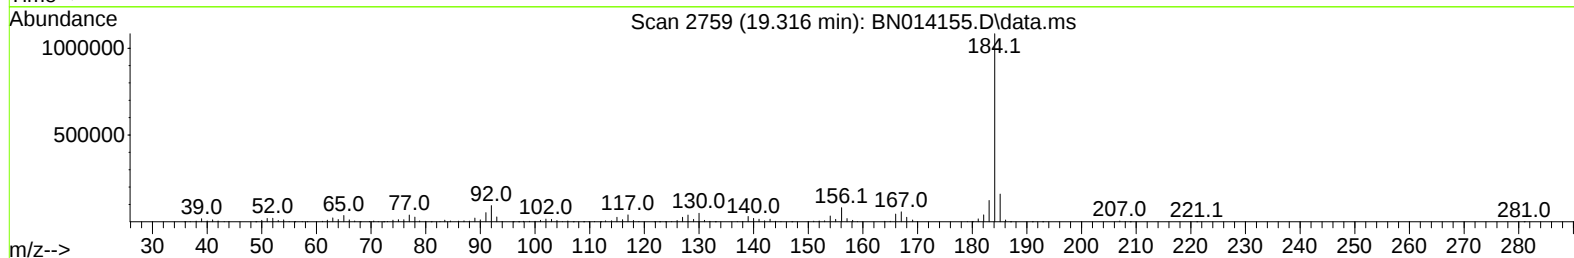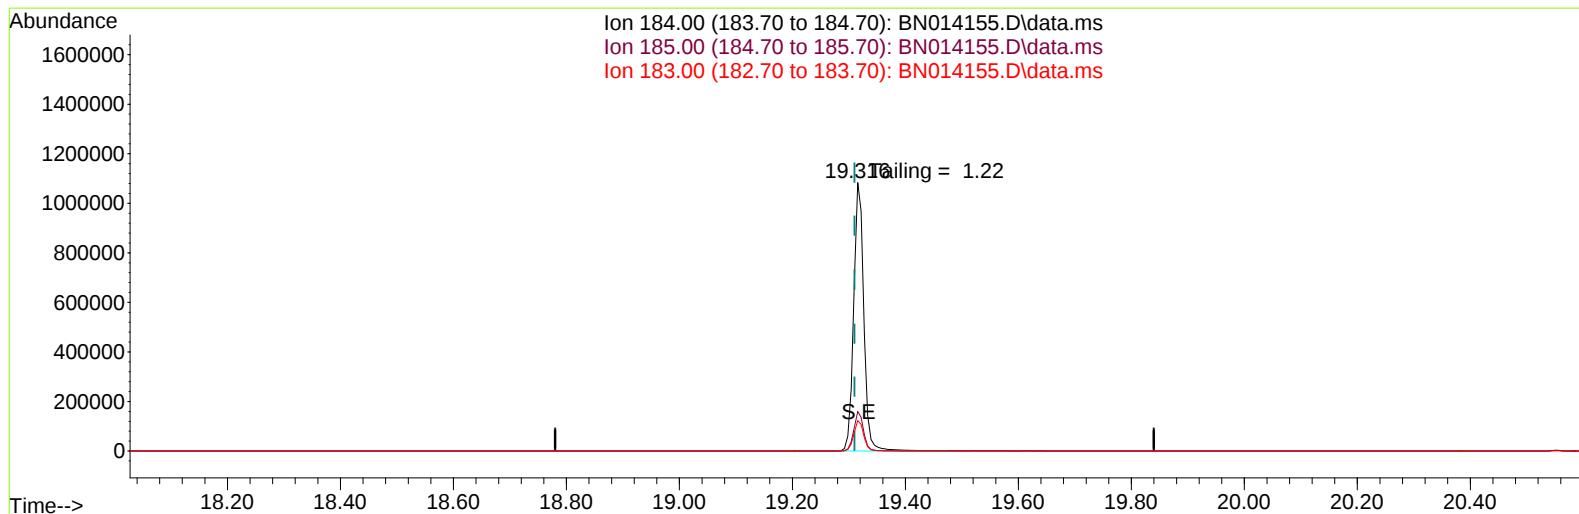

TIC: BN014155.D\data.ms

(77) Benzidine

19.316min (+ 0.006) 0.00 ng

response 1359312

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.76
183.00	13.20	11.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/31/2021	BNA_N	<u>BN014155.D</u>
Compound Name	Response	Retention Time
DDT	704894	20.551
DDD	10110	20.11
DDE	1175	19.604
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11285	716179	1.58