




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030556.D
Acq On : 30 Mar 2024 19:22
Operator : MA/JU
Sample : PB159892BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK892

Manual IntegrationsAPPROVED

Quant Time: Mar 31 13:07:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2024
Supervised By :mohammad ahmed 04/02/2024

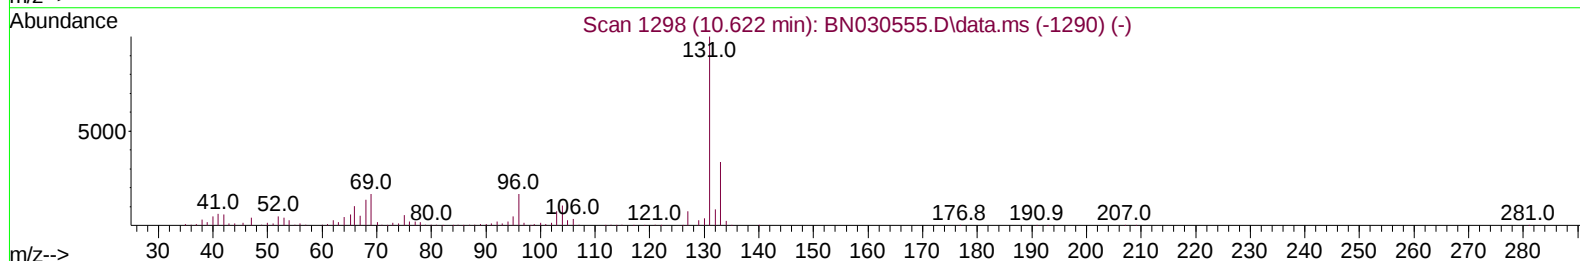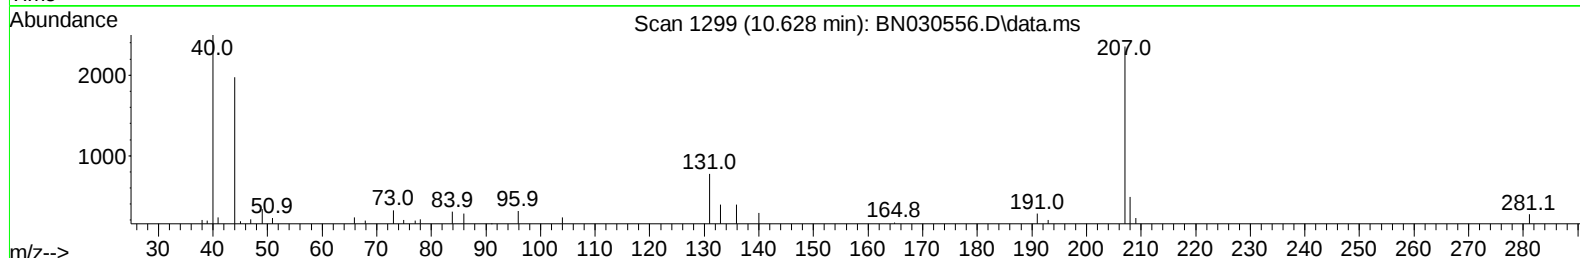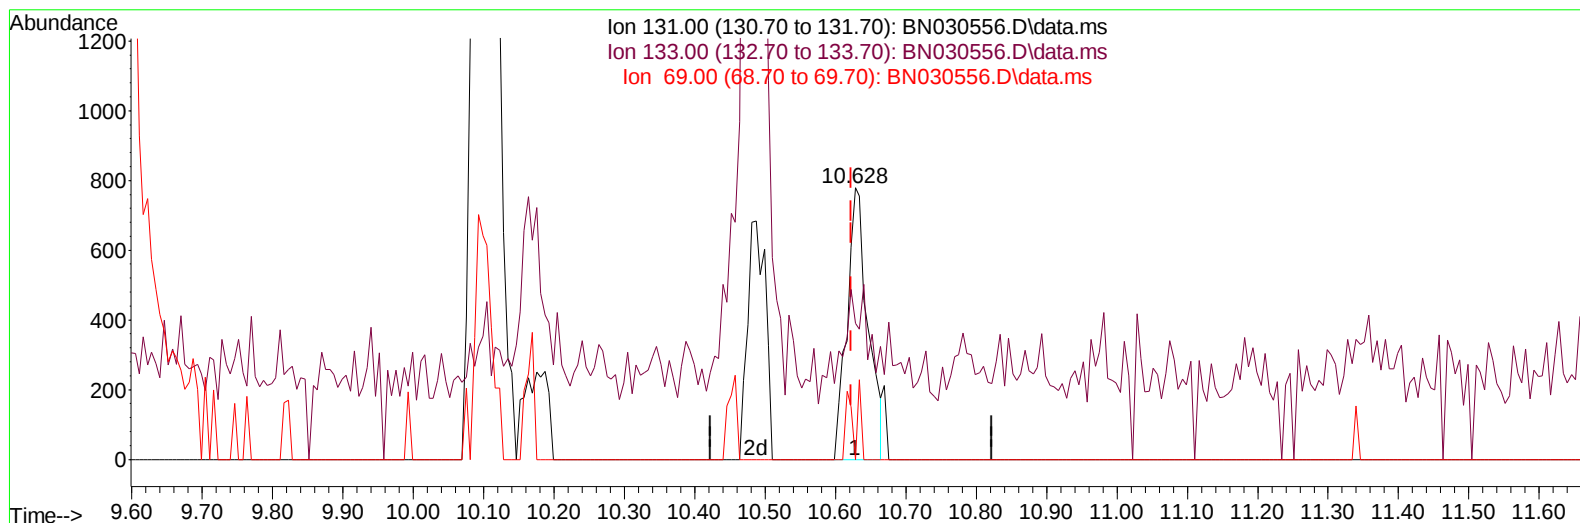

TIC: BN030556.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.628min (+ 0.006) 0.09 ng/u1

response 1595

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.70	50.19#
69.00	16.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030556.D
Acq On : 30 Mar 2024 19:22
Operator : MA/JU
Sample : PB159892BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK892

Manual IntegrationsAPPROVED

Quant Time: Mar 31 13:07:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2024
Supervised By :mohammad ahmed 04/02/2024

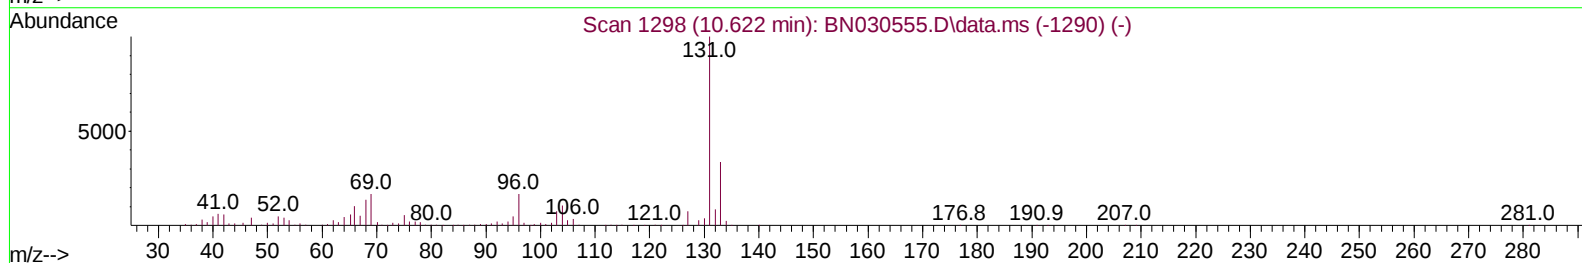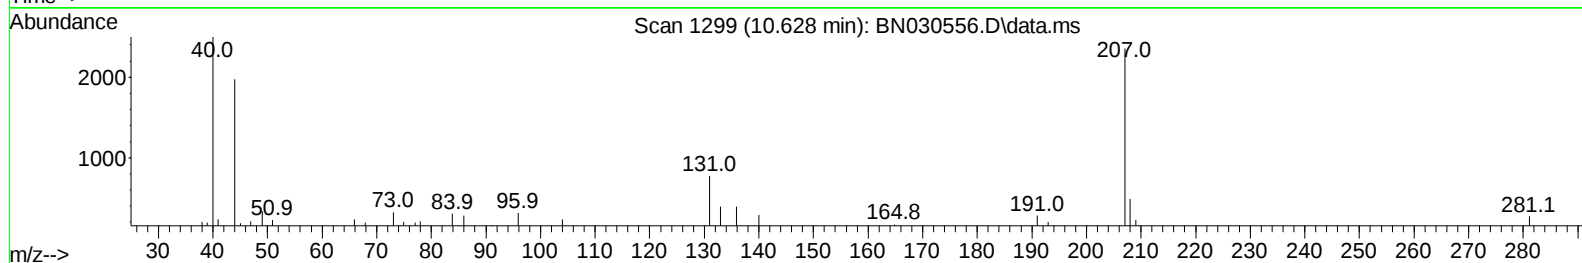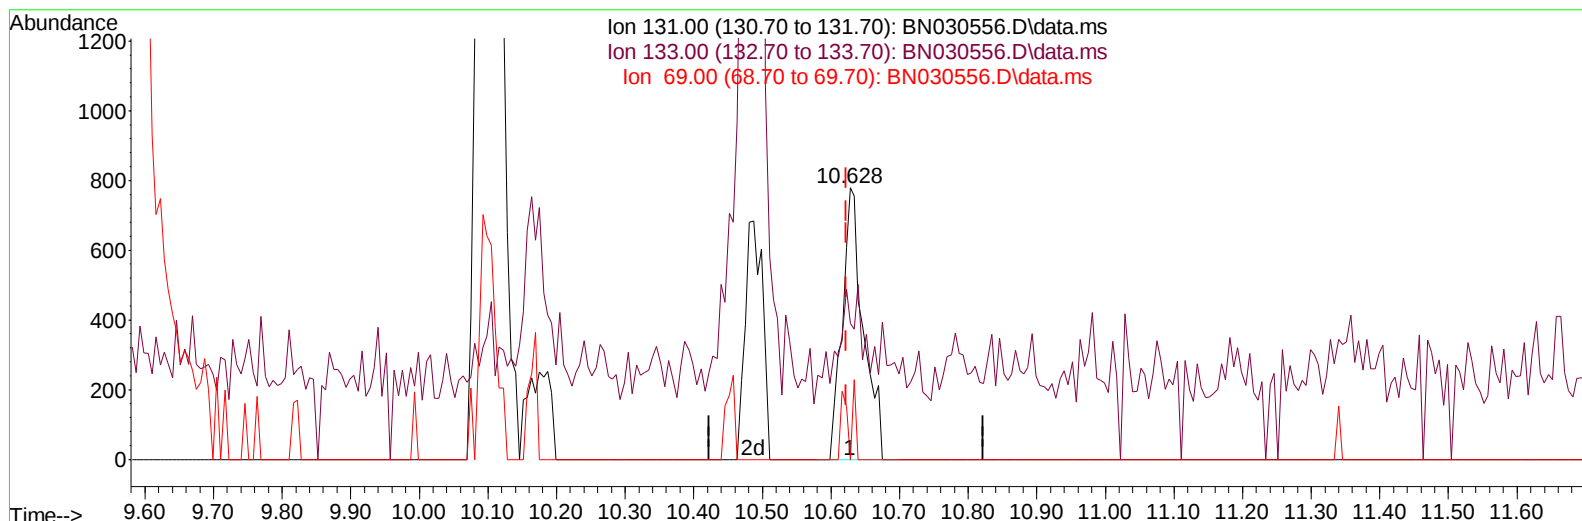

TIC: BN030556.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.628min (+ 0.006) 0.09 ng/ul m

response 1670

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.70	50.19#
69.00	16.20	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030556.D
 Acq On : 30 Mar 2024 19:22
 Operator : MA/JU
 Sample : PB159892BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK892

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/01/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Mar 31 13:09:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	184608	20.000	ng/ul	0.00
20) Naphthalene-d8	10.481	136	804250	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.340	164	527956	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.087	188	1125842	20.000	ng/ul	0.00
79) Chrysene-d12	21.328	240	1077347	20.000	ng/ul	0.00
88) Perylene-d12	24.280	264	1181587	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	28306	7.189	ng/uL	0.00
4) Pyridine-d5	3.599	84	303780	25.732	ng/ul	0.00
7) Phenol-d5	6.864	99	466117	31.212	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	314388	34.084	ng/ul	0.00
11) 2-Chlorophenol-d4	7.228	132	404745	35.727	ng/ul	0.00
15) 4-Methylphenol-d8	8.399	113	357184	28.538	ng/ul	0.00
21) Nitrobenzene-d5	8.852	128	200282	35.899	ng/ul	0.00
24) 2-Nitrophenol-d4	9.569	143	192108	37.640	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	376389	33.686	ng/ul	0.00
31) 4-Chloroaniline-d4	10.628	131	1670m	0.091	ng/ul	0.00
46) Dimethylphthalate-d6	13.757	166	1342598	38.089	ng/ul	0.00
49) Acenaphthylene-d8	14.034	160	1420483	35.049	ng/ul	0.00
54) 4-Nitrophenol-d4	14.540	143	231549	34.342	ng/ul	0.00
60) Fluorene-d10	15.340	176	1148631	37.238	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.451	200	139887	28.150	ng/ul	0.00
73) Anthracene-d10	17.187	188	1817309	37.464	ng/ul	0.00
81) Pyrene-d10	19.486	212	2227819	38.462	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.069	264	1992717	36.601	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030556.D
Acq On : 30 Mar 2024 19:22
Operator : MA/JU
Sample : PB159892BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK892

Manual IntegrationsAPPROVED

Quant Time: Mar 31 13:09:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2024
Supervised By :mohammad ahmed 04/02/2024

