

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030545.D
 Acq On : 30 Mar 2024 11:29
 Operator : MA/JU
 Sample : P1929-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL5

Quant Time: Mar 31 12:33:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	225264	20.000	ng/u1	0.00
20) Naphthalene-d8	10.481	136	994697	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.339	164	643908	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.092	188	1389906	20.000	ng/u1	0.00
79) Chrysene-d12	21.327	240	1321419	20.000	ng/u1	0.00
88) Perylene-d12	24.274	264	1490187	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	34617	7.205	ng/uL	0.00
4) Pyridine-d5	3.605	84	150403	10.441	ng/u1	0.00
7) Phenol-d5	6.863	99	155656	8.542	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	504956	44.864	ng/u1	0.00
11) 2-Chlorophenol-d4	7.228	132	484998	35.084	ng/u1	0.00
15) 4-Methylphenol-d8	8.399	113	305397	19.997	ng/u1	0.00
21) Nitrobenzene-d5	8.857	128	326026	47.249	ng/u1	0.00
24) 2-Nitrophenol-d4	9.569	143	298523	47.292	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	543913	39.359	ng/u1	0.00
31) 4-Chloroaniline-d4	10.622	131	818768	35.989	ng/u1	0.00
46) Dimethylphthalate-d6	13.757	166	2001477	46.556	ng/u1	0.00
49) Acenaphthylene-d8	14.034	160	2313314	46.800	ng/u1	0.00
54) 4-Nitrophenol-d4	14.534	143	53903	6.555	ng/u1	0.00
60) Fluorene-d10	15.339	176	1745588	46.400	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.451	200	219524	35.782	ng/u1	0.00
73) Anthracene-d10	17.186	188	2844151	47.493	ng/u1	0.00
81) Pyrene-d10	19.486	212	3326988	46.829	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.074	264	3495772	50.911	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.234	88	5723	1.112	ng/uL	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030545.D
Acq On : 30 Mar 2024 11:29
Operator : MA/JU
Sample : P1929-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL5

Quant Time: Mar 31 12:33:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

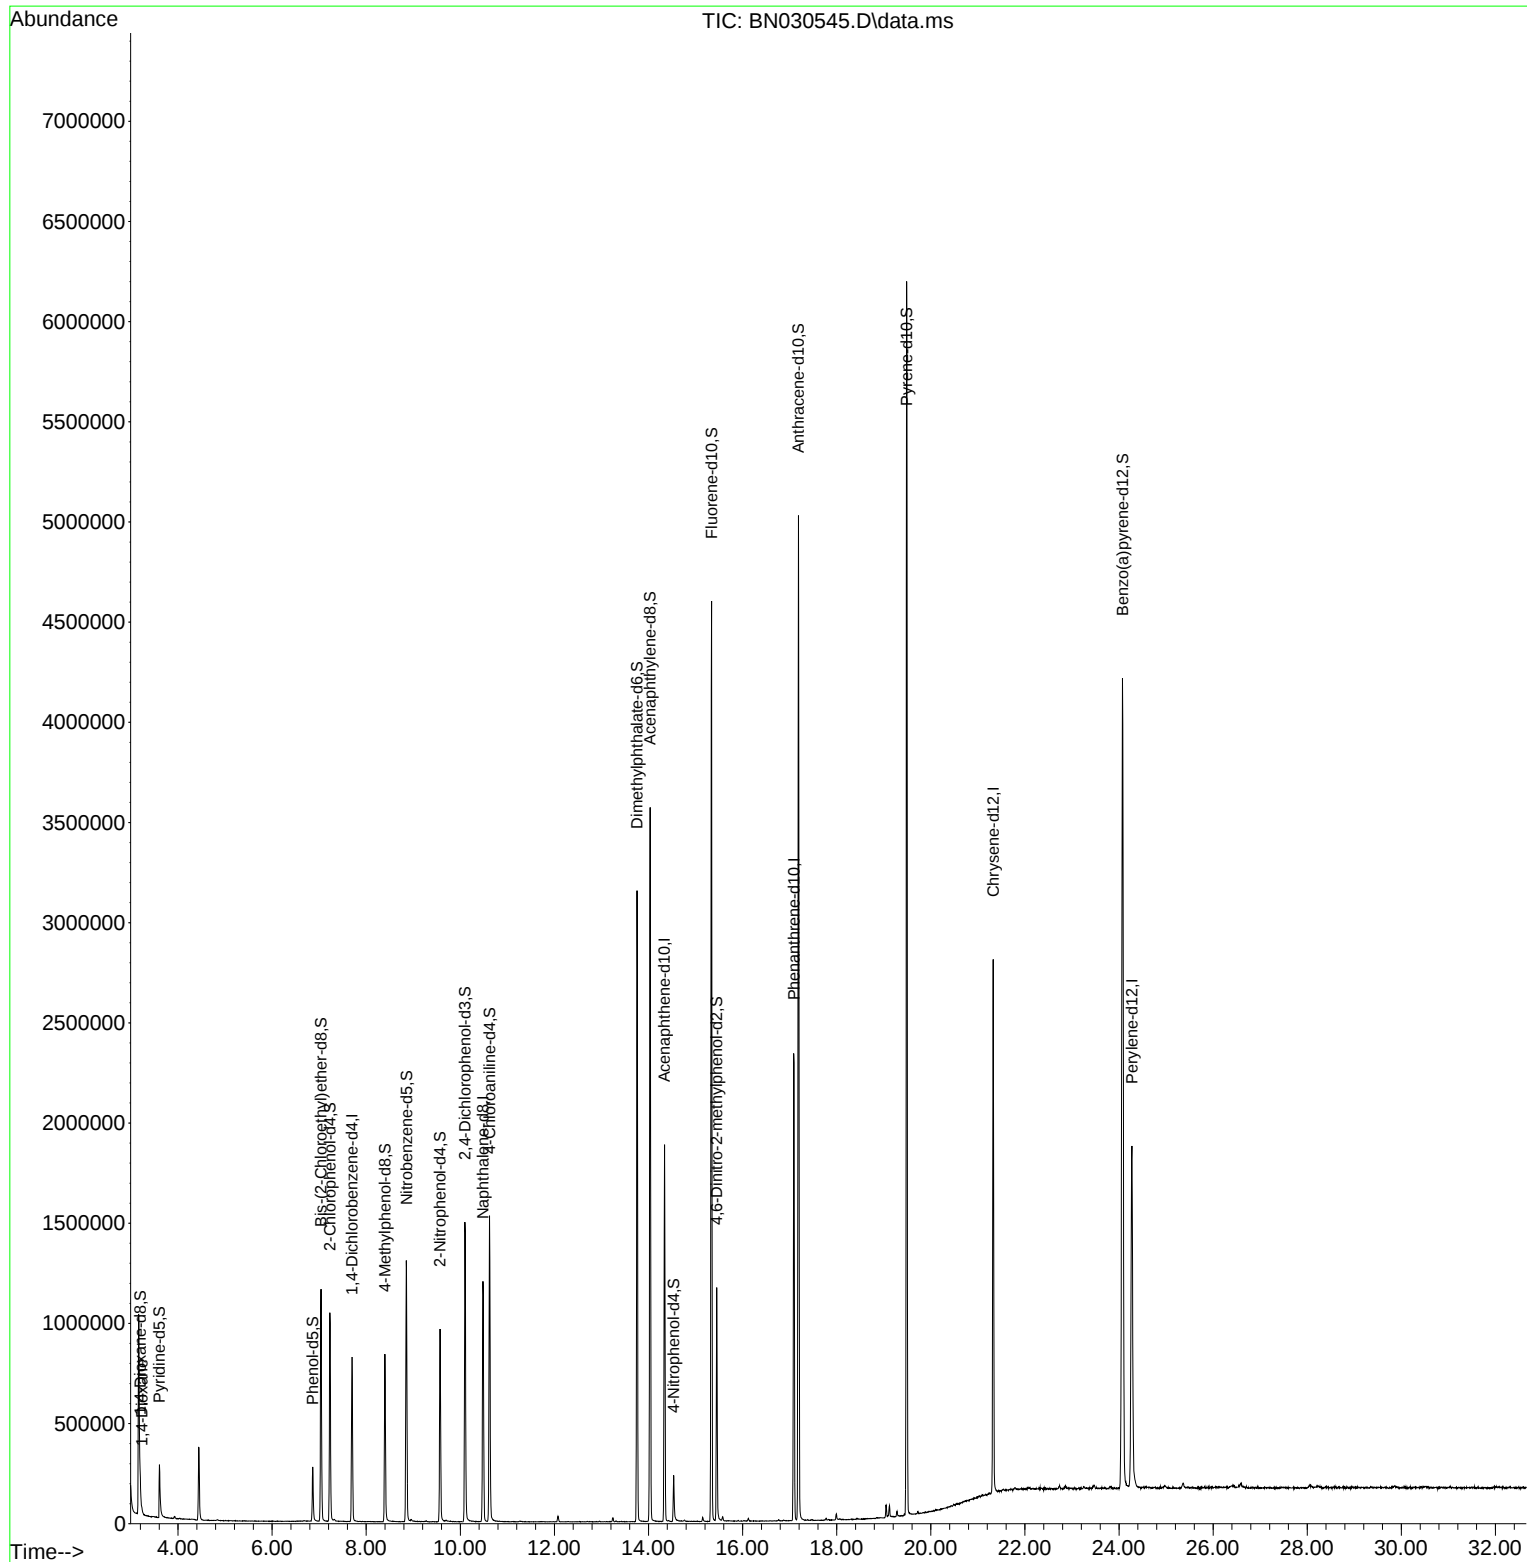

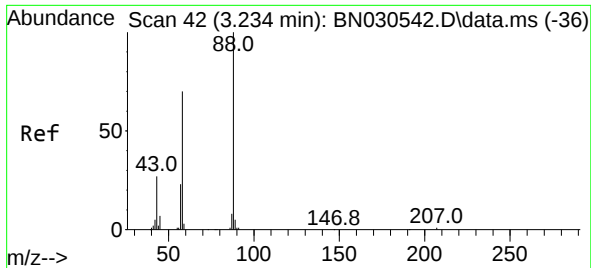

#2
 1,4-Dioxane
 Concen: 1.112 ng/uL
 RT: 3.234 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BN030545.D
 Acq: 30 Mar 2024 11:29

Instrument :
 BNA_N
 ClientSampleId :
 C0AL5

Tgt Ion: 88 Resp: 5723

Ion	Ratio	Lower	Upper
88	100		
43	25.8	23.8	35.8
58	60.8	56.6	84.8

