

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030551.D
 Acq On : 30 Mar 2024 15:25
 Operator : MA/JU
 Sample : P1931-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07C5

Quant Time: Mar 31 12:44:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	214882	20.000	ng/ul	0.00
20) Naphthalene-d8	10.481	136	940646	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.340	164	613736	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.086	188	1299876	20.000	ng/ul	0.00
79) Chrysene-d12	21.327	240	1295851	20.000	ng/ul	0.00
88) Perylene-d12	24.268	264	1475244	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	13317	2.906	ng/uL	0.00
4) Pyridine-d5	3.605	84	87642	6.378	ng/ul	0.00
7) Phenol-d5	6.863	99	255938	14.724	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	170434	15.874	ng/ul	0.00
11) 2-Chlorophenol-d4	7.228	132	209956	15.922	ng/ul	0.00
15) 4-Methylphenol-d8	8.399	113	190078	13.047	ng/ul	0.00
21) Nitrobenzene-d5	8.852	128	99424	15.237	ng/ul	0.00
24) 2-Nitrophenol-d4	9.569	143	85084	14.254	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	189200	14.478	ng/ul	0.00
31) 4-Chloroaniline-d4	10.622	131	25535	1.187	ng/ul	0.00
46) Dimethylphthalate-d6	13.757	166	685896	16.739	ng/ul	0.00
49) Acenaphthylene-d8	14.034	160	756949	16.067	ng/ul	0.00
54) 4-Nitrophenol-d4	14.540	143	86960	11.095	ng/ul	0.00
60) Fluorene-d10	15.334	176	619176	17.268	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.451	200	51557	8.986	ng/ul	0.00
73) Anthracene-d10	17.186	188	991987	17.712	ng/ul	0.00
81) Pyrene-d10	19.486	212	1259366	18.076	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.068	264	1303493	19.176	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.516	105	31529	1.371	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030551.D
Acq On : 30 Mar 2024 15:25
Operator : MA/JU
Sample : P1931-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C5

Quant Time: Mar 31 12:44:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

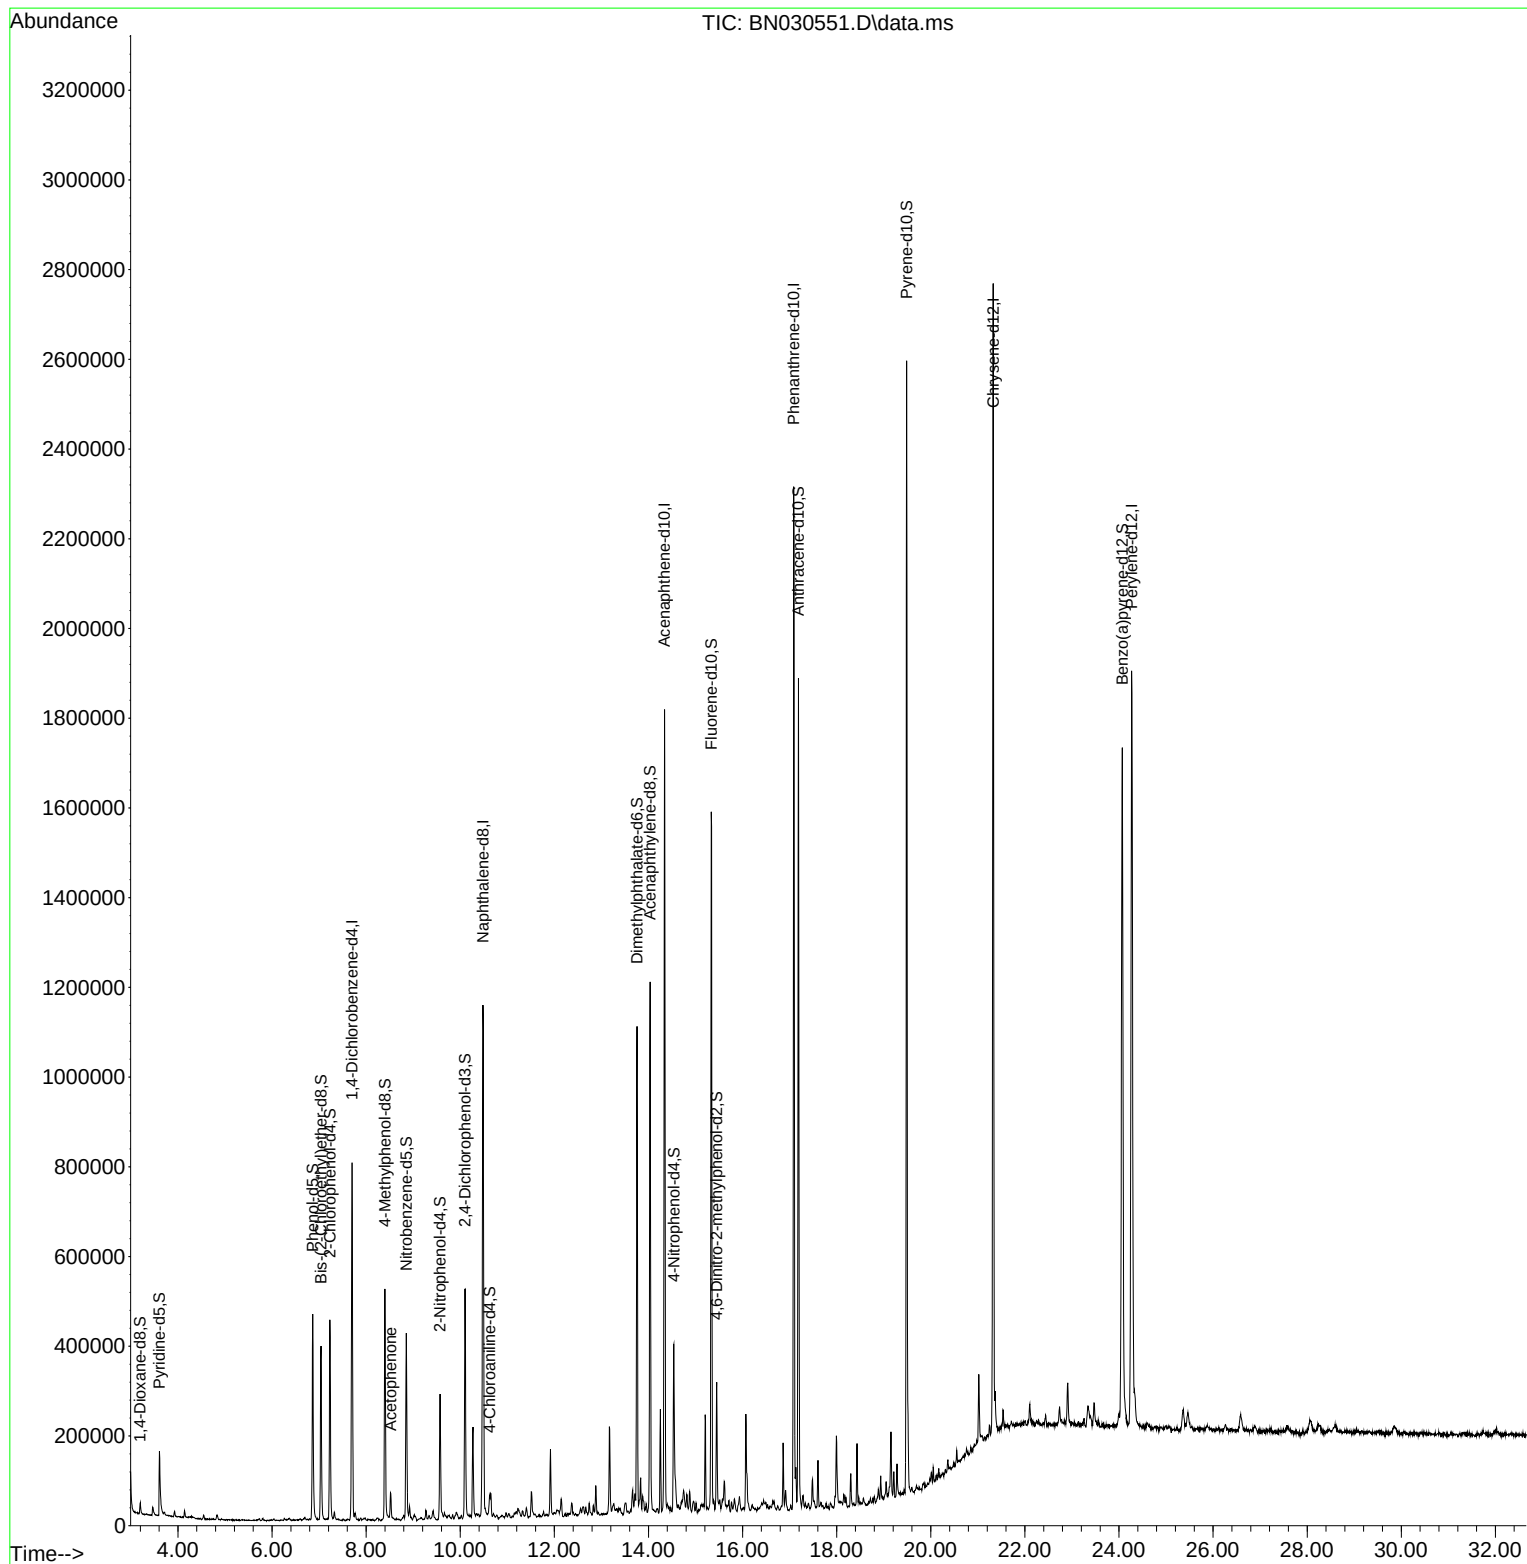

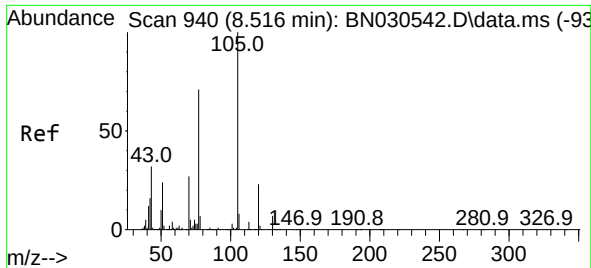

#16
 Acetophenone
 Concen: 1.371 ng/ul
 RT: 8.516 min Scan# 94
 Delta R.T. -0.000 min
 Lab File: BN030551.D
 Acq: 30 Mar 2024 15:25

Instrument :
 BNA_N
 ClientSampleId :
 E07C5

Tgt Ion:105 Resp: 31529
 Ion Ratio Lower Upper
 105 100
 77 76.6 61.2 91.8
 51 26.4 21.0 31.4

