

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030552.D
 Acq On : 30 Mar 2024 16:05
 Operator : MA/JU
 Sample : P1931-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07C7

Quant Time: Mar 31 12:44:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	224399	20.000	ng/u1	0.00
20) Naphthalene-d8	10.481	136	978578	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.340	164	633754	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.086	188	1324995	20.000	ng/u1	0.00
79) Chrysene-d12	21.327	240	1313503	20.000	ng/u1	0.00
88) Perylene-d12	24.268	264	1444374	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	7889	1.648	ng/uL	0.00
4) Pyridine-d5	3.617	84	31029	2.162	ng/u1	0.02
7) Phenol-d5	6.863	99	123529	6.805	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	84748	7.559	ng/u1	0.00
11) 2-Chlorophenol-d4	7.228	132	100350	7.287	ng/u1	0.00
15) 4-Methylphenol-d8	8.399	113	96177	6.322	ng/u1	0.00
21) Nitrobenzene-d5	8.852	128	46746	6.886	ng/u1	0.00
24) 2-Nitrophenol-d4	9.575	143	38341	6.174	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.104	165	89653	6.594	ng/u1	0.00
31) 4-Chloroaniline-d4	10.622	131	14694	0.657	ng/u1	0.00
46) Dimethylphthalate-d6	13.757	166	340866	8.056	ng/u1	0.00
49) Acenaphthylene-d8	14.034	160	367261	7.549	ng/u1	0.00
54) 4-Nitrophenol-d4	14.534	143	31101	3.843	ng/u1	0.00
60) Fluorene-d10	15.334	176	303058	8.185	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.451	200	16574	2.834	ng/u1	0.00
73) Anthracene-d10	17.186	188	474750	8.316	ng/u1	0.00
81) Pyrene-d10	19.486	212	611587	8.660	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.063	264	613397	9.217	ng/u1	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.522	105	29025	1.208	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030552.D
Acq On : 30 Mar 2024 16:05
Operator : MA/JU
Sample : P1931-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C7


Quant Time: Mar 31 12:44:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

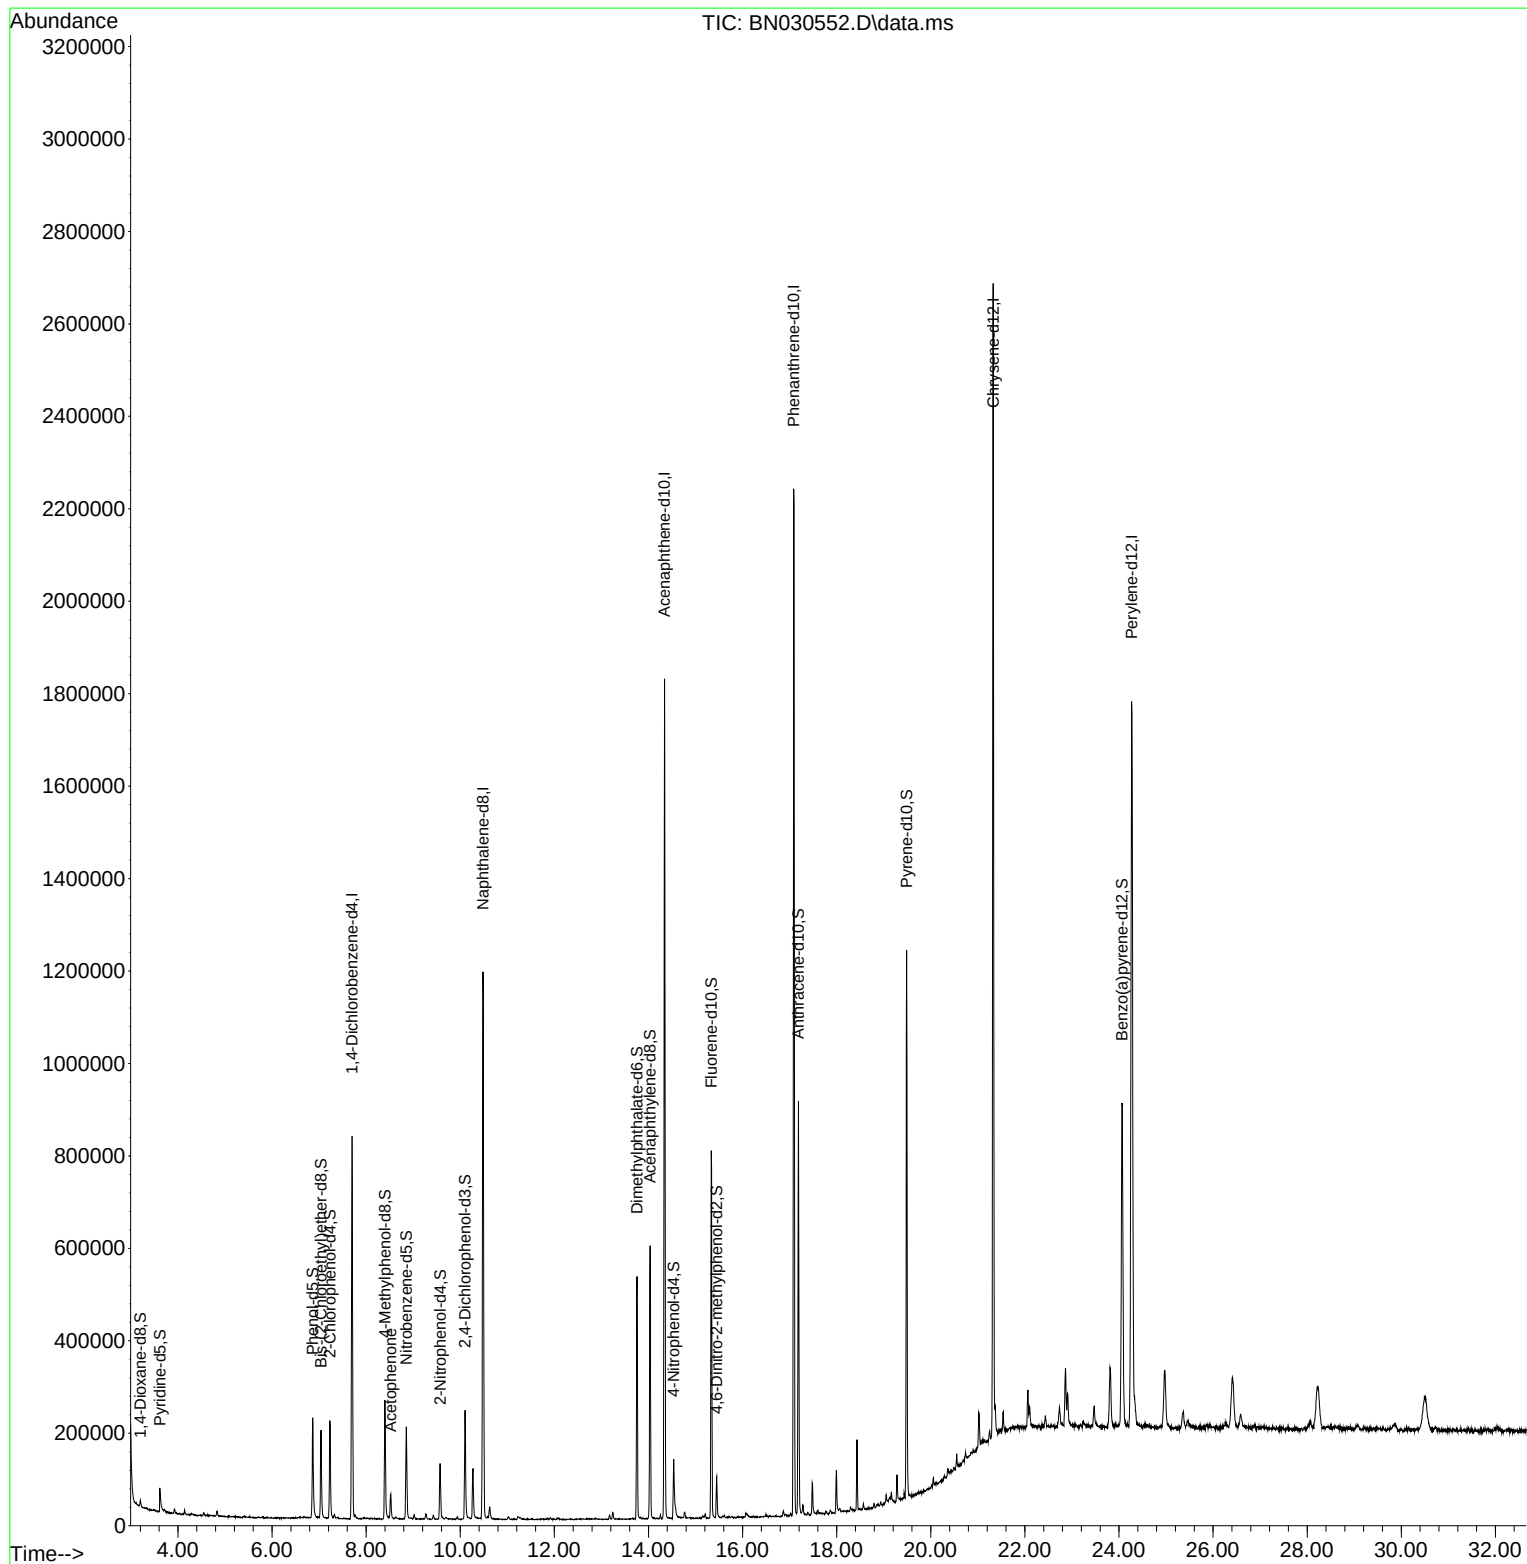

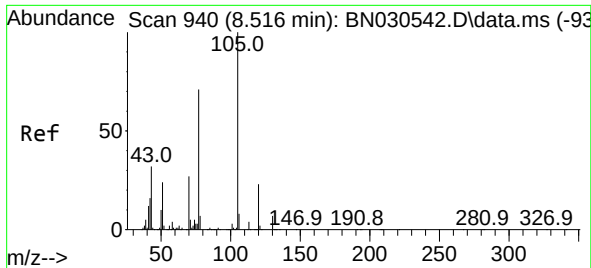

#16
 Acetophenone
 Concen: 1.208 ng/ul
 RT: 8.522 min Scan# 941
 Delta R.T. 0.006 min
 Lab File: BN030552.D
 Acq: 30 Mar 2024 16:05

Instrument :
 BNA_N
 ClientSampleId :
 E07C7

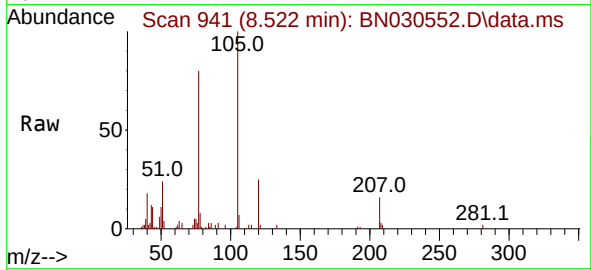

Tgt Ion:	105	Resp:	29025
Ion	Ratio	Lower	Upper
105	100		
77	80.1	61.2	91.8
51	23.7	21.0	31.4

