

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030558.D
 Acq On : 30 Mar 2024 20:42
 Operator : MA/JU
 Sample : P1931-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07C3

Quant Time: Apr 01 05:11:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.699	152	257271	20.000	ng/u1	0.00
20) Naphthalene-d8	10.481	136	1102541	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.339	164	689409	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.086	188	1440376	20.000	ng/u1	0.00
79) Chrysene-d12	21.327	240	1266542	20.000	ng/u1	0.00
88) Perylene-d12	24.268	264	1160939	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	6418	1.170	ng/uL	0.00
4) Pyridine-d5	3.616	84	28164	1.712	ng/u1	0.02
7) Phenol-d5	6.863	99	124277	5.971	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	78622	6.116	ng/u1	0.00
11) 2-Chlorophenol-d4	7.228	132	96193	6.093	ng/u1	0.00
15) 4-Methylphenol-d8	8.399	113	88736	5.087	ng/u1	0.00
21) Nitrobenzene-d5	8.851	128	43017	5.624	ng/u1	0.00
24) 2-Nitrophenol-d4	9.569	143	35150	5.024	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.098	165	92237	6.022	ng/u1	0.00
31) 4-Chloroaniline-d4	10.622	131	56150	2.227	ng/u1	0.00
46) Dimethylphthalate-d6	13.757	166	323576	7.030	ng/u1	0.00
49) Acenaphthylene-d8	14.034	160	365980	6.915	ng/u1	0.00
54) 4-Nitrophenol-d4	14.539	143	7342	0.834	ng/u1	0.00
60) Fluorene-d10	15.333	176	308316	7.655	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	4562	0.718	ng/u1	0.00
73) Anthracene-d10	17.186	188	500190	8.060	ng/u1	0.00
81) Pyrene-d10	19.486	212	624562	9.172	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.068	264	446515	8.347	ng/u1	0.00
Target Compounds						
					Qvalue	
80) Fluoranthene	19.151	202	82004	1.013	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030558.D
Acq On : 30 Mar 2024 20:42
Operator : MA/JU
Sample : P1931-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C3

Quant Time: Apr 01 05:11:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

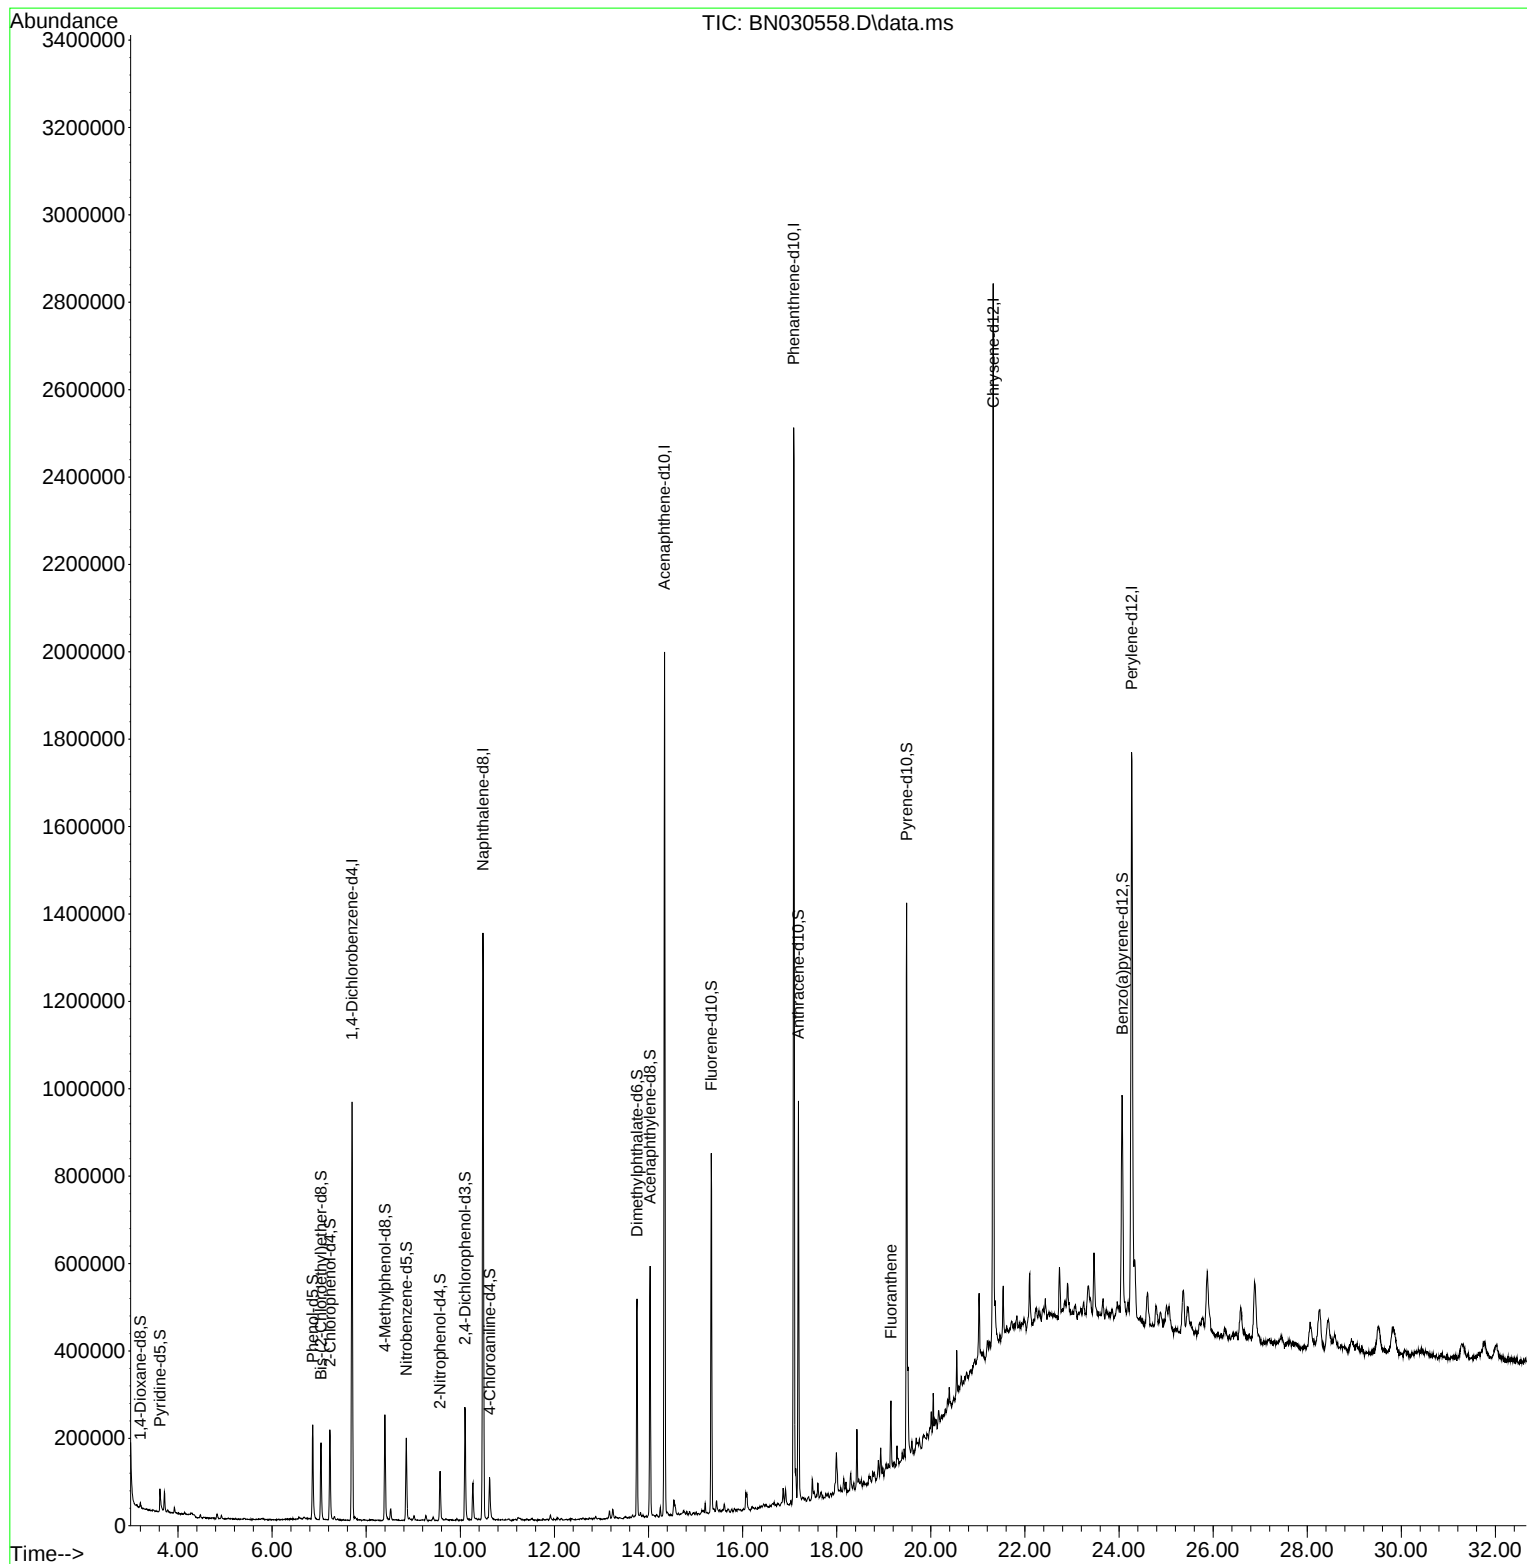

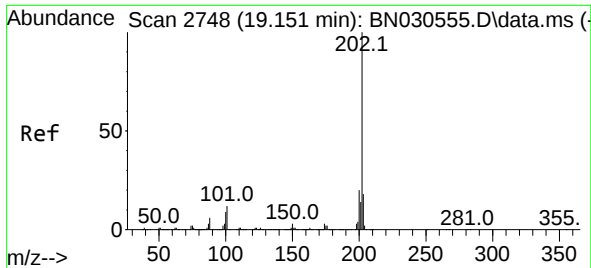

#80
Fluoranthene
Concen: 1.013 ng/ul
RT: 19.151 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN030558.D
Acq: 30 Mar 2024 20:42

Instrument :
BNA_N
ClientSampleId :
E07C3

Tgt Ion:202 Resp: 82004
Ion Ratio Lower Upper
202 100
101 11.9 9.0 13.6
100 8.3 6.8 10.2

