

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030543.D
 Acq On : 30 Mar 2024 10:11
 Operator : MA/JU
 Sample : PB159892BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK892

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030543.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	46	rVB	65498	93558	1.28%	0.134%
2	3.605	102	105	121	rBV	578390	1009896	13.87%	1.442%
3	3.928	155	160	170	rVB2	11834	24202	0.33%	0.035%
4	6.864	652	659	675	rBV	1066412	1706599	23.44%	2.437%
5	7.040	683	689	699	rBV	929249	1441366	19.79%	2.059%
6	7.228	715	721	733	rBV	1080886	1711833	23.51%	2.445%
7	7.699	794	801	816	rBV	923300	1493038	20.50%	2.132%
8	8.399	912	920	936	rBV	1358950	2163347	29.71%	3.090%
9	8.852	990	997	1013	rBV	1049113	1712683	23.52%	2.446%
10	9.569	1112	1119	1130	rBV	782062	1253819	17.22%	1.791%
11	10.099	1202	1209	1229	rBV	1289899	2170743	29.81%	3.100%
12	10.481	1267	1274	1286	rBV	1367675	2256560	30.99%	3.223%
13	10.622	1290	1298	1310	rBV	435957	748570	10.28%	1.069%
14	12.075	1538	1545	1552	rBV2	23441	39884	0.55%	0.057%
15	13.240	1738	1743	1750	rBV4	12525	20405	0.28%	0.029%
16	13.757	1824	1831	1846	rBV	2654516	3549747	48.75%	5.070%
17	14.034	1871	1878	1889	rBV	2858493	4267007	58.60%	6.094%
18	14.340	1923	1930	1938	rBV	2170833	3138414	43.10%	4.482%
19	14.534	1956	1963	1982	rBV	1127077	1720128	23.62%	2.457%
20	15.340	2092	2100	2112	rBV	3659511	5317440	73.02%	7.595%
21	15.451	2112	2119	2135	rVV	905211	1254449	17.23%	1.792%
22	15.575	2136	2140	2149	rVB2	16712	29540	0.41%	0.042%
23	16.122	2227	2233	2237	rBV4	11451	15702	0.22%	0.022%
24	16.769	2336	2343	2346	rBV6	5840	10020	0.14%	0.014%
25	16.875	2357	2361	2369	rVB3	5471	10113	0.14%	0.014%
26	17.087	2391	2397	2407	rBV	2649839	3793618	52.09%	5.418%
27	17.187	2408	2414	2426	rVV2	4133008	5863471	80.52%	8.374%
28	19.051	2726	2731	2735	rBV2	46928	66577	0.91%	0.095%
29	19.122	2738	2743	2750	rVB	39555	59448	0.82%	0.085%
30	19.486	2799	2805	2817	rBV2	4958450	6810528	93.52%	9.727%
31	21.327	3112	3118	3128	rBV	3040185	4281613	58.80%	6.115%
32	24.074	3575	3585	3601	rVB2	3049517	7282188	100.00%	10.401%
33	24.274	3610	3619	3640	rVB	1951053	4699943	64.54%	6.713%




Sum of corrected areas: 70016449

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030543.D
Acq On : 30 Mar 2024 10:11
Operator : MA/JU
Sample : PB159892BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK892

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

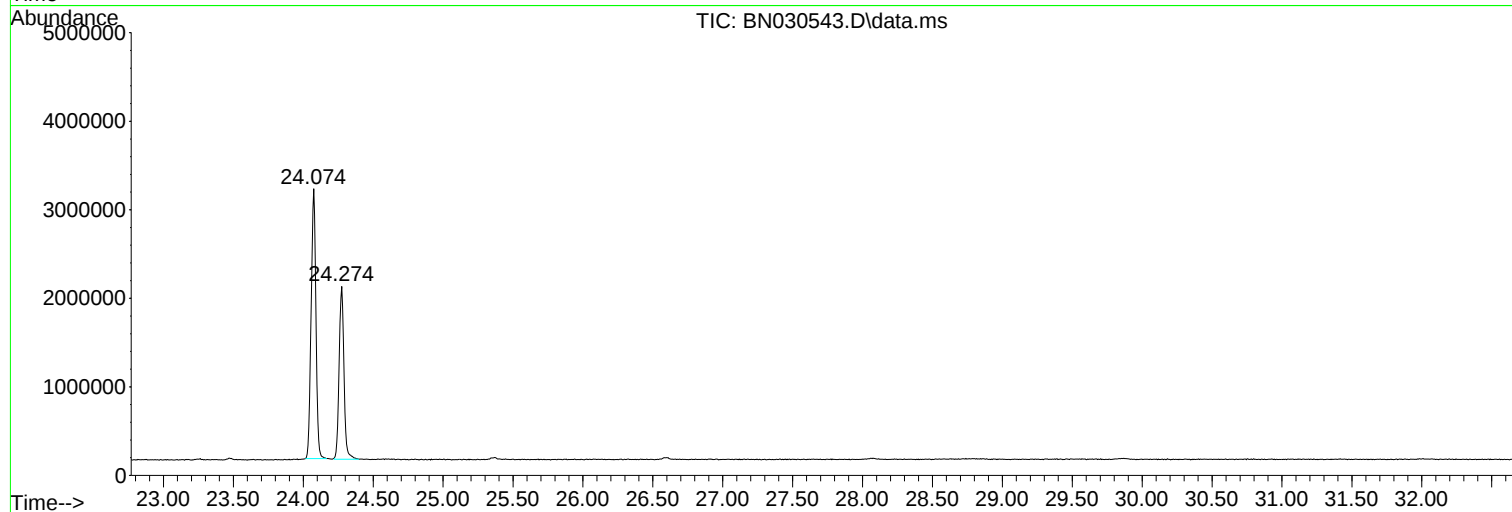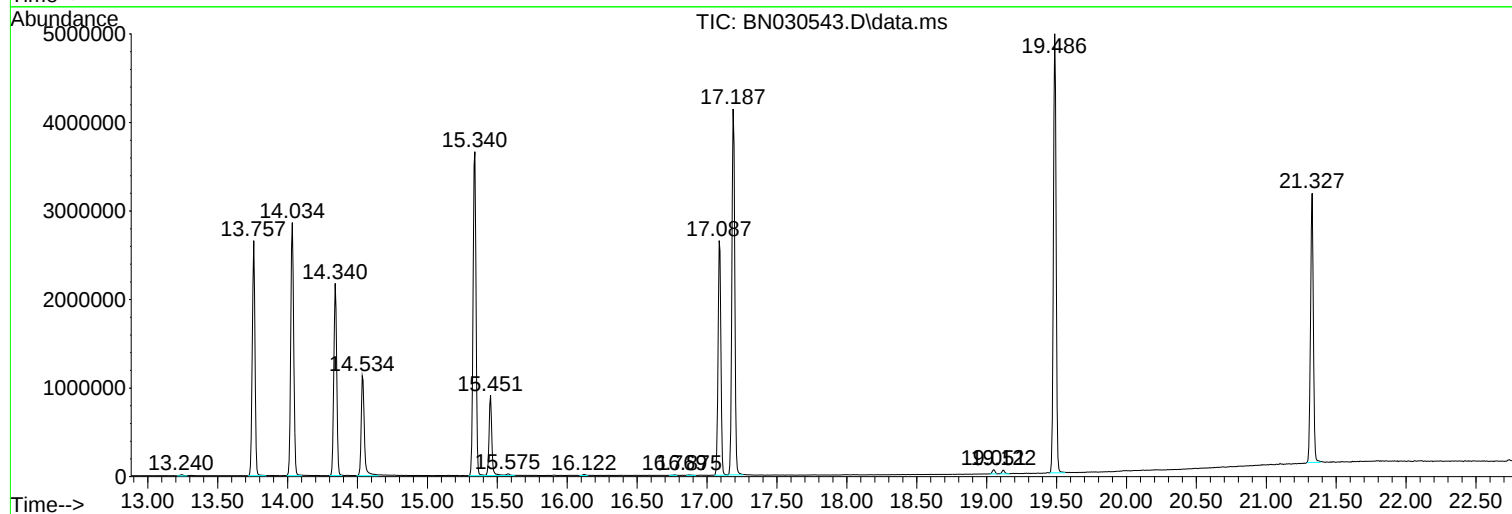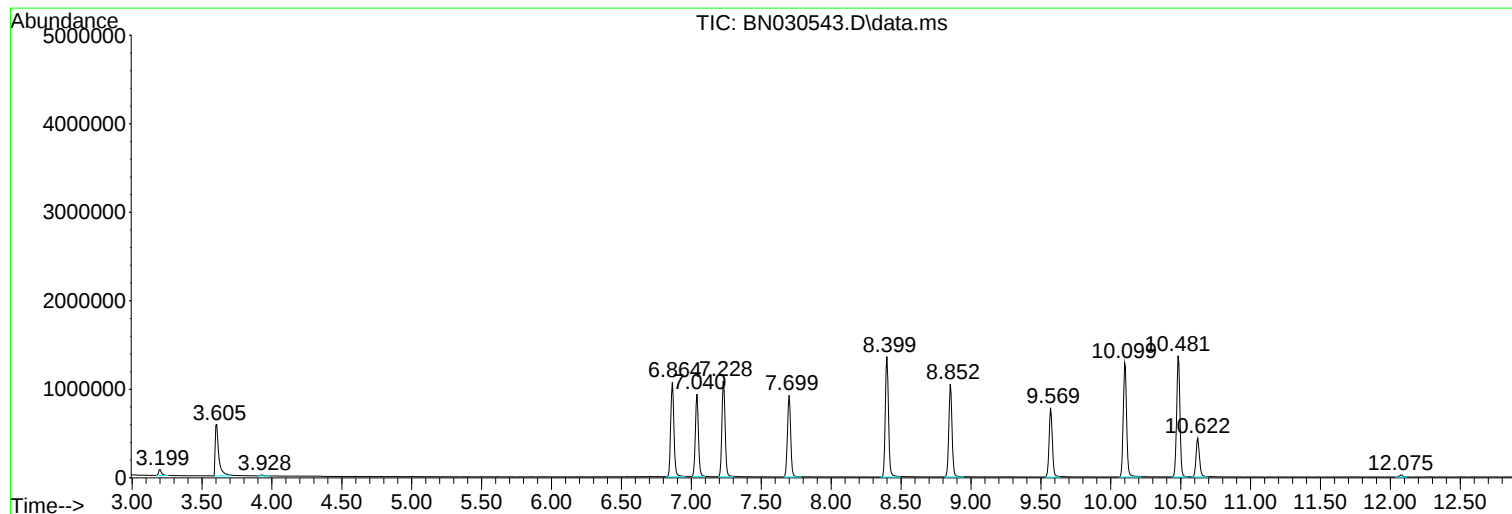

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030543.D
Acq On : 30 Mar 2024 10:11
Operator : MA/JU
Sample : PB159892BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK892

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030543.D
Acq On : 30 Mar 2024 10:11
Operator : MA/JU
Sample : PB159892BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK892

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc