

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030544.D
 Acq On : 30 Mar 2024 10:50
 Operator : MA/JU
 Sample : P1929-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030544.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	25	30	57	rVB2	1013410	2128582	19.16%	2.306%
2	3.605	103	105	125	rBV	269214	519909	4.68%	0.563%
3	3.928	156	160	168	rVB	12278	18624	0.17%	0.020%
4	4.440	242	247	262	rBV	369456	683921	6.16%	0.741%
5	4.834	308	314	321	rVB7	5093	11672	0.11%	0.013%
6	6.863	654	659	672	rVB	337067	541529	4.88%	0.587%
7	7.040	682	689	701	rBV	1336453	2120796	19.09%	2.298%
8	7.228	714	721	734	rBV	1198227	1990413	17.92%	2.157%
9	7.316	734	736	745	rVB7	9335	17853	0.16%	0.019%
10	7.699	793	801	810	rBV	999307	1630872	14.68%	1.767%
11	8.399	913	920	936	rBV	999214	1608336	14.48%	1.743%
12	8.852	990	997	1011	rBV	1533825	2541418	22.88%	2.754%
13	9.269	1062	1068	1073	rVB	8189	14022	0.13%	0.015%
14	9.569	1110	1119	1137	rBV	1114291	1839057	16.56%	1.993%
15	9.693	1137	1140	1149	rVB8	6942	15472	0.14%	0.017%
16	10.099	1202	1209	1223	rBV	1755105	2890299	26.02%	3.132%
17	10.481	1267	1274	1289	rBV	1455279	2445482	22.02%	2.650%
18	10.622	1289	1298	1313	rBV	1711242	2866929	25.81%	3.106%
19	12.075	1539	1545	1554	rVB2	34697	58248	0.52%	0.063%
20	13.245	1738	1744	1749	rVB	19869	31869	0.29%	0.035%
21	13.757	1824	1831	1844	rBV	3711173	5023877	45.23%	5.443%
22	14.034	1868	1878	1892	rBV	4198418	6133967	55.22%	6.646%
23	14.340	1923	1930	1940	rBV	2316882	3346470	30.13%	3.626%
24	14.422	1942	1944	1950	rVB6	7488	11246	0.10%	0.012%
25	14.534	1957	1963	1978	rBV	295820	480212	4.32%	0.520%
26	14.763	1997	2002	2006	rVB3	8088	12181	0.11%	0.013%
27	15.151	2064	2068	2075	rBV2	17382	24634	0.22%	0.027%
28	15.340	2093	2100	2112	rBV	5160105	7612222	68.53%	8.247%
29	15.451	2112	2119	2132	rVV	1407802	1876712	16.90%	2.033%
30	15.575	2135	2140	2145	rVB	24087	38218	0.34%	0.041%
31	16.122	2229	2233	2239	rVB4	19529	27954	0.25%	0.030%
32	17.086	2391	2397	2407	rBV	2848345	4063466	36.58%	4.403%
33	17.186	2408	2414	2433	rVB2	5731134	8482294	76.37%	9.190%
34	17.775	2510	2514	2519	rVB2	25618	35135	0.32%	0.038%
35	17.992	2546	2551	2557	rBV2	58132	79451	0.72%	0.086%
36	19.051	2726	2731	2735	rBV2	77343	110098	0.99%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030544.D
Acq On : 30 Mar 2024 10:50
Operator : MA/JU
Sample : P1929-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.092	2735	2738	2740	rVV	31439	41299	0.37%	0.045%
38	19.122	2740	2743	2749	rVB	65694	86529	0.78%	0.094%
39	19.280	2766	2770	2779	rBV2	53252	78659	0.71%	0.085%
40	19.486	2799	2805	2815	rBV	7099350	9943745	89.52%	10.774%
41	21.327	3112	3118	3129	rBV	3293573	4561080	41.06%	4.942%
42	24.080	3575	3586	3605	rBV2	4608560	11107461	100.00%	12.034%
43	24.274	3610	3619	3643	rVB	2134764	5145220	46.32%	5.575%




Sum of corrected areas: 92297433

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030544.D
Acq On : 30 Mar 2024 10:50
Operator : MA/JU
Sample : P1929-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

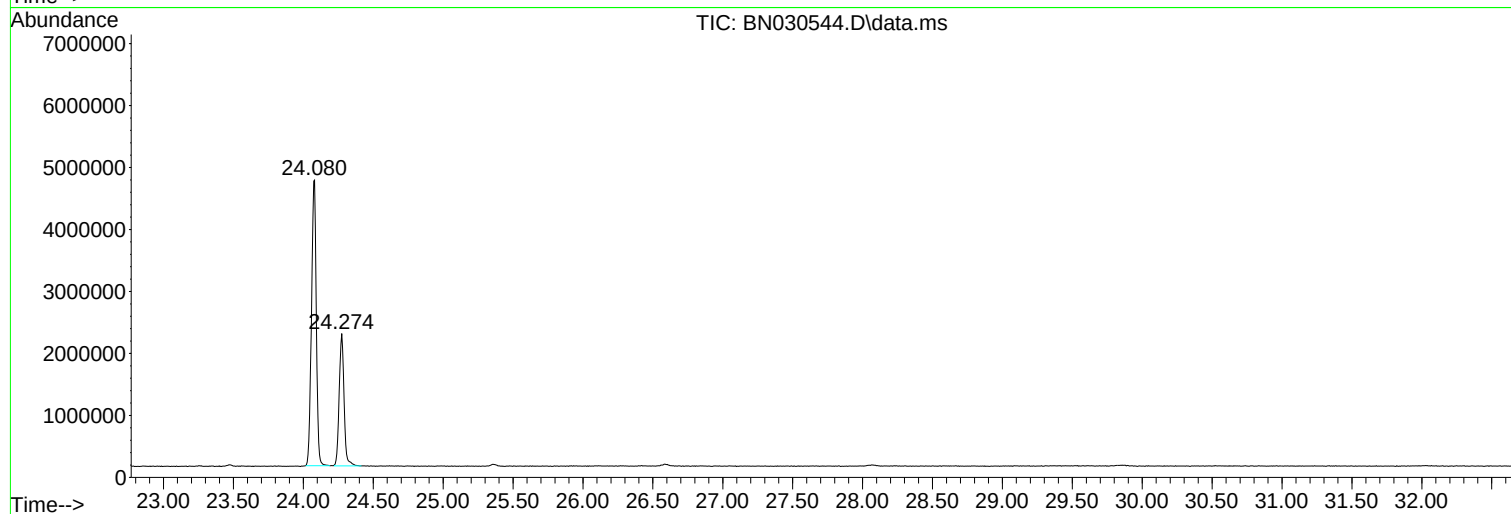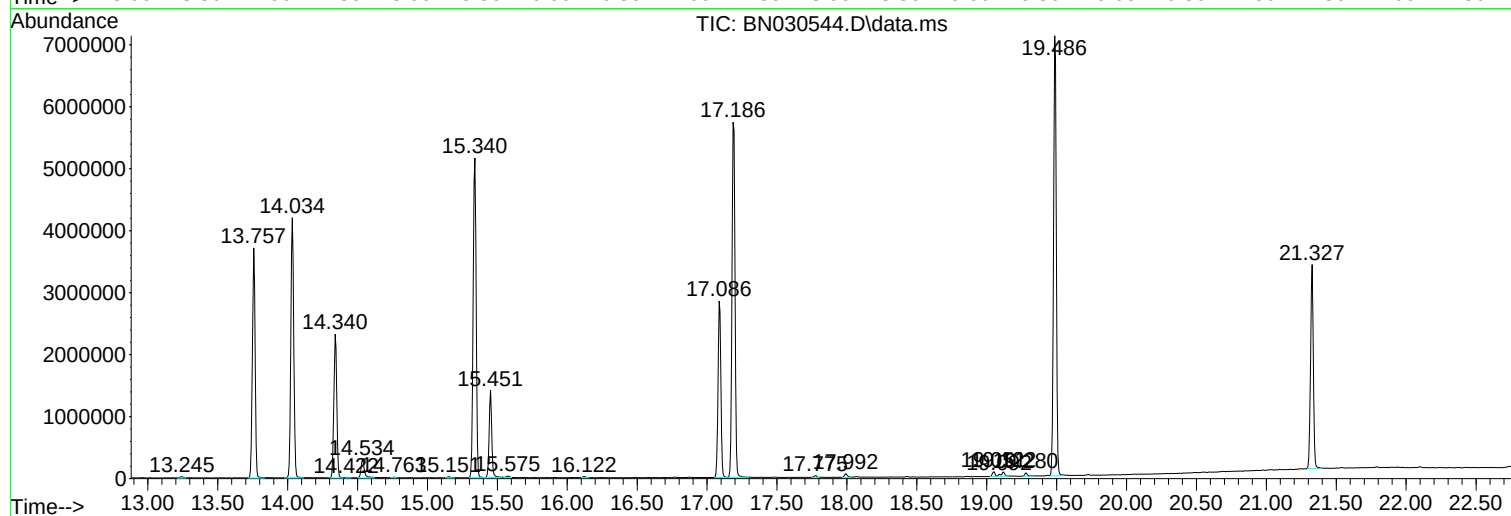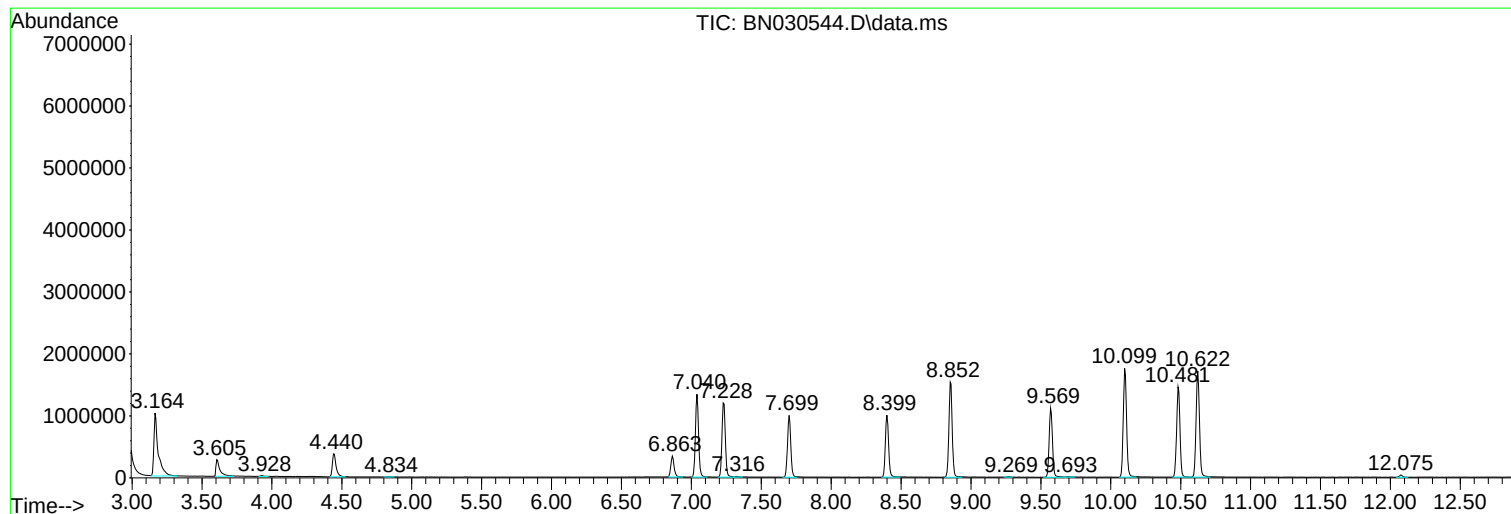

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030544.D
Acq On : 30 Mar 2024 10:50
Operator : MA/JU
Sample : P1929-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030544.D
Acq On : 30 Mar 2024 10:50
Operator : MA/JU
Sample : P1929-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc