

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030545.D
 Acq On : 30 Mar 2024 11:29
 Operator : MA/JU
 Sample : P1929-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	25	30	55	rVB2	1005860	1863021	19.41%	2.367%
2	3.605	102	105	124	rBV	263557	425473	4.43%	0.541%
3	3.928	157	160	166	rVB2	11793	18263	0.19%	0.023%
4	4.440	241	247	259	rBV	362655	589406	6.14%	0.749%
5	6.863	653	659	677	rBV	270665	439773	4.58%	0.559%
6	7.040	681	689	704	rBV	1157888	1823116	19.00%	2.317%
7	7.228	714	721	733	rBV	1041325	1665803	17.36%	2.117%
8	7.322	734	737	743	rVB5	8518	16285	0.17%	0.021%
9	7.699	794	801	810	rBV	820653	1316600	13.72%	1.673%
10	8.399	912	920	936	rBV	837118	1331037	13.87%	1.691%
11	8.852	989	997	1010	rBV	1304494	2182718	22.74%	2.774%
12	8.957	1012	1015	1021	rVB5	9108	15601	0.16%	0.020%
13	9.569	1113	1119	1133	rBV	960872	1559555	16.25%	1.982%
14	10.099	1201	1209	1228	rBV	1495694	2499930	26.05%	3.177%
15	10.481	1266	1274	1289	rBV	1199375	2014592	20.99%	2.560%
16	10.622	1289	1298	1318	rBV	1525544	2596184	27.05%	3.299%
17	12.075	1539	1545	1552	rBV2	28276	46336	0.48%	0.059%
18	13.245	1738	1744	1750	rBV2	20359	33895	0.35%	0.043%
19	13.757	1824	1831	1846	rBV	3149171	4282150	44.62%	5.442%
20	14.034	1870	1878	1895	rBV	3563693	5289896	55.12%	6.722%
21	14.339	1923	1930	1941	rBV	1880171	2747836	28.63%	3.492%
22	14.534	1957	1963	1977	rBV	230294	374216	3.90%	0.476%
23	15.151	2063	2068	2075	rBV2	20850	30193	0.31%	0.038%
24	15.339	2093	2100	2111	rBV	4594273	6556231	68.32%	8.332%
25	15.451	2113	2119	2135	rVV	1165951	1612477	16.80%	2.049%
26	15.575	2136	2140	2147	rVB3	20950	34964	0.36%	0.044%
27	16.122	2229	2233	2238	rVB3	14349	20530	0.21%	0.026%
28	16.769	2337	2343	2348	rVB6	7524	10697	0.11%	0.014%
29	17.086	2391	2397	2407	rBV	2331646	3368638	35.10%	4.281%
30	17.186	2408	2414	2435	rVB2	5014839	7387381	76.98%	9.388%
31	17.775	2509	2514	2518	rBV3	9867	13227	0.14%	0.017%
32	17.992	2546	2551	2559	rBV3	30843	47235	0.49%	0.060%
33	19.051	2726	2731	2735	rBV2	64495	90606	0.94%	0.115%
34	19.122	2739	2743	2747	rVB	54750	71214	0.74%	0.090%
35	19.280	2766	2770	2774	rBV2	26296	36298	0.38%	0.046%
36	19.486	2799	2805	2814	rVV	6156757	8700865	90.66%	11.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030545.D
Acq On : 30 Mar 2024 11:29
Operator : MA/JU
Sample : P1929-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.727	2843	2846	2849	rVB	11736	12548	0.13%	0.016%
38	21.327	3112	3118	3129	rBV	2657704	3811192	39.71%	4.843%
39	24.074	3575	3585	3601	rBV2	4034856	9596792	100.00%	12.195%
40	24.274	3610	3619	3637	rVB	1699387	4158917	43.34%	5.285%




Sum of corrected areas: 78691691

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030545.D
Acq On : 30 Mar 2024 11:29
Operator : MA/JU
Sample : P1929-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

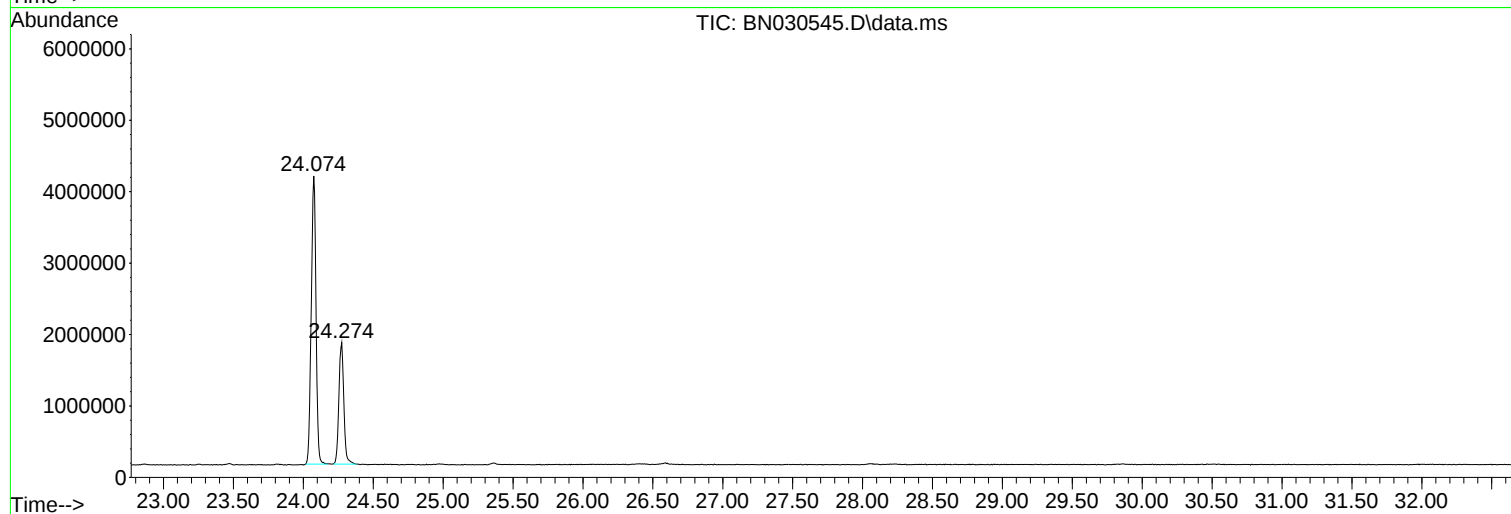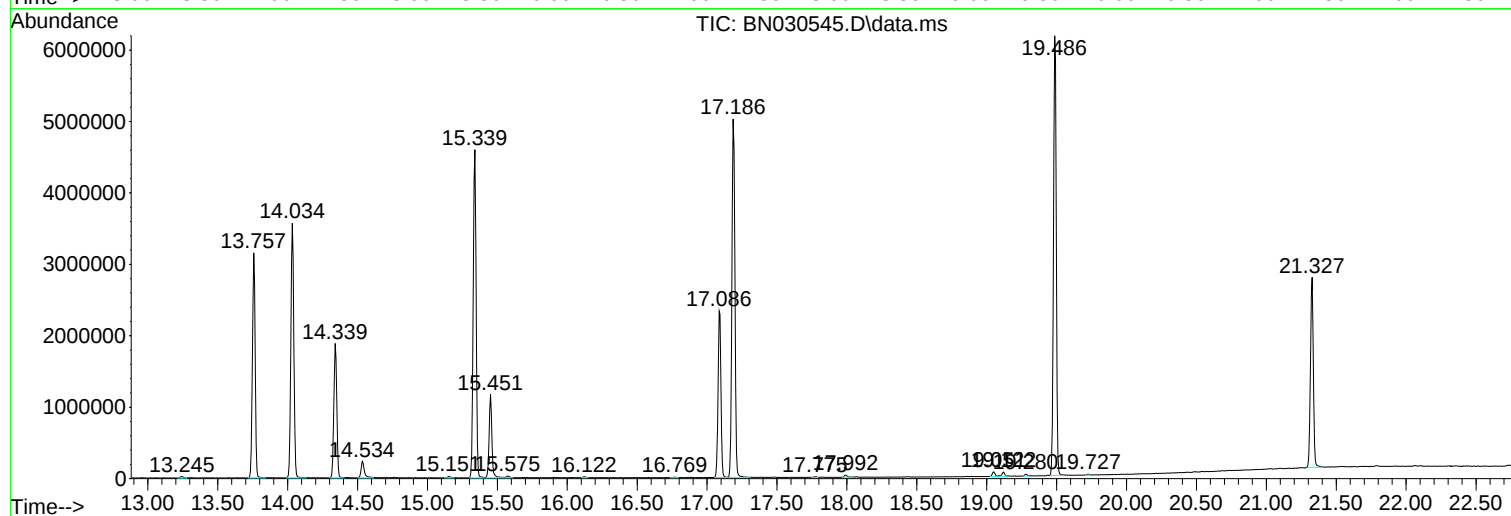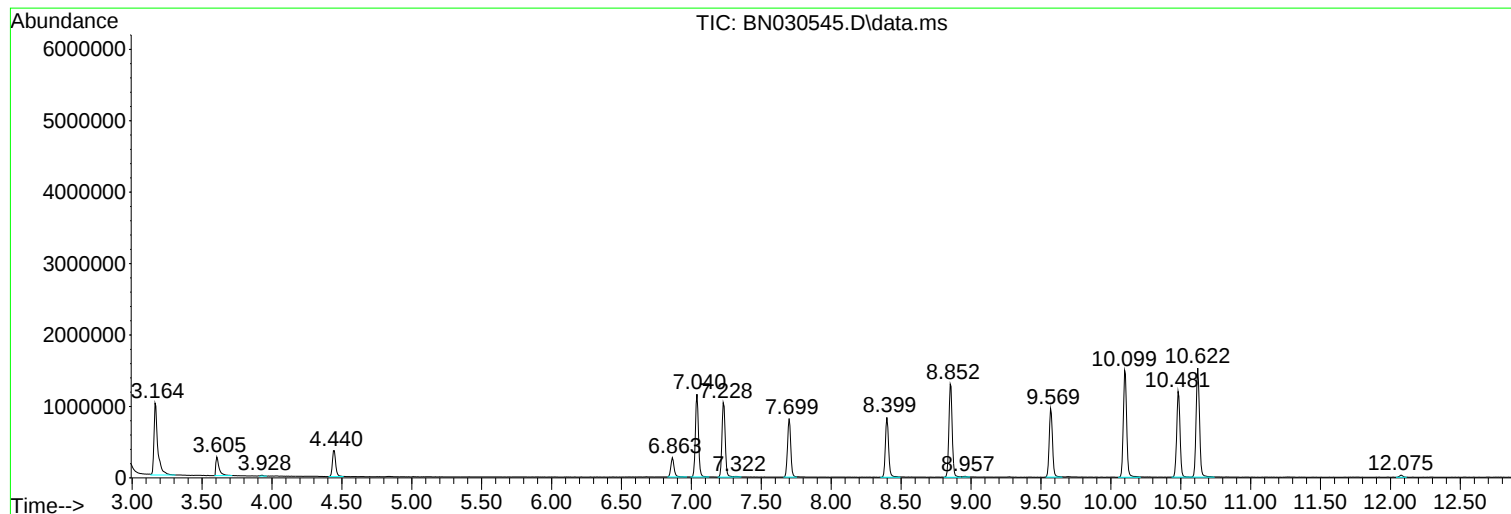

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030545.D
Acq On : 30 Mar 2024 11:29
Operator : MA/JU
Sample : P1929-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030545.D
Acq On : 30 Mar 2024 11:29
Operator : MA/JU
Sample : P1929-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc