

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030547.D
 Acq On : 30 Mar 2024 12:48
 Operator : MA/JU
 Sample : P1929-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	40	rBV	43940	61200	0.75%	0.095%
2	3.605	103	105	121	rBV	179937	309150	3.76%	0.477%
3	3.922	156	159	167	rVB	11173	18242	0.22%	0.028%
4	5.769	469	473	478	rVB5	6971	10779	0.13%	0.017%
5	6.863	652	659	677	rVB	222420	360681	4.39%	0.557%
6	7.040	682	689	703	rBV	939746	1475780	17.97%	2.279%
7	7.228	713	721	734	rBV	857878	1363931	16.61%	2.107%
8	7.316	734	736	741	rVB6	5424	8891	0.11%	0.014%
9	7.699	793	801	810	rBV	778305	1216198	14.81%	1.878%
10	8.398	913	920	938	rBV	679224	1082822	13.18%	1.672%
11	8.851	990	997	1010	rBV	1075400	1742385	21.22%	2.691%
12	9.569	1112	1119	1133	rBV	754185	1225342	14.92%	1.893%
13	10.098	1202	1209	1223	rBV	1184691	2026320	24.67%	3.130%
14	10.487	1266	1275	1286	rBV	1064274	1843230	22.44%	2.847%
15	10.622	1289	1298	1312	rBV	1102391	1871950	22.79%	2.891%
16	12.075	1536	1545	1553	rVB	22691	37123	0.45%	0.057%
17	13.245	1734	1744	1750	rBV2	18995	43150	0.53%	0.067%
18	13.757	1824	1831	1843	rBV	2560803	3529732	42.98%	5.452%
19	14.033	1867	1878	1891	rBV	2982872	4367919	53.18%	6.746%
20	14.339	1923	1930	1942	rBV	1756363	2522710	30.72%	3.896%
21	14.533	1957	1963	1976	rBV	178709	302190	3.68%	0.467%
22	14.763	1998	2002	2006	rVB7	6665	9881	0.12%	0.015%
23	15.151	2063	2068	2075	rBV2	15964	29167	0.36%	0.045%
24	15.339	2093	2100	2110	rBV	3816010	5504046	67.02%	8.501%
25	15.451	2112	2119	2131	rVV	879250	1208288	14.71%	1.866%
26	15.575	2136	2140	2148	rVB3	15907	29373	0.36%	0.045%
27	16.122	2229	2233	2239	rVB5	13147	19437	0.24%	0.030%
28	17.086	2391	2397	2407	rBV	2045702	3047916	37.11%	4.707%
29	17.186	2408	2414	2429	rVV2	4235108	6260174	76.22%	9.669%
30	17.992	2548	2551	2557	rBV4	27644	39505	0.48%	0.061%
31	19.051	2728	2731	2735	rVB	67203	78804	0.96%	0.122%
32	19.121	2740	2743	2746	rVB	50345	65986	0.80%	0.102%
33	19.486	2799	2805	2814	rBV	5446327	7528833	91.67%	11.628%
34	21.327	3113	3118	3123	rBV2	2337708	3338498	40.65%	5.156%
35	24.074	3576	3585	3598	rVB2	3549472	8212982	100.00%	12.685%
36	24.274	3610	3619	3636	rVB	1531710	3953461	48.14%	6.106%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030547.D
Acq On : 30 Mar 2024 12:48
Operator : MA/JU
Sample : P1929-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 64746076

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030547.D
Acq On : 30 Mar 2024 12:48
Operator : MA/JU
Sample : P1929-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAL8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

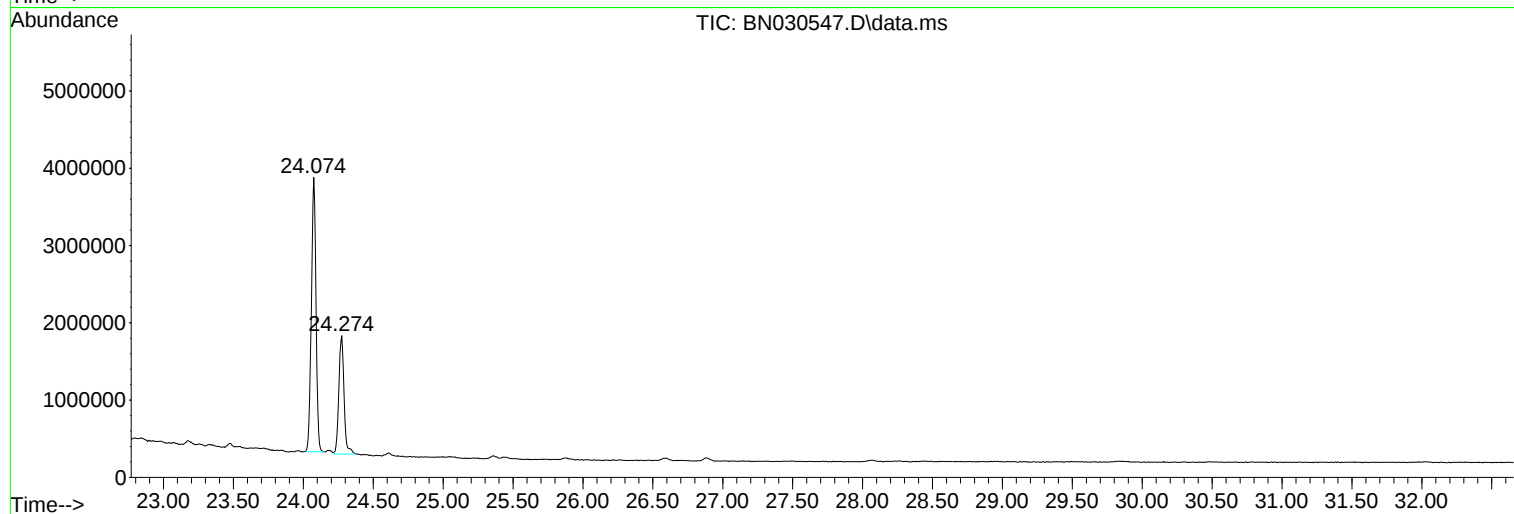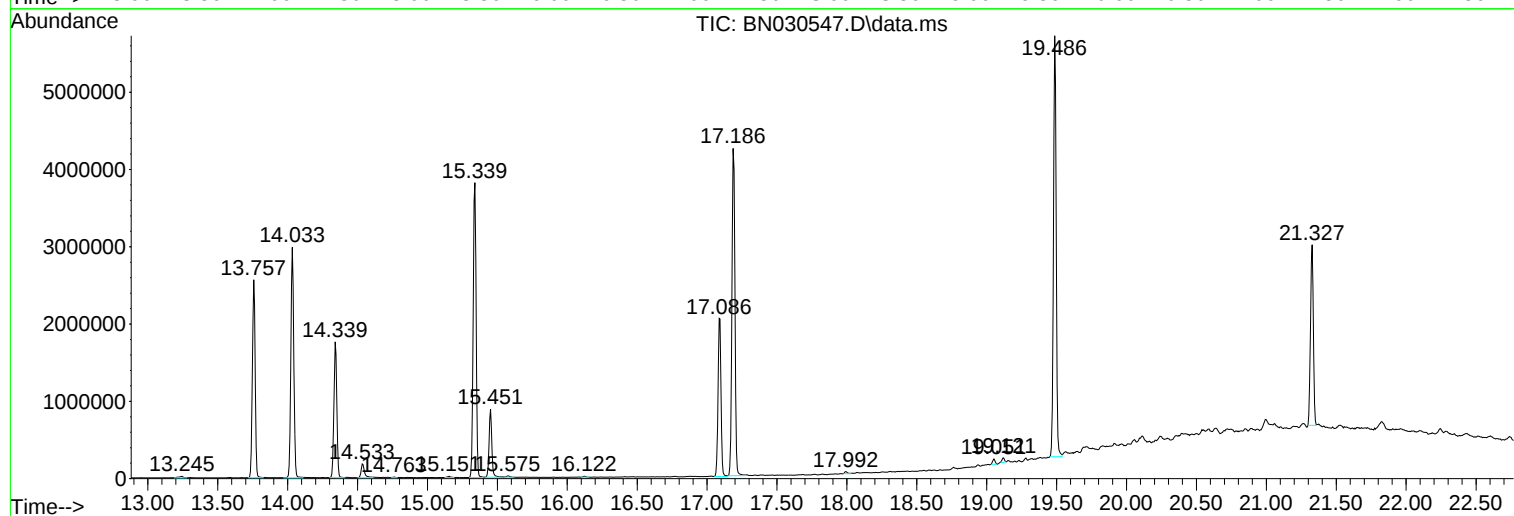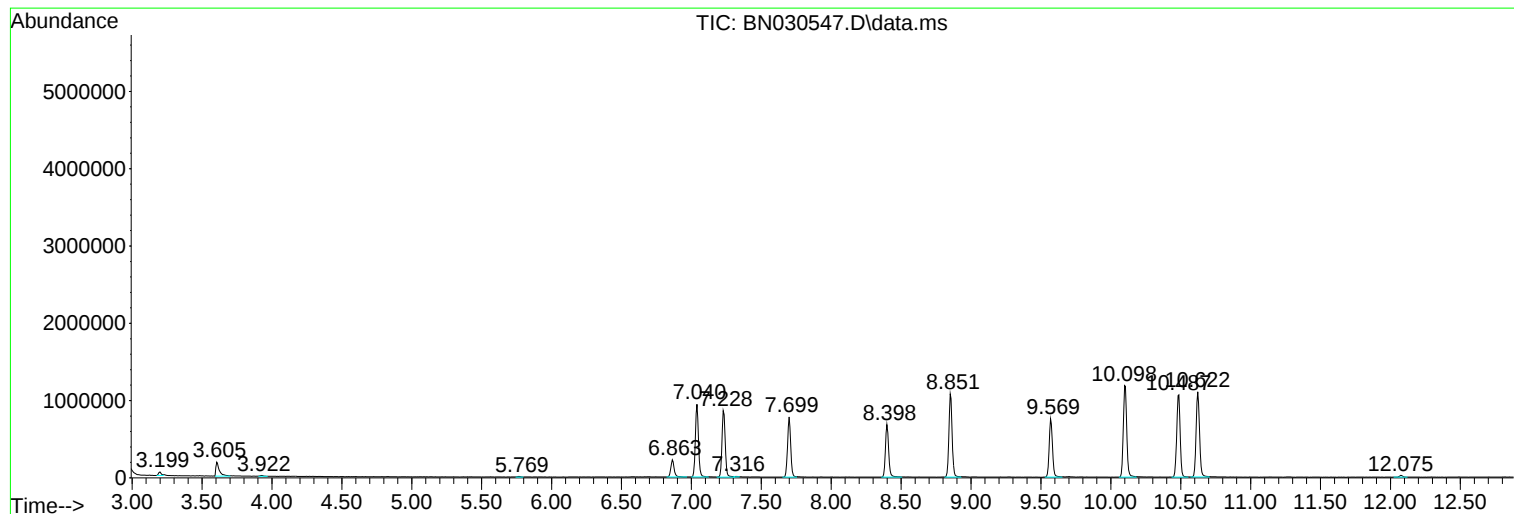

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030547.D
Acq On : 30 Mar 2024 12:48
Operator : MA/JU
Sample : P1929-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030547.D
Acq On : 30 Mar 2024 12:48
Operator : MA/JU
Sample : P1929-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AL8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------