

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030550.D
 Acq On : 30 Mar 2024 14:46
 Operator : MA/JU
 Sample : P1931-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07C4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030550.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	42	rVB2	12711	18604	0.42%	0.062%
2	3.611	104	106	120	rBV	49241	91906	2.09%	0.307%
3	3.928	156	160	166	rVB	10721	16142	0.37%	0.054%
4	4.828	307	313	320	rBV4	9312	20775	0.47%	0.069%
5	6.864	652	659	669	rBV	175783	306084	6.95%	1.022%
6	7.040	683	689	701	rBV	166529	268005	6.08%	0.895%
7	7.228	715	721	730	rBV	173379	285175	6.47%	0.953%
8	7.328	733	738	741	rVB4	6819	9055	0.21%	0.030%
9	7.699	792	801	810	rBV	833023	1312208	29.78%	4.383%
10	8.246	886	894	898	rVV9	3734	9403	0.21%	0.031%
11	8.399	914	920	929	rBV	209812	341111	7.74%	1.139%
12	8.522	934	941	946	rVV	40344	66792	1.52%	0.223%
13	8.852	991	997	1005	rVV	169804	286886	6.51%	0.958%
14	8.922	1005	1009	1020	rVV6	14296	26984	0.61%	0.090%
15	9.016	1020	1025	1029	rVV8	6295	12967	0.29%	0.043%
16	9.269	1063	1068	1073	rBV3	8153	12543	0.28%	0.042%
17	9.334	1075	1079	1084	rBV6	4113	7681	0.17%	0.026%
18	9.422	1086	1094	1098	rVV9	5727	11346	0.26%	0.038%
19	9.569	1111	1119	1130	rBV	106717	192893	4.38%	0.644%
20	9.922	1175	1179	1185	rVB10	7896	16308	0.37%	0.054%
21	10.105	1200	1210	1220	rBV	202133	352289	8.00%	1.177%
22	10.269	1233	1238	1247	rBV	58444	94305	2.14%	0.315%
23	10.481	1264	1274	1290	rBV	1185374	2060545	46.77%	6.883%
24	10.622	1292	1298	1302	rBV	30353	65382	1.48%	0.218%
25	10.781	1320	1325	1329	rVB7	4371	8003	0.18%	0.027%
26	10.975	1354	1358	1361	rBV5	5057	8081	0.18%	0.027%
27	11.028	1363	1367	1373	rVB8	4944	9191	0.21%	0.031%
28	11.157	1381	1389	1390	rBV7	5676	10435	0.24%	0.035%
29	11.234	1397	1402	1406	rBV7	5415	11049	0.25%	0.037%
30	11.322	1412	1417	1424	rVV10	5696	11758	0.27%	0.039%
31	11.404	1424	1431	1437	rVB7	9926	21164	0.48%	0.071%
32	11.510	1444	1449	1458	rBV	23338	46112	1.05%	0.154%
33	11.587	1460	1462	1469	rVB7	4984	7345	0.17%	0.025%
34	11.769	1487	1493	1497	rBV8	6777	10971	0.25%	0.037%
35	11.916	1512	1518	1524	rBV	61970	93239	2.12%	0.311%
36	12.057	1537	1542	1545	rBV6	5568	9837	0.22%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030550.D
 Acq On : 30 Mar 2024 14:46
 Operator : MA/JU
 Sample : P1931-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07C4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	12.146	1550	1557	1563	rVB4	17148	36262	0.82%	0.121%
38	12.375	1589	1596	1599	rBV2	13833	22703	0.52%	0.076%
39	12.557	1624	1627	1630	rVB5	6052	7805	0.18%	0.026%
40	12.599	1630	1634	1635	rBV4	7468	8198	0.19%	0.027%
41	12.740	1654	1658	1664	rBV4	7738	12342	0.28%	0.041%
42	12.828	1669	1673	1677	rBV3	7492	11369	0.26%	0.038%
43	12.881	1677	1682	1688	rVV2	25271	37482	0.85%	0.125%
44	13.169	1724	1731	1739	rBV	74359	119963	2.72%	0.401%
45	13.240	1739	1743	1753	rVV5	13776	33949	0.77%	0.113%
46	13.498	1782	1787	1788	rBV5	8826	11959	0.27%	0.040%
47	13.663	1810	1815	1818	rBV3	18781	30764	0.70%	0.103%
48	13.716	1819	1824	1826	rVV5	13945	24053	0.55%	0.080%
49	13.757	1826	1831	1837	rVV	488550	664956	15.09%	2.221%
50	13.834	1837	1844	1848	rVB3	29078	51441	1.17%	0.172%
51	13.875	1848	1851	1858	rBV6	13025	26462	0.60%	0.088%
52	14.034	1869	1878	1888	rBV	509078	774976	17.59%	2.589%
53	14.181	1899	1903	1909	rVB9	6411	13684	0.31%	0.046%
54	14.251	1909	1915	1920	rBV	86709	115046	2.61%	0.384%
55	14.340	1923	1930	1938	rBV	1915744	2795760	63.45%	9.338%
56	14.534	1958	1963	1977	rBV2	117076	243658	5.53%	0.814%
57	14.745	1995	1999	2007	rVV6	15507	36821	0.84%	0.123%
58	14.816	2007	2011	2015	rVB5	13689	20439	0.46%	0.068%
59	14.875	2018	2021	2027	rVB6	17112	25233	0.57%	0.084%
60	14.957	2029	2035	2041	rBV7	9315	20763	0.47%	0.069%
61	15.010	2041	2044	2050	rVB6	8188	13083	0.30%	0.044%
62	15.204	2073	2077	2083	rVB	73237	89722	2.04%	0.300%
63	15.334	2091	2099	2106	rBV	712335	1027025	23.31%	3.431%
64	15.445	2113	2118	2125	rBV	97187	152865	3.47%	0.511%
65	15.569	2134	2139	2142	rBV7	8598	15576	0.35%	0.052%
66	15.610	2142	2146	2151	rVB3	22474	36794	0.84%	0.123%
67	15.710	2160	2163	2168	rVB5	9976	13924	0.32%	0.047%
68	15.769	2168	2173	2177	rBV7	7811	12706	0.29%	0.042%
69	15.834	2177	2184	2190	rVV10	9268	19996	0.45%	0.067%
70	15.934	2192	2201	2211	rBV3	17838	45669	1.04%	0.153%
71	16.069	2220	2224	2240	rVB	75766	139237	3.16%	0.465%
72	16.204	2243	2247	2250	rBV4	4493	7432	0.17%	0.025%
73	16.645	2316	2322	2324	rBV6	6517	9771	0.22%	0.033%
74	16.863	2353	2359	2363	rBV2	46339	61814	1.40%	0.206%
75	16.916	2363	2368	2373	rVB5	14271	23122	0.52%	0.077%
76	17.087	2391	2397	2403	rBV	2357561	3384558	76.82%	11.305%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030550.D
 Acq On : 30 Mar 2024 14:46
 Operator : MA/JU
 Sample : P1931-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07C4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

77	17.187	2409	2414	2424	rVB	807617	1138250	25.83%	3.802%
78	17.281	2426	2430	2434	rVB6	12553	20762	0.47%	0.069%
79	17.486	2460	2465	2469	rBV5	28994	43520	0.99%	0.145%
80	17.598	2481	2484	2489	rBV	32513	40599	0.92%	0.136%
81	17.775	2510	2514	2518	rBV6	6436	7206	0.16%	0.024%
82	17.992	2541	2551	2559	rBV3	78805	156050	3.54%	0.521%
83	18.151	2574	2578	2583	rBV7	11132	20909	0.47%	0.070%
84	18.198	2583	2586	2592	rVB3	9783	12419	0.28%	0.041%
85	18.298	2598	2603	2612	rBV4	25748	45295	1.03%	0.151%
86	18.434	2621	2626	2630	rBV3	57212	69497	1.58%	0.232%
87	18.563	2645	2648	2652	rVV5	7528	10023	0.23%	0.033%
88	18.763	2679	2682	2685	rBV4	7479	9338	0.21%	0.031%
89	18.792	2685	2687	2694	rVV6	6802	10181	0.23%	0.034%
90	18.886	2701	2703	2708	rVB3	10884	11581	0.26%	0.039%
91	18.933	2708	2711	2717	rBV6	16644	24779	0.56%	0.083%
92	19.151	2744	2748	2753	rVB	70198	98940	2.25%	0.330%
93	19.216	2756	2759	2763	rVB3	21481	28108	0.64%	0.094%
94	19.281	2767	2770	2780	rVB4	28717	43504	0.99%	0.145%
95	19.486	2799	2805	2815	rBV	1191992	1681990	38.17%	5.618%
96	19.663	2831	2835	2841	rBV2	64696	83956	1.91%	0.280%
97	21.022	3062	3066	3072	rBV4	84343	130117	2.95%	0.435%
98	21.327	3112	3118	3124	rBV	2736319	3944977	89.54%	13.177%
99	24.063	3576	3583	3598	rVB2	657839	1568084	35.59%	5.238%
100	24.274	3610	3619	3638	rVB	1723201	4406007	100.00%	14.717%




Sum of corrected areas: 29938048

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030550.D
Acq On : 30 Mar 2024 14:46
Operator : MA/JU
Sample : P1931-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

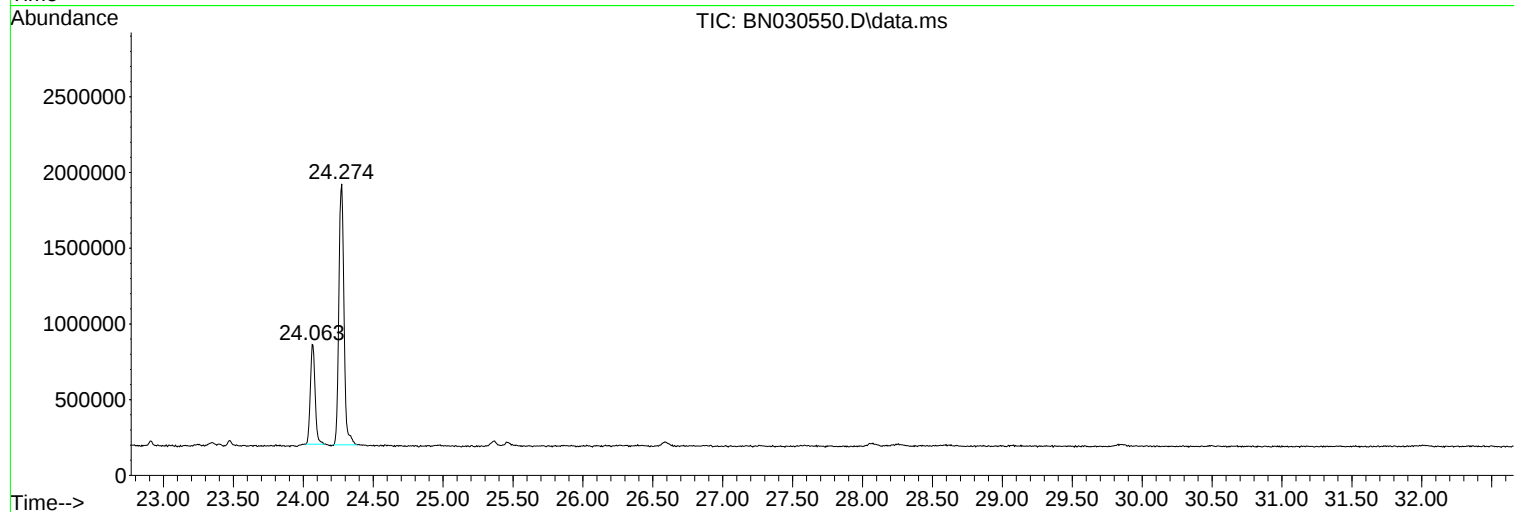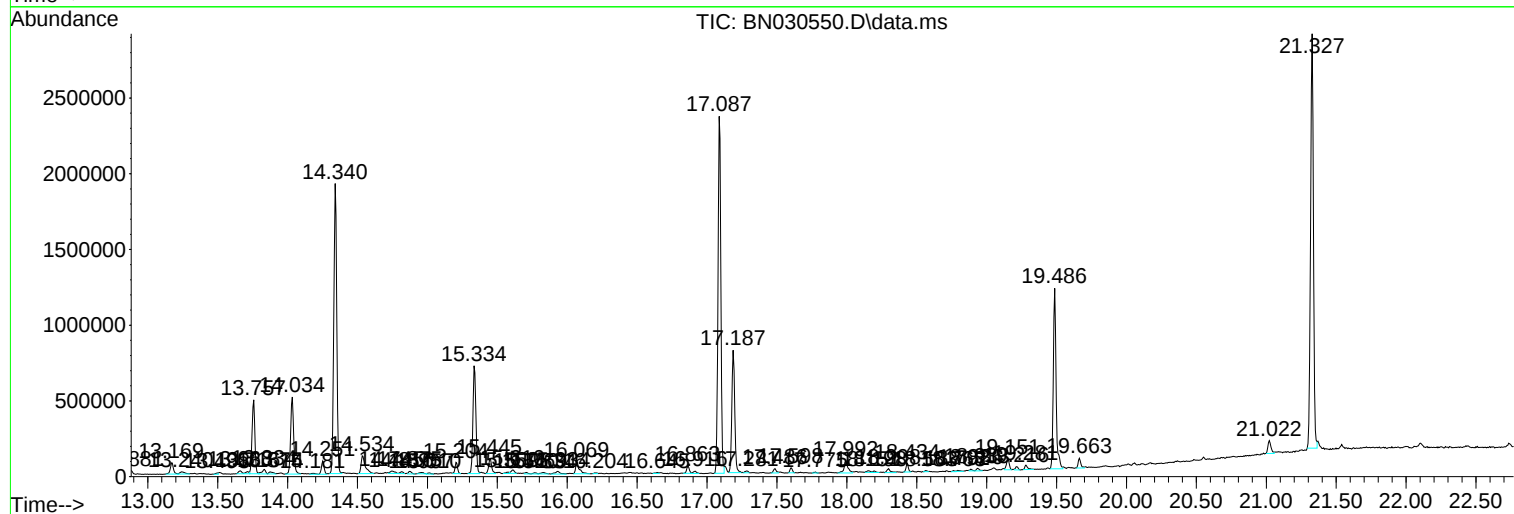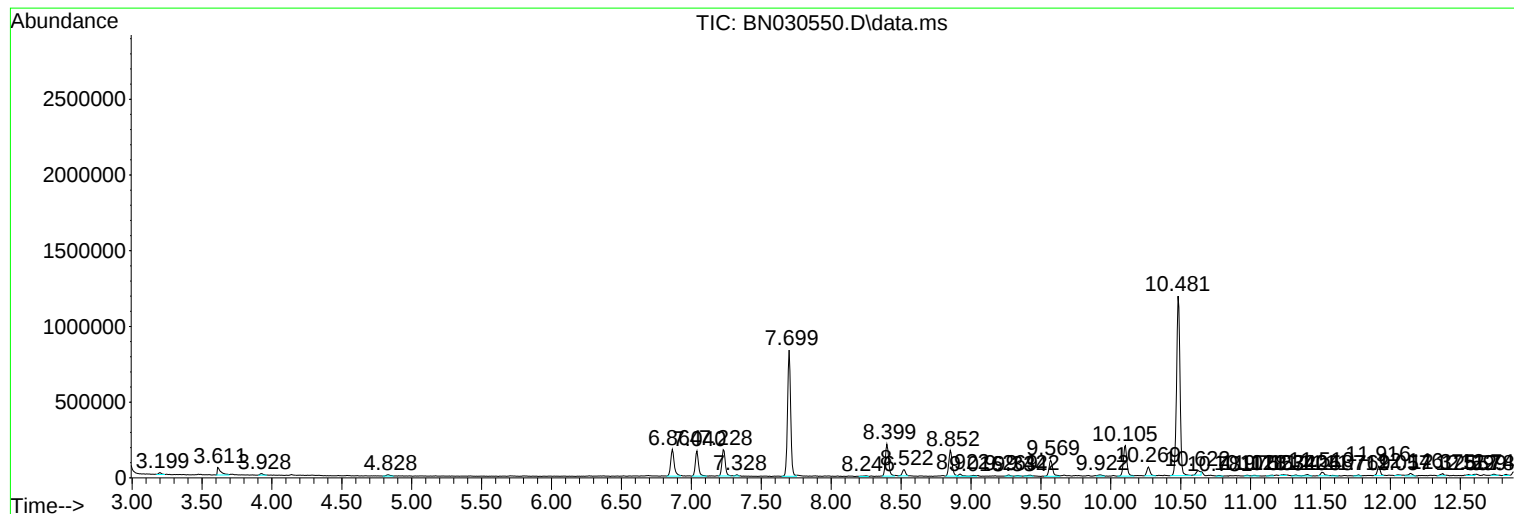

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030550.D
Acq On : 30 Mar 2024 14:46
Operator : MA/JU
Sample : P1931-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030550.D
Acq On : 30 Mar 2024 14:46
Operator : MA/JU
Sample : P1931-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc