

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030552.D
 Acq On : 30 Mar 2024 16:05
 Operator : MA/JU
 Sample : P1931-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07C7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030552.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	33	36	42	rVB	15663	23166	0.59%	0.079%
2	3.611	105	106	118	rBV	50199	89077	2.27%	0.305%
3	3.928	156	160	164	rVB2	9674	13401	0.34%	0.046%
4	4.140	193	196	202	rVB6	10503	12863	0.33%	0.044%
5	4.552	261	266	271	rVB8	7181	11267	0.29%	0.039%
6	4.828	309	313	318	rVB3	9949	14480	0.37%	0.050%
7	6.863	650	659	673	rBV	216846	378946	9.65%	1.299%
8	7.040	683	689	701	rVB	189613	303862	7.74%	1.042%
9	7.228	714	721	733	rBV	211598	352890	8.99%	1.210%
10	7.328	733	738	745	rVV9	8696	16682	0.42%	0.057%
11	7.399	745	750	754	rVB6	3461	5379	0.14%	0.018%
12	7.699	793	801	809	rBV	828893	1317847	33.57%	4.517%
13	8.399	913	920	931	rVV	257483	421817	10.75%	1.446%
14	8.522	934	941	949	rVB	52440	91197	2.32%	0.313%
15	8.852	990	997	1007	rBV	199612	339144	8.64%	1.163%
16	9.022	1021	1026	1030	rVB8	9363	15279	0.39%	0.052%
17	9.269	1062	1068	1074	rBV2	11596	20845	0.53%	0.071%
18	9.422	1088	1094	1102	rVB7	8335	14514	0.37%	0.050%
19	9.569	1113	1119	1126	rBV	119751	206452	5.26%	0.708%
20	9.693	1136	1140	1145	rBV6	3190	5769	0.15%	0.020%
21	9.934	1174	1181	1185	rBV6	6260	10150	0.26%	0.035%
22	10.104	1203	1210	1220	rBV	234366	403752	10.29%	1.384%
23	10.269	1232	1238	1247	rBV	108408	182469	4.65%	0.625%
24	10.481	1267	1274	1287	rBV	1183317	1982341	50.50%	6.795%
25	10.628	1293	1299	1307	rVB	25861	52516	1.34%	0.180%
26	11.016	1360	1365	1366	rBV5	5332	6142	0.16%	0.021%
27	11.228	1397	1401	1405	rBV5	5857	11086	0.28%	0.038%
28	11.263	1405	1407	1412	rVB6	3224	5365	0.14%	0.018%
29	11.910	1512	1517	1523	rBV7	4136	7856	0.20%	0.027%
30	12.081	1541	1546	1550	rVB5	4175	6988	0.18%	0.024%
31	13.175	1728	1732	1737	rVB4	8852	13505	0.34%	0.046%
32	13.240	1737	1743	1750	rBV3	15040	25251	0.64%	0.087%
33	13.757	1825	1831	1841	rBV	525116	734815	18.72%	2.519%
34	13.828	1841	1843	1849	rVB6	4200	5746	0.15%	0.020%
35	14.034	1871	1878	1888	rVB	589573	843192	21.48%	2.890%
36	14.251	1912	1915	1919	rBV3	8582	10032	0.26%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030552.D
 Acq On : 30 Mar 2024 16:05
 Operator : MA/JU
 Sample : P1931-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07C7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	14.340	1921	1930	1941	rBV	1817984	2714835	69.16%	9.306%
38	14.534	1958	1963	1981	rBV	129510	265375	6.76%	0.910%
39	14.769	1998	2003	2007	rVB4	12382	19536	0.50%	0.067%
40	15.151	2063	2068	2073	rBV6	6705	14102	0.36%	0.048%
41	15.204	2074	2077	2081	rVB4	10311	13661	0.35%	0.047%
42	15.334	2093	2099	2113	rBV	794606	1142959	29.12%	3.918%
43	15.451	2113	2119	2128	rBV	89404	140345	3.58%	0.481%
44	15.581	2137	2141	2143	rBV3	3018	4055	0.10%	0.014%
45	15.610	2144	2146	2150	rVB4	5574	5459	0.14%	0.019%
46	15.769	2168	2173	2175	rVV5	2945	5380	0.14%	0.018%
47	15.828	2179	2183	2186	rBV5	3297	5259	0.13%	0.018%
48	16.069	2221	2224	2227	rBV4	8883	12777	0.33%	0.044%
49	16.581	2305	2311	2315	rBV9	3493	6487	0.17%	0.022%
50	16.869	2355	2360	2364	rBV4	12097	19198	0.49%	0.066%
51	16.916	2364	2368	2371	rVB6	3881	6680	0.17%	0.023%
52	17.022	2382	2386	2391	rBV7	6573	7819	0.20%	0.027%
53	17.086	2391	2397	2408	rVV	2221079	3256037	82.94%	11.161%
54	17.186	2408	2414	2425	rVV	895662	1235014	31.46%	4.234%
55	17.281	2426	2430	2436	rVB6	21129	32319	0.82%	0.111%
56	17.386	2445	2448	2455	rVB4	6615	10779	0.27%	0.037%
57	17.481	2458	2464	2475	rBV2	69787	113536	2.89%	0.389%
58	17.598	2481	2484	2488	rVB5	8300	10725	0.27%	0.037%
59	17.769	2510	2513	2518	rVB5	6372	11061	0.28%	0.038%
60	17.869	2526	2530	2535	rBV7	6965	10917	0.28%	0.037%
61	17.992	2546	2551	2559	rBV2	94163	140296	3.57%	0.481%
62	18.292	2599	2602	2606	rBV6	8997	11815	0.30%	0.041%
63	18.433	2621	2626	2630	rBV	152278	177599	4.52%	0.609%
64	18.569	2645	2649	2653	rBV2	12571	15533	0.40%	0.053%
65	18.792	2685	2687	2691	rVB3	9143	10978	0.28%	0.038%
66	18.933	2709	2711	2716	rVB4	6810	7020	0.18%	0.024%
67	19.051	2728	2731	2735	rBV5	16398	20559	0.52%	0.070%
68	19.163	2747	2750	2754	rVB6	17463	21648	0.55%	0.074%
69	19.280	2766	2770	2777	rBV	59229	83114	2.12%	0.285%
70	19.433	2794	2796	2799	rVB4	11722	8279	0.21%	0.028%
71	19.486	2799	2805	2813	rBV	1185570	1637276	41.71%	5.612%
72	20.057	2898	2902	2906	rBV4	21461	33318	0.85%	0.114%
73	21.022	3062	3066	3071	rBV3	74982	125138	3.19%	0.429%
74	21.327	3112	3118	3123	rBV	2490516	3730761	95.04%	12.789%
75	22.063	3239	3243	3246	rBV3	77501	121037	3.08%	0.415%
76	22.863	3375	3379	3383	rBV2	96671	144172	3.67%	0.494%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030552.D
Acq On : 30 Mar 2024 16:05
Operator : MA/JU
Sample : P1931-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

77	23.810	3536	3540	3549	rVB3	124434	280474	7.14%	0.961%
78	24.063	3576	3583	3595	rVB2	694232	1657213	42.22%	5.681%
79	24.268	3610	3618	3628	rBV2	1550355	3925556	100.00%	13.457%




Sum of corrected areas: 29172184

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030552.D
Acq On : 30 Mar 2024 16:05
Operator : MA/JU
Sample : P1931-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

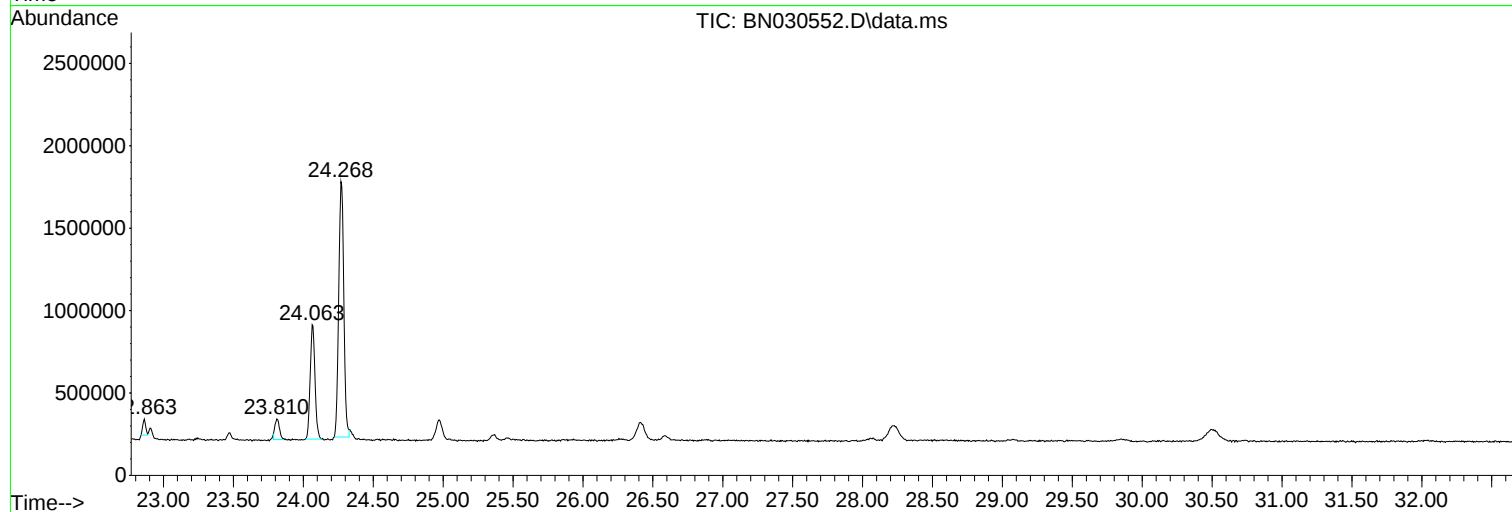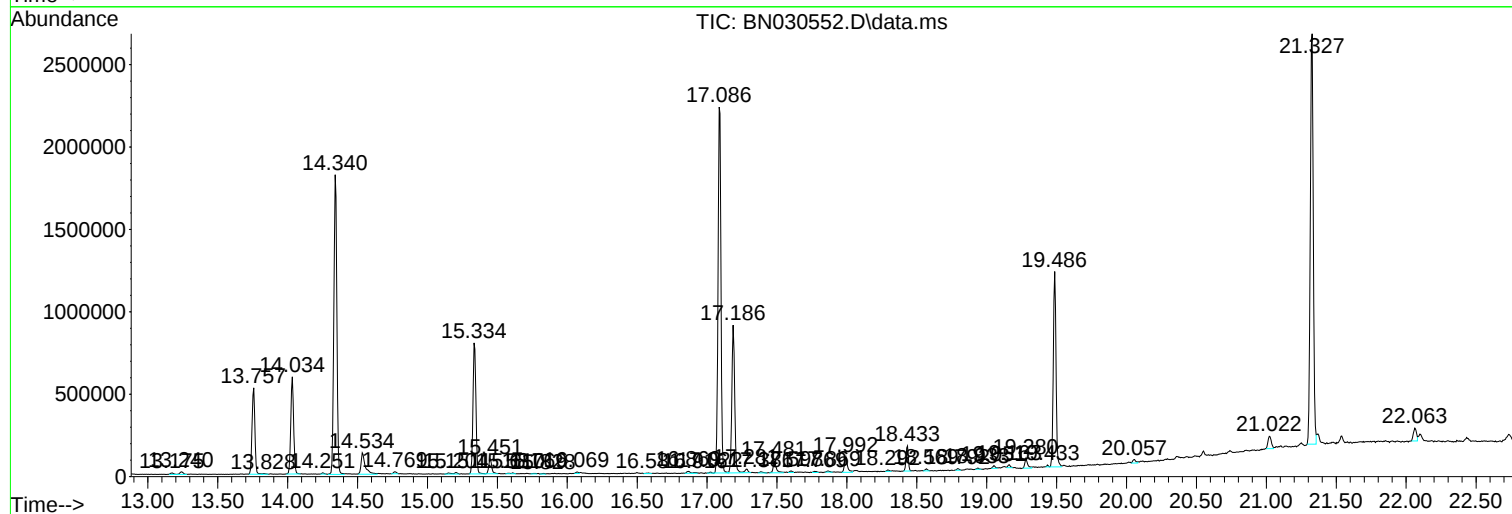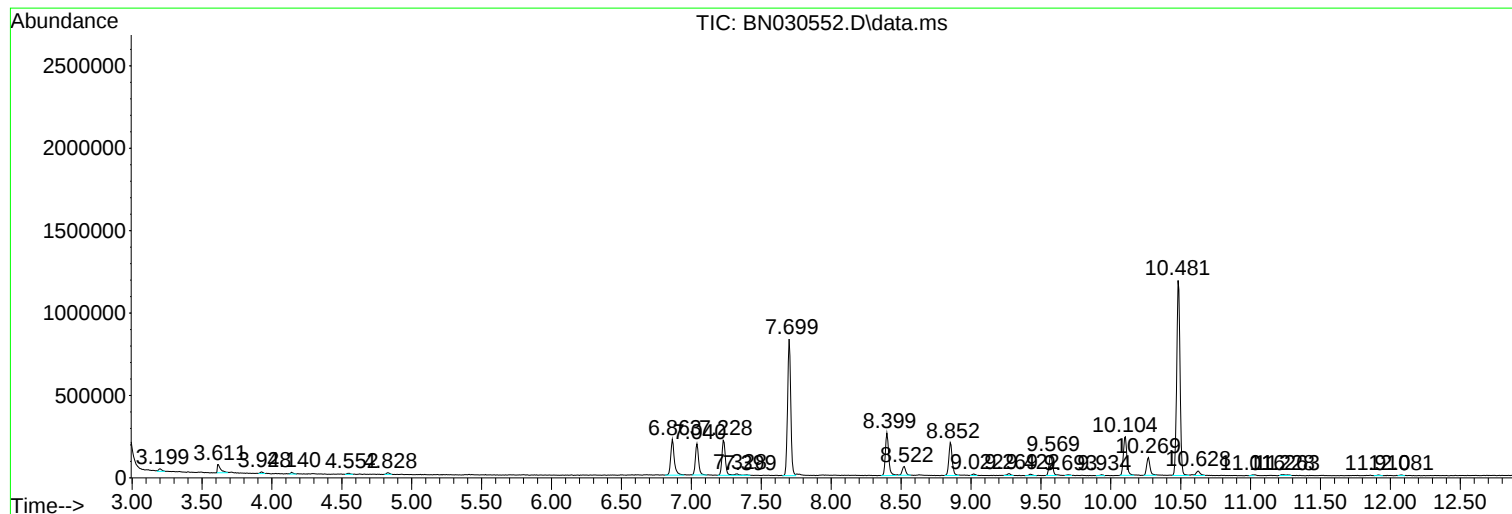

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030552.D
Acq On : 30 Mar 2024 16:05
Operator : MA/JU
Sample : P1931-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030552.D
Acq On : 30 Mar 2024 16:05
Operator : MA/JU
Sample : P1931-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc