

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030557.D
 Acq On : 30 Mar 2024 20:02
 Operator : MA/JU
 Sample : PB159886BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK886

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030557.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	31	36	46	rVB	62030	94851	1.46%	0.151%
2	3.599	101	104	127	rBV	568662	955990	14.69%	1.523%
3	3.922	156	159	165	rVB2	10416	14604	0.22%	0.023%
4	6.863	652	659	677	rBV	1020759	1580711	24.29%	2.518%
5	7.040	682	689	703	rBV	845368	1319270	20.27%	2.101%
6	7.228	714	721	733	rBV	988015	1587302	24.39%	2.528%
7	7.698	793	801	817	rBV	851797	1356813	20.85%	2.161%
8	8.398	913	920	933	rBV	1259426	1975973	30.36%	3.147%
9	8.851	990	997	1010	rBV	963653	1553170	23.87%	2.474%
10	9.569	1111	1119	1131	rBV	692834	1149257	17.66%	1.831%
11	10.098	1200	1209	1224	rBV	1164635	1984730	30.50%	3.161%
12	10.481	1263	1274	1285	rBV	1194800	2042684	31.39%	3.254%
13	10.622	1291	1298	1314	rBV	386863	652403	10.03%	1.039%
14	12.075	1539	1545	1551	rVB2	19875	33696	0.52%	0.054%
15	13.245	1739	1744	1749	rBV2	14094	20319	0.31%	0.032%
16	13.757	1824	1831	1842	rBV	2357920	3151179	48.42%	5.019%
17	14.033	1871	1878	1895	rBV	2629097	3803930	58.46%	6.059%
18	14.339	1923	1930	1940	rBV	1891756	2789847	42.87%	4.444%
19	14.539	1957	1964	1984	rBV	1013874	1570571	24.14%	2.502%
20	15.339	2093	2100	2113	rBV	3287264	4730273	72.69%	7.535%
21	15.451	2113	2119	2133	rVV	789143	1085996	16.69%	1.730%
22	15.574	2136	2140	2145	rVB3	14309	22063	0.34%	0.035%
23	16.122	2228	2233	2237	rBV5	9141	13946	0.21%	0.022%
24	16.763	2340	2342	2348	rVB5	4743	8297	0.13%	0.013%
25	17.086	2391	2397	2407	rBV	2291607	3380571	51.95%	5.385%
26	17.186	2408	2414	2427	rVV	3524133	5176032	79.54%	8.245%
27	19.051	2726	2731	2737	rBV3	46527	66031	1.01%	0.105%
28	19.121	2738	2743	2750	rVV	35854	52902	0.81%	0.084%
29	19.439	2794	2797	2799	rBV4	7629	8607	0.13%	0.014%
30	19.486	2799	2805	2818	rBV	4518240	6126238	94.14%	9.758%
31	21.327	3112	3118	3130	rBV	2577720	3748494	57.60%	5.971%
32	24.074	3575	3585	3598	rBV2	2694724	6507412	100.00%	10.365%
33	24.268	3610	3618	3638	rVB2	1707720	4216631	64.80%	6.716%




Sum of corrected areas: 62780793

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030557.D
Acq On : 30 Mar 2024 20:02
Operator : MA/JU
Sample : PB159886BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK886

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

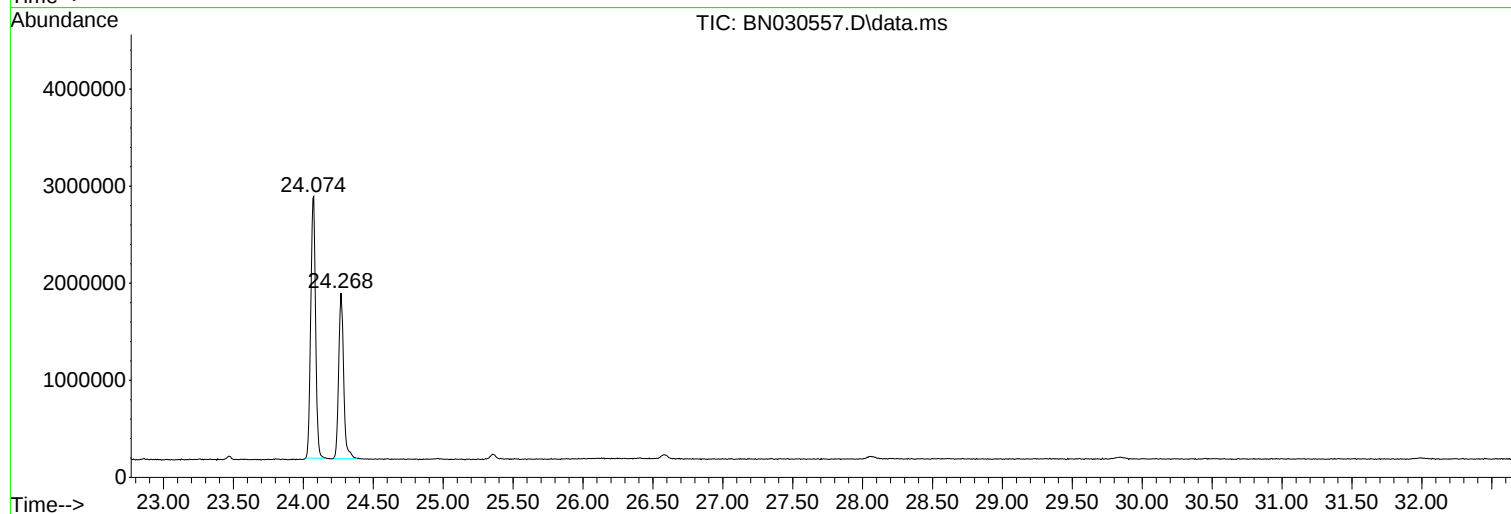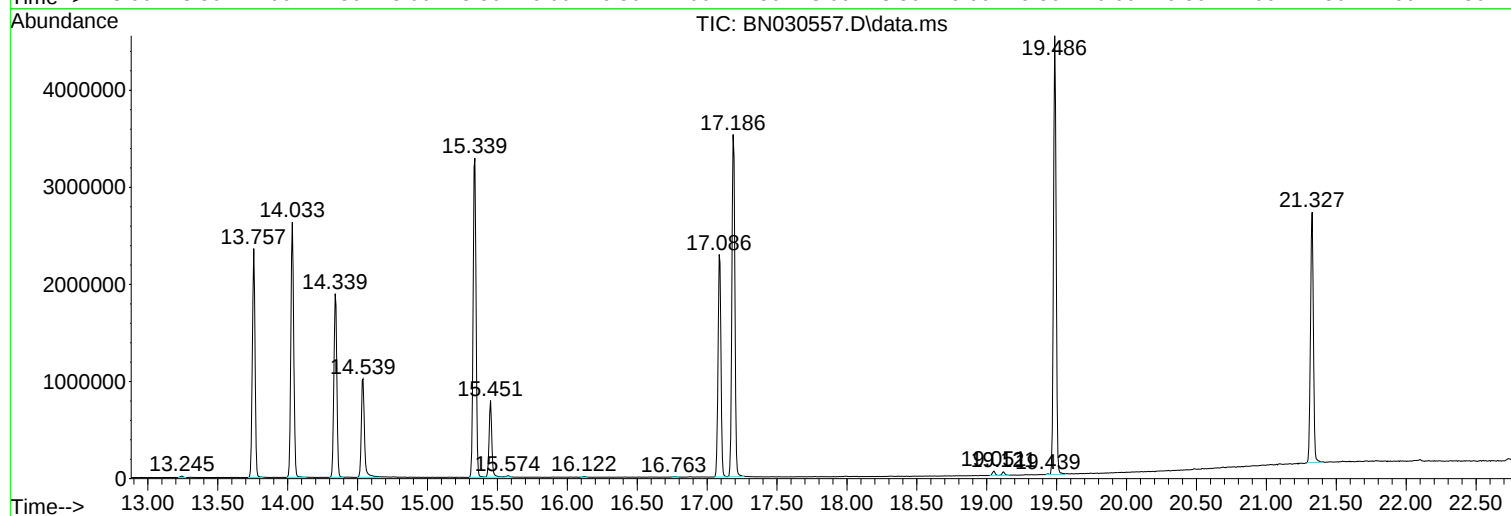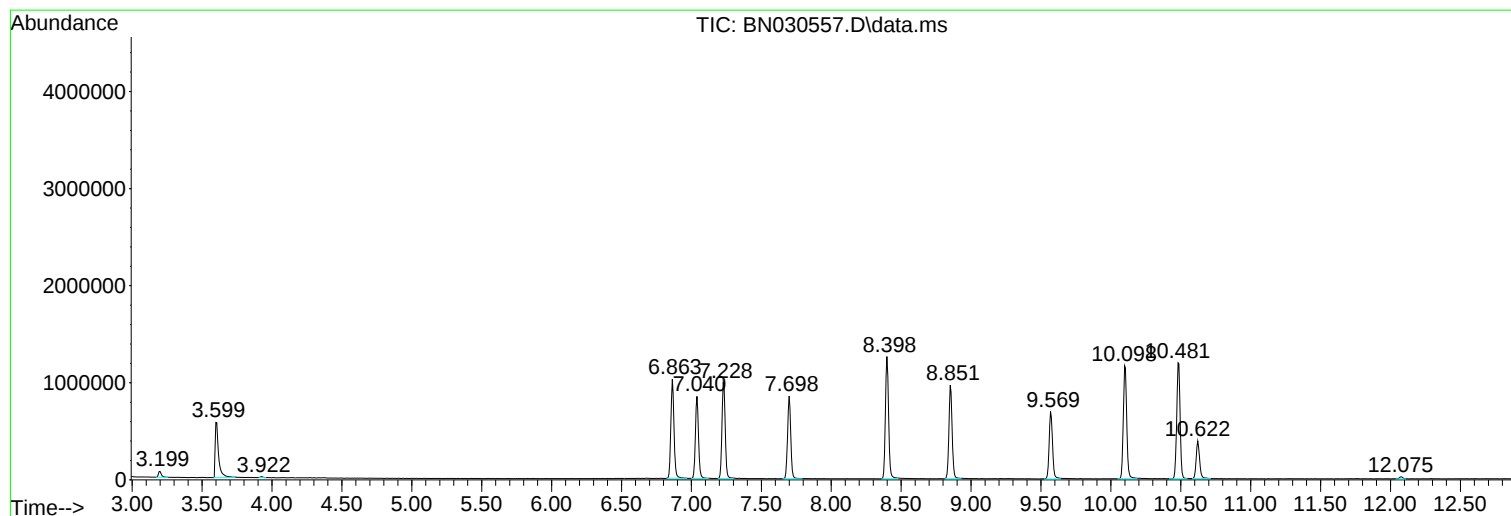

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030557.D
Acq On : 30 Mar 2024 20:02
Operator : MA/JU
Sample : PB159886BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK886

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030557.D
Acq On : 30 Mar 2024 20:02
Operator : MA/JU
Sample : PB159886BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK886

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------