

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030558.D
 Acq On : 30 Mar 2024 20:42
 Operator : MA/JU
 Sample : P1931-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030558.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	33	36	44	rVB2	14281	23386	0.65%	0.081%
2	3.616	104	107	118	rBV	51450	88043	2.43%	0.306%
3	3.711	120	123	132	rVB	46076	62641	1.73%	0.218%
4	3.922	156	159	166	rVB	13369	17060	0.47%	0.059%
5	4.475	249	253	261	rVB5	8379	13456	0.37%	0.047%
6	4.828	309	313	319	rVB3	10891	18912	0.52%	0.066%
7	4.922	324	329	336	rVB3	7963	11127	0.31%	0.039%
8	5.410	410	412	416	rVB4	2635	3768	0.10%	0.013%
9	5.775	469	474	476	rBV5	2464	4084	0.11%	0.014%
10	5.810	479	480	485	rVB4	3726	3988	0.11%	0.014%
11	6.569	607	609	616	rVV6	4770	8346	0.23%	0.029%
12	6.863	653	659	670	rBV	215803	358045	9.88%	1.246%
13	7.040	682	689	700	rBV	176509	283367	7.82%	0.986%
14	7.228	715	721	733	rBV	206652	338064	9.33%	1.176%
15	7.322	733	737	743	rVV7	7915	14430	0.40%	0.050%
16	7.699	792	801	808	rBV	958033	1502760	41.47%	5.228%
17	7.763	810	812	819	rVB7	6185	10964	0.30%	0.038%
18	8.399	911	920	931	rBV	242299	396900	10.95%	1.381%
19	8.522	936	941	948	rVB	25639	44074	1.22%	0.153%
20	8.851	991	997	1006	rBV	189292	314128	8.67%	1.093%
21	8.922	1006	1009	1014	rVB6	3899	5550	0.15%	0.019%
22	9.016	1019	1025	1029	rVV6	9742	16365	0.45%	0.057%
23	9.269	1064	1068	1073	rVB2	11573	19050	0.53%	0.066%
24	9.422	1090	1094	1101	rVB5	8413	13960	0.39%	0.049%
25	9.569	1111	1119	1126	rBV	113668	197643	5.45%	0.688%
26	9.928	1175	1180	1186	rVB7	4957	7847	0.22%	0.027%
27	10.098	1201	1209	1219	rBV	260016	438297	12.10%	1.525%
28	10.269	1231	1238	1248	rBV	85202	148088	4.09%	0.515%
29	10.481	1265	1274	1288	rBV	1343065	2251649	62.14%	7.833%
30	10.622	1288	1298	1312	rVB	96711	196384	5.42%	0.683%
31	11.234	1397	1402	1404	rBV3	6136	11344	0.31%	0.039%
32	11.516	1446	1450	1455	rBV6	3638	6009	0.17%	0.021%
33	11.763	1487	1492	1494	rBV6	2816	3973	0.11%	0.014%
34	11.916	1511	1518	1525	rBV5	12439	25581	0.71%	0.089%
35	12.057	1538	1542	1543	rBV4	5004	5922	0.16%	0.021%
36	12.069	1543	1544	1549	rVV4	5422	8023	0.22%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030558.D
 Acq On : 30 Mar 2024 20:42
 Operator : MA/JU
 Sample : P1931-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	12.145	1552	1557	1563	rVB9	4380	9239	0.25%	0.032%
38	12.363	1592	1594	1600	rBV6	2839	4966	0.14%	0.017%
39	12.604	1630	1635	1641	rBV8	3199	6106	0.17%	0.021%
40	12.740	1655	1658	1661	rBV5	3976	5131	0.14%	0.018%
41	12.781	1663	1665	1670	rVB6	3358	5590	0.15%	0.019%
42	12.828	1670	1673	1675	rBV4	3582	4834	0.13%	0.017%
43	12.881	1679	1682	1687	rVB4	6337	8115	0.22%	0.028%
44	13.169	1724	1731	1736	rBV3	17634	30580	0.84%	0.106%
45	13.239	1738	1743	1750	rVB2	20466	36751	1.01%	0.128%
46	13.304	1752	1754	1758	rBV5	3720	4423	0.12%	0.015%
47	13.510	1783	1789	1795	rVB10	4210	8075	0.22%	0.028%
48	13.663	1811	1815	1819	rBV5	5023	6064	0.17%	0.021%
49	13.716	1820	1824	1825	rBV4	3416	4352	0.12%	0.015%
50	13.757	1825	1831	1838	rVV	498274	689922	19.04%	2.400%
51	13.828	1841	1843	1848	rVB5	9306	11593	0.32%	0.040%
52	14.034	1867	1878	1887	rBV	575450	861418	23.77%	2.997%
53	14.175	1899	1902	1905	rVB5	3627	3763	0.10%	0.013%
54	14.251	1910	1915	1919	rBV2	23084	32692	0.90%	0.114%
55	14.339	1922	1930	1937	rBV	1977185	2979478	82.22%	10.365%
56	14.539	1958	1964	1977	rBV8	36460	104753	2.89%	0.364%
57	14.751	1996	2000	2001	rBV4	4443	4862	0.13%	0.017%
58	14.816	2008	2011	2015	rVB6	9083	12488	0.34%	0.043%
59	14.875	2015	2021	2028	rVB9	9034	16748	0.46%	0.058%
60	14.969	2029	2037	2040	rBV8	5730	13080	0.36%	0.046%
61	15.016	2040	2045	2048	rVB4	7137	10678	0.29%	0.037%
62	15.057	2048	2052	2053	rBV4	3583	5166	0.14%	0.018%
63	15.204	2074	2077	2080	rVB	22541	24407	0.67%	0.085%
64	15.333	2093	2099	2106	rBV	821392	1158735	31.98%	4.031%
65	15.445	2113	2118	2127	rBV4	24302	43341	1.20%	0.151%
66	15.610	2143	2146	2152	rVB2	17264	25449	0.70%	0.089%
67	15.828	2180	2183	2187	rBV6	6845	10714	0.30%	0.037%
68	16.069	2220	2224	2226	rBV2	39420	53808	1.48%	0.187%
69	16.863	2355	2359	2363	rVV3	32370	41537	1.15%	0.144%
70	16.910	2363	2367	2376	rVB2	35452	61123	1.69%	0.213%
71	17.086	2391	2397	2403	rBV	2460461	3578180	98.75%	12.448%
72	17.128	2403	2404	2408	rVV	75693	74883	2.07%	0.261%
73	17.186	2408	2414	2425	rVB2	913788	1309623	36.14%	4.556%
74	17.480	2461	2464	2469	rBV2	43936	61746	1.70%	0.215%
75	17.598	2481	2484	2489	rVB	33742	45194	1.25%	0.157%
76	17.992	2547	2551	2560	rVB4	88143	163574	4.51%	0.569%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
 Data File : BN030558.D
 Acq On : 30 Mar 2024 20:42
 Operator : MA/JU
 Sample : P1931-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

77	18.151	2574	2578	2582	rBV4	27394	41761	1.15%	0.145%
78	18.298	2599	2603	2610	rBV2	38139	60881	1.68%	0.212%
79	18.427	2621	2625	2629	rBV	131809	164969	4.55%	0.574%
80	18.763	2680	2682	2686	rBV2	18921	24949	0.69%	0.087%
81	18.933	2708	2711	2716	rVB4	59256	72742	2.01%	0.253%
82	19.151	2744	2748	2754	rBV	150979	204173	5.63%	0.710%
83	19.280	2767	2770	2772	rBV2	44499	46374	1.28%	0.161%
84	19.486	2800	2805	2809	rBV	1269663	1722233	47.53%	5.991%
85	20.051	2898	2901	2904	rBV	86571	95756	2.64%	0.333%
86	20.551	2983	2986	2991	rBV	95133	99387	2.74%	0.346%
87	21.027	3064	3067	3071	rVB	135578	174785	4.82%	0.608%
88	21.327	3112	3118	3123	rBV2	2399186	3623650	100.00%	12.606%
89	24.062	3578	3583	3593	rVB2	474197	1060403	29.26%	3.689%
90	24.268	3611	3618	3626	rBV	1247064	2947211	81.33%	10.253%




Sum of corrected areas: 28745683

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030558.D
Acq On : 30 Mar 2024 20:42
Operator : MA/JU
Sample : P1931-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

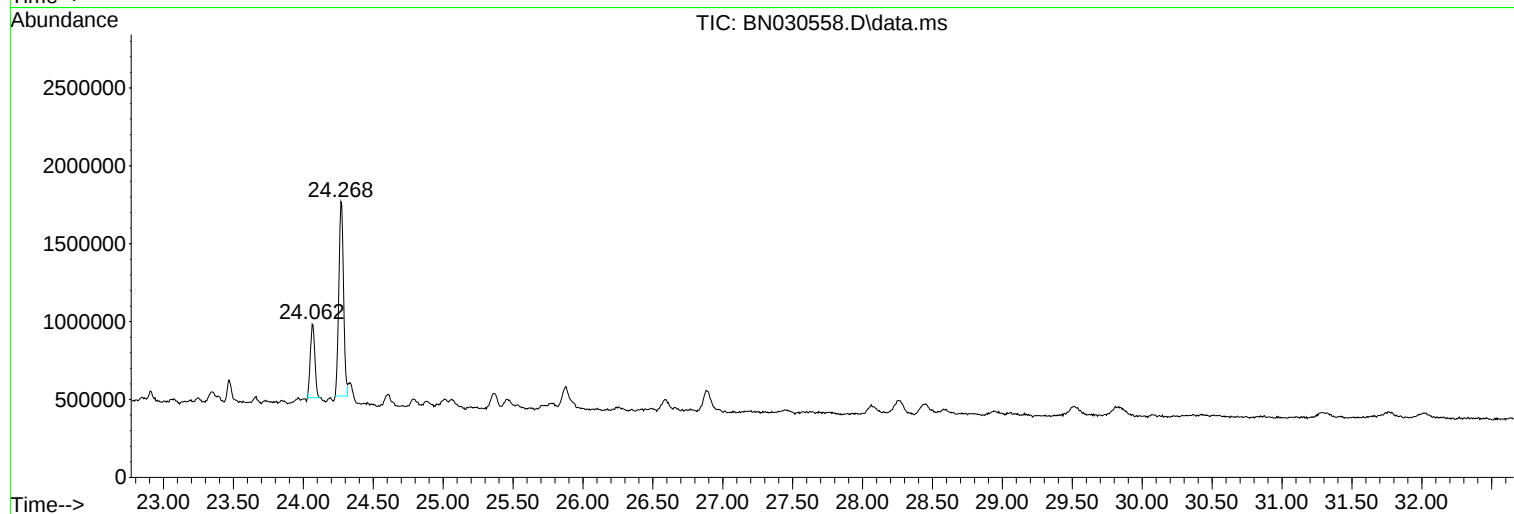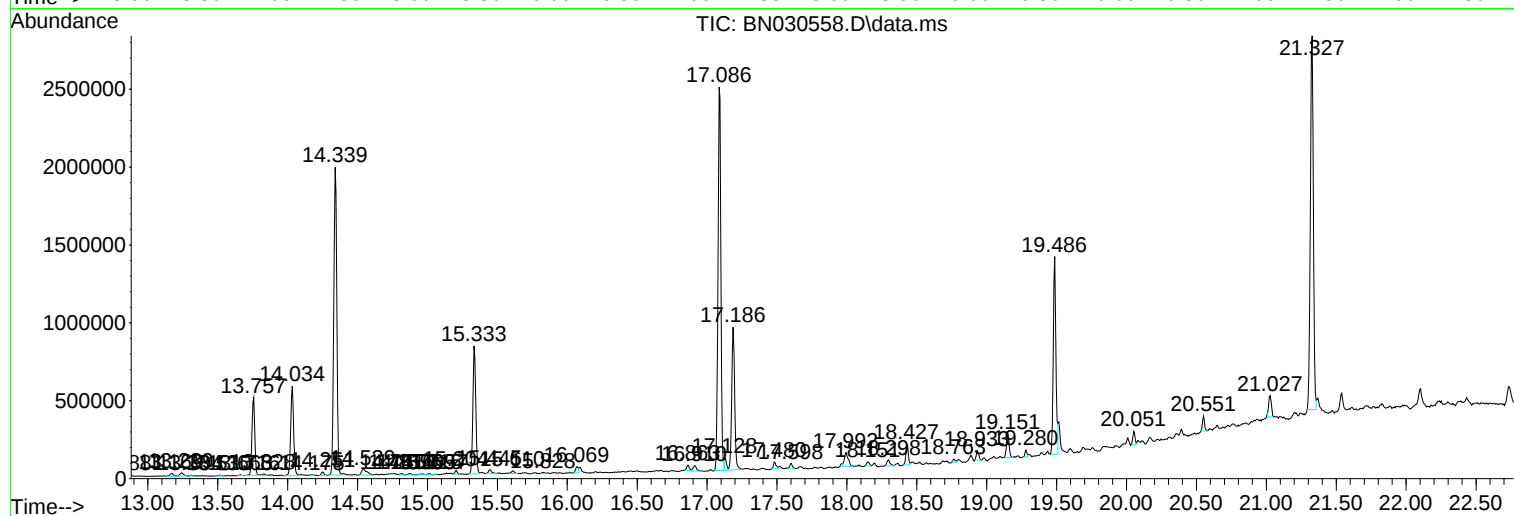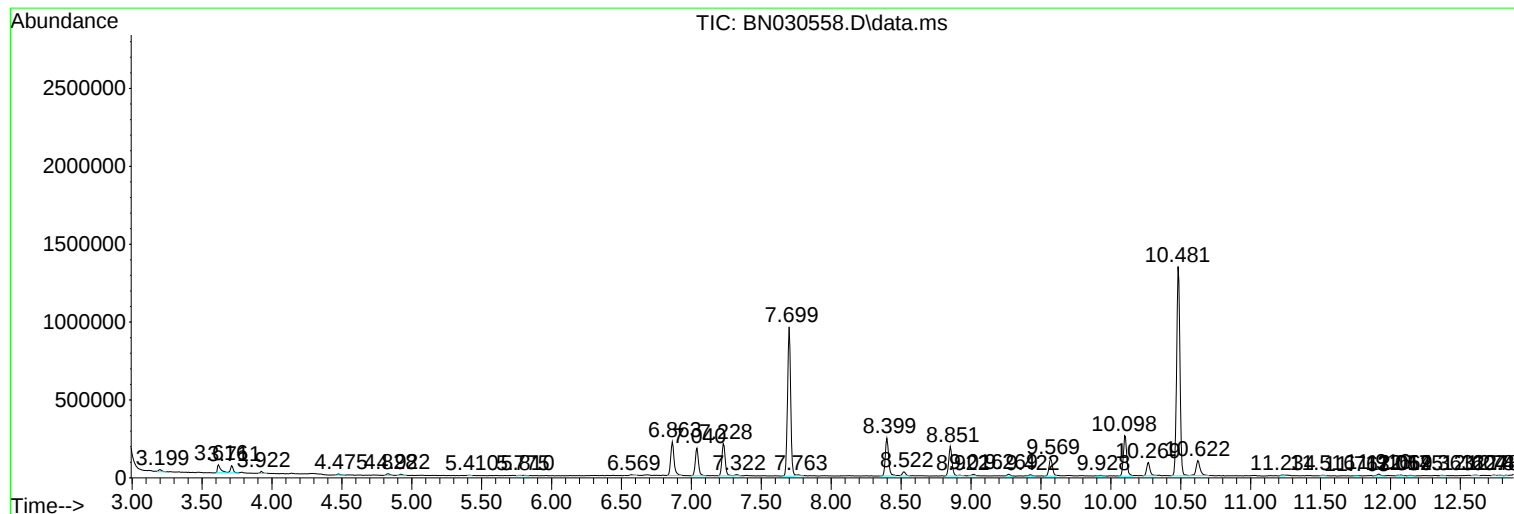

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030558.D
Acq On : 30 Mar 2024 20:42
Operator : MA/JU
Sample : P1931-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033124\
Data File : BN030558.D
Acq On : 30 Mar 2024 20:42
Operator : MA/JU
Sample : P1931-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07C3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc