
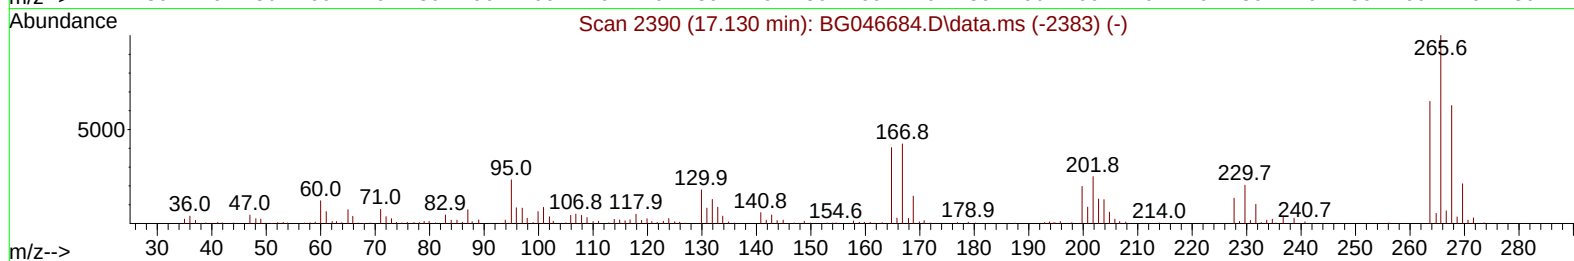
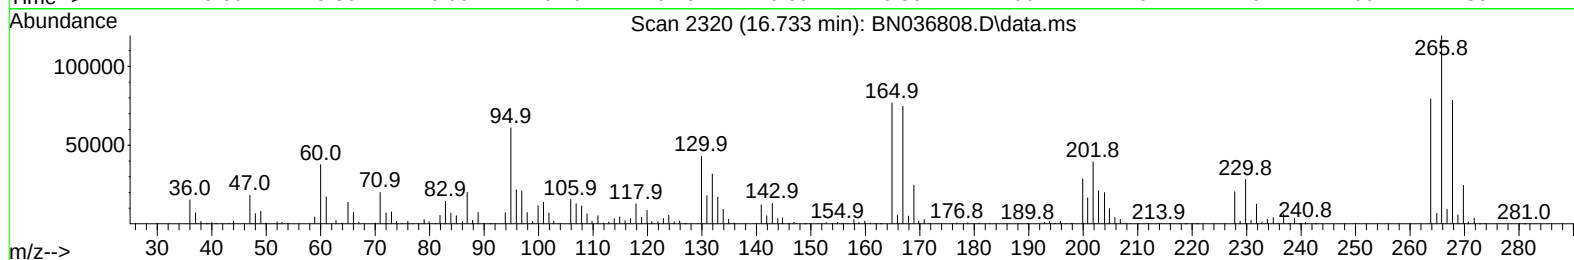


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033125\
Data File : BN036808.D
Acq On : 31 Mar 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 12:42:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 29 04:33:53 2025
Response via : Initial Calibration

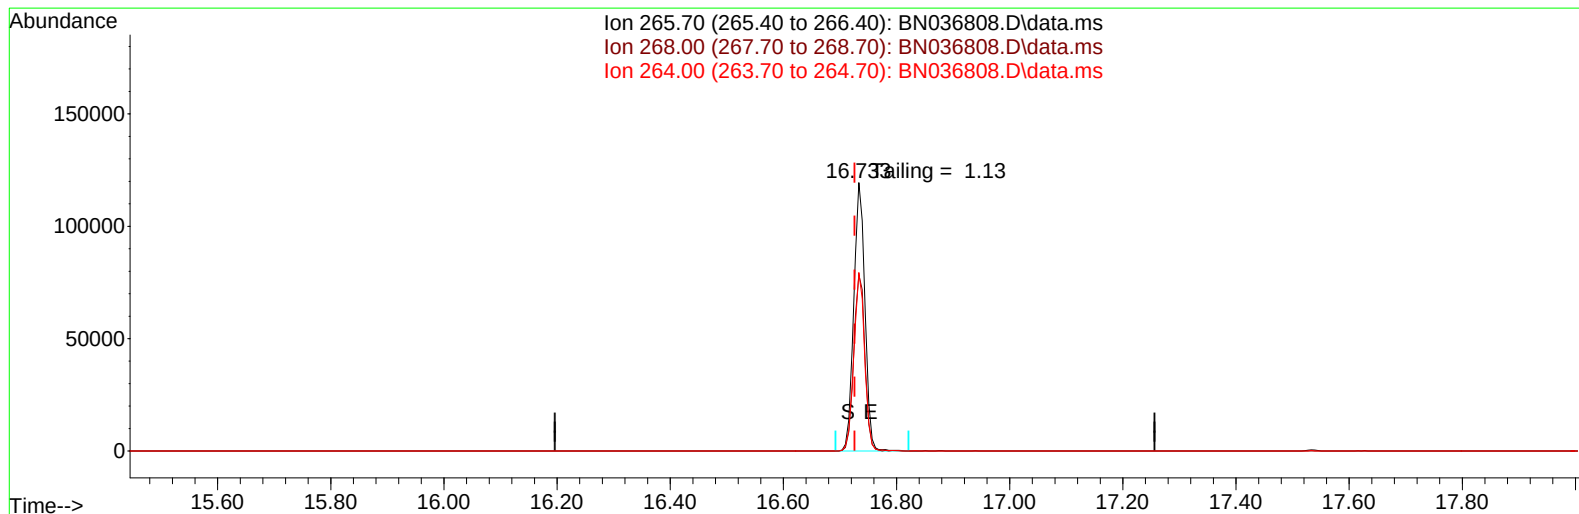

TIC: BN036808.D\data.ms

(70) Pentachlorophenol (C)




16.733min (+ 0.007) 18057.26 ng

response 163532

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.65
264.00	61.60	66.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033125\
Data File : BN036808.D
Acq On : 31 Mar 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 12:45:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 29 04:33:53 2025
Response via : Initial Calibration

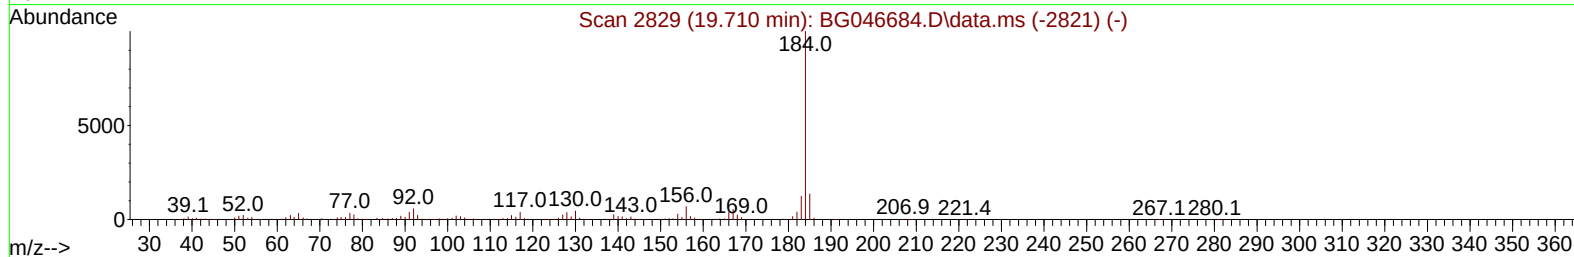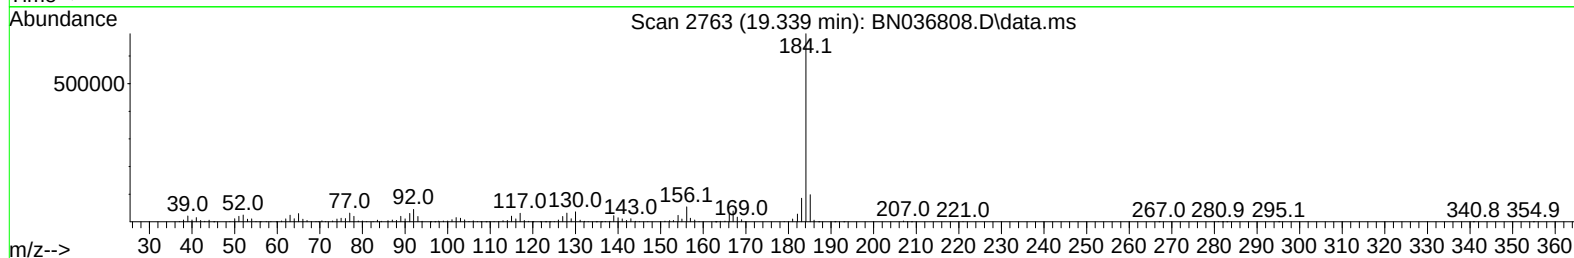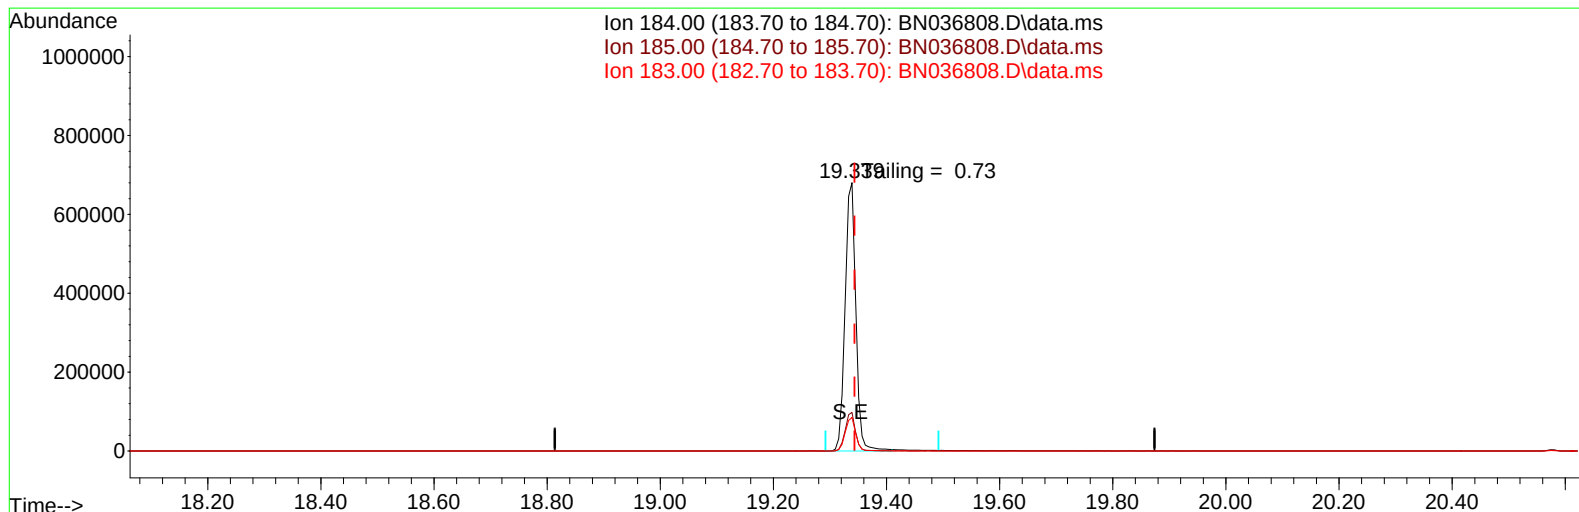

TIC: BN036808.D\data.ms

(77) Benzidine

19.339min (-0.005) 0.00 ng

response 903894

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.38
183.00	13.20	12.51
0.00	0.00	0.00