
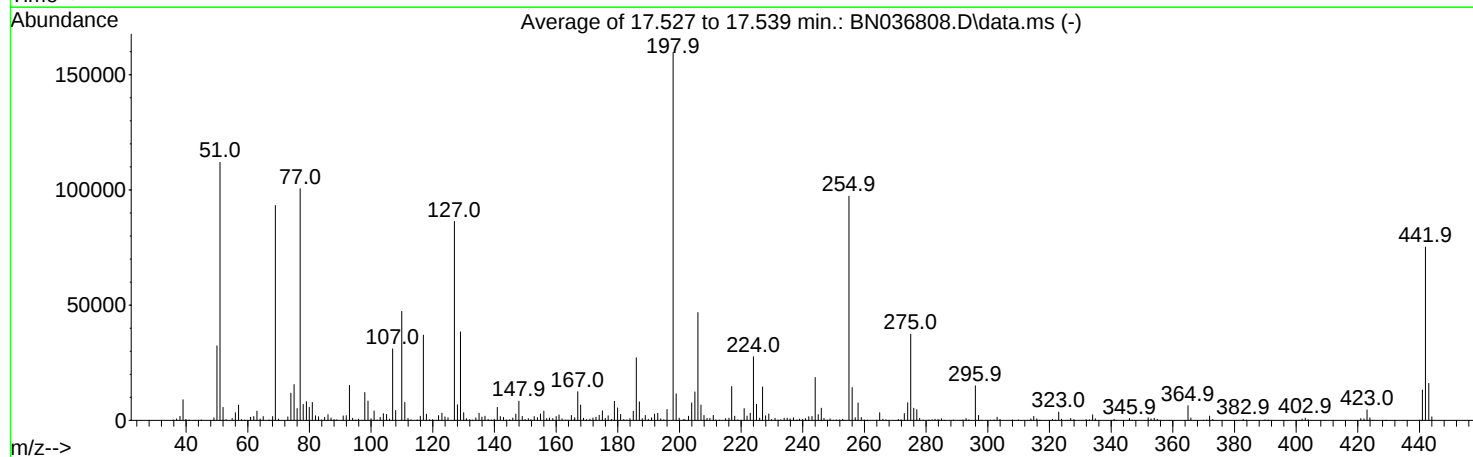


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033125\
Data File : BN036808.D
Acq On : 31 Mar 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 16:06:28 2025

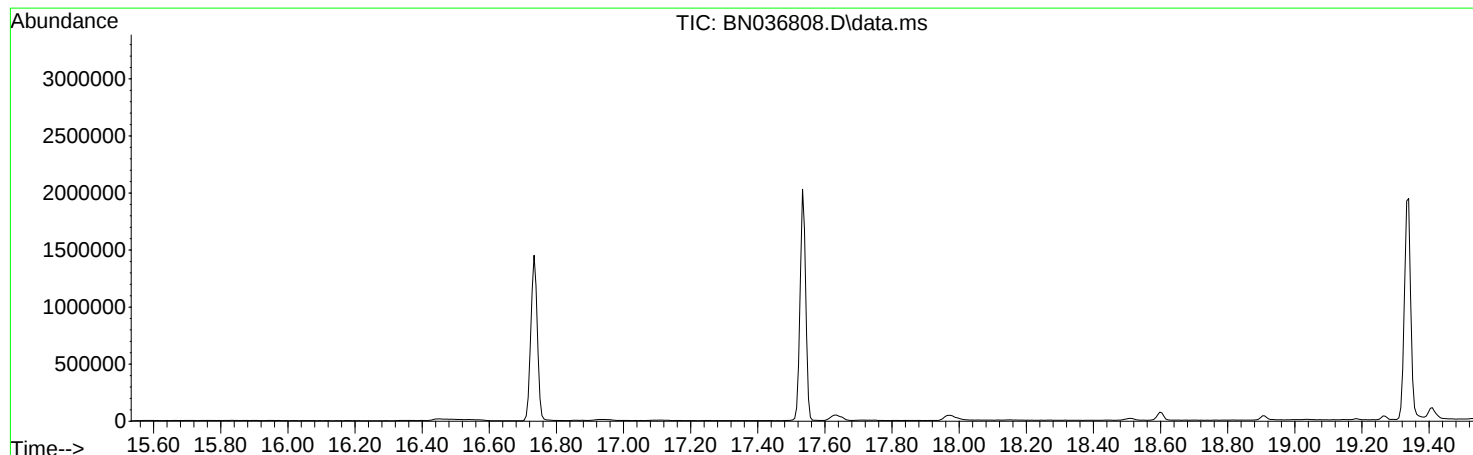

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	70.2	112056	PASS
68	69	0.00	2	1.8	1674	PASS
69	198	0.00	100	58.4	93275	PASS
70	69	0.00	2	0.6	564	PASS
127	198	10	80	54.1	86363	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	159677	PASS
199	198	5	9	7.2	11540	PASS
275	198	10	60	23.4	37339	PASS
365	198	1	100	4.0	6395	PASS
441	198	0.01	100	8.3	13207	PASS
442	442	50	100	100.0	75192	PASS
443	442	15	24	21.3	16045	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/31/2025	BNA_N	<u>BN036808.D</u>
Compound Name	Response	Retention Time
DDT	562026	20.58
DDD	7640	20.186
DDE	699	19.627
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8339	570365	1.46

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033125\
Data File : BN036808.D
Acq On : 31 Mar 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 31 12:42:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 29 04:33:53 2025
Response via : Initial Calibration

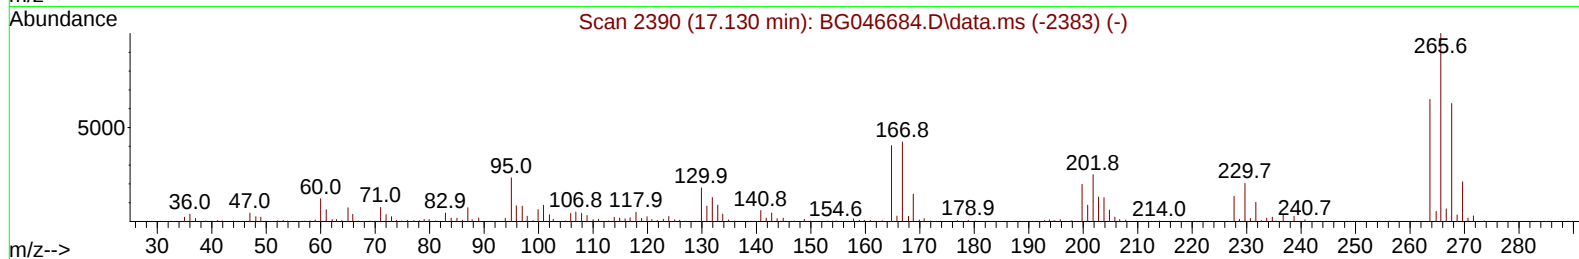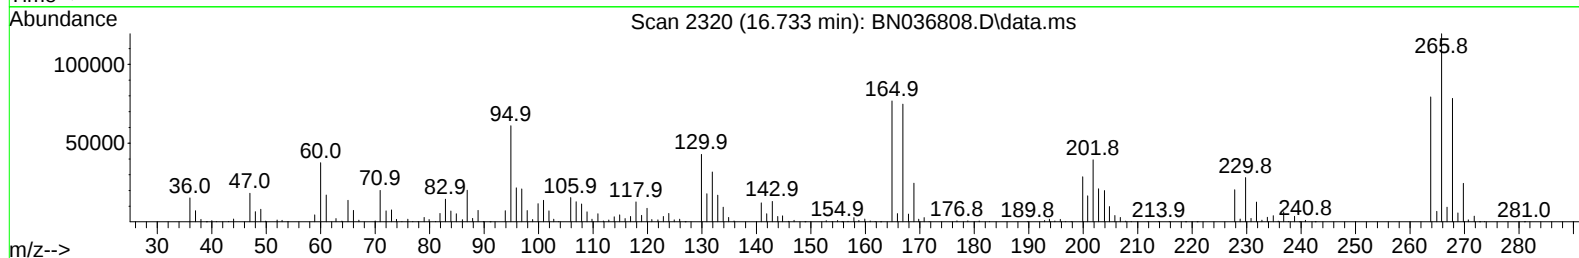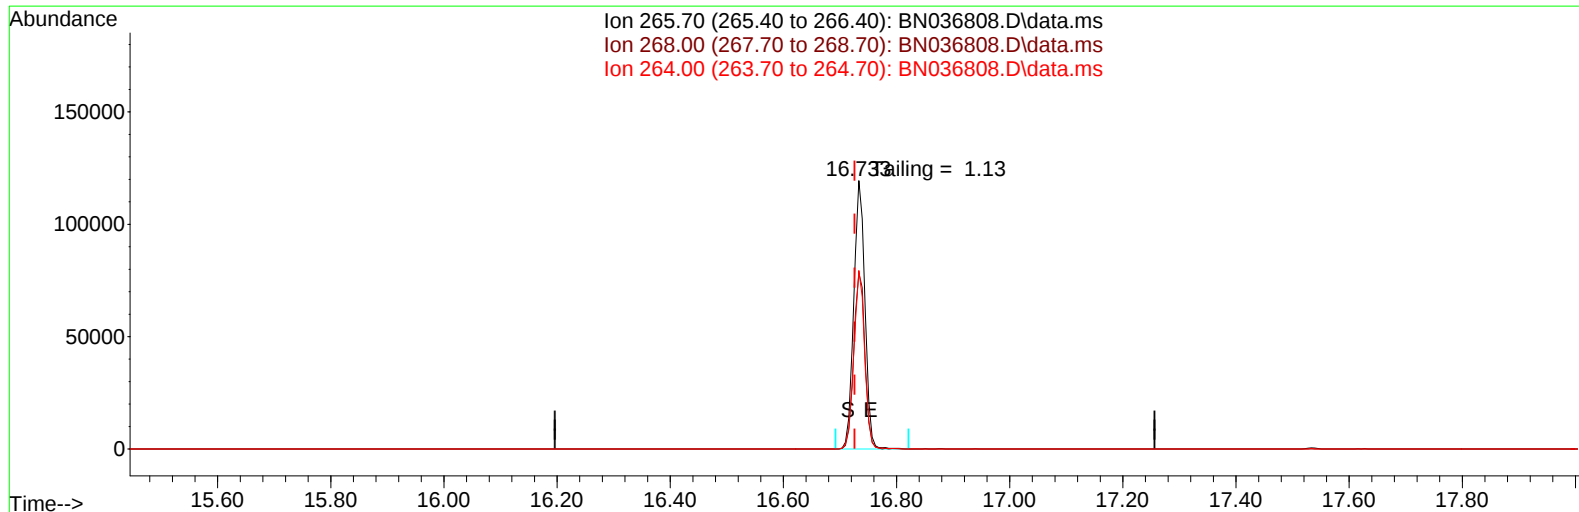

TIC: BN036808.D\data.ms

(70) Pentachlorophenol (C)

16.733min (+ 0.007) 18057.26 ng




response 163532

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.65
264.00	61.60	66.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN033125\
Data File : BN036808.D
Acq On : 31 Mar 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Mar 31 12:45:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 29 04:33:53 2025
Response via : Initial Calibration

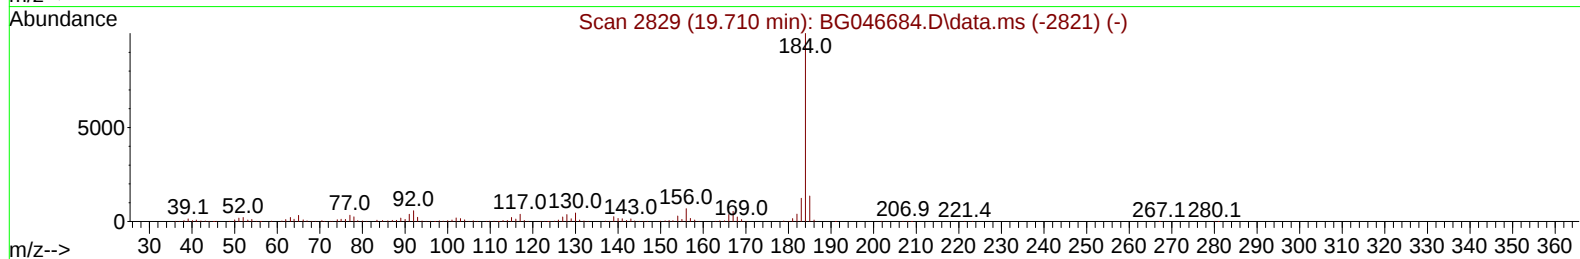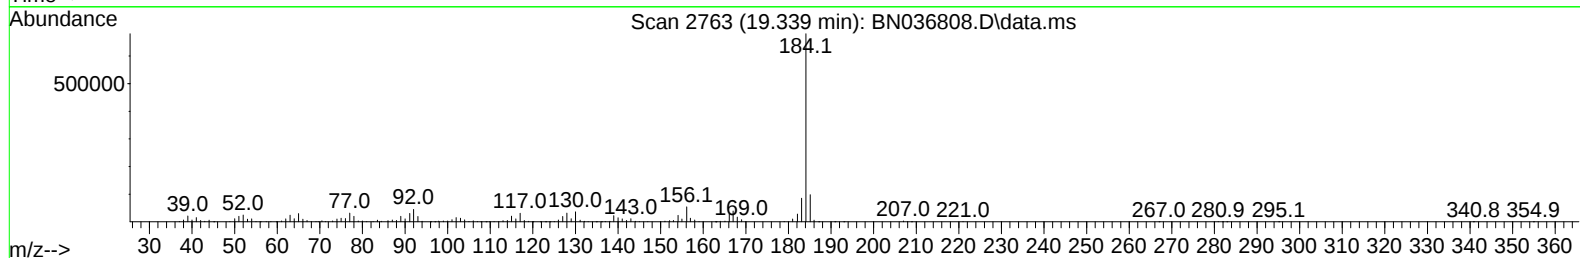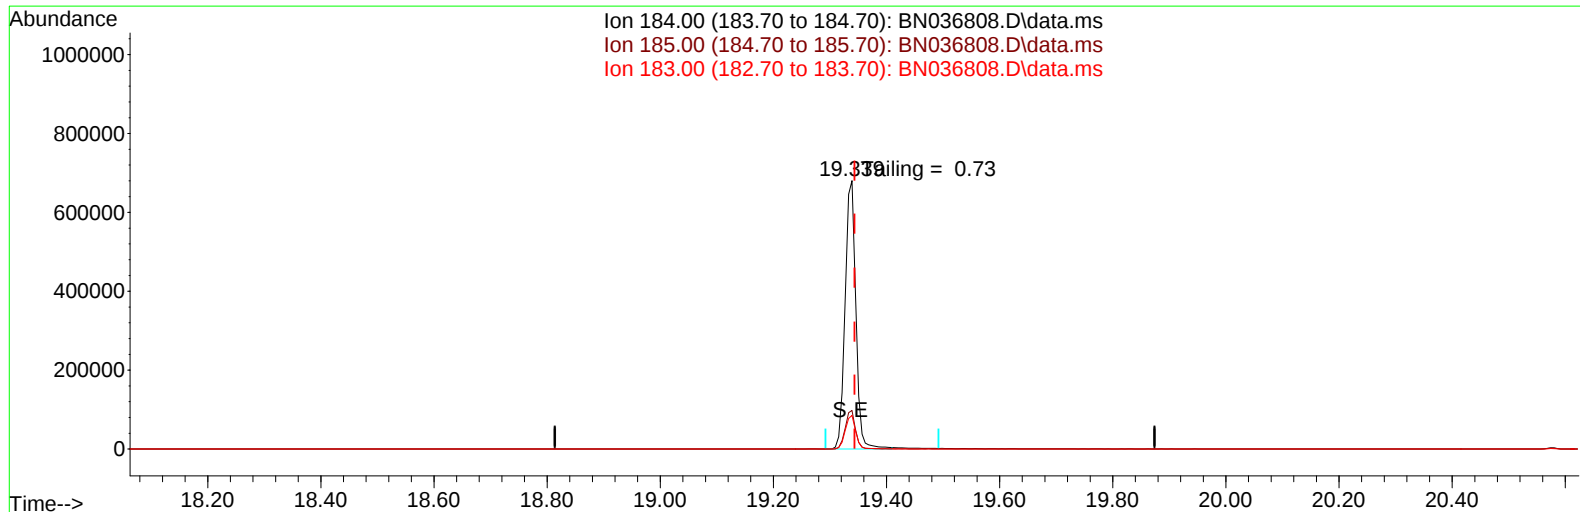

TIC: BN036808.D\data.ms

(77) Benzidine

19.339min (-0.005) 0.00 ng

response 903894

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.38
183.00	13.20	12.51
0.00	0.00	0.00