
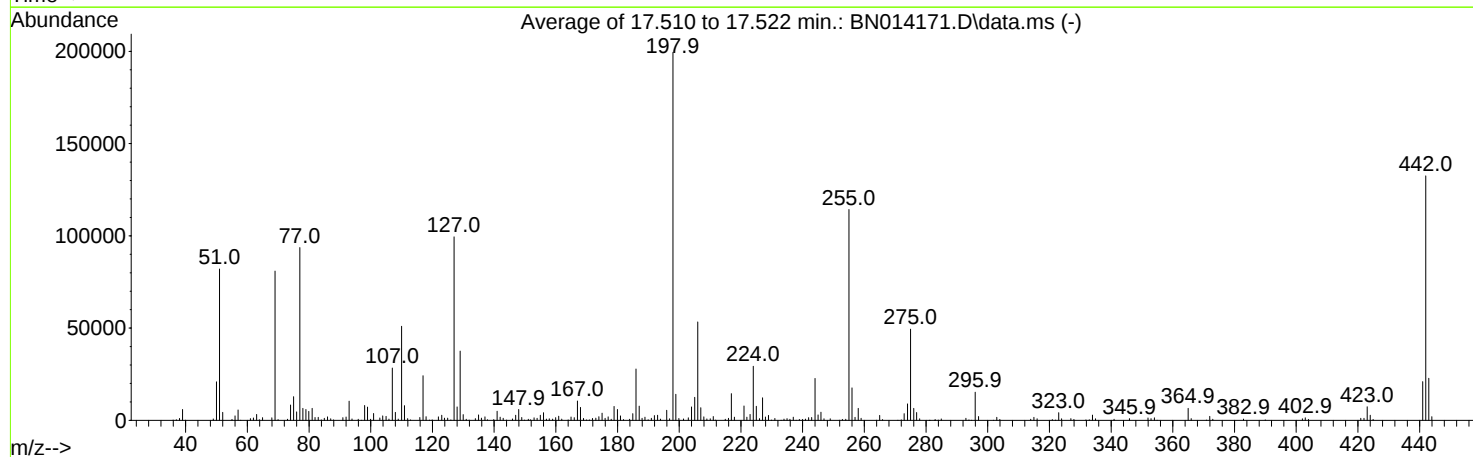


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040121\
 Data File : BN014171.D
 Acq On : 01 Apr 2021 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN032621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 31 12:15:38 2021

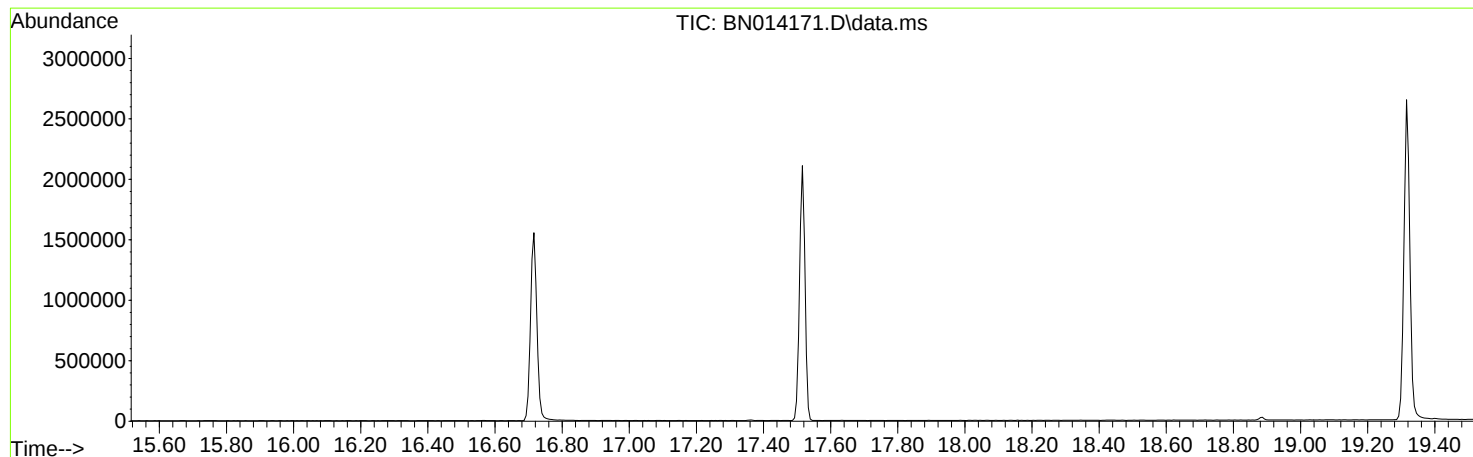

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	82016	PASS
68	69	0.00	2	1.7	1366	PASS
69	198	0.00	100	40.6	80872	PASS
70	69	0.00	2	0.5	428	PASS
127	198	10	80	49.9	99496	PASS
197	198	0.00	2	0.4	897	PASS
198	198	100	100	100.0	199381	PASS
199	198	5	9	7.1	14172	PASS
275	198	10	60	24.8	49421	PASS
365	198	1	100	3.3	6539	PASS
441	198	0.01	100	10.5	21022	PASS
442	442	50	100	100.0	132491	PASS
443	442	15	24	17.2	22781	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/1/2021	BNA_N	<u>BN014171.D</u>
Compound Name	Response	Retention Time
DDT	683625	20.557
DDD	6398	20.116
DDE	1054	19.604
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7452	691077	1.08

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040121\
 Data File : BN014171.D
 Acq On : 01 Apr 2021 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 01 10:56:58 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 26 11:50:50 2021
 Response via : Initial Calibration

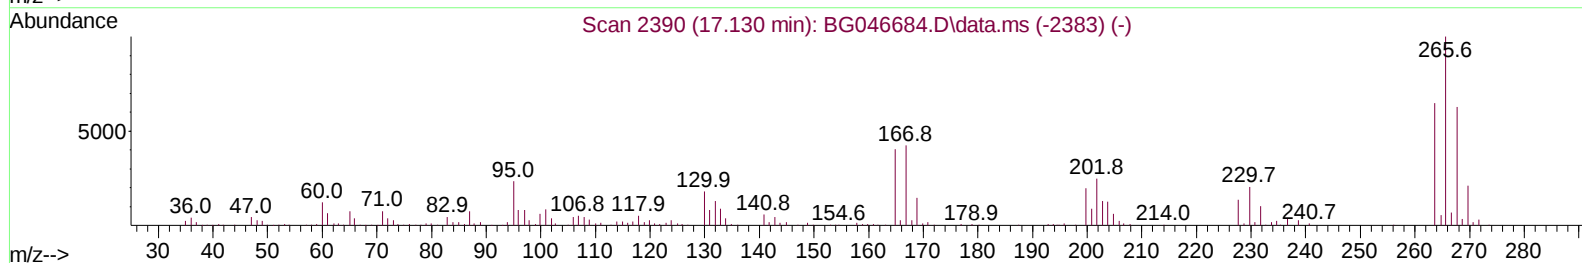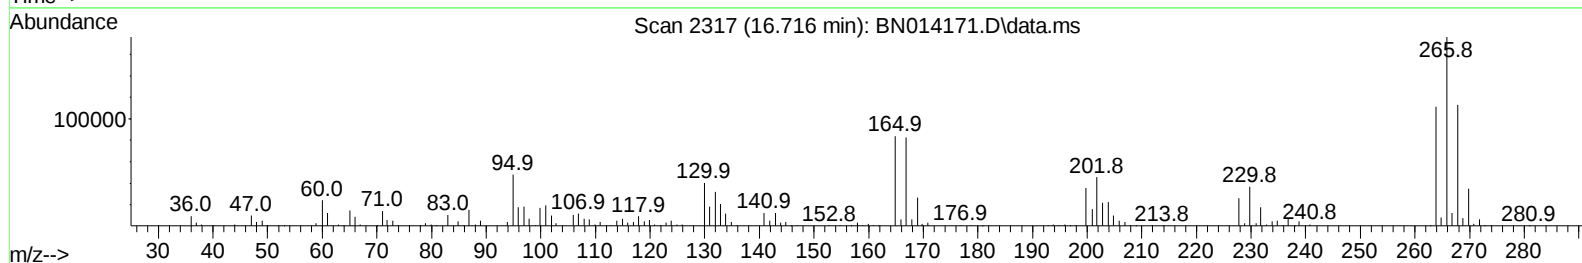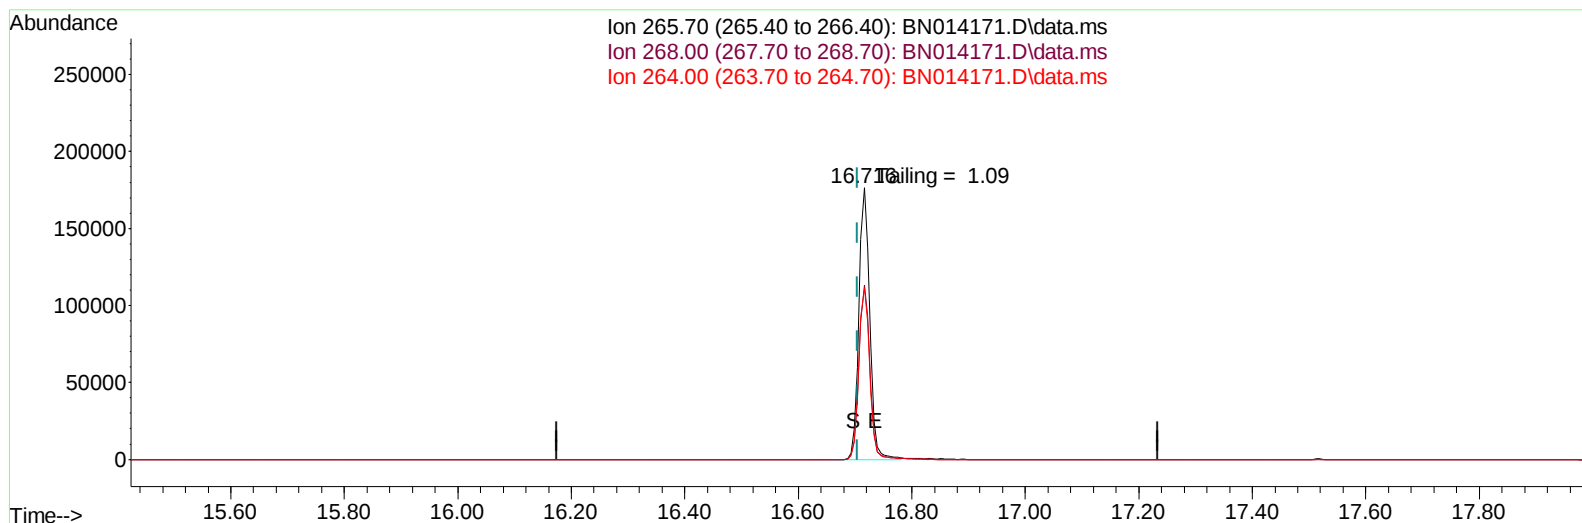

TIC: BN014171.D\data.ms




(70) Pentachlorophenol (C)**16.716min (+ 0.012) 22650.80 ng****response 234818**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.28
264.00	61.60	63.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040121\
 Data File : BN014171.D
 Acq On : 01 Apr 2021 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 01 10:56:58 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 26 11:50:50 2021
 Response via : Initial Calibration

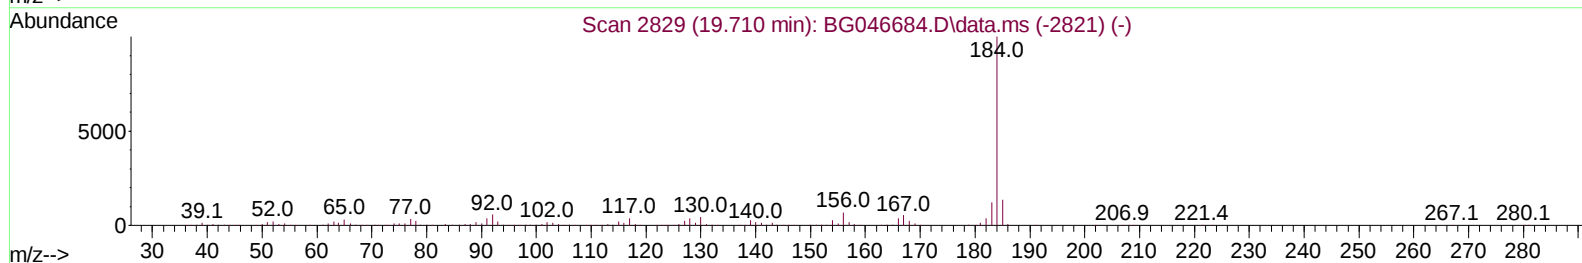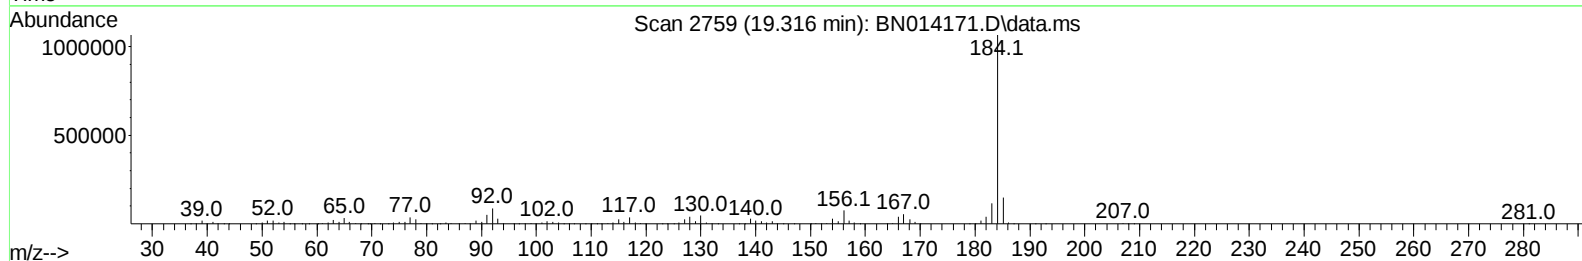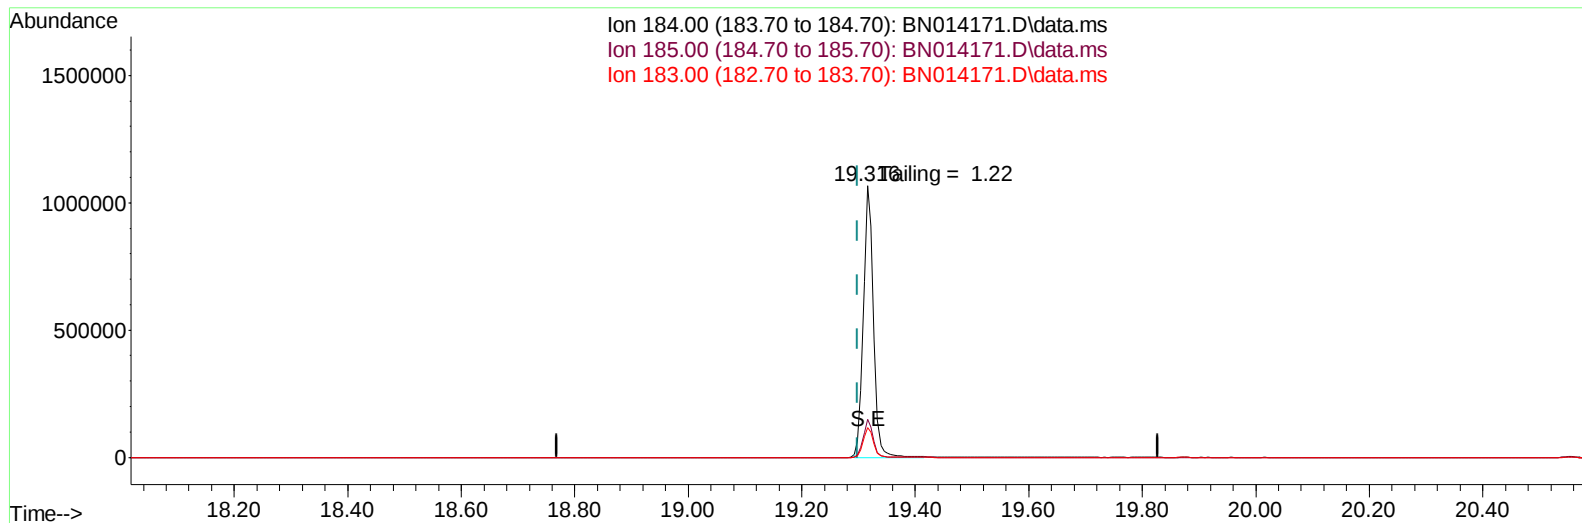

TIC: BN014171.D\data.ms

(77) Benzidine

19.316min (+ 0.018) 0.00 ng

response 1337443

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	10.95
0.00	0.00	0.00