

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA N\DATA\BN040218\
 Data File : BN000697.D
 Acq On : 02 Apr 2018 16:22
 Operator : JU/SJ
 Sample : J2082-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ET2R1

Quant Time: Apr 03 02:11:21 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 03 02:09:38 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.41	152	167604	20.00	ng/ul	0.00
18) Naphthalene-d8	11.24	136	749038	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.02	164	415219	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.75	188	909975	20.00	ng/ul	0.00
75) Chrysene-d12	21.87	240	915299	20.00	ng/ul	0.00
83) Perylene-d12	24.35	264	803604	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.58	96	18522	3.95	ng/uL	0.00
5) Phenol-d5	7.55	99	390699	24.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.71	67	235191	26.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.93	132	283024	23.94	ng/ul	0.00
13) 4-Methylphenol-d8	9.12	113	322709	26.50	ng/ul	0.00
19) Nitrobenzene-d5	9.58	128	142980	23.50	ng/ul	0.00
22) 2-Nitrophenol-d4	10.31	143	156287	24.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.87	165	266955	23.63	ng/ul	0.00
29) 4-Chloroaniline-d4	11.37	131	405490	34.97	ng/ul	0.00
43) Dimethylphthalate-d6	14.41	166	904328	27.57	ng/ul	0.00
46) Acenaphthylene-d8	14.72	160	1132679	26.17	ng/ul	0.00
51) 4-Nitrophenol-d4	15.23	143	112737	18.51	ng/ul	0.00
57) Fluorene-d10	16.01	176	755307	27.02	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.12	200	73516	14.11	ng/ul	0.00
70) Anthracene-d10	17.85	188	1167502	26.69	ng/ul	0.00
76) Pyrene-d10	20.11	212	1276666	25.27	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.19	264	1045008	27.55	ng/ul	0.00


Target Compounds				Ovalue	
44) Dimethylphthalate	14.46	163	167028	5.148	ng/ul# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA N\DATA\BN040218\
Data File : BN000697.D
Acq On : 02 Apr 2018 16:22
Operator : JU/SJ
Sample : J2082-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
ET2R1

Quant Time: Apr 03 02:11:21 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\SOM-EPA-BN031918.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 03 02:09:38 2018
Response via : Initial Calibration

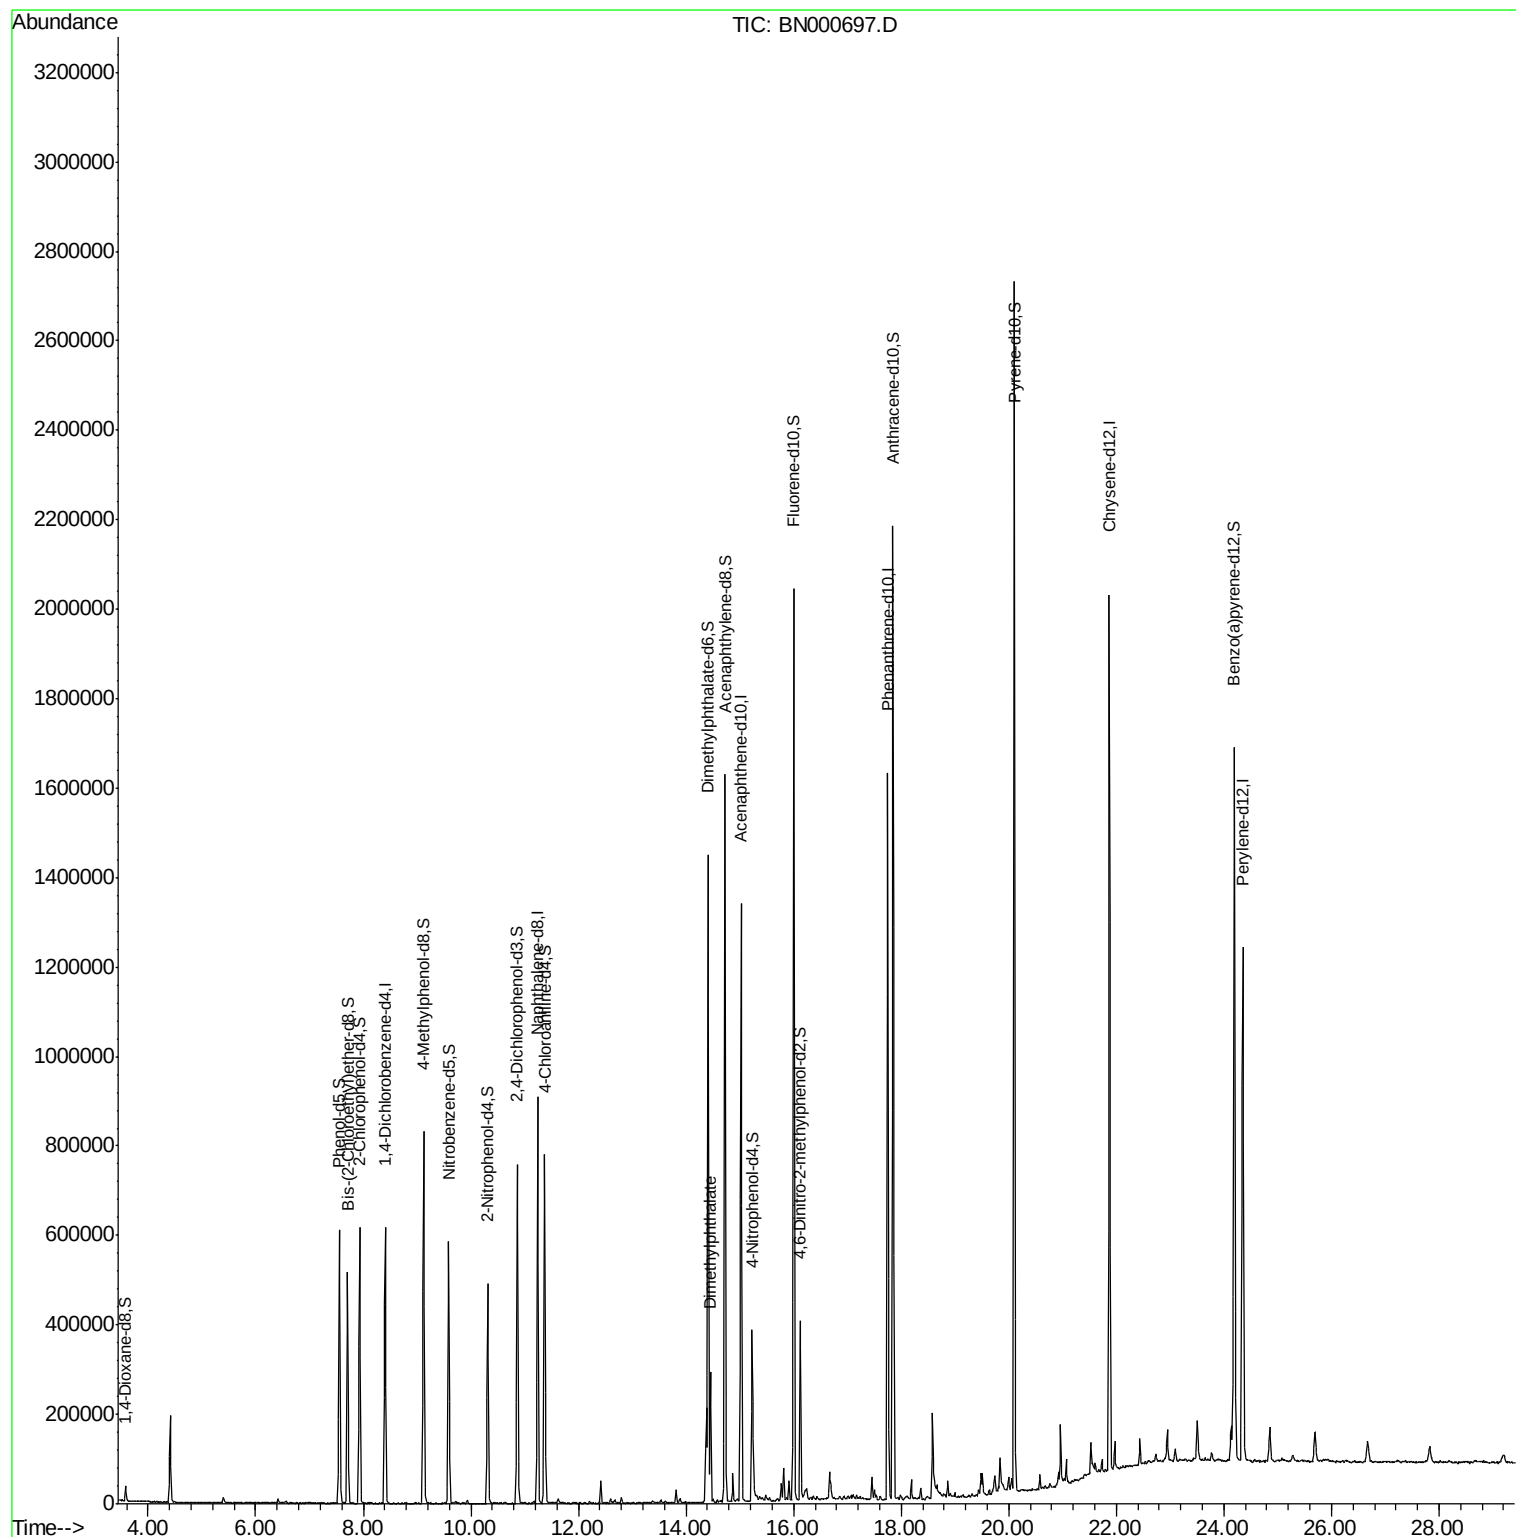

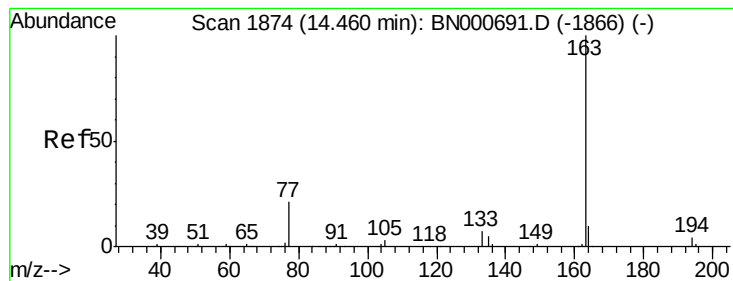

#44

Dimethylphthalate

Concen: 5.148 ng/ul

RT: 14.46 min Scan# 1874

Delta R.T. 0.00 min

Lab File: BN000697.D

Acq: 02 Apr 2018 16:22

Instrument :

BNA_N

ClientSampleId :

ET2R1


Tot Ion:163 Resp: 167028

Ion Ratio Lower Upper

163 100

194 3.8 4.0 6.0#

164 9.8 8.4 12.6

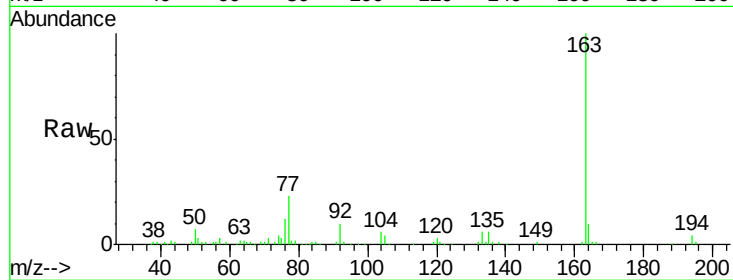

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

