


Data Path : Z:\HPCHEM1\BNA_N\Data\BN040218\
 Data File : BN000690.D
 Acq On : 02 Apr 2018 10:58
 Operator : JU/SJ
 Sample : DFTPP90
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP90

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN031918.M
 Title : SVOA CALIBRATION
 Last Update : Tue Apr 03 02:09:38 2018

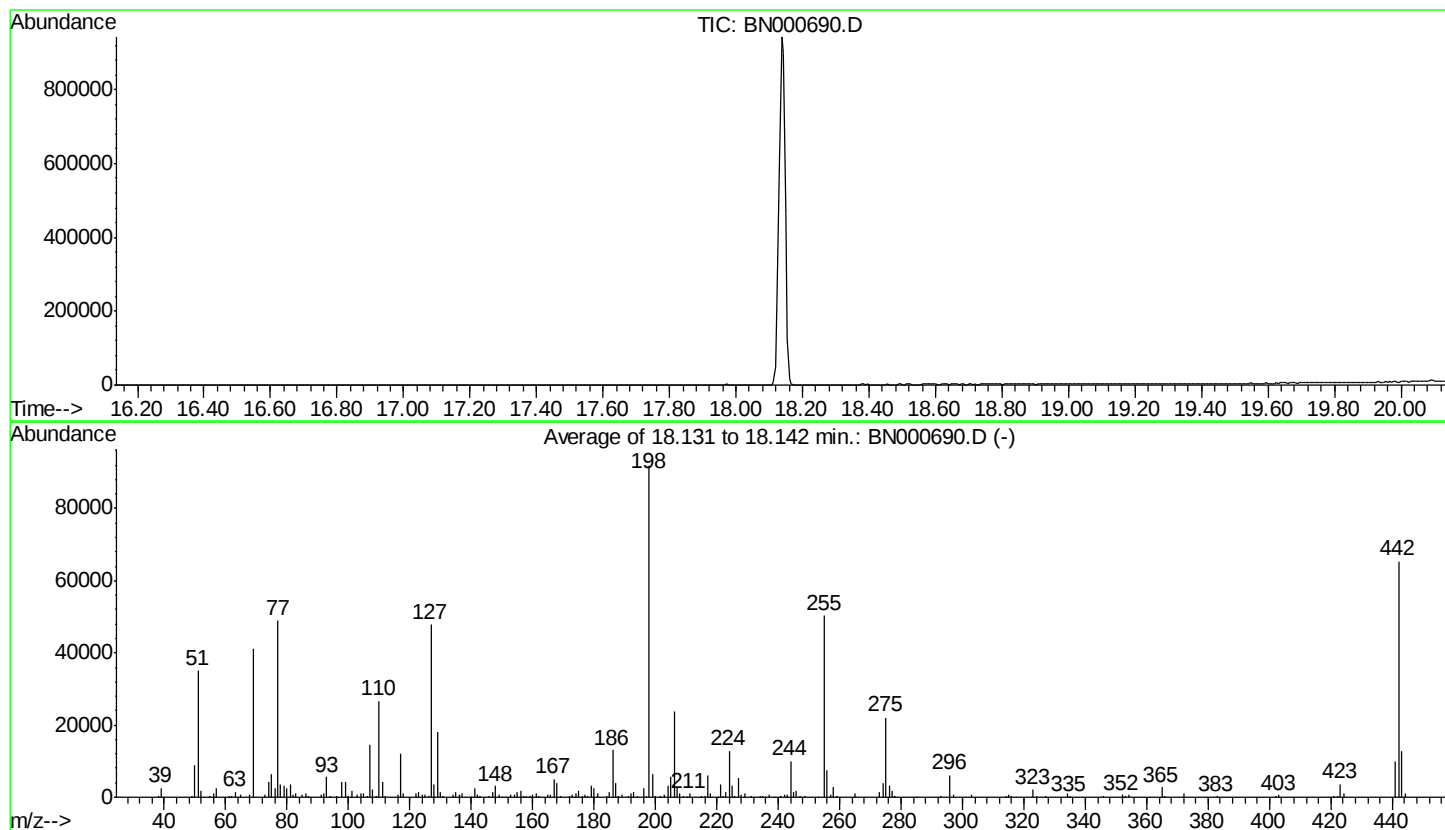

AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	34965	PASS
68	69	0.00	2	1.8	744	PASS
69	198	0.00	100	44.8	41178	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	47773	PASS
197	198	0.00	2	0.5	465	PASS
198	198	100	100	100.0	91880	PASS
199	198	5	9	6.9	6333	PASS
275	198	10	60	23.9	21994	PASS
365	198	1	100	3.1	2813	PASS
441	443	0.01	100	78.5	10070	PASS
442	198	50	100	71.1	65285	PASS
443	442	15	24	19.7	12830	PASS

m/z	Abundance
39.00	2357.0
40.00	417.0
44.00	414.0
49.10	321.0
50.00	7672.0
51.00	29664.0
52.00	1662.0
55.00	336.0
56.00	940.0
57.00	2211.0
61.00	435.0
62.00	450.0
63.00	1265.0
65.00	709.0
67.90	614.0
69.00	35384.0
73.00	599.0
74.00	3674.0
75.00	5757.0
76.00	1921.0
77.10	40424.0
78.00	3215.0
79.00	2807.0
80.00	1995.0
81.00	3001.0
82.00	749.0
83.00	779.0
85.00	612.0
86.00	978.0
87.00	427.0
90.90	777.0
91.90	756.0
93.00	4407.0
94.00	349.0
98.00	3475.0
99.00	3963.0
100.00	336.0
101.00	1432.0
103.00	599.0
104.00	990.0
105.00	934.0
106.00	359.0
107.00	11942.0
108.00	2047.0
109.10	453.0
110.00	21936.0
111.00	3435.0
111.90	411.0
115.90	583.0
117.00	9688.0
118.00	777.0
121.90	664.0
123.00	1328.0
124.00	578.0
124.90	506.0
127.00	38008.0
128.00	3001.0
129.00	14628.0
130.00	1230.0
130.90	328.0
133.90	422.0
135.00	1168.0
136.00	523.0
137.00	944.0
141.00	1956.0
141.90	645.0
142.90	374.0
146.00	329.0
147.00	1087.0
148.00	2292.0
149.00	600.0
152.90	584.0
154.00	458.0
155.00	1033.0
156.00	1472.0
159.90	666.0
161.00	807.0
165.00	571.0
165.90	505.0
167.00	3681.0
168.00	3378.0
169.00	492.0
172.00	418.0
173.00	453.0
174.00	580.0
175.00	1548.0
176.00	414.0
177.00	668.0
179.00	2488.0
180.00	1862.0
181.00	992.0

Instrument :
BNA_N
ClientSampleId :
DFTPP90

185.00	1220.0
186.00	9765.0
187.00	2958.0
188.00	326.0
189.00	548.0
191.00	340.0
192.00	792.0
193.00	861.0
196.00	1991.0
197.10	548.0
198.00	67760.0
199.00	4701.0
200.00	367.0
203.00	474.0
204.00	2396.0
205.00	3998.0
206.10	17928.0
207.10	2862.0
208.00	666.0
209.00	393.0
211.00	736.0
216.00	332.0
217.00	4273.0
218.00	706.0
221.10	2422.0
223.00	1001.0
224.10	9149.0
225.00	2247.0
226.00	372.0
227.00	3414.0
228.00	637.0
229.00	885.0
231.00	362.0
237.00	473.0
242.00	457.0
243.10	552.0
244.10	6907.0
245.10	961.0
246.00	1327.0
255.00	35720.0
256.00	5295.0
257.00	479.0
258.00	2047.0
258.90	354.0
265.00	824.0
273.00	1021.0
274.00	2878.0
275.10	15008.0
276.00	2261.0
277.00	1257.0
277.90	319.0
292.90	346.0
296.00	4195.0
297.00	596.0
303.00	502.0
315.00	439.0
323.00	1293.0
334.00	674.0
346.00	337.0
352.00	466.0
353.00	355.0
354.00	439.0
365.00	2018.0
372.00	673.0
403.00	306.0
423.00	2017.0
424.10	841.0
441.10	5425.0
442.10	35600.0
443.10	7220.0
444.10	612.0

Instrument :
BNA_N
ClientSampleId :
DFTPP90

m/z	Abundance
38.00	558.0
39.00	2809.0
40.00	534.0
44.00	330.0
49.00	434.0
50.00	10455.0
51.00	41288.0
52.00	2253.0
55.00	400.0
55.90	1195.0
57.00	2948.0
61.00	529.0
62.00	608.0
63.00	1796.0
65.00	1144.0
68.00	912.0
69.00	47584.0
73.00	573.0
74.00	4892.0
75.00	7497.0
76.10	2947.0
77.10	57664.0
78.00	4128.0
79.00	4058.0
80.00	2997.0
81.00	3955.0
82.00	1018.0
83.00	1136.0
84.90	1023.0
86.00	1201.0
86.90	599.0
91.00	775.0
92.00	1067.0
93.00	6678.0
94.00	455.0
96.10	345.0
98.00	5310.0
99.00	4811.0
100.00	399.0
101.00	2249.0
103.00	760.0
104.00	1392.0
105.00	1394.0
106.10	487.0
107.00	16752.0
108.00	2571.0
109.00	556.0
110.00	30968.0
111.00	4840.0
112.00	593.0
116.00	945.0
117.00	14529.0
118.00	1239.0
122.00	1125.0
123.00	1628.0
124.00	829.0
125.00	744.0
126.10	368.0
127.00	55360.0
128.00	4227.0
129.00	21264.0
130.00	1924.0
131.00	375.0
133.90	665.0
135.00	1719.0
136.00	726.0
137.00	1222.0
140.00	319.0
141.00	3015.0
141.90	901.0
142.90	672.0
145.90	523.0
147.00	1602.0
148.00	3649.0
149.00	889.0
150.00	318.0
153.00	880.0
154.00	658.0
155.00	1618.0
156.00	2189.0
156.90	355.0
157.90	523.0
159.00	429.0
160.00	904.0
161.00	1254.0
162.00	415.0
165.00	956.0
166.00	851.0
167.00	5901.0
168.00	4496.0
169.00	558.0

Instrument :
BNA_N
ClientSampleId :
DFTPP90

172.00	491.0
172.90	682.0
174.00	1155.0
175.00	2404.0
176.10	542.0
177.00	910.0
178.10	363.0
179.00	3689.0
180.00	3183.0
181.00	1259.0
184.00	343.0
185.00	1795.0
186.00	15293.0
187.00	4226.0
188.00	441.0
189.00	892.0
191.00	482.0
192.00	1351.0
193.00	1541.0
194.00	365.0
196.00	2930.0
198.00	106488.0
199.00	7621.0
200.00	605.0
201.40	445.0
203.00	815.0
204.00	3988.0
205.00	6898.0
206.10	27272.0
207.00	4229.0
208.00	1190.0
209.00	384.0
211.00	1043.0
215.10	318.0
216.00	604.0
217.00	6829.0
218.00	1083.0
221.00	3669.0
221.90	1048.0
223.00	1595.0
224.00	14980.0
225.10	3681.0
225.90	425.0
227.00	6454.0
228.00	975.0
229.00	1422.0
231.00	473.0
234.00	426.0
235.00	419.0
237.00	686.0
238.90	313.0
241.00	382.0
242.00	670.0
243.00	855.0
244.10	11454.0
245.10	1563.0
246.00	2199.0
247.00	453.0
248.90	387.0
255.00	57512.0
256.00	8488.0
257.00	735.0
258.00	3578.0
259.10	484.0
265.00	1396.0
273.00	1695.0
274.00	4364.0
275.10	25008.0
276.00	3760.0
277.00	2187.0
278.10	432.0
293.00	475.0
296.00	6686.0
297.00	950.0
303.10	749.0
314.00	329.0
315.00	719.0
315.90	437.0
323.10	2239.0
324.10	350.0
326.90	521.0
334.10	1417.0
335.00	358.0
346.00	430.0
352.00	695.0
353.00	400.0
354.00	874.0
365.00	2858.0
366.00	489.0
372.00	1144.0
383.00	346.0
402.00	514.0
403.10	748.0
421.10	606.0
422.00	669.0

Instrument :
BNA_N
ClientSampleId :
DFTPP90

423.10	4055.0
424.00	1466.0
441.10	11478.0
442.10	71432.0
443.10	14687.0
444.10	1424.0

Instrument :
BNA_N
ClientSampleId :
DFTPP90

m/z	Abundance
38.00	426.0
39.00	2386.0
40.00	420.0
44.00	317.0
49.10	362.0
50.00	8254.0
51.10	33944.0
52.10	1663.0
55.00	412.0
56.00	1017.0
57.00	2591.0
61.00	496.0
62.00	522.0
63.00	1407.0
65.00	822.0
68.00	706.0
69.00	40568.0
73.00	642.0
74.00	4530.0
75.00	6414.0
76.00	2182.0
77.00	48520.0
78.00	3706.0
79.00	3083.0
80.00	2171.0
81.00	3331.0
82.00	859.0
83.00	818.0
85.00	874.0
86.00	1075.0
87.00	541.0
91.00	942.0
92.00	990.0
93.00	5605.0
93.90	393.0
96.00	346.0
98.00	4131.0
99.00	4172.0
100.00	305.0
101.00	1921.0
102.90	614.0
104.00	1269.0
105.00	1161.0
105.90	339.0
107.00	14572.0
108.00	2245.0
109.00	423.0
110.00	27424.0
111.00	4074.0
112.00	510.0
116.00	899.0
117.00	12523.0
118.00	1081.0
122.00	964.0
123.00	1488.0
124.00	742.0
125.00	672.0
126.10	363.0
127.00	49952.0
128.00	3531.0
129.00	18464.0
130.00	1542.0
134.00	571.0
135.00	1605.0
136.00	693.0
137.00	978.0
141.00	2592.0
142.00	796.0
142.90	564.0
146.00	488.0
147.00	1320.0
148.00	3194.0
149.00	677.0
151.10	380.0
153.00	842.0
154.00	592.0
155.00	1217.0
156.00	2091.0
157.00	411.0
157.90	467.0
159.00	387.0
160.00	715.0
161.00	1171.0
162.00	361.0
165.00	962.0
166.00	731.0
167.00	5417.0
168.00	3560.0
169.00	543.0
171.90	436.0
173.00	715.0

Instrument :
BNA_N
ClientSampleId :
DFTPP90

174.00	1228.0
175.00	1871.0
176.10	644.0
177.00	923.0
178.00	352.0
179.00	3658.0
180.00	2796.0
181.00	1243.0
183.90	316.0
185.00	1703.0
186.00	13904.0
187.00	4103.0
188.00	529.0
189.00	948.0
191.00	415.0
192.00	1306.0
193.00	1498.0
194.00	312.0
196.00	2872.0
197.20	848.0
198.00	101392.0
199.00	6678.0
199.90	463.0
201.50	483.0
203.00	728.0
204.00	3744.0
205.00	5986.0
206.10	26440.0
207.00	4192.0
208.00	976.0
209.10	328.0
210.00	445.0
210.30	457.0
211.00	994.0
215.00	318.0
216.00	547.0
217.00	6700.0
218.00	964.0
220.30	312.0
221.10	4174.0
223.00	1432.0
224.10	14674.0
225.00	3793.0
226.10	364.0
227.00	6290.0
228.00	776.0
229.00	1402.0
231.10	521.0
234.00	437.0
235.00	350.0
236.00	301.0
237.00	558.0
241.00	443.0
242.10	789.0
243.00	922.0
244.10	11647.0
245.00	1506.0
246.00	2225.0
247.00	436.0
248.90	468.0
253.00	328.0
255.00	57552.0
256.00	8255.0
257.00	720.0
258.00	3317.0
259.00	566.0
265.00	1325.0
273.00	1893.0
274.10	4737.0
275.10	25968.0
276.10	3338.0
277.00	2275.0
278.00	438.0
285.10	423.0
293.00	556.0
296.00	7714.0
297.00	1144.0
303.10	794.0
314.10	303.0
314.90	760.0
316.00	475.0
323.00	2463.0
324.10	445.0
327.00	593.0
334.00	1441.0
335.00	481.0
346.00	599.0
352.10	853.0
353.00	510.0
354.10	749.0
365.00	3565.0
366.00	598.0
372.10	1132.0
382.90	363.0
402.00	568.0

Instrument :
BNA_N
ClientSampleId :
DFTPP90

403.00	815.0
421.00	555.0
422.00	743.0
423.10	5028.0
424.00	1337.0
441.10	13307.0
442.10	88824.0
443.10	16584.0
444.10	1525.0

Instrument :
BNA_N
ClientSampleId :
DFTPP90

Scan 2493 (18.101 min): BN000690.D
DFTPP90

m/z	Abundance
40.00	373.0
44.00	360.0
207.10	738.0

Instrument :
BNA_N
ClientSampleId :
DFTPP90