

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
 Data File : BN014190.D
 Acq On : 02 Apr 2021 14:00
 Operator : CG/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Apr 02 14:32:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 02 14:32:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.684	152	4735	0.40	ng	0.00
7) Naphthalene-d8	10.454	136	17382	0.40	ng	0.00
13) Acenaphthene-d10	14.321	164	9924	0.40	ng	0.00
19) Phenanthrene-d10	17.055	188	21060	0.40	ng	0.00
29) Chrysene-d12	21.247	240	22437	0.40	ng	0.00
36) Perylene-d12	23.466	264	21759	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.284	112	5295	0.44	ng	0.00
5) Phenol-d6	6.855	99	6665	0.43	ng	0.00
8) Nitrobenzene-d5	8.832	82	5068	0.43	ng	0.00
11) 2-Methylnaphthalene-d10	12.053	152	15092	0.57	ng	0.00
14) 2,4,6-Tribromophenol	15.805	330	1344	0.42	ng	0.00
15) 2-Fluorobiphenyl	12.938	172	14951	0.40	ng	0.00
27) Fluoranthene-d10	19.096	212	33205	0.60	ng	0.00
31) Terphenyl-d14	19.697	244	21379	0.41	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.231	88	2444	0.40	ng	100
3) n-Nitrosodimethylamine	3.569	42	1477	0.31	ng	# 96
6) bis(2-Chloroethyl)ether	7.112	93	5392	0.44	ng	100
9) Naphthalene	10.505	128	18612	0.43	ng	100
10) Hexachlorobutadiene	10.796	225	3530	0.45	ng	# 100
12) 2-Methylnaphthalene	12.124	142	12532	0.45	ng	100
16) Acenaphthylene	14.029	152	15677	0.41	ng	100
17) Acenaphthene	14.372	154	11303	0.41	ng	100
18) Fluorene	15.361	166	14488	0.44	ng	100
20) 4,6-Dinitro-2-methylph...	15.450	198	1025	0.39	ng	100
21) 4-Bromophenyl-phenylether	16.264	248	4658	0.43	ng	100
22) Hexachlorobenzene	16.373	284	5183	0.43	ng	100
23) Atrazine	16.532	200	3133	0.42	ng	100
24) Pentachlorophenol	16.714	266	859	0.23	ng	97
25) Phenanthrene	17.104	178	24360	0.43	ng	100
26) Anthracene	17.189	178	20378	0.43	ng	100
28) Fluoranthene	19.126	202	28514	0.48	ng	100
30) Pyrene	19.488	202	29125	0.40	ng	100
32) Benzo(a)anthracene	21.237	228	28854	0.46	ng	100
33) Chrysene	21.279	228	30246	0.44	ng	100
34) Bis(2-ethylhexyl)phtha...	21.173	149	11750	0.62	ng	100
35) Indeno(1,2,3-cd)pyrene	25.687	276	35534	0.50	ng	100
37) Benzo(b)fluoranthene	22.798	252	32477	0.42	ng	100
38) Benzo(k)fluoranthene	22.843	252	30899	0.41	ng	100
39) Benzo(a)pyrene	23.367	252	28316	0.43	ng	100
40) Dibenzo(a,h)anthracene	25.701	278	29927	0.44	ng	100
41) Benzo(g,h,i)perylene	26.372	276	31466	0.44	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
Data File : BN014190.D
Acq On : 02 Apr 2021 14:00
Operator : CG/JU
Sample : SSTDICCC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Quant Time: Apr 02 14:32:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 02 14:32:17 2021
Response via : Initial Calibration

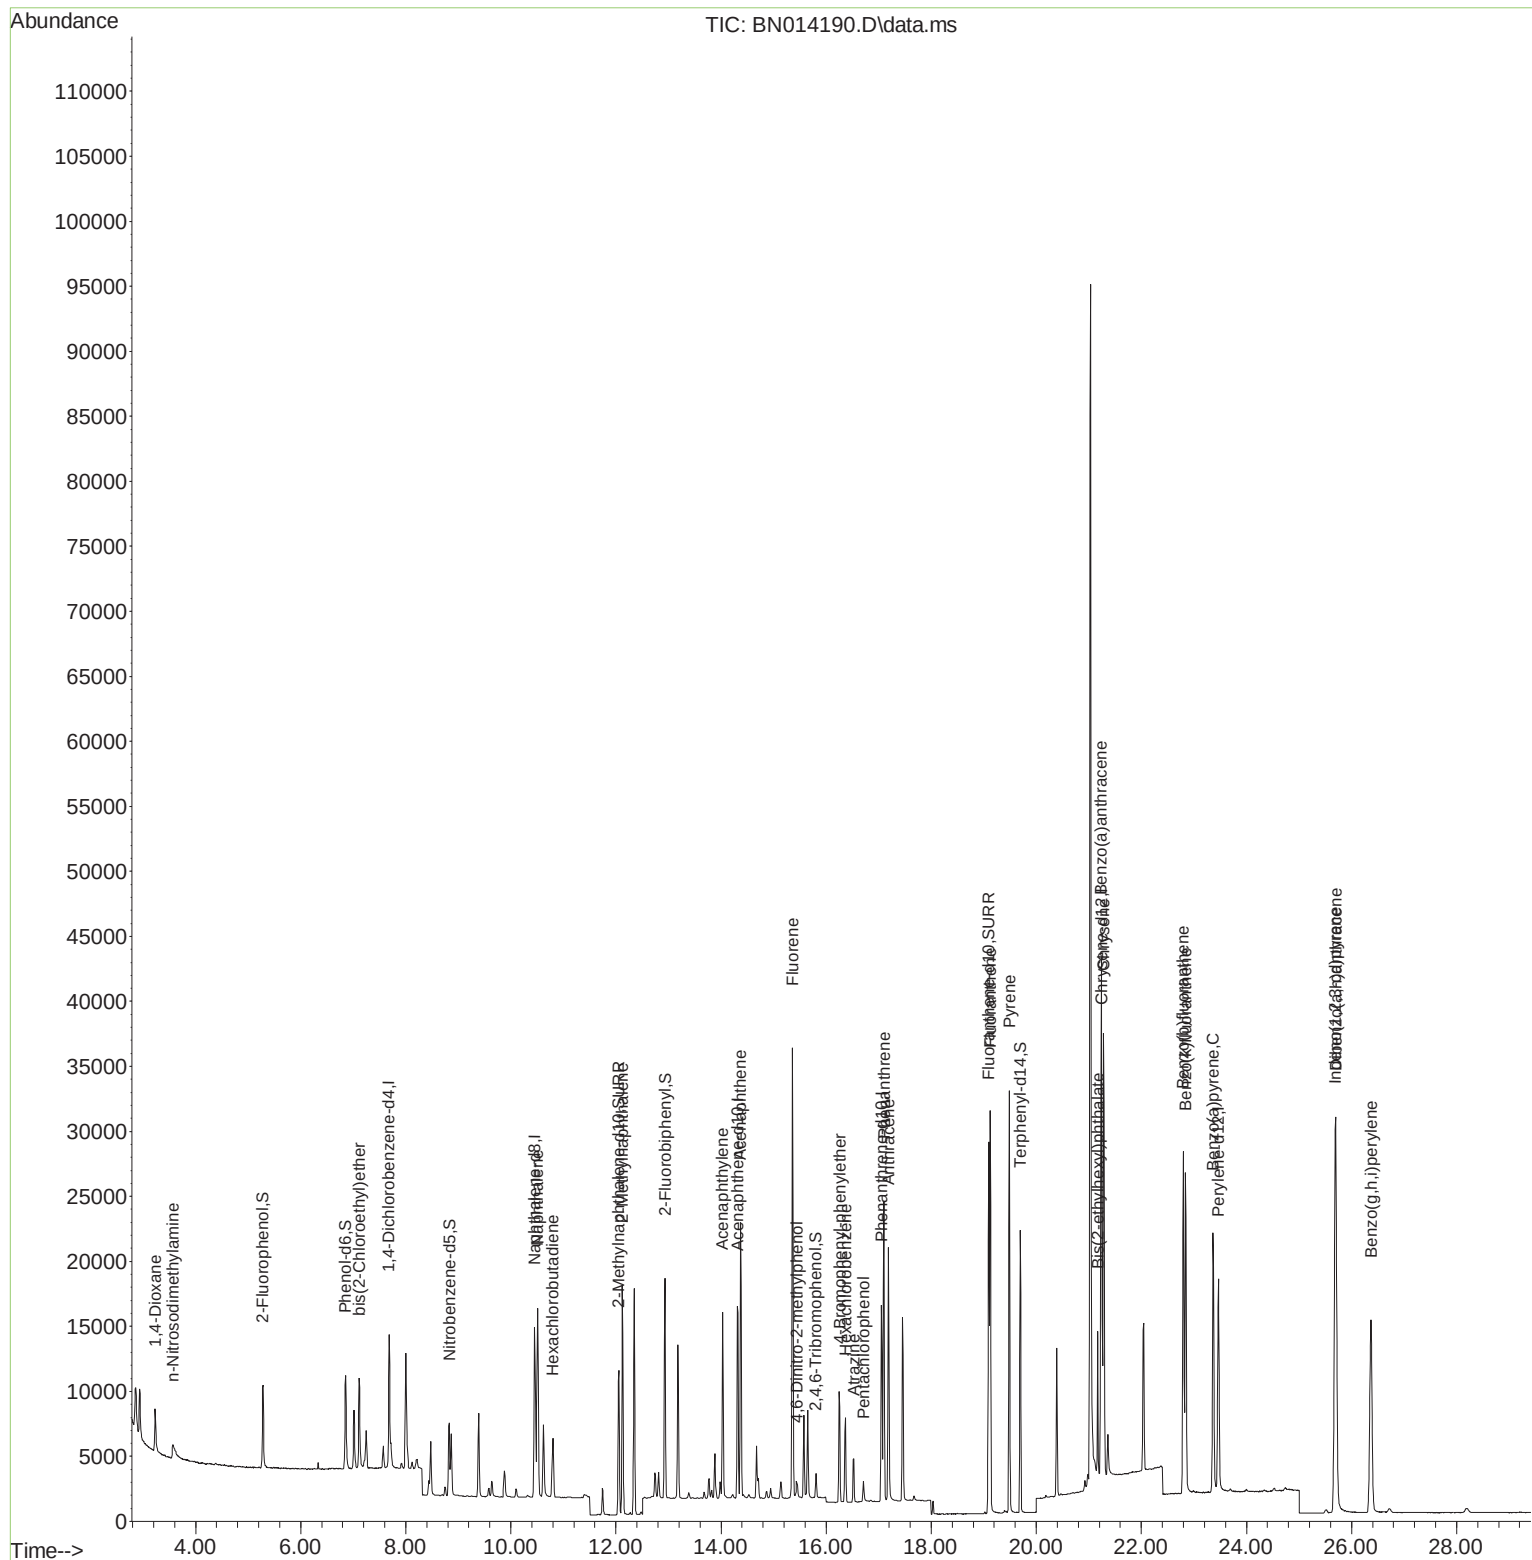




Abundance Scan 609 (7.684 min): BN014190.D\data.ms (-602) (#1)

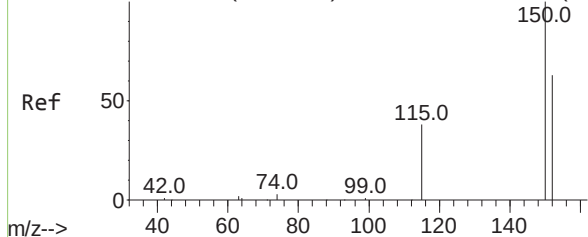


1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.684 min Scan# 609
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:152 Resp: 4735
Ion Ratio Lower Upper
152 100
150 157.8 126.2 189.4
115 62.2 49.8 74.6

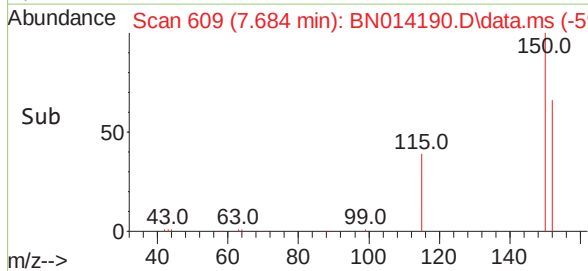
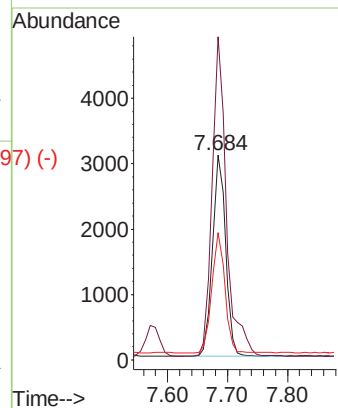
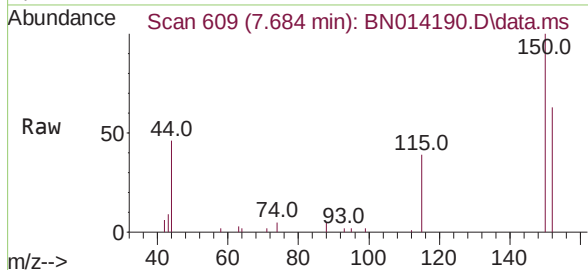



Abundance Scan 56 (3.231 min): BN014190.D\data.ms (-53) (#2)

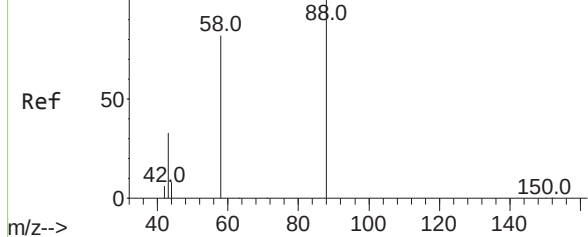

1,4-Dioxane
Concen: 0.40 ng
RT: 3.231 min Scan# 56
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Tgt Ion: 88 Resp: 2444
Ion Ratio Lower Upper
88 100
58 79.0 63.2 94.8
43 31.4 25.1 37.7


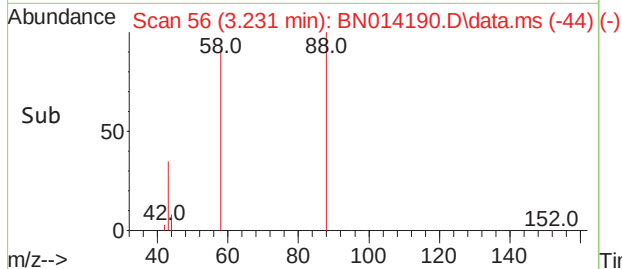
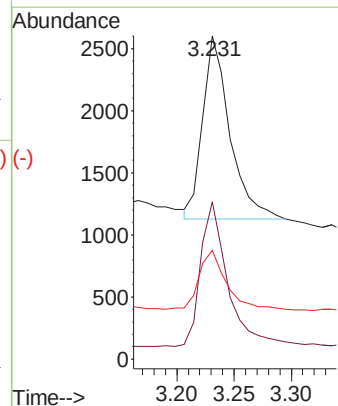
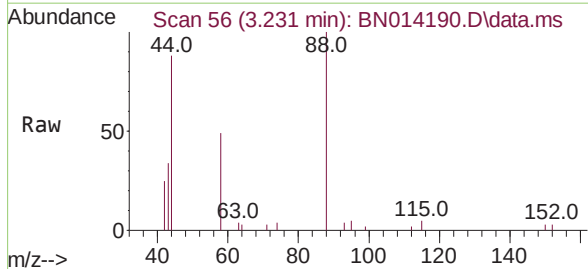


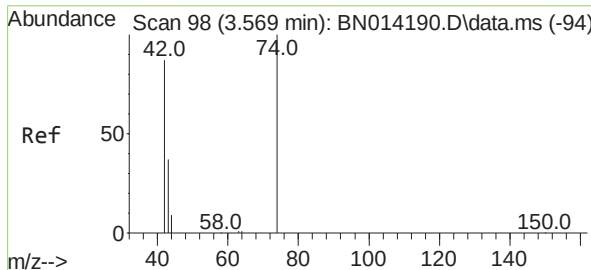

n-Nitrosodimethylamine
Concen: 0.31 ng
RT: 3.569 min Scan# 98
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00




Instrument :
BNA_N
ClientSampled :
SSTDICCC0.4


Tgt Ion: 42 Resp: 1477
Ion Ratio Lower Upper
42 100
74 127.5 98.8 148.2
44 0.0 0.0 0.0

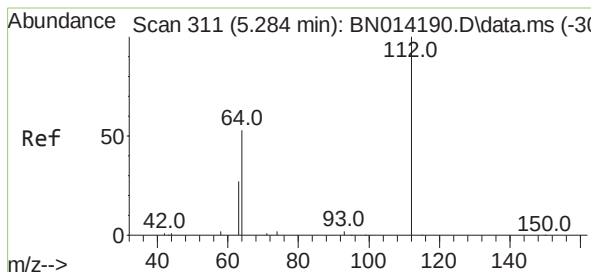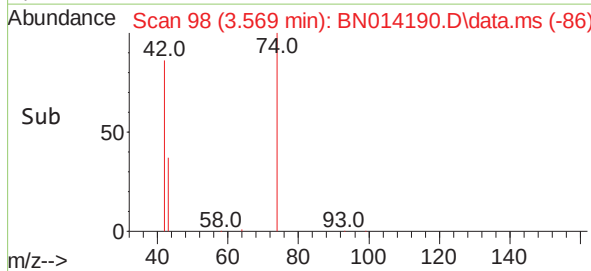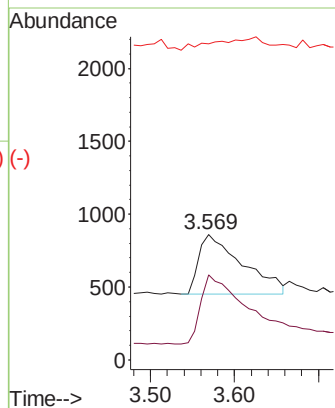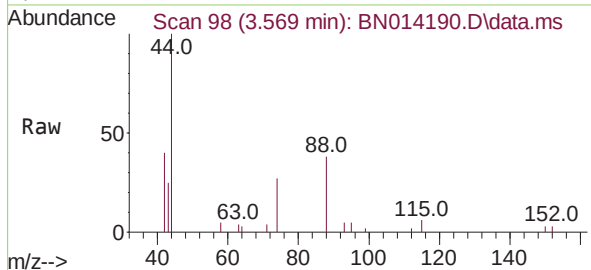

2-Fluorophenol
Concen: 0.44 ng
RT: 5.284 min Scan# 311
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Tgt Ion: 112 Resp: 5295
Ion Ratio Lower Upper
112 100
64 60.4 48.3 72.5
63 32.2 25.8 38.6


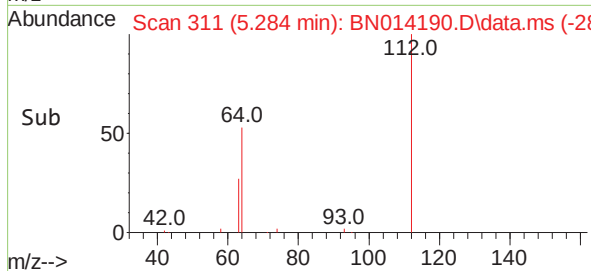
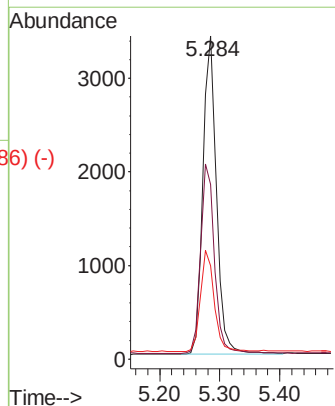
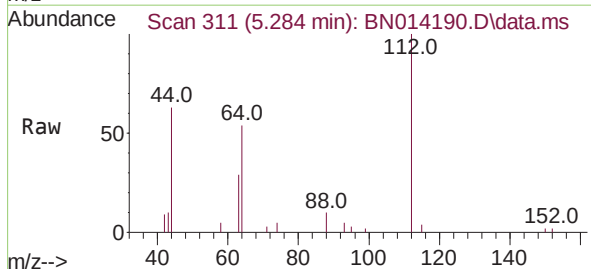


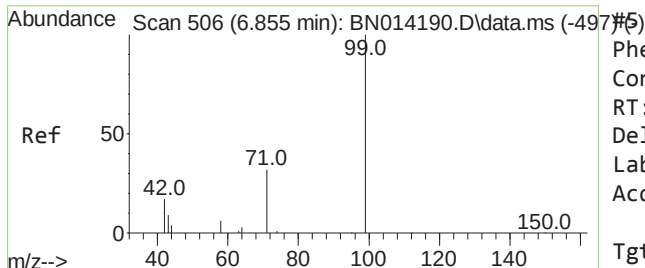

Phenol-d6
 Concen: 0.43 ng
 RT: 6.855 min Scan# 506
 Delta R.T. 0.000 min
 Lab File: BN014190.D
 Acq: 02 Apr 2021 14:00




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Tgt Ion:	99	Resp:	6665
Ion	Ratio	Lower	Upper
99	100		
42	22.2	17.8	26.6
71	33.3	26.6	40.0

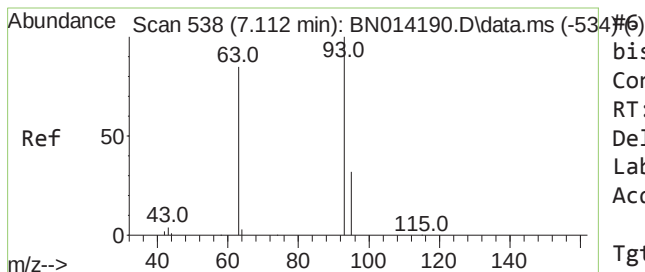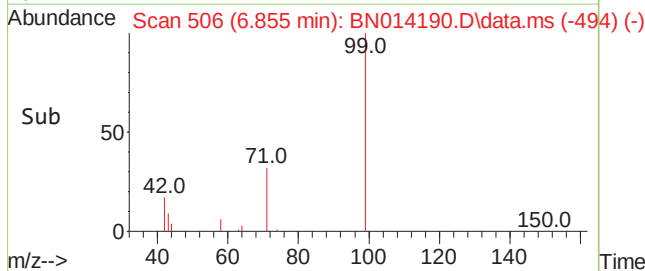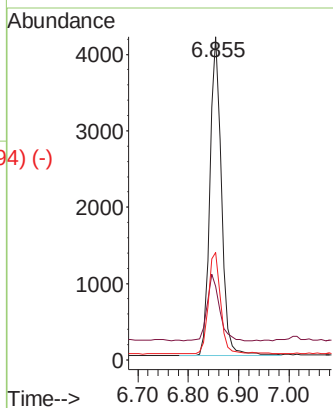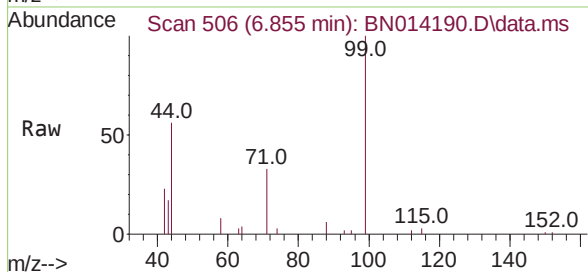


bis(2-Chloroethyl)ether
 Concen: 0.44 ng
 RT: 7.112 min Scan# 538
 Delta R.T. 0.000 min
 Lab File: BN014190.D
 Acq: 02 Apr 2021 14:00

Tgt Ion:	93	Resp:	5392
Ion	Ratio	Lower	Upper
93	100		
63	80.3	64.2	96.4
95	33.3	26.6	40.0

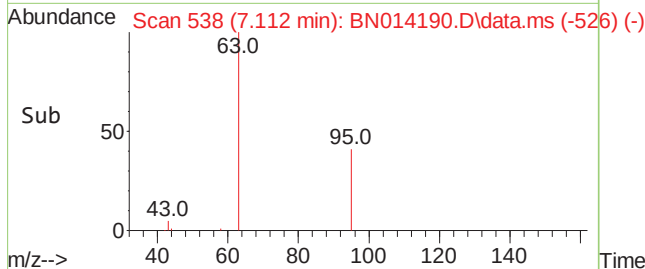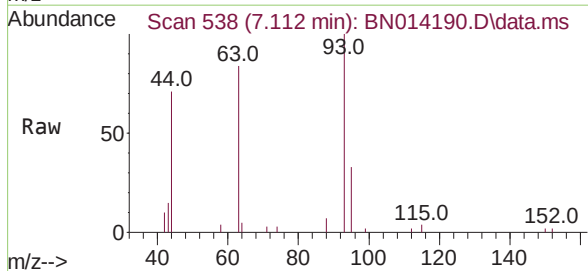




Abundance Scan 856 (10.454 min): BN014190.D\data.ms (-856) (-)

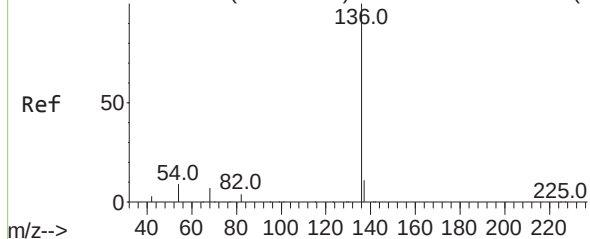


Naphthalene-d8
Concen: 0.40 ng
RT: 10.454 min Scan# 856
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	136	Resp:	17382
Ion	Ratio	Lower	Upper
136	100		
137	11.4	9.1	13.7
54	10.3	8.2	12.4
68	7.6	6.1	9.1

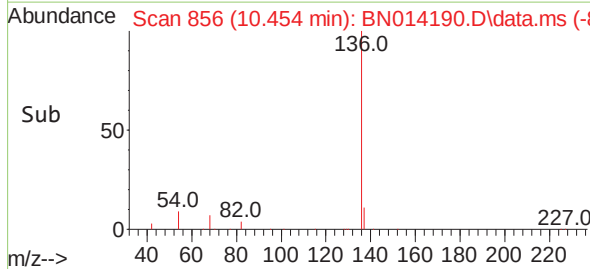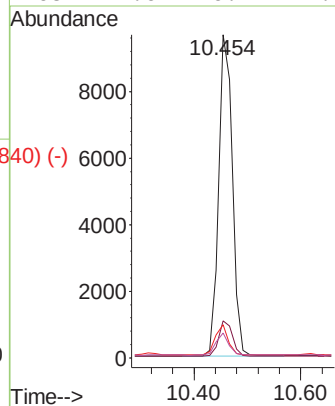
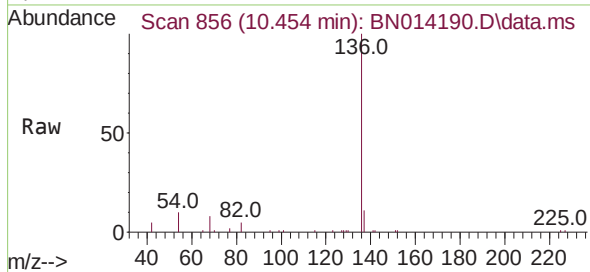


Abundance Scan 728 (8.832 min): BN014190.D\data.ms (-728) (-)

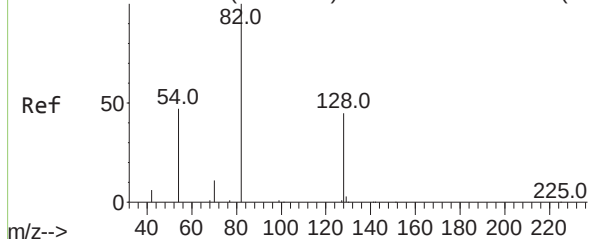


Nitrobenzene-d5
Concen: 0.43 ng
RT: 8.832 min Scan# 728
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00


Tgt Ion:	82	Resp:	5068
Ion	Ratio	Lower	Upper
82	100		
128	46.0	36.8	55.2
54	48.4	38.7	58.1

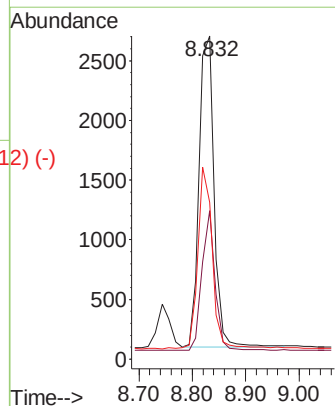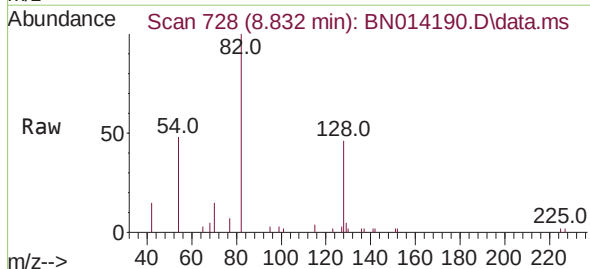

Abundance Scan 728 (8.832 min): BN014190.D\data.ms (-712) (-)

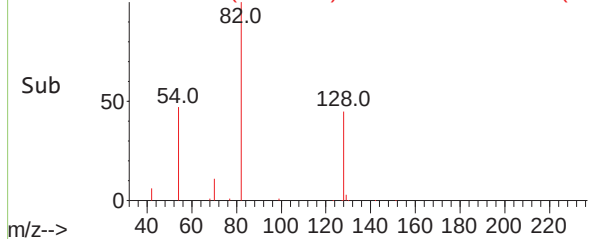




Abundance Scan 860 (10.505 min): BN014190.D\data.ms (-853) (-)




Naphthalene
Concen: 0.43 ng
RT: 10.505 min Scan# 860
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	128	Resp:	18612
Ion	Ratio	Lower	Upper
128	100		
129	11.4	9.1	13.7
127	13.2	10.6	15.8

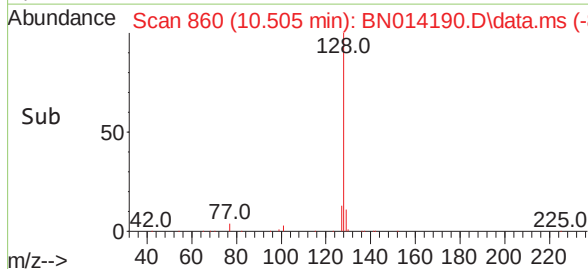

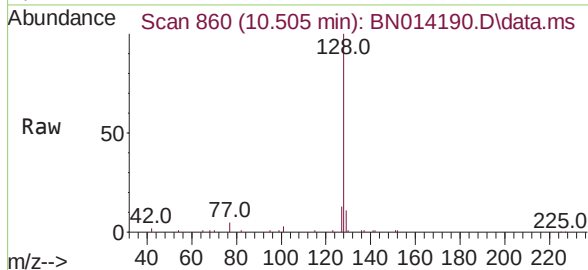


Abundance Scan 883 (10.796 min): BN014190.D\data.ms (-877) (-)




Hexachlorobutadiene
Concen: 0.45 ng
RT: 10.796 min Scan# 883
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Tgt Ion:	225	Resp:	3530
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.5	50.8	76.2

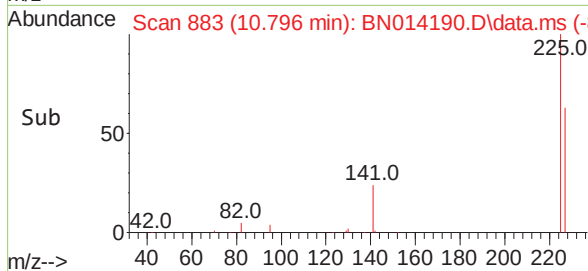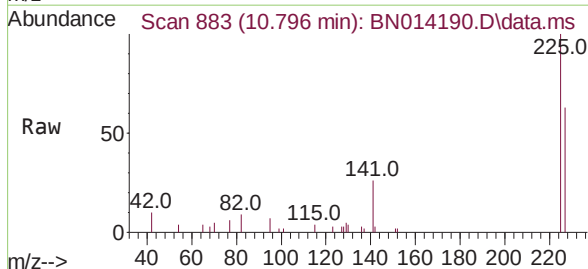




Abundance Scan 1062 (12.053 min): BN014190.D\data.ms (-1017) (-)




2-Methylnaphthalene-d10
Concen: 0.57 ng
RT: 12.053 min Scan# 1062
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:152 Resp: 15092
Ion Ratio Lower Upper
152 100
151 20.1 16.1 24.1

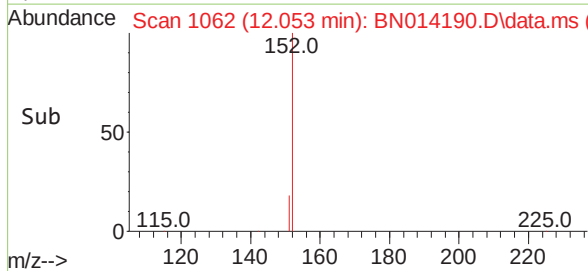
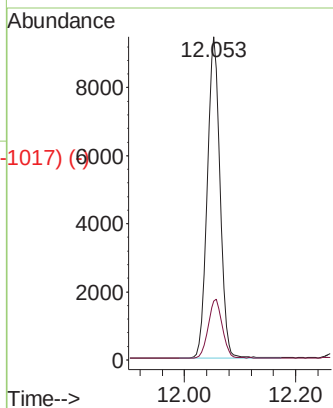
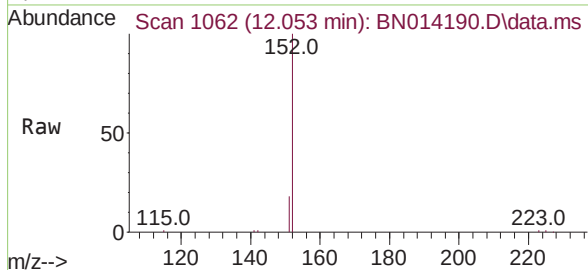


Abundance Scan 1078 (12.124 min): BN014190.D\data.ms (-1056) (-)

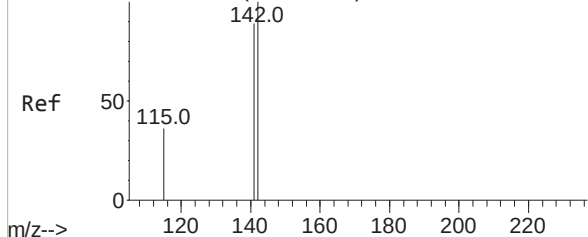

2-Methylnaphthalene
Concen: 0.45 ng
RT: 12.124 min Scan# 1078
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00


Tgt Ion:142 Resp: 12532
Ion Ratio Lower Upper
142 100
141 89.5 71.6 107.4
115 36.5 29.2 43.8

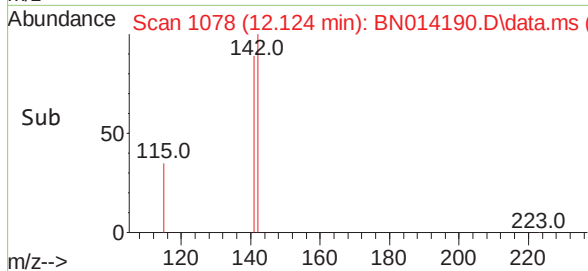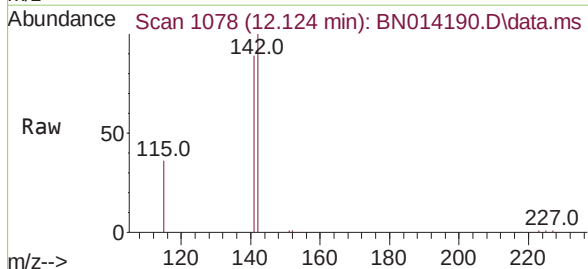




Abundance Scan 1307 (14.321 min): BN014190.D\data.ms (-1291) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.321 min Scan# 1307
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

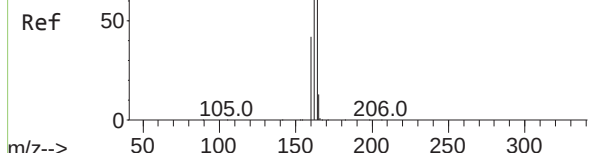





Tgt Ion:	164	Resp:	9924
Ion	Ratio	Lower	Upper
164	100		
162	96.8	77.4	116.2
160	42.8	34.2	51.4

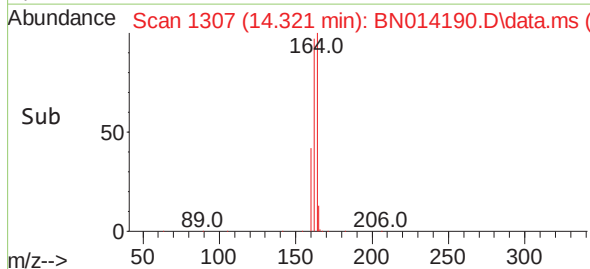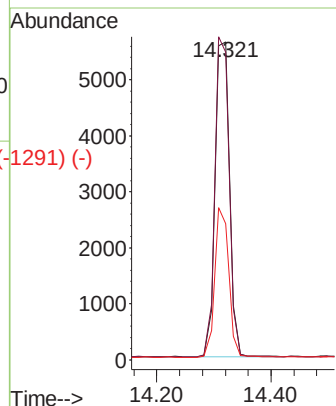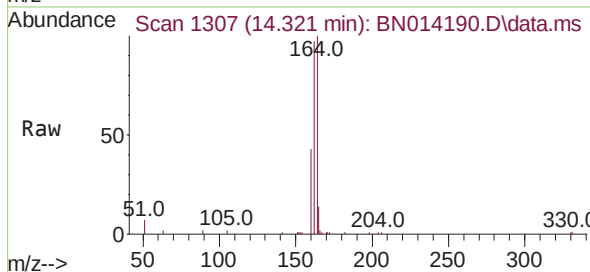


Abundance Scan 1424 (15.805 min): BN014190.D\data.ms (-1416) (-)

2,4,6-Tribromophenol
Concen: 0.42 ng
RT: 15.805 min Scan# 1424
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Tgt Ion:	330	Resp:	1344
Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	36.8	29.8	44.6

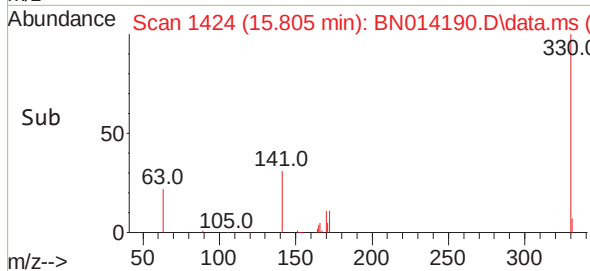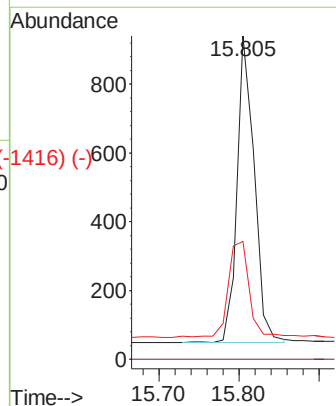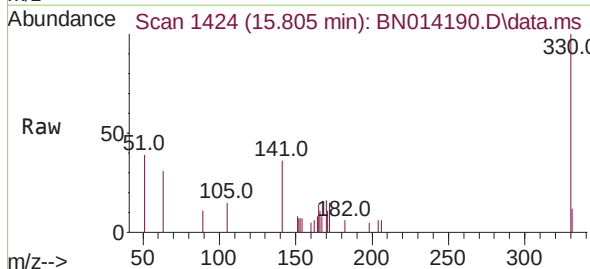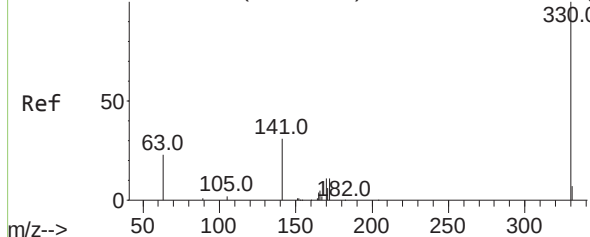




Abundance Scan 1198 (12.938 min): BN014190.D\data.ms (-1190) (-)

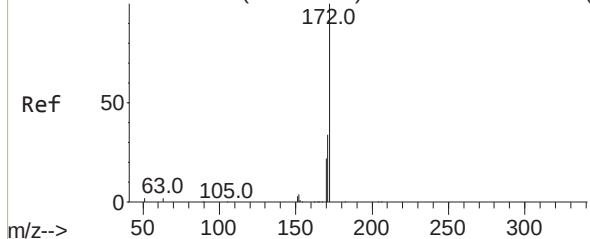


2-Fluorobiphenyl
Concen: 0.40 ng
RT: 12.938 min Scan# 1198
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	172	Resp:	14951
Ion	Ratio	Lower	Upper
172	100		
171	34.1	27.3	40.9
170	22.6	18.1	27.1

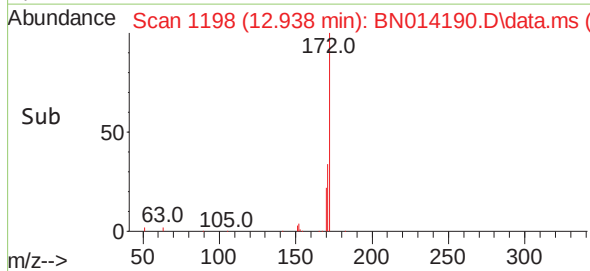
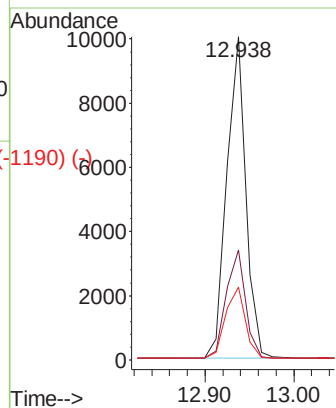
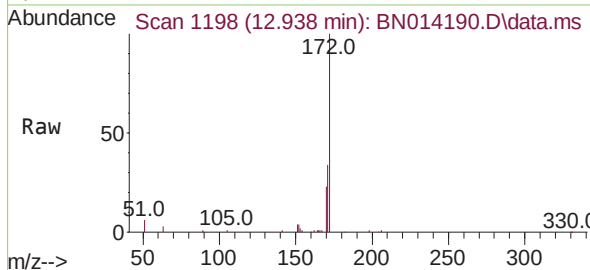


Abundance Scan 1284 (14.029 min): BN014190.D\data.ms (-1268) (-)

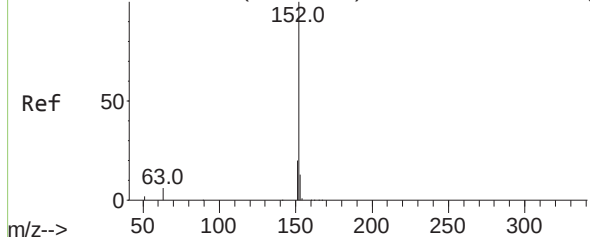

Acenaphthylene
Concen: 0.41 ng
RT: 14.029 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00


Tgt Ion:	152	Resp:	15677
Ion	Ratio	Lower	Upper
152	100		
151	18.9	15.1	22.7
153	13.1	10.5	15.7

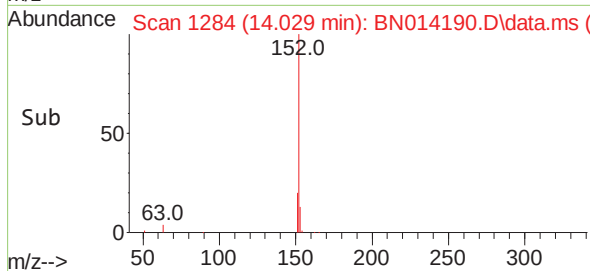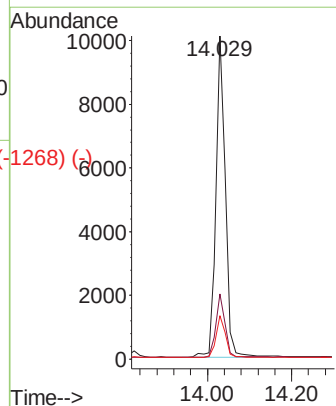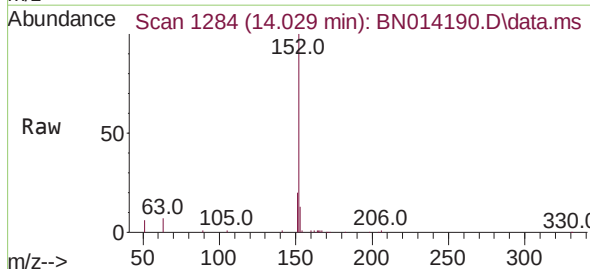




Abundance Scan 1311 (14.372 min): BN014190.D\data.ms (-1303) (-)

Acenaphthene
Concen: 0.41 ng
RT: 14.372 min Scan# 1311
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

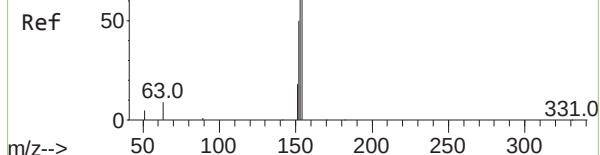


Tgt Ion:	154	Resp:	11303
Ion	Ratio	Lower	Upper
154	100		
153	112.0	89.2	133.8
152	54.9	43.8	65.6

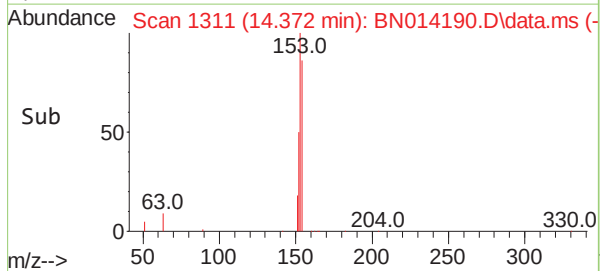
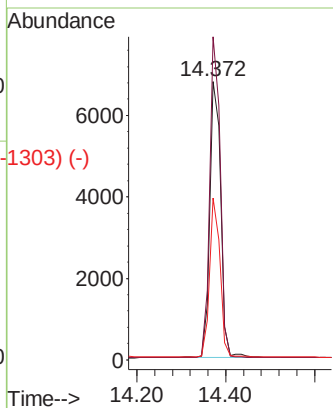
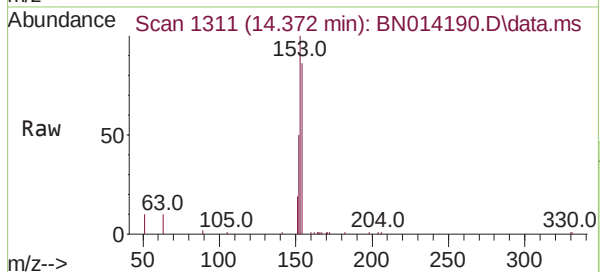



Abundance Scan 1389 (15.361 min): BN014190.D\data.ms (-1373) (-)

Fluorene
Concen: 0.44 ng
RT: 15.361 min Scan# 1389
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

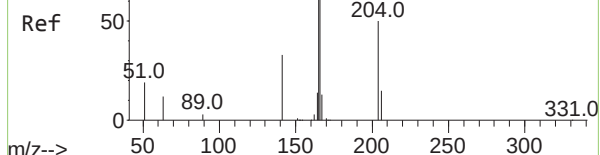

Tgt Ion:	166	Resp:	14488
Ion	Ratio	Lower	Upper
166	100		
165	98.1	78.5	117.7
167	13.6	10.9	16.3


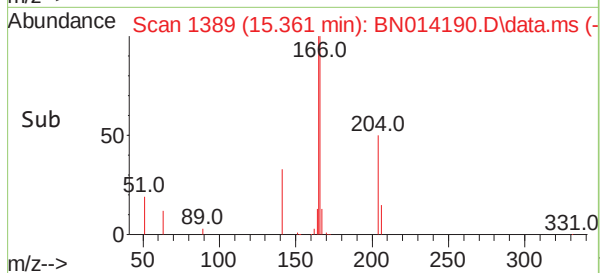

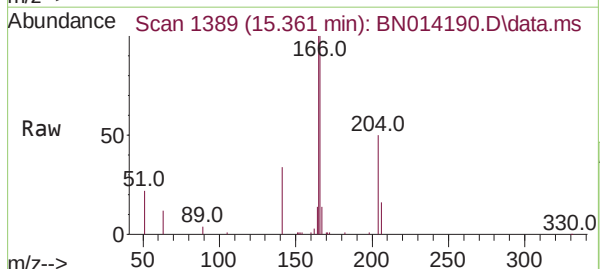


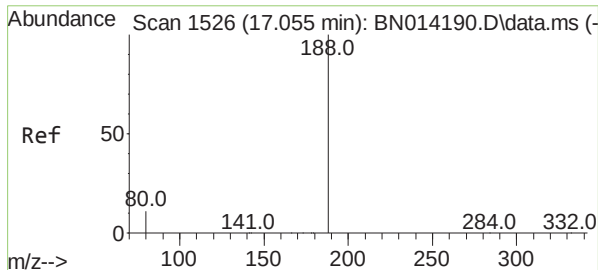

#129 (-)
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.055 min Scan# 1526
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	188	Resp:	21060
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	11.9	9.5	14.3

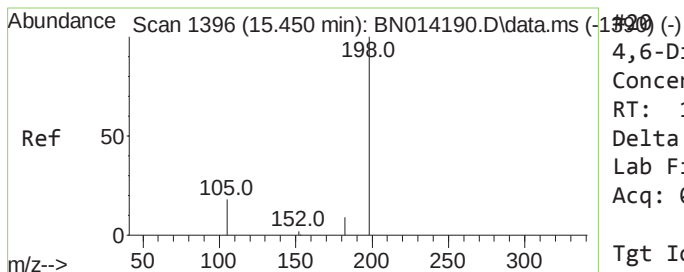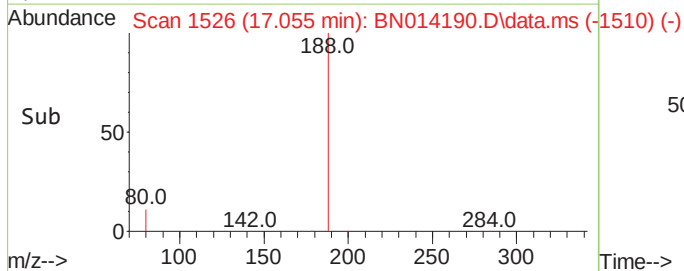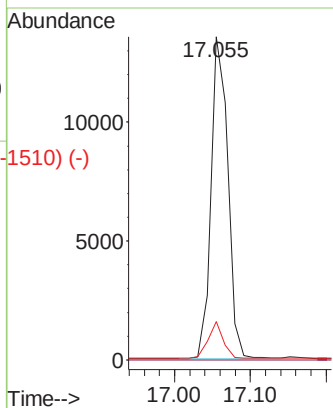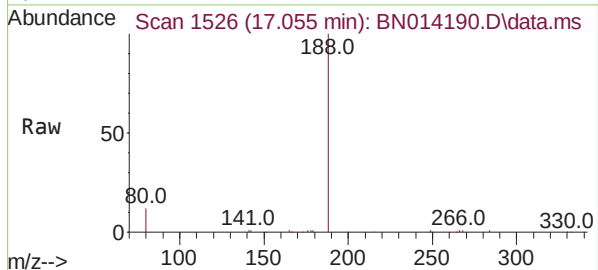


#200 (-)
4,6-Dinitro-2-methylphenol
Concen: 0.39 ng
RT: 15.450 min Scan# 1396
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Tgt Ion:	198	Resp:	1025
Ion	Ratio	Lower	Upper
198	100		
51	74.2	59.4	89.0
105	37.2	29.8	44.6

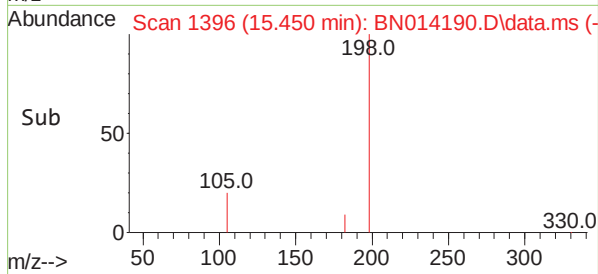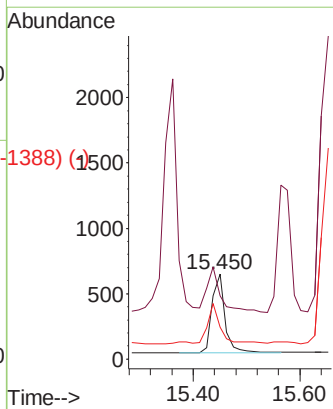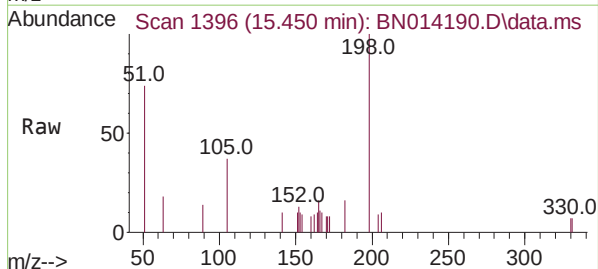




Abundance Scan 1461 (16.264 min): BN014190.D\data.ms (-1453) (-)

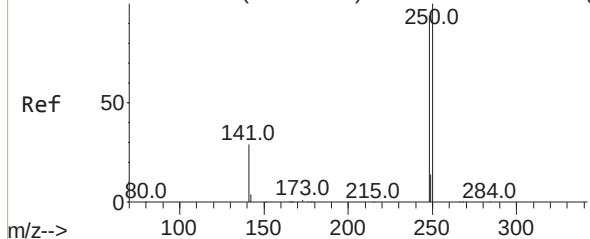


4-Bromophenyl-phenylether
Concen: 0.43 ng
RT: 16.264 min Scan# 1461
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	248	Resp:	4658
Ion	Ratio	Lower	Upper
248	100		
250	107.0	85.6	128.4
141	32.6	26.1	39.1

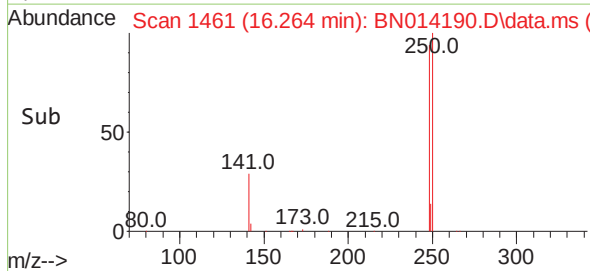
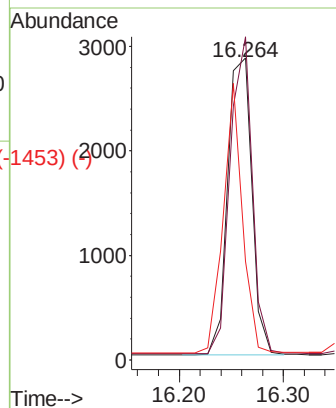
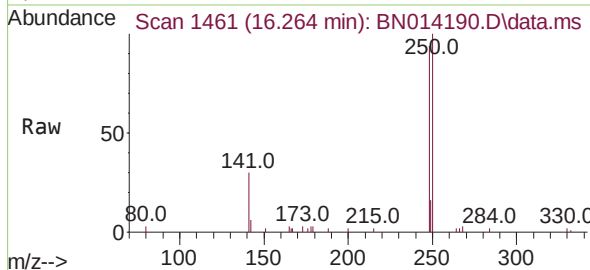


Abundance Scan 1470 (16.373 min): BN014190.D\data.ms (-1462) (-)

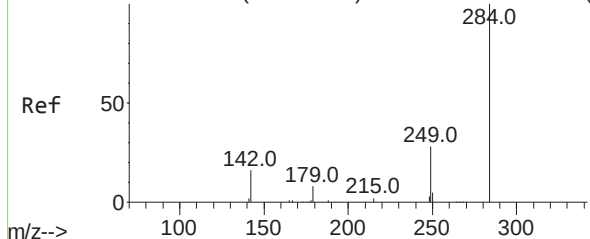

Hexachlorobenzene
Concen: 0.43 ng
RT: 16.373 min Scan# 1470
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00


Tgt Ion:	284	Resp:	5183
Ion	Ratio	Lower	Upper
284	100		
142	35.7	28.6	42.8
249	31.6	25.3	37.9

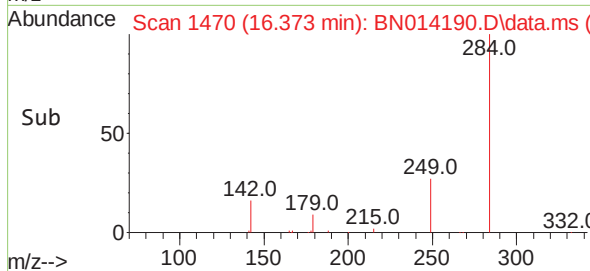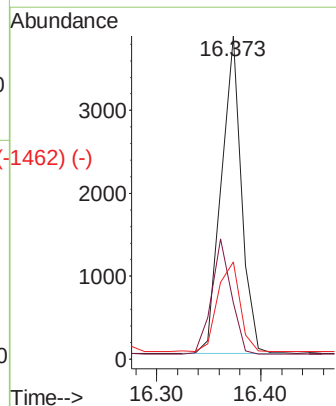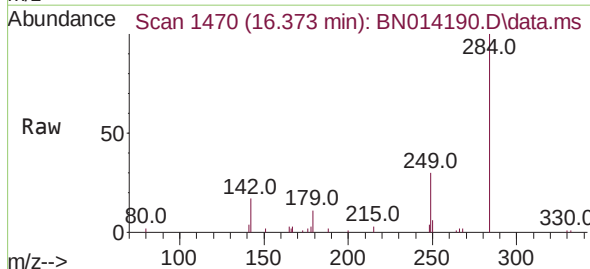



Abundance Scan 1483 (16.532 min): BN014190.D\data.ms (-1425) (-)

Atrazine
Concen: 0.42 ng
RT: 16.532 min Scan# 1483
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00


Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

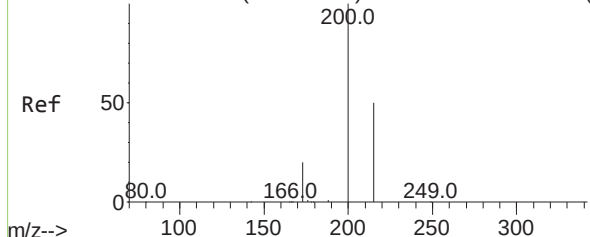

Tgt Ion:	200	Resp:	3133
Ion	Ratio	Lower	Upper
200	100		
173	22.0	17.6	26.4
215	51.7	41.4	62.0

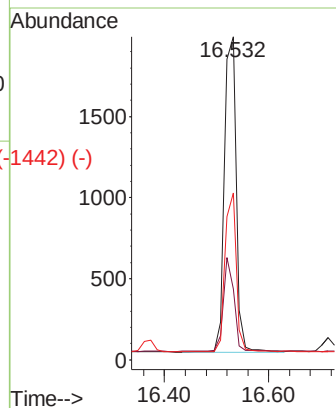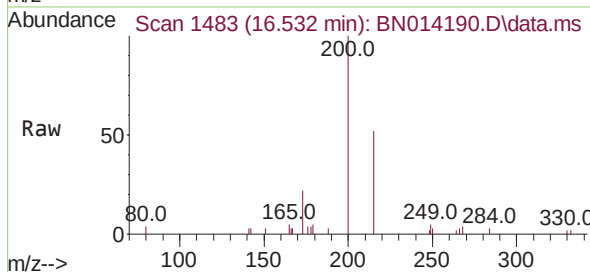



Abundance Scan 1483 (16.532 min): BN014190.D\data.ms (-1442) (-)

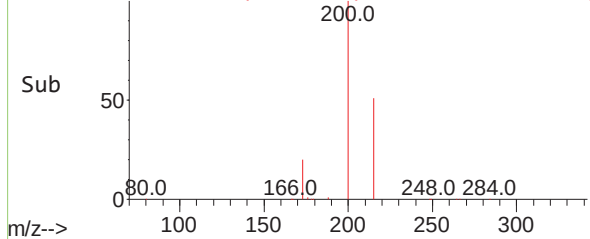


Abundance Scan 1498 (16.714 min): BN014190.D\data.ms (-1421) (-)

Pentachlorophenol
Concen: 0.23 ng
RT: 16.714 min Scan# 1498
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00


Tgt Ion:	266	Resp:	859
Ion	Ratio	Lower	Upper
266	100		
264	66.9	51.8	77.8
268	61.6	47.7	71.5

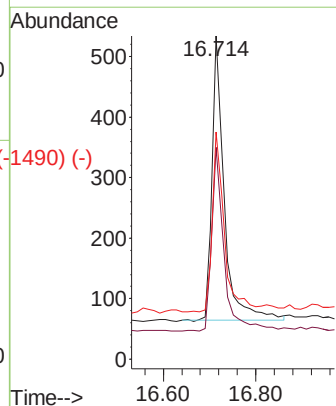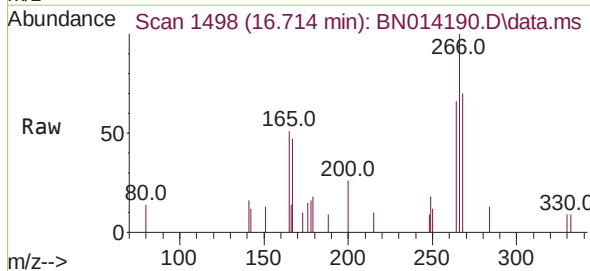

Abundance Scan 1498 (16.714 min): BN014190.D\data.ms (-1490) (-)

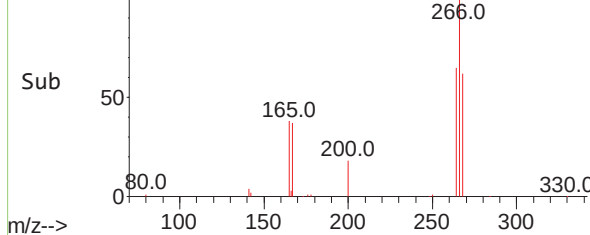




Abundance Scan 1530 (17.104 min): BN014190.D\data.ms (-1525) (-)

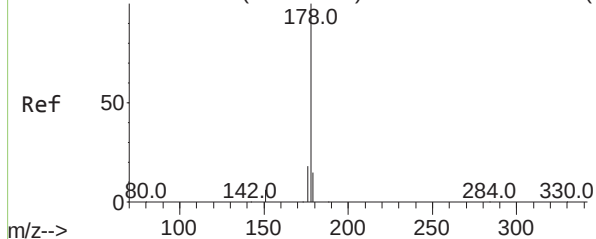


Phenanthrene
Concen: 0.43 ng
RT: 17.104 min Scan# 1530
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:178 Resp: 24360
Ion Ratio Lower Upper
178 100
176 19.0 15.2 22.8
179 15.4 12.3 18.5

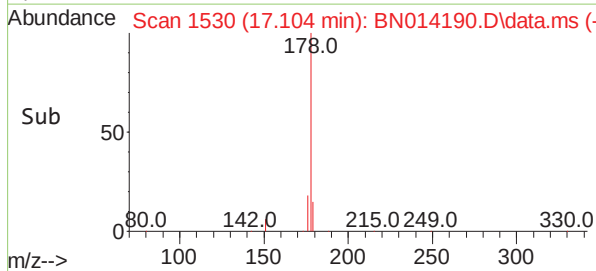
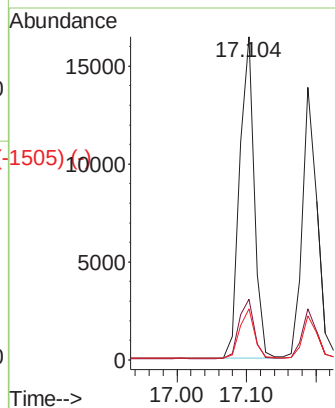
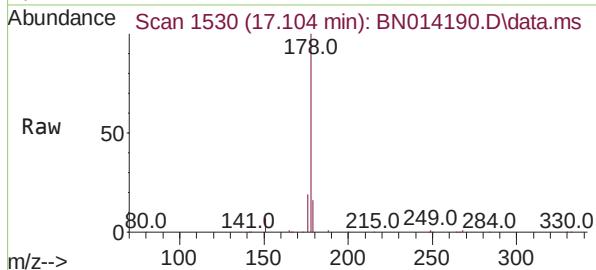


Abundance Scan 1537 (17.189 min): BN014190.D\data.ms (-1526) (-)

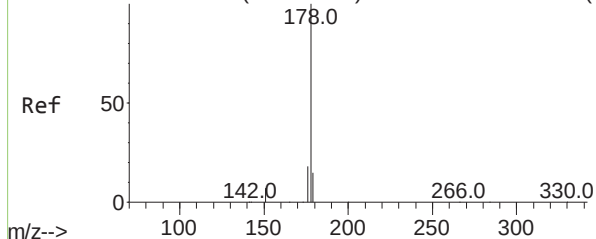


Anthracene
Concen: 0.43 ng
RT: 17.189 min Scan# 1537
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Tgt Ion:178 Resp: 20378
Ion Ratio Lower Upper
178 100
176 18.2 14.6 22.0
179 15.5 12.4 18.6

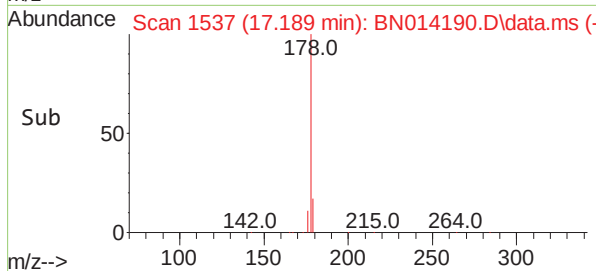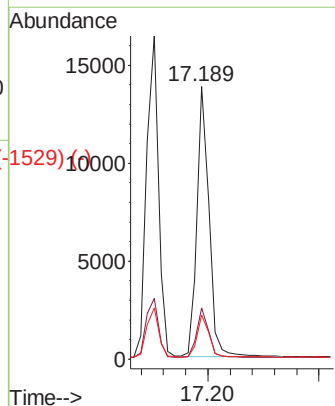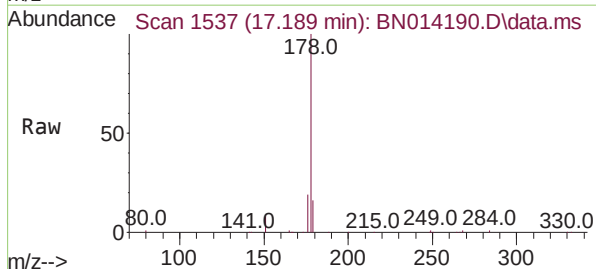




Abundance Scan 1824 (19.096 min): BN014190.D\data.ms (-1824) (-)

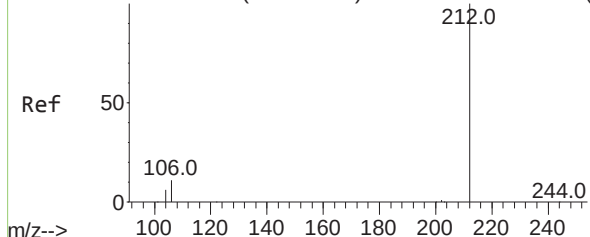


Fluoranthene-d10
Concen: 0.60 ng
RT: 19.096 min Scan# 1824
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	212	Resp:	33205
Ion	Ratio	Lower	Upper
212	100		
106	12.4	9.9	14.9
104	7.0	5.6	8.4

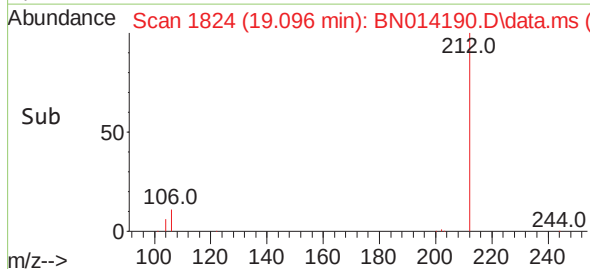
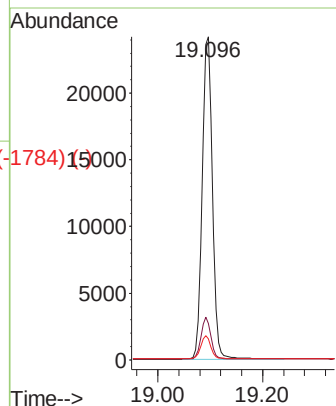
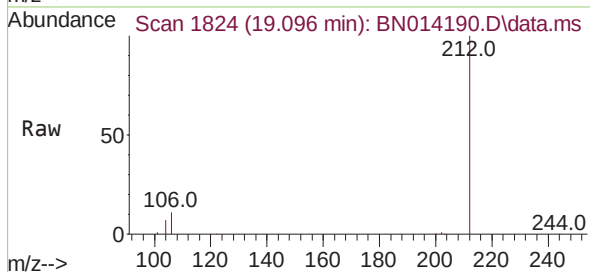


Abundance Scan 1830 (19.126 min): BN014190.D\data.ms (-1828) (-)

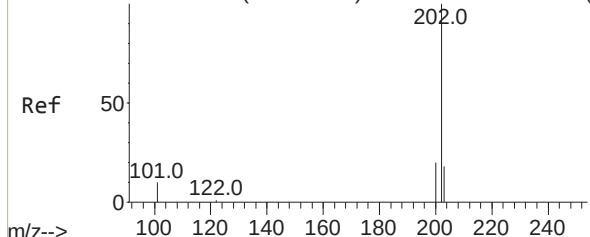

Fluoranthene
Concen: 0.48 ng
RT: 19.126 min Scan# 1830
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Tgt Ion:	202	Resp:	28514
Ion	Ratio	Lower	Upper
202	100		
101	10.6	8.5	12.7
203	17.4	13.9	20.9

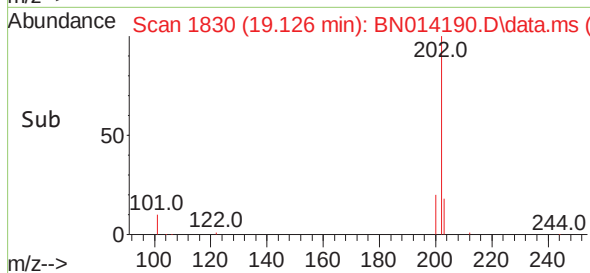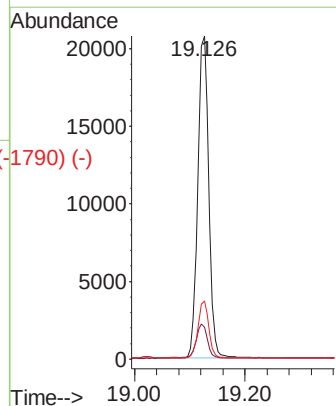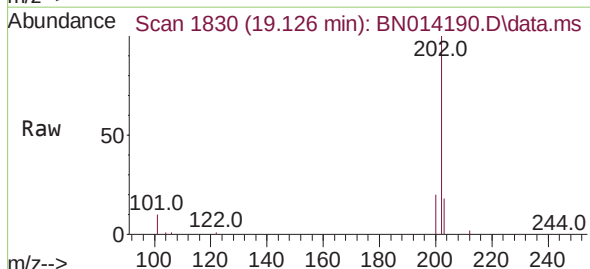

Abundance Scan 2124 (21.247 min): BN014190.D\data.ms (-2105) (-)

Chrysene-d12

Concen: 0.40 ng

RT: 21.247 min Scan# 2124

Delta R.T. 0.000 min

Lab File: BN014190.D

Acq: 02 Apr 2021 14:00

Tgt Ion:240 Resp: 22437

Ion Ratio Lower Upper

240 100

120 9.1 7.3 10.9

236 26.0 20.8 31.2

Abundance Scan 2124 (21.247 min): BN014190.D\data.ms

Ref 50

240.0

91.0 120.0 212.0 279.0

m/z-->

Abundance Scan 2124 (21.247 min): BN014190.D\data.ms

Raw 50

91.0 120.0 149.0 212.0 279.0

m/z-->

Abundance Scan 2124 (21.247 min): BN014190.D\data.ms (-2105) (-)

Sub 50

240.0

120.0 167.0 212.0 279.0

m/z-->

Abundance

21.247

15000

10000

5000

0

Time-->

21.20 21.40

Abundance Scan 1903 (19.488 min): BN014190.D\data.ms (-1863) (-)

Pyrene

Concen: 0.40 ng

RT: 19.488 min Scan# 1903

Delta R.T. 0.000 min

Lab File: BN014190.D

Acq: 02 Apr 2021 14:00

Tgt Ion:202 Resp: 29125

Ion Ratio Lower Upper

202 100

200 20.4 16.3 24.5

203 17.4 13.9 20.9

Abundance Scan 1903 (19.488 min): BN014190.D\data.ms

Ref 50

202.0

101.0 122.0 244.0

m/z-->

Abundance Scan 1903 (19.488 min): BN014190.D\data.ms

Raw 50

101.0 122.0 244.0

m/z-->

Abundance Scan 1903 (19.488 min): BN014190.D\data.ms (-1863) (-)

Sub 50

202.0

101.0 122.0

m/z-->

Abundance

19.488

20000

15000

10000

5000

0


Time-->

19.40 19.60




Abundance Scan 1945 (19.697 min): BN014190.D\data.ms (-1934) (-)

Terphenyl-d14
Concen: 0.41 ng
RT: 19.697 min Scan# 1945
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

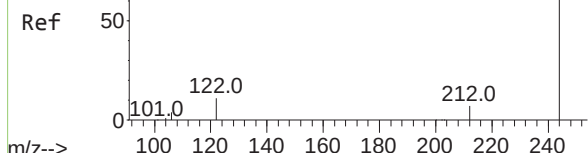





Tgt Ion:	244	Resp:	21379
Ion	Ratio	Lower	Upper
244	100		
212	7.6	6.1	9.1
122	11.2	9.0	13.4

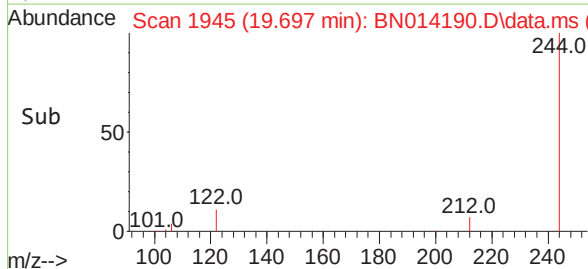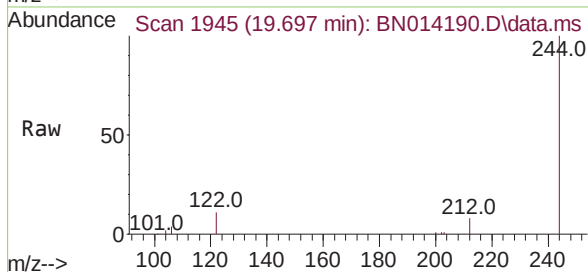


Abundance Scan 2123 (21.237 min): BN014190.D\data.ms (-2139) (-)

Benzo(a)anthracene
Concen: 0.46 ng
RT: 21.237 min Scan# 2123
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Tgt Ion:	228	Resp:	28854
Ion	Ratio	Lower	Upper
228	100		
226	25.7	20.6	30.8
229	20.2	16.2	24.2

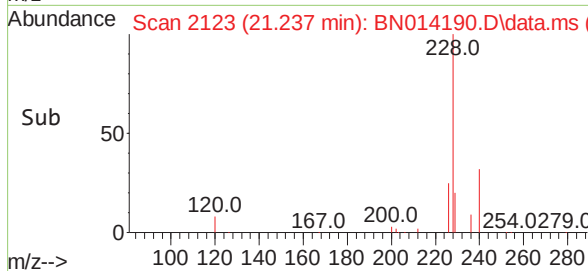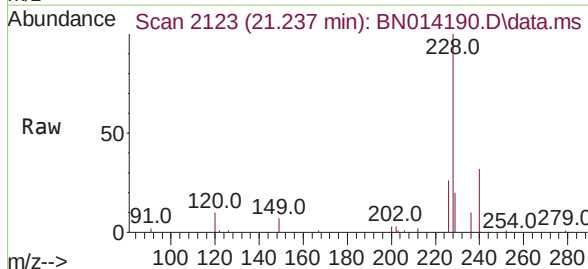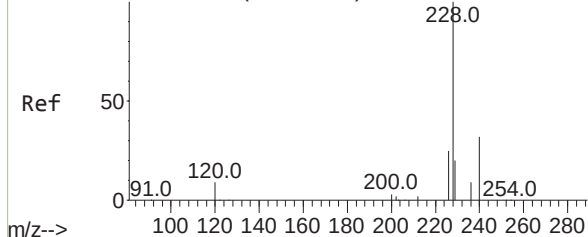



Abundance Scan 2127 (21.279 min): BN014190.D\data.ms (-2118) (-)

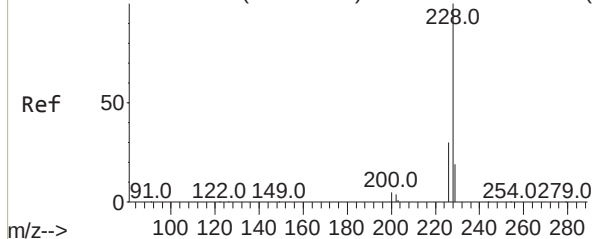


Chrysene
Concen: 0.44 ng
RT: 21.279 min Scan# 2127
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	228	Resp:	30246
Ion	Ratio	Lower	Upper
228	100		
226	30.4	24.3	36.5
229	19.2	15.4	23.0

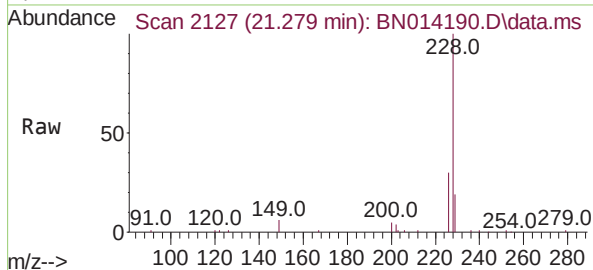

Abundance Scan 2127 (21.279 min): BN014190.D\data.ms (-2118) (-)


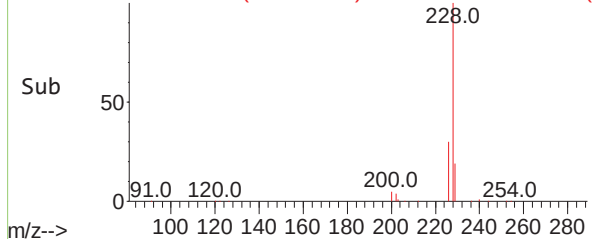


Abundance Scan 2117 (21.173 min): BN014190.D\data.ms (-2118) (-)

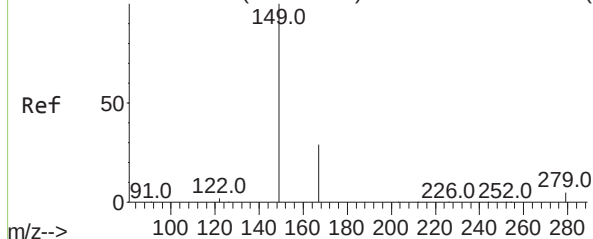


Bis(2-ethylhexyl)phthalate
Concen: 0.62 ng
RT: 21.173 min Scan# 2117
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00


Tgt Ion:	149	Resp:	11750
Ion	Ratio	Lower	Upper
149	100		
167	25.7	20.6	30.8
279	4.3	3.4	5.2

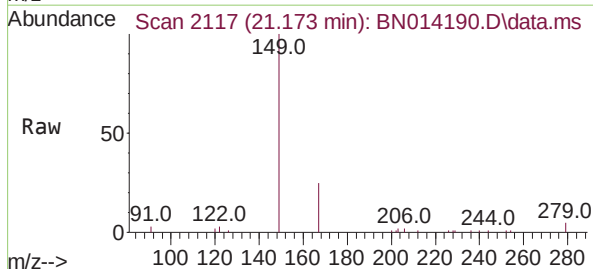

Abundance Scan 2117 (21.173 min): BN014190.D\data.ms (-2108) (-)

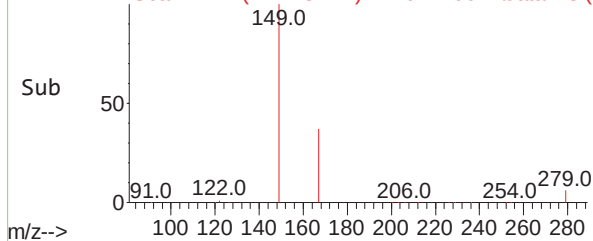


Abundance Scan 3192 (25.687 min): BN014190.D\data.ms (-3135) (-)

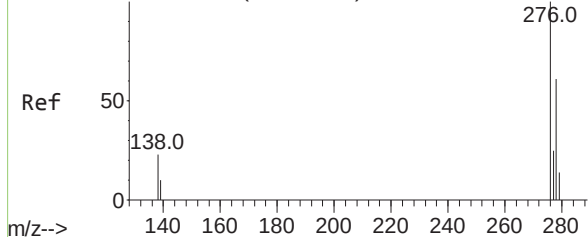


Indeno(1,2,3-cd)pyrene
Concen: 0.50 ng
RT: 25.687 min Scan# 3192
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00


Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

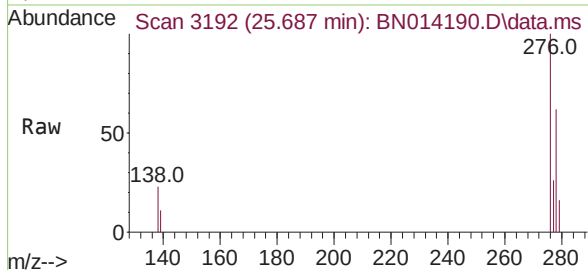


Tgt Ion:	276	Resp:	35534
Ion	Ratio	Lower	Upper
276	100		
138	23.7	19.0	28.4
277	24.8	19.9	29.9




Abundance Scan 3192 (25.687 min): BN014190.D\data.ms (-3163) (-)




Abundance Scan 2543 (23.466 min): BN014190.D\data.ms (-2525) (-)

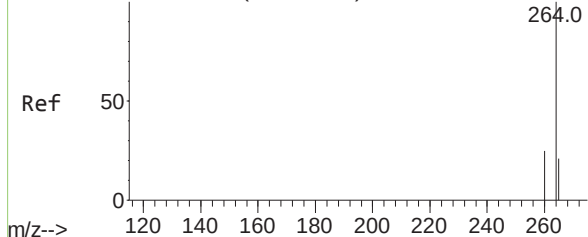


Perylene-d12
Concen: 0.40 ng
RT: 23.466 min Scan# 2543
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

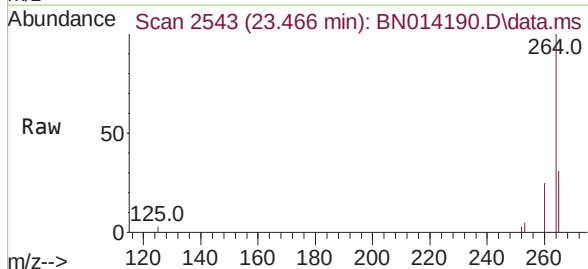


Tgt Ion:	264	Resp:	21759
Ion	Ratio	Lower	Upper
264	100		
260	25.1	20.1	30.1
265	31.2	25.0	37.4



Abundance Scan 2543 (23.466 min): BN014190.D\data.ms (-2499) (-)





Abundance Scan 2348 (22.798 min): BN014190.D\data.ms (-2348) (-)




Benzo(b)fluoranthene
Concen: 0.42 ng
RT: 22.798 min Scan# 2348
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Tgt Ion:	252	Resp:	32477
Ion Ratio	Lower	Upper	
252	100		
253	23.5	18.8	28.2
125	11.1	8.9	13.3


Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

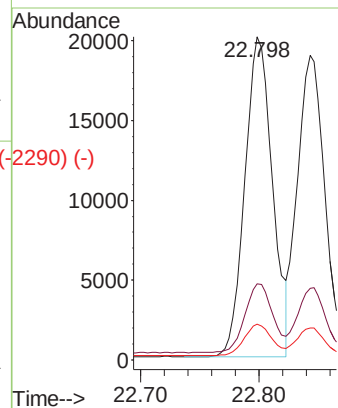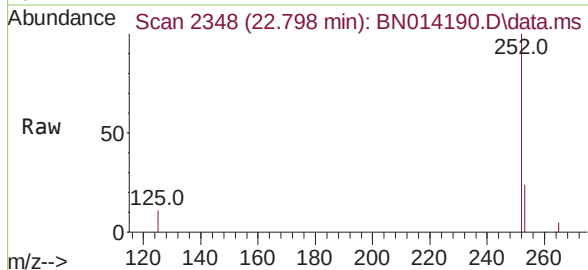

Abundance Scan 2348 (22.798 min): BN014190.D\data.ms (-2290) (-)


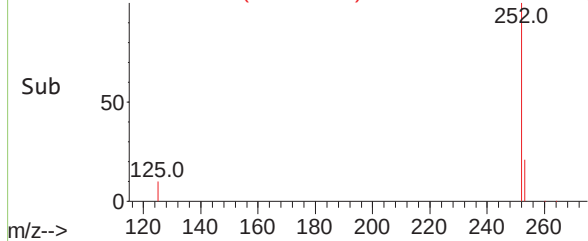


Abundance Scan 2361 (22.843 min): BN014190.D\data.ms (-2361) (-)




Benzo(k)fluoranthene
Concen: 0.41 ng
RT: 22.843 min Scan# 2361
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00


Tgt Ion:	252	Resp:	30899
Ion Ratio	Lower	Upper	
252	100		
253	23.6	18.9	28.3
125	10.6	8.5	12.7

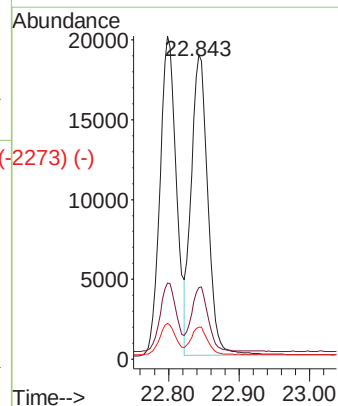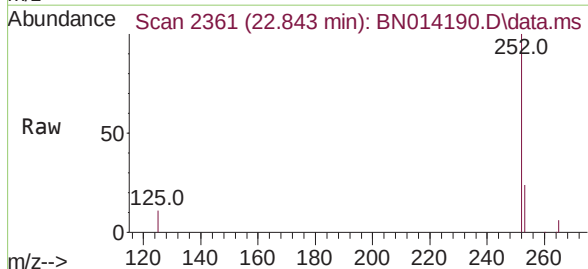

Abundance Scan 2361 (22.843 min): BN014190.D\data.ms (-2273) (-)





Abundance Scan 2514 (23.367 min): BN014190.D\data.ms (-252.0) (-)




Benzo(a)pyrene
Concen: 0.43 ng
RT: 23.367 min Scan# 2514
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	252	Resp:	28316
Ion Ratio	Lower	Upper	
252	100		
253	24.5	19.6	29.4
125	12.4	9.9	14.9

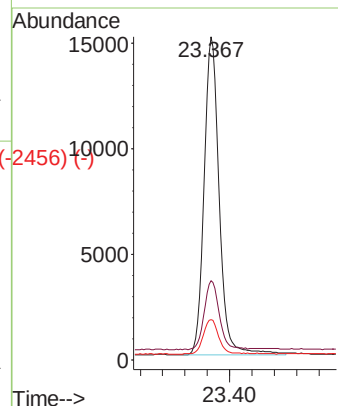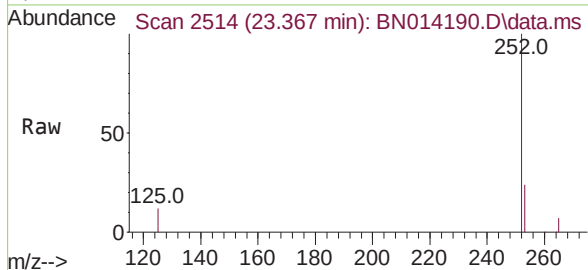

Abundance Scan 2514 (23.367 min): BN014190.D\data.ms (-252.0) (-)


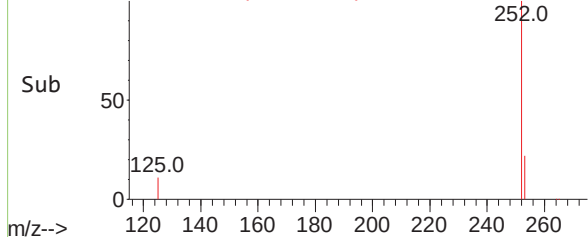


Abundance Scan 3196 (25.701 min): BN014190.D\data.ms (-278.0) (-)




Dibenzo(a,h)anthracene
Concen: 0.44 ng
RT: 25.701 min Scan# 3196
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00


Tgt Ion:	278	Resp:	29927
Ion Ratio	Lower	Upper	
278	100		
139	16.4	13.1	19.7
279	24.9	19.9	29.9

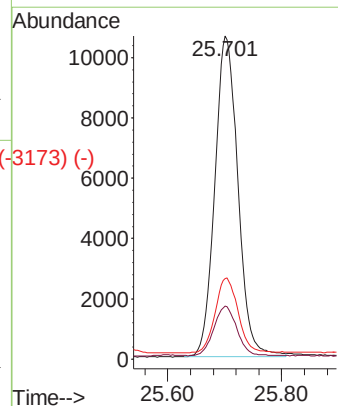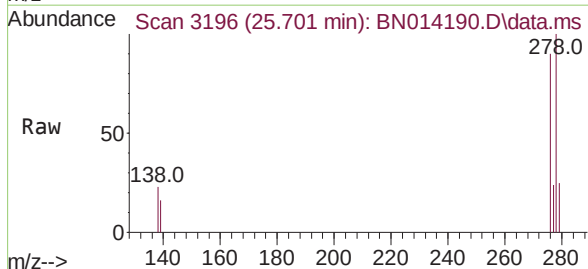

Abundance Scan 3196 (25.701 min): BN014190.D\data.ms (-278.0) (-)




Abundance Scan 3392 (26.372 min): BN014190.D\data.ms (-3334) (-)

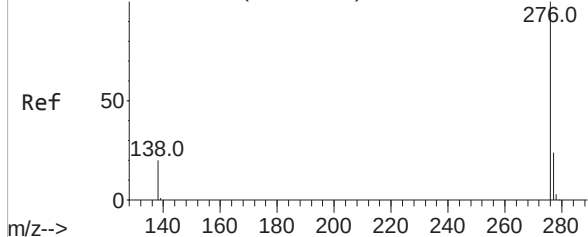


Benzo(g,h,i)perylene
Concen: 0.44 ng
RT: 26.372 min Scan# 3392
Delta R.T. 0.000 min
Lab File: BN014190.D
Acq: 02 Apr 2021 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Abundance Scan 3392 (26.372 min): BN014190.D\data.ms

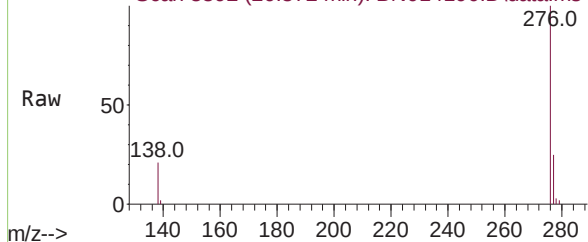

Tgt Ion:	276	Resp:	31466
Ion	Ratio	Lower	Upper
276	100		
277	24.9	19.9	29.9
138	20.5	16.4	24.6

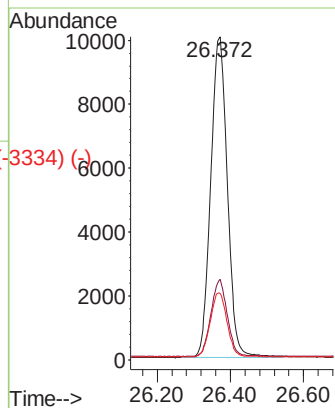

Abundance Scan 3392 (26.372 min): BN014190.D\data.ms (-3334) (-)

