

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
 Data File : BN014193.D
 Acq On : 02 Apr 2021 15:48
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Apr 02 16:18:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 02 15:44:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.684	152	5385	0.40	ng	0.00
7) Naphthalene-d8	10.454	136	18185	0.40	ng	0.00
13) Acenaphthene-d10	14.308	164	10652	0.40	ng	-0.01
19) Phenanthrene-d10	17.055	188	22020	0.40	ng	0.00
29) Chrysene-d12	21.247	240	23781	0.40	ng	0.00
36) Perylene-d12	23.463	264	21620	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.284	112	62396	4.52	ng	0.00
5) Phenol-d6	6.855	99	82937	4.73	ng	0.00
8) Nitrobenzene-d5	8.819	82	69160	5.59	ng	-0.01
11) 2-Methylnaphthalene-d10	12.053	152	193354	7.00	ng	0.00
14) 2,4,6-Tribromophenol	15.805	330	22599	6.60	ng	0.00
15) 2-Fluorobiphenyl	12.938	172	188962	4.73	ng	0.00
27) Fluoranthene-d10	19.096	212	438458	7.61	ng	0.00
31) Terphenyl-d14	19.697	244	261503	4.77	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.223	88	28640	4.13	ng	98
3) n-Nitrosodimethylamine	3.537	42	27969	5.24	ng	# 92
6) bis(2-Chloroethyl)ether	7.112	93	66627	4.77	ng	100
9) Naphthalene	10.505	128	232084	5.17	ng	99
10) Hexachlorobutadiene	10.796	225	42360	5.15	ng	# 100
12) 2-Methylnaphthalene	12.124	142	158449	5.39	ng	99
16) Acenaphthylene	14.029	152	236520	5.80	ng	100
17) Acenaphthene	14.372	154	153716	5.21	ng	98
18) Fluorene	15.361	166	193355	5.43	ng	99
20) 4,6-Dinitro-2-methylph...	15.450	198	21214	7.74	ng	# 46
21) 4-Bromophenyl-phenylether	16.252	248	62968	5.56	ng	# 66
22) Hexachlorobenzene	16.373	284	66386	5.25	ng	99
23) Atrazine	16.532	200	48228	6.23	ng	97
24) Pentachlorophenol	16.714	266	21457	5.45	ng	96
25) Phenanthrene	17.104	178	312904	5.29	ng	100
26) Anthracene	17.189	178	288931	5.81	ng	100
28) Fluoranthene	19.126	202	370162	5.99	ng	100
30) Pyrene	19.488	202	375744	4.84	ng	100
32) Benzo(a)anthracene	21.237	228	386965	5.87	ng	99
33) Chrysene	21.279	228	386613	5.31	ng	100
34) Bis(2-ethylhexyl)phtha...	21.162	149	170268	8.47	ng	97
35) Indeno(1,2,3-cd)pyrene	25.687	276	440301	5.82	ng	100
37) Benzo(b)fluoranthene	22.798	252	395419	5.19	ng	96
38) Benzo(k)fluoranthene	22.843	252	391461	5.25	ng	97
39) Benzo(a)pyrene	23.367	252	355597	5.43	ng	95
40) Dibenzo(a,h)anthracene	25.701	278	370595	5.51	ng	97
41) Benzo(g,h,i)perylene	26.372	276	380549	5.32	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
Data File : BN014193.D
Acq On : 02 Apr 2021 15:48
Operator : CG/JU
Sample : SSTDIC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Apr 02 16:18:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 02 15:44:53 2021
Response via : Initial Calibration









1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.684 min Scan# 609
 Delta R.T. 0.000 min
 Lab File: BN014193.D
 Acq: 02 Apr 2021 15:48




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:	152	Resp:	5385
Ion	Ratio	Lower	Upper
152	100		
150	155.4	126.2	189.4
115	59.8	49.8	74.6



1,4-Dioxane
 Concen: 4.13 ng
 RT: 3.223 min Scan# 55
 Delta R.T. -0.008 min
 Lab File: BN014193.D
 Acq: 02 Apr 2021 15:48

Tgt Ion:	88	Resp:	28640
Ion	Ratio	Lower	Upper
88	100		
58	79.9	63.2	94.8
43	33.0	25.1	37.7









n-Nitrosodimethylamine
 Concen: 5.24 ng
 RT: 3.537 min Scan# 94
 Delta R.T. -0.032 min
 Lab File: BN014193.D
 Acq: 02 Apr 2021 15:48




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:	42	Resp:	27969
Ion	Ratio	Lower	Upper
42	100		
74	114.4	98.8	148.2
44	5.9	0.0	0.0#



2-Fluorophenol
 Concen: 4.52 ng
 RT: 5.284 min Scan# 311
 Delta R.T. 0.000 min
 Lab File: BN014193.D
 Acq: 02 Apr 2021 15:48

Tgt Ion:	112	Resp:	62396
Ion	Ratio	Lower	Upper
112	100		
64	60.0	48.3	72.5
63	31.7	25.8	38.6









Phenol-d6
 Concen: 4.73 ng
 RT: 6.855 min Scan# 506
 Delta R.T. 0.000 min
 Lab File: BN014193.D
 Acq: 02 Apr 2021 15:48




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:	99	Resp:	82937
Ion	Ratio	Lower	Upper
99	100		
42	21.9	17.8	26.6
71	33.5	26.6	40.0




bis(2-Chloroethyl)ether
 Concen: 4.77 ng
 RT: 7.112 min Scan# 538
 Delta R.T. 0.000 min
 Lab File: BN014193.D
 Acq: 02 Apr 2021 15:48

Tgt Ion:	93	Resp:	66627
Ion	Ratio	Lower	Upper
93	100		
63	80.5	64.2	96.4
95	32.9	26.6	40.0





Abundance Scan 856 (10.454 min): BN014190.D\data.ms (-856#7-)

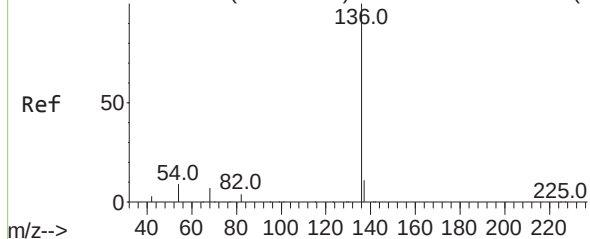


Naphthalene-d8
Concen: 0.40 ng
RT: 10.454 min Scan# 856
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	18185
Ion	Ratio	Lower	Upper
136	100		
137	11.4	9.1	13.7
54	9.6	8.2	12.4
68	7.2	6.1	9.1



Abundance Scan 856 (10.454 min): BN014193.D\data.ms (-840) (-)





Abundance Scan 728 (8.832 min): BN014190.D\data.ms (-724#8)




Nitrobenzene-d5
Concen: 5.59 ng
RT: 8.819 min Scan# 727
Delta R.T. -0.013 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48


Tgt Ion:	82	Resp:	69160
Ion	Ratio	Lower	Upper
82	100		
128	31.5	36.8	55.2#
54	60.9	38.7	58.1#



Abundance Scan 727 (8.819 min): BN014193.D\data.ms (-712) (-)





Abundance Scan 860 (10.505 min): BN014190.D\data.ms (-853) (-)




Naphthalene
Concen: 5.17 ng
RT: 10.505 min Scan# 860
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	128	Resp:	232084
Ion	Ratio	Lower	Upper
128	100		
129	10.9	9.1	13.7
127	13.0	10.6	15.8



Abundance Scan 860 (10.505 min): BN014193.D\data.ms (-852) (-)





Abundance Scan 883 (10.796 min): BN014190.D\data.ms (-877) (-)





Hexachlorobutadiene
Concen: 5.15 ng
RT: 10.796 min Scan# 883
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:	225	Resp:	42360
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.9	50.8	76.2



Abundance Scan 883 (10.796 min): BN014193.D\data.ms (-875) (-)









Scan 1062 (12.053 min): BN014190.D\data.ms (-1019) (-)
 2-Methylnaphthalene-d10
 Concen: 7.00 ng
 RT: 12.053 min Scan# 1062
 Delta R.T. 0.000 min
 Lab File: BN014193.D
 Acq: 02 Apr 2021 15:48




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:152 Resp: 193354
 Ion Ratio Lower Upper
 152 100
 151 20.0 16.1 24.1



Scan 1078 (12.124 min): BN014190.D\data.ms (-1049) (-)
 2-Methylnaphthalene
 Concen: 5.39 ng
 RT: 12.124 min Scan# 1078
 Delta R.T. 0.000 min
 Lab File: BN014193.D
 Acq: 02 Apr 2021 15:48


Tgt Ion:142 Resp: 158449
 Ion Ratio Lower Upper
 142 100
 141 88.7 71.6 107.4
 115 35.2 29.2 43.8






Abundance Scan 1307 (14.321 min): BN014190.D\data.ms (-1291) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.308 min Scan# 1306
Delta R.T. -0.013 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

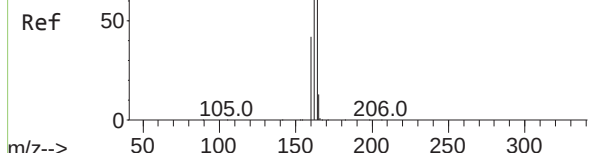


Tgt Ion:	164	Resp:	10652
Ion	Ratio	Lower	Upper
164	100		
162	104.5	77.4	116.2
160	49.1	34.2	51.4






Abundance Scan 1424 (15.805 min): BN014190.D\data.ms (-1291) (-)


2,4,6-Tribromophenol
Concen: 6.60 ng
RT: 15.805 min Scan# 1424
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48



Tgt Ion:	330	Resp:	22599
Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	37.5	29.8	44.6





Abundance Scan 1198 (12.938 min): BN014190.D\data.ms (-1190) (-)

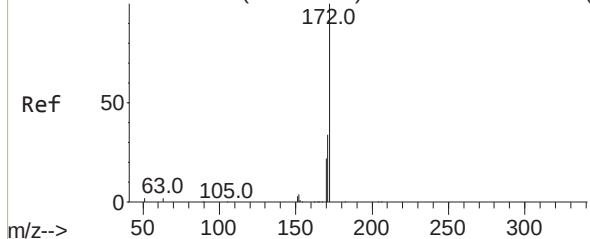


2-Fluorobiphenyl
Concen: 4.73 ng
RT: 12.938 min Scan# 1198
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	172	Resp:	188962
Ion	Ratio	Lower	Upper
172	100		
171	33.6	27.3	40.9
170	22.0	18.1	27.1



Abundance Scan 1198 (12.938 min): BN014193.D\data.ms (-1190) (-)





Abundance Scan 1284 (14.029 min): BN014190.D\data.ms (-1215) (-)




Acenaphthylene
Concen: 5.80 ng
RT: 14.029 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:	152	Resp:	236520
Ion	Ratio	Lower	Upper
152	100		
151	19.2	15.1	22.7
153	13.0	10.5	15.7




Abundance Scan 1284 (14.029 min): BN014193.D\data.ms (-1268) (-)






Abundance Scan 1311 (14.372 min): BN014190.D\data.ms (-1303) (-)

Acenaphthene
Concen: 5.21 ng
RT: 14.372 min Scan# 1311
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0







Tgt Ion	Ratio	Lower	Upper
154	100		
153	109.5	89.2	133.8
152	52.7	43.8	65.6




Abundance Scan 1389 (15.361 min): BN014190.D\data.ms (-1303) (-)

Fluorene
Concen: 5.43 ng
RT: 15.361 min Scan# 1389
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion	Ratio	Lower	Upper
166	100		
165	97.3	78.5	117.7
167	13.4	10.9	16.3







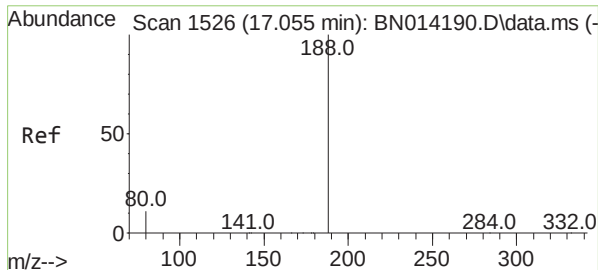

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.055 min Scan# 1526
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	188	Resp:	22020
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	11.8	9.5	14.3




4,6-Dinitro-2-methylphenol
Concen: 7.74 ng
RT: 15.450 min Scan# 1396
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:	198	Resp:	21214
Ion	Ratio	Lower	Upper
198	100		
51	18.2	59.4	89.0#
105	18.8	29.8	44.6#






Abundance Scan 1461 (16.264 min): BN014190.D\data.ms (-1424) (-)




4-Bromophenyl-phenylether
Concen: 5.56 ng
RT: 16.252 min Scan# 1460
Delta R.T. -0.012 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:248 Resp: 62968
Ion Ratio Lower Upper
248 100
250 88.7 85.6 128.4
141 82.6 26.1 39.1#






Abundance Scan 1470 (16.373 min): BN014190.D\data.ms (-1426) (-)



Hexachlorobenzene
Concen: 5.25 ng
RT: 16.373 min Scan# 1470
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48


Tgt Ion:284 Resp: 66386
Ion Ratio Lower Upper
284 100
142 35.2 28.6 42.8
249 31.1 25.3 37.9






Abundance Scan 1483 (16.532 min): BN014190.D\data.ms (-1425) (-)

Atrazine
Concen: 6.23 ng
RT: 16.532 min Scan# 1483
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion:	200	Resp:	48228
Ion	Ratio	Lower	Upper
200	100		
173	19.7	17.6	26.4
215	50.2	41.4	62.0






Abundance Scan 1498 (16.714 min): BN014190.D\data.ms (-1421) (-)

Pentachlorophenol
Concen: 5.45 ng
RT: 16.714 min Scan# 1498
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Tgt Ion:	266	Resp:	21457
Ion	Ratio	Lower	Upper
266	100		
264	62.9	51.8	77.8
268	63.6	47.7	71.5





Abundance Scan 1530 (17.104 min): BN014190.D\data.ms (-1525) (-)

Phenanthrene
Concen: 5.29 ng
RT: 17.104 min Scan# 1530
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Tgt Ion:178 Resp: 312904
Ion Ratio Lower Upper
178 100
176 18.8 15.2 22.8
179 15.4 12.3 18.5






Abundance Scan 1530 (17.104 min): BN014193.D\data.ms (-1505) (-)




Abundance Scan 1537 (17.189 min): BN014190.D\data.ms (-1526) (-)

Anthracene
Concen: 5.81 ng
RT: 17.189 min Scan# 1537
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48


Tgt Ion:178 Resp: 288931
Ion Ratio Lower Upper
178 100
176 18.2 14.6 22.0
179 15.4 12.4 18.6



Abundance Scan 1537 (17.189 min): BN014193.D\data.ms (-1529) (-)






Abundance Scan 1824 (19.096 min): BN014190.D\data.ms (-1824) (-)

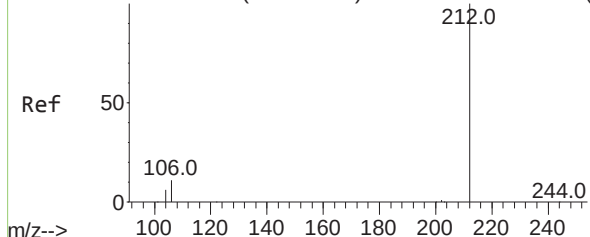


Fluoranthene-d10
Concen: 7.61 ng
RT: 19.096 min Scan# 1824
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:212 Resp: 438458
Ion Ratio Lower Upper
212 100
106 12.5 9.9 14.9
104 6.9 5.6 8.4






Abundance Scan 1830 (19.126 min): BN014190.D\data.ms (-1828) (-)

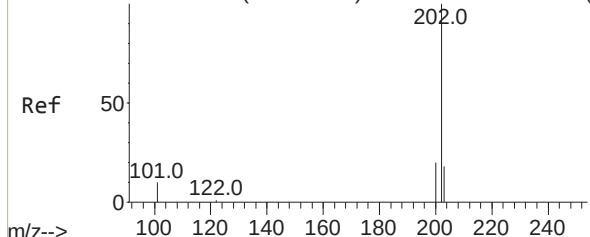


Fluoranthene
Concen: 5.99 ng
RT: 19.126 min Scan# 1830
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:202 Resp: 370162
Ion Ratio Lower Upper
202 100
101 10.8 8.5 12.7
203 17.4 13.9 20.9





Abundance Scan 2124 (21.247 min): BN014190.D\data.ms (-2124) (-)




Chrysene-d12
Concen: 0.40 ng
RT: 21.247 min Scan# 2124
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	240	Resp:	23781
Ion	Ratio	Lower	Upper
240	100		
120	9.3	7.3	10.9
236	26.3	20.8	31.2



Abundance Scan 2124 (21.247 min): BN014193.D\data.ms (-2105) (-)





Abundance Scan 1903 (19.488 min): BN014190.D\data.ms (-1930) (-)




Pyrene
Concen: 4.84 ng
RT: 19.488 min Scan# 1903
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:	202	Resp:	375744
Ion	Ratio	Lower	Upper
202	100		
200	20.4	16.3	24.5
203	17.5	13.9	20.9




Abundance Scan 1903 (19.488 min): BN014193.D\data.ms (-1863) (-)






Abundance Scan 1945 (19.697 min): BN014190.D\data.ms (-1934) (-)

Terphenyl-d14
Concen: 4.77 ng
RT: 19.697 min Scan# 1945
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0







Tgt Ion:	244	Resp:	261503
Ion	Ratio	Lower	Upper
244	100		
212	7.2	6.1	9.1
122	10.3	9.0	13.4




Abundance Scan 2123 (21.237 min): BN014190.D\data.ms (-2139) (-)

Benzo(a)anthracene
Concen: 5.87 ng
RT: 21.237 min Scan# 2123
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:	228	Resp:	386965
Ion	Ratio	Lower	Upper
228	100		
226	25.2	20.6	30.8
229	20.2	16.2	24.2

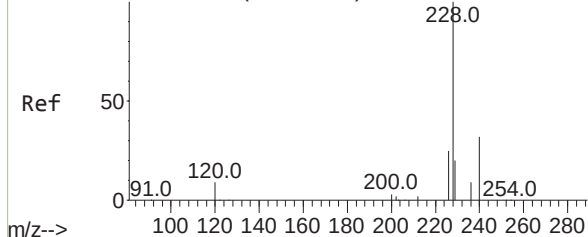


Abundance Scan 2127 (21.279 min): BN014190.D\data.ms (-2118) (-)


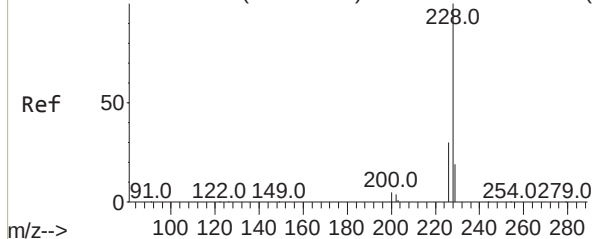


Chrysene
Concen: 5.31 ng
RT: 21.279 min Scan# 2127
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Tgt Ion:	228	Resp:	386613
Ion	Ratio	Lower	Upper
228	100		
226	30.1	24.3	36.5
229	19.1	15.4	23.0






Abundance Scan 2117 (21.173 min): BN014190.D\data.ms (-2114) (-)




Bis(2-ethylhexyl)phthalate
Concen: 8.47 ng
RT: 21.162 min Scan# 2116
Delta R.T. -0.011 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:	149	Resp:	170268
Ion	Ratio	Lower	Upper
149	100		
167	27.3	20.6	30.8
279	4.0	3.4	5.2




Abundance Scan 3192 (25.687 min): BN014190.D\data.ms (-3135) (-)





Indeno(1,2,3-cd)pyrene
Concen: 5.82 ng
RT: 25.687 min Scan# 3192
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion:	276	Resp:	440301
Ion	Ratio	Lower	Upper
276	100		
138	23.8	19.0	28.4
277	24.8	19.9	29.9





Abundance Scan 2543 (23.466 min): BN014190.D\data.ms (-2525) (-)




Perylene-d12
Concen: 0.40 ng
RT: 23.463 min Scan# 2542
Delta R.T. -0.003 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48



Tgt Ion:	264	Resp:	21620
Ion	Ratio	Lower	Upper
264	100		
260	24.5	20.1	30.1
265	30.0	25.0	37.4






Abundance Scan 2348 (22.798 min): BN014190.D\data.ms (-2348) (-)




Benzo(b)fluoranthene
Concen: 5.19 ng
RT: 22.798 min Scan# 2348
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:252 Resp: 395419
Ion Ratio Lower Upper
252 100
253 21.8 18.8 28.2
125 9.4 8.9 13.3






Abundance Scan 2361 (22.843 min): BN014190.D\data.ms (-2361) (-)



Benzo(k)fluoranthene
Concen: 5.25 ng
RT: 22.843 min Scan# 2361
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48


Tgt Ion:252 Resp: 391461
Ion Ratio Lower Upper
252 100
253 21.9 18.9 28.3
125 9.3 8.5 12.7





Abundance Scan 2514 (23.367 min): BN014190.D\data.ms (-2509) (-)

Benzo(a)pyrene
Concen: 5.43 ng
RT: 23.367 min Scan# 2514
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Tgt Ion:	252	Resp:	355597
Ion	Ratio	Lower	Upper
252	100		
253	21.7	19.6	29.4
125	10.5	9.9	14.9





Abundance Scan 2514 (23.367 min): BN014193.D\data.ms (-2456) (-)




Abundance Scan 3196 (25.701 min): BN014190.D\data.ms (-3149) (-)

Dibenzo(a,h)anthracene
Concen: 5.51 ng
RT: 25.701 min Scan# 3196
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48


Tgt Ion:	278	Resp:	370595
Ion	Ratio	Lower	Upper
278	100		
139	15.6	13.1	19.7
279	23.2	19.9	29.9



Abundance Scan 3196 (25.701 min): BN014193.D\data.ms (-3173) (-)




Abundance Scan 3392 (26.372 min): BN014190.D\data.ms (-3341) (-)

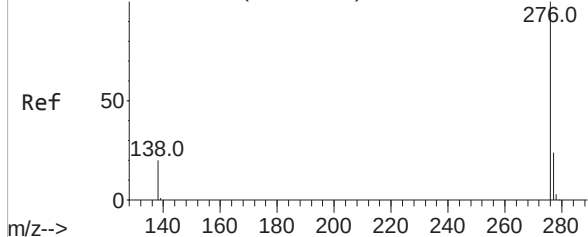


Benzo(g,h,i)perylene
Concen: 5.32 ng
RT: 26.372 min Scan# 3392
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Abundance Scan 3392 (26.372 min): BN014193.D\data.ms



Tgt Ion:	276	Resp:	380549
Ion	Ratio	Lower	Upper
276	100		
277	23.7	19.9	29.9
138	20.2	16.4	24.6



Abundance Scan 3392 (26.372 min): BN014193.D\data.ms (-3334) (-)

