
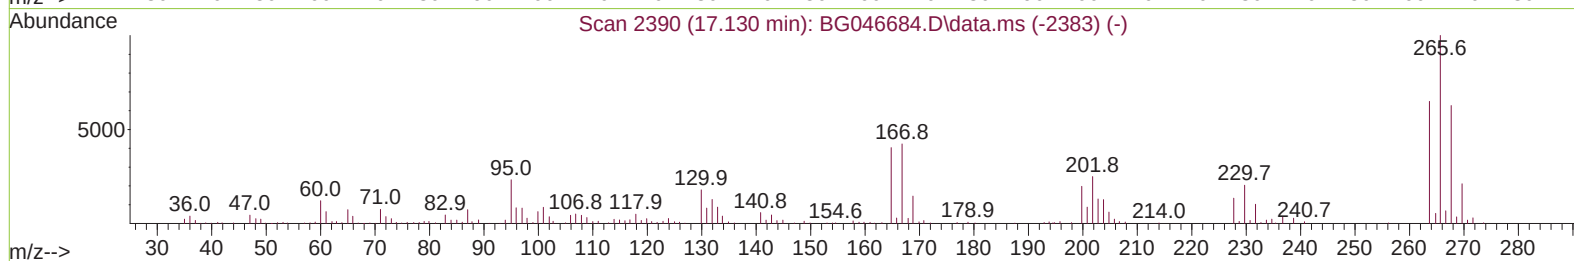
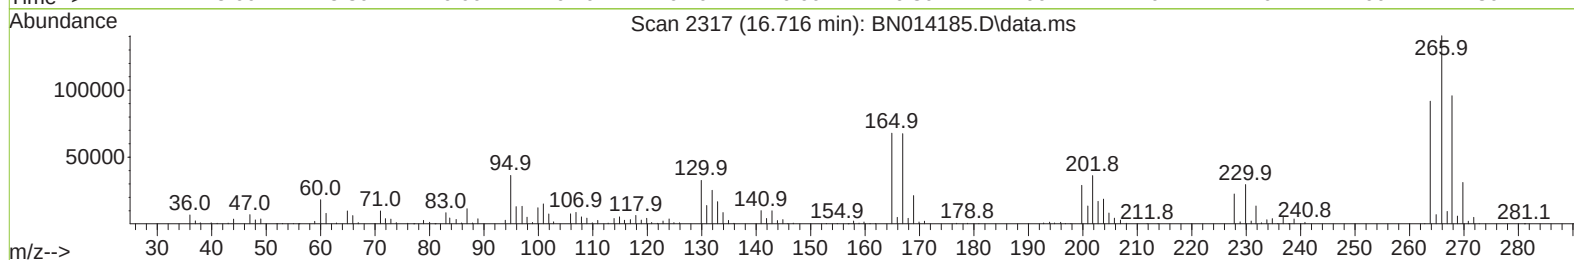


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
Data File : BN014185.D
Acq On : 02 Apr 2021 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 02:22:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

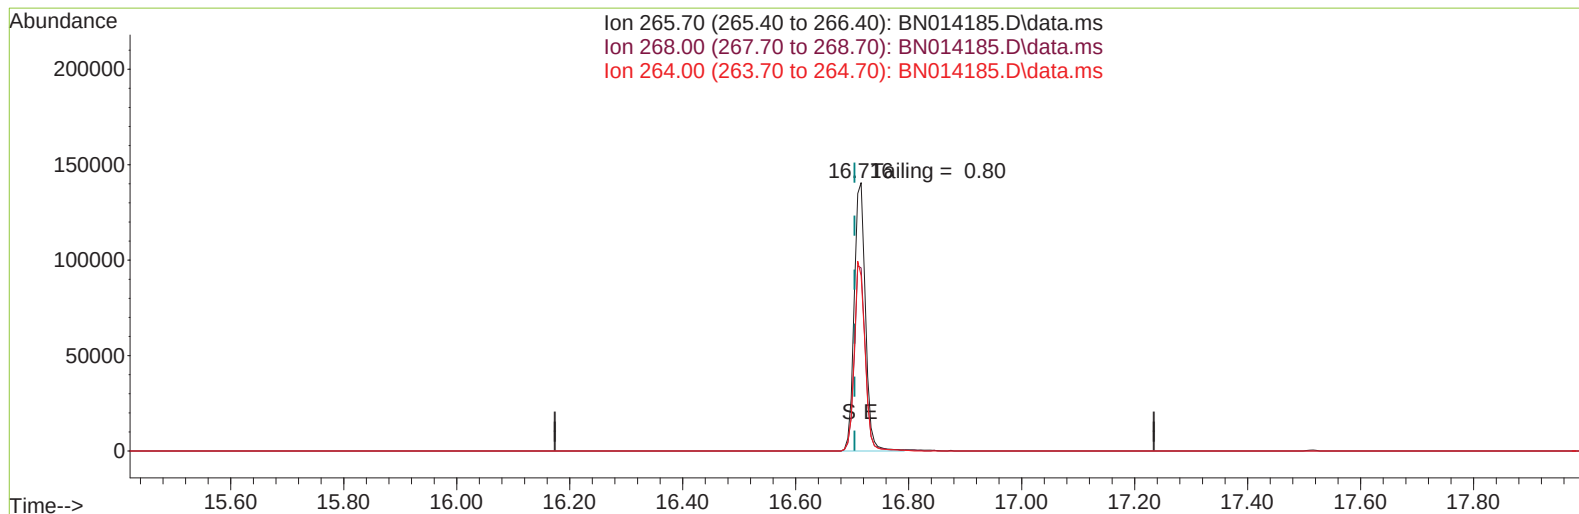

TIC: BN014185.D\data.ms

(70) Pentachlorophenol (C)




16.716min (+ 0.012) 23067.48 ng

response 195329

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.19
264.00	61.60	65.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
Data File : BN014185.D
Acq On : 02 Apr 2021 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 02:22:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

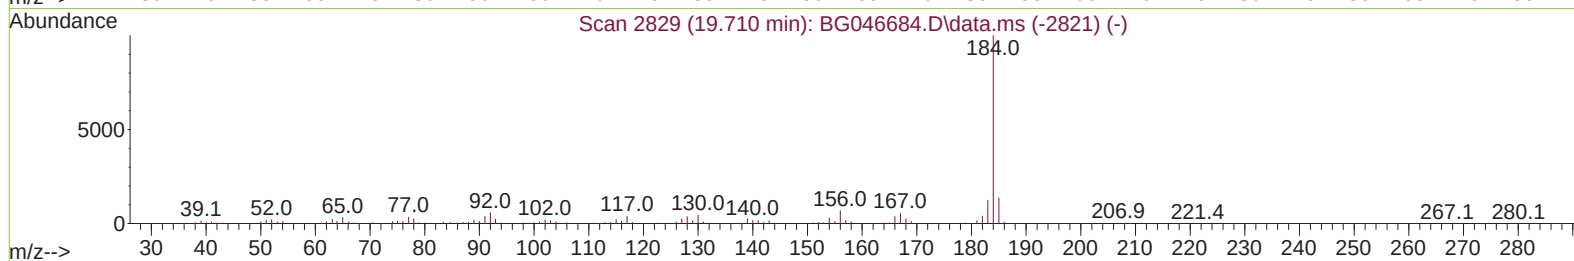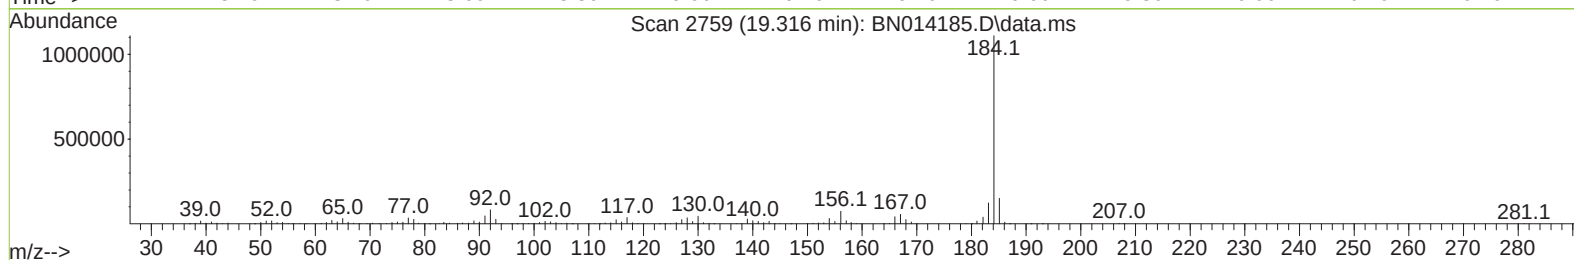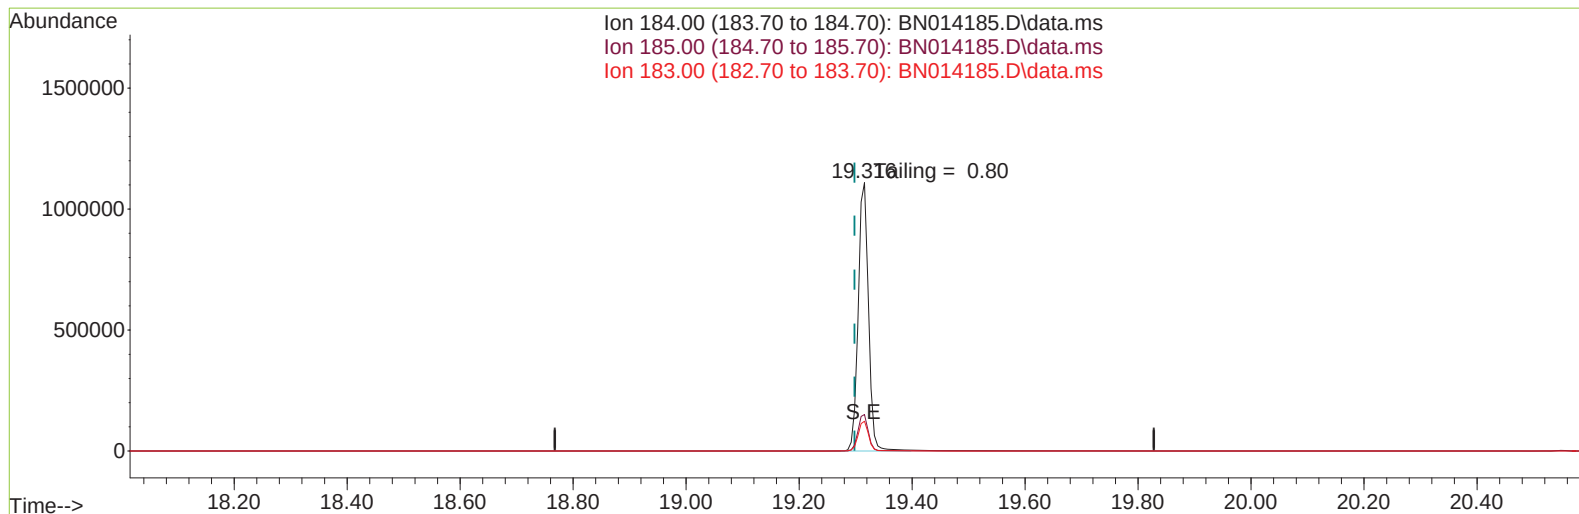

TIC: BN014185.D\data.ms

(77) Benzidine

19.316min (+ 0.018) 0.00 ng

response 1420920

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	11.11
0.00	0.00	0.00