

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
 Data File : BN014187.D
 Acq On : 02 Apr 2021 12:13
 Operator : CG/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Manual Integrations
 APPROVED

mohammad
 4/5/2021 11:56:01 AM

Quant Time: Apr 02 14:35:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 02 14:32:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.684	152	4163	0.40	ng	0.00
7) Naphthalene-d8	10.454	136	15212	0.40	ng	0.00
13) Acenaphthene-d10	14.308	164	8606	0.40	ng	-0.01
19) Phenanthrene-d10	17.055	188	18035	0.40	ng	0.00
29) Chrysene-d12	21.247	240	20348	0.40	ng	0.00
36) Perylene-d12	23.466	264	21273	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.284	112	2501	0.23	ng	0.00
5) Phenol-d6	6.855	99	3123	0.23	ng	0.00
8) Nitrobenzene-d5	8.832	82	2325	0.22	ng	0.00
11) 2-Methylnaphthalene-d10	12.053	152	6646	0.29	ng	0.00
14) 2,4,6-Tribromophenol	15.805	330	649	0.23	ng	0.00
15) 2-Fluorobiphenyl	12.938	172	6486	0.20	ng	0.00
27) Fluoranthene-d10	19.096	212	14738	0.31	ng	0.00
31) Terphenyl-d14	19.697	244	9037	0.19	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.231	88	1141	0.21	ng	96
3) n-Nitrosodimethylamine	3.577	42	677	0.16	ng	# 96
6) bis(2-Chloroethyl)ether	7.112	93	2374	0.22	ng	99
9) Naphthalene	10.505	128	8236	0.22	ng	98
10) Hexachlorobutadiene	10.796	225	1560	0.23	ng	# 99
12) 2-Methylnaphthalene	12.124	142	5429	0.22	ng	99
16) Acenaphthylene	14.029	152	6733	0.20	ng	99
17) Acenaphthene	14.372	154	4881	0.20	ng	98
18) Fluorene	15.361	166	6303	0.22	ng	99
20) 4,6-Dinitro-2-methylph...	15.450	198	476	0.21	ng	# 51
21) 4-Bromophenyl-phenylether	16.264	248	2017	0.22	ng	98
22) Hexachlorobenzene	16.373	284	2228	0.22	ng	99
23) Atrazine	16.532	200	1447	0.23	ng	96
24) Pentachlorophenol	16.714	266	496	0.15	ng	90
25) Phenanthrene	17.104	178	10765	0.22	ng	100
26) Anthracene	17.189	178	8857	0.22	ng	100
28) Fluoranthene	19.126	202	12694	0.25	ng	100
30) Pyrene	19.488	202	13458	0.20	ng	100
32) Benzo(a)anthracene	21.237	228	13055	0.23	ng	99
33) Chrysene	21.279	228	13507	0.22	ng	99
34) Bis(2-ethylhexyl)phtha...	21.173	149	6524	0.38	ng	99
35) Indeno(1,2,3-cd)pyrene	25.691	276	17461	0.27	ng	100
37) Benzo(b)fluoranthene	22.802	252	15440m	0.21	ng	
38) Benzo(k)fluoranthene	22.843	252	14683	0.20	ng	94
39) Benzo(a)pyrene	23.370	252	13619	0.21	ng	# 92
40) Dibenzo(a,h)anthracene	25.704	278	14740	0.22	ng	96
41) Benzo(g,h,i)perylene	26.372	276	15513	0.22	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
Data File : BN014187.D
Acq On : 02 Apr 2021 12:13
Operator : CG/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Manual Integrations
APPROVED

mohammad
4/5/2021 11:56:01 AM


Quant Time: Apr 02 14:35:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 02 14:32:17 2021
Response via : Initial Calibration





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.684 min Scan# 609
 Delta R.T. 0.000 min
 Lab File: BN014187.D
 Acq: 02 Apr 2021 12:13




Instrument :
 BNA_N
 ClientSampled :
 SSTDICC0.2




Tgt Ion:152 Resp: 4163
 Ion Ratio Lower Upper
 152 100
 150 156.9 126.2 189.4
 115 61.6 49.8 74.6

Manual Integrations
 APPROVED



mohammad
 4/5/2021 11:56:01 AM




#2
 1,4-Dioxane
 Concen: 0.21 ng
 RT: 3.231 min Scan# 56
 Delta R.T. 0.000 min
 Lab File: BN014187.D
 Acq: 02 Apr 2021 12:13



Tgt Ion: 88 Resp: 1141
 Ion Ratio Lower Upper
 88 100
 58 76.8 63.2 94.8
 43 35.4 25.1 37.7



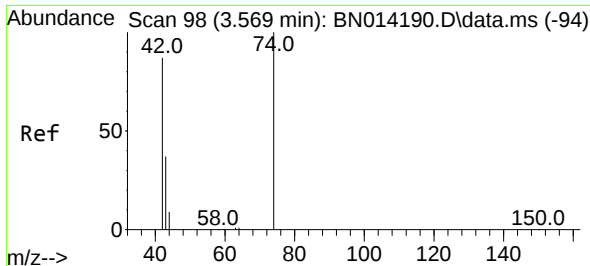





#3
n-Nitrosodimethylamine
Concen: 0.16 ng
RT: 3.577 min Scan# 99
Delta R.T. 0.008 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13

Tgt Ion: 42 Resp: 677
Ion Ratio Lower Upper
42 100
74 119.4 98.8 148.2
44 16.4 0.0 0.0#

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
4/5/2021 11:56:01 AM




#4
2-Fluorophenol
Concen: 0.23 ng
RT: 5.284 min Scan# 311
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13

Tgt Ion: 112 Resp: 2501
Ion Ratio Lower Upper
112 100
64 59.5 48.3 72.5
63 33.1 25.8 38.6






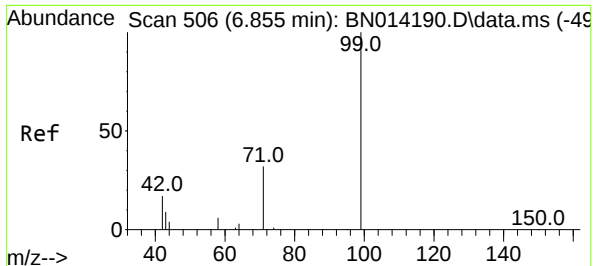


#5
Phenol-d6
Concen: 0.23 ng
RT: 6.855 min Scan# 506
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13





Tgt Ion: 99 Resp: 3123
Ion Ratio Lower Upper
99 100
42 24.2 17.8 26.6
71 33.2 26.6 40.0



#6
bis(2-Chloroethyl)ether
Concen: 0.22 ng
RT: 7.112 min Scan# 538
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Tgt Ion: 93 Resp: 2374
Ion Ratio Lower Upper
93 100
63 80.0 64.2 96.4
95 33.8 26.6 40.0



Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Manual Integrations
APPROVED

mohammad
4/5/2021 11:56:01 AM



#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.454 min Scan# 856
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Tgt Ion	Ratio	Lower	Upper
136	100		
137	11.6	9.1	13.7
54	10.7	8.2	12.4
68	7.9	6.1	9.1

Manual Integrations
APPROVED



mohammad
4/5/2021 11:56:01 AM




#8
Nitrobenzene-d5
Concen: 0.22 ng
RT: 8.832 min Scan# 728
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13



Tgt Ion	Ratio	Lower	Upper
82	100		
128	48.9	36.8	55.2
54	52.3	38.7	58.1









#9
Naphthalene
Concen: 0.22 ng
RT: 10.505 min Scan# 860
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13

Tgt Ion:	128	Resp:	8236
Ion Ratio	Lower	Upper	
128	100		
129	12.2	9.1	13.7
127	13.8	10.6	15.8

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
4/5/2021 11:56:01 AM



#10
Hexachlorobutadiene
Concen: 0.23 ng
RT: 10.796 min Scan# 883
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13

Tgt Ion:	225	Resp:	1560
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	62.7	50.8	76.2



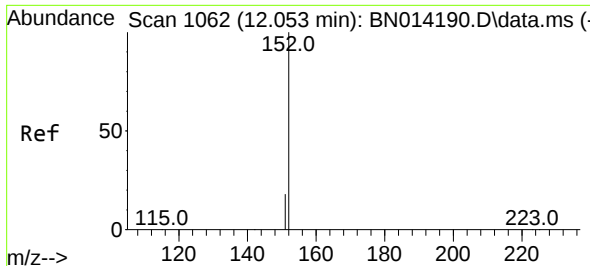





#11
2-Methylnaphthalene-d10
Concen: 0.29 ng
RT: 12.053 min Scan# 1062
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13

Tgt Ion:152 Resp: 6646
Ion Ratio Lower Upper
152 100
151 20.2 16.1 24.1

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
4/5/2021 11:56:01 AM



#12
2-Methylnaphthalene
Concen: 0.22 ng
RT: 12.124 min Scan# 1078
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13


Tgt Ion:142 Resp: 5429
Ion Ratio Lower Upper
142 100
141 90.4 71.6 107.4
115 37.5 29.2 43.8





#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.308 min Scan# 1306
Delta R.T. -0.013 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Tgt Ion:164 Resp: 8606
Ion Ratio Lower Upper
164 100
162 103.8 77.4 116.2
160 48.9 34.2 51.4

Manual Integrations
APPROVED



mohammad
4/5/2021 11:56:01 AM




#14
2,4,6-Tribromophenol
Concen: 0.23 ng
RT: 15.805 min Scan# 1424
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Tgt Ion:330 Resp: 649
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 44.8 29.8 44.6#









#15
2-Fluorobiphenyl
Concen: 0.20 ng
RT: 12.938 min Scan# 1198
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13





Tgt Ion:172 Resp: 6486
Ion Ratio Lower Upper
172 100
171 34.8 27.3 40.9
170 23.0 18.1 27.1



#16
Acenaphthylene
Concen: 0.20 ng
RT: 14.029 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Tgt Ion:152 Resp: 6733
Ion Ratio Lower Upper
152 100
151 19.8 15.1 22.7
153 13.3 10.5 15.7



Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Manual Integrations
APPROVED

mohammad
4/5/2021 11:56:01 AM



#17
Acenaphthene
Concen: 0.20 ng
RT: 14.372 min Scan# 1311
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2




Tgt Ion:154 Resp: 4881
Ion Ratio Lower Upper
154 100
153 113.0 89.2 133.8
152 56.0 43.8 65.6

Manual Integrations
APPROVED



mohammad
4/5/2021 11:56:01 AM




#18
Fluorene
Concen: 0.22 ng
RT: 15.361 min Scan# 1389
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Tgt Ion:166 Resp: 6303
Ion Ratio Lower Upper
166 100
165 96.8 78.5 117.7
167 13.9 10.9 16.3





#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.055 min Scan# 1526
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.4	9.5	14.3

Manual Integrations
APPROVED



mohammad
4/5/2021 11:56:01 AM




#20
4,6-Dinitro-2-methylphenol
Concen: 0.21 ng
RT: 15.450 min Scan# 1396
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Tgt Ion	Ratio	Lower	Upper
198	100		
51	121.6	59.4	89.0#
105	59.0	29.8	44.6#





#21
4-Bromophenyl-phenylether
Concen: 0.22 ng
RT: 16.264 min Scan# 1461
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Tgt Ion	Ratio	Lower	Upper
248	100		
250	108.7	85.6	128.4
141	35.3	26.1	39.1

Manual Integrations
APPROVED



mohammad
4/5/2021 11:56:01 AM




#22
Hexachlorobenzene
Concen: 0.22 ng
RT: 16.373 min Scan# 1470
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13



Tgt Ion	Ratio	Lower	Upper
284	100		
142	35.5	28.6	42.8
249	30.7	25.3	37.9









#23
Atrazine
Concen: 0.23 ng
RT: 16.532 min Scan# 1483
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13

Tgt Ion:	200	Resp:	1447
Ion Ratio	Lower	Upper	
200	100		
173	25.2	17.6	26.4
215	53.9	41.4	62.0

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
4/5/2021 11:56:01 AM




#24
Pentachlorophenol
Concen: 0.15 ng
RT: 16.714 min Scan# 1498
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13

Tgt Ion:	266	Resp:	496
Ion Ratio	Lower	Upper	
266	100		
264	59.3	51.8	77.8
268	69.6	47.7	71.5






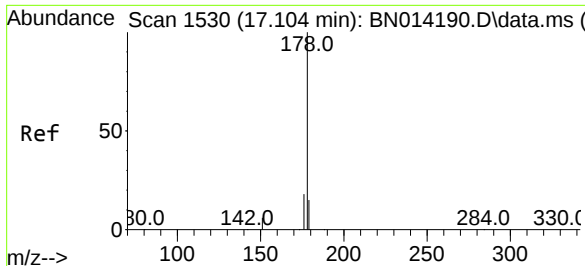


#25
Phenanthrene
Concen: 0.22 ng
RT: 17.104 min Scan# 1530
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13





Tgt Ion:178 Resp: 10765
Ion Ratio Lower Upper
178 100
176 19.0 15.2 22.8
179 15.4 12.3 18.5



#26
Anthracene
Concen: 0.22 ng
RT: 17.189 min Scan# 1537
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Tgt Ion:178 Resp: 8857
Ion Ratio Lower Upper
178 100
176 18.0 14.6 22.0
179 15.5 12.4 18.6




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED




mohammad
4/5/2021 11:56:01 AM




#27
Fluoranthene-d10
Concen: 0.31 ng
RT: 19.096 min Scan# 1824
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13





Tgt Ion:212 Resp: 14738
Ion Ratio Lower Upper
212 100
106 12.4 9.9 14.9
104 7.0 5.6 8.4



#28
Fluoranthene
Concen: 0.25 ng
RT: 19.126 min Scan# 1830
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Tgt Ion:202 Resp: 12694
Ion Ratio Lower Upper
202 100
101 10.7 8.5 12.7
203 17.3 13.9 20.9




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED



mohammad
4/5/2021 11:56:01 AM



#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.247 min Scan# 2124
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Tgt Ion:240 Resp: 20348
Ion Ratio Lower Upper
240 100
120 9.7 7.3 10.9
236 26.0 20.8 31.2




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED



mohammad
4/5/2021 11:56:01 AM




#30
Pyrene
Concen: 0.20 ng
RT: 19.488 min Scan# 1903
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Tgt Ion:202 Resp: 13458
Ion Ratio Lower Upper
202 100
200 20.2 16.3 24.5
203 17.4 13.9 20.9





#31
Terphenyl-d14
Concen: 0.19 ng
RT: 19.697 min Scan# 1945
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13



Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Tgt Ion:244 Resp: 9037
Ion Ratio Lower Upper
244 100
212 8.0 6.1 9.1
122 11.5 9.0 13.4

Manual Integrations
APPROVED



mohammad
4/5/2021 11:56:01 AM




#32
Benzo(a)anthracene
Concen: 0.23 ng
RT: 21.237 min Scan# 2123
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Tgt Ion:228 Resp: 13055
Ion Ratio Lower Upper
228 100
226 26.0 20.6 30.8
229 20.7 16.2 24.2





#33
Chrysene
Concen: 0.22 ng
RT: 21.279 min Scan# 2127
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Tgt Ion: 228 Resp: 13507
Ion Ratio Lower Upper
228 100
226 30.9 24.3 36.5
229 19.5 15.4 23.0

Manual Integrations
APPROVED



mohammad
4/5/2021 11:56:01 AM




#34
Bis(2-ethylhexyl)phthalate
Concen: 0.38 ng
RT: 21.173 min Scan# 2117
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Tgt Ion: 149 Resp: 6524
Ion Ratio Lower Upper
149 100
167 25.3 20.6 30.8
279 3.8 3.4 5.2






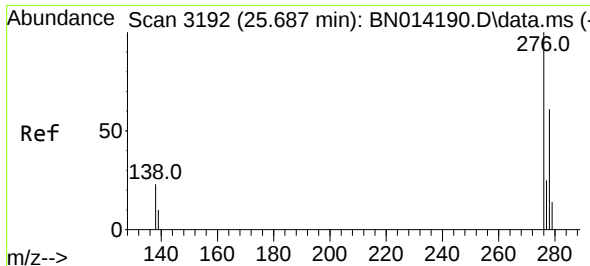


#35
Indeno(1,2,3-cd)pyrene
Concen: 0.27 ng
RT: 25.691 min Scan# 3193
Delta R.T. 0.003 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13





Tgt Ion:	276	Resp:	17461
Ion Ratio	Lower	Upper	
276	100		
138	23.5	19.0	28.4
277	24.8	19.9	29.9



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.466 min Scan# 2543
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13




Tgt Ion:	264	Resp:	21273
Ion Ratio	Lower	Upper	
264	100		
260	24.2	20.1	30.1
265	31.1	25.0	37.4



Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED

mohammad
4/5/2021 11:56:01 AM



#37

Benzo(b)fluoranthene

Concen: 0.21 ng m

RT: 22.802 min Scan# 2349

Delta R.T. 0.003 min

Lab File: BN014187.D

Acq: 02 Apr 2021 12:13

Tgt Ion:	252	Resp:	15440
Ion Ratio	Lower	Upper	
252	100		
253	26.8	18.8	28.2
125	13.4	8.9	13.3#

Instrument :





BNA_N

ClientSampleId :

SSTDIC0.2

Manual Integrations
APPROVED

mohammad
4/5/2021 11:56:01 AM



#38

Benzo(k)fluoranthene

Concen: 0.20 ng




RT: 22.843 min Scan# 2361


Delta R.T. 0.000 min

Lab File: BN014187.D

Acq: 02 Apr 2021 12:13

Tgt Ion:	252	Resp:	14683
Ion Ratio	Lower	Upper	
252	100		
253	27.0	18.9	28.3
125	12.2	8.5	12.7









#39
Benzo(a)pyrene
Concen: 0.21 ng
RT: 23.370 min Scan# 2515
Delta R.T. 0.003 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13

Tgt Ion:	252	Resp:	13619
Ion Ratio	Lower	Upper	
252	100		
253	28.4	19.6	29.4
125	15.6	9.9	14.9#

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
4/5/2021 11:56:01 AM




#40
Dibenzo(a,h)anthracene
Concen: 0.22 ng
RT: 25.704 min Scan# 3197
Delta R.T. 0.003 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13

Tgt Ion:	278	Resp:	14740
Ion Ratio	Lower	Upper	
278	100		
139	17.2	13.1	19.7
279	27.3	19.9	29.9





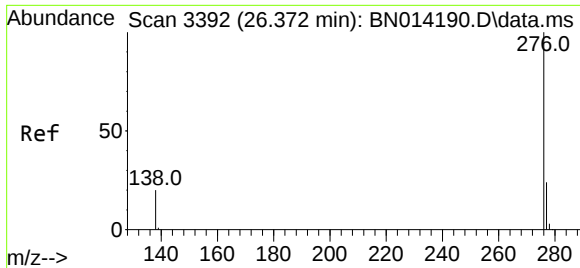

#41
Benzo(g,h,i)perylene
Concen: 0.22 ng
RT: 26.372 min Scan# 3392
Delta R.T. 0.000 min
Lab File: BN014187.D
Acq: 02 Apr 2021 12:13



Tgt Ion:	276	Resp:	15513
Ion Ratio	Lower	Upper	
276	100		
277	25.5	19.9	29.9
138	21.8	16.4	24.6



Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED

mohammad
4/5/2021 11:56:01 AM