

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
 Data File : BN014189.D
 Acq On : 02 Apr 2021 13:24
 Operator : CG/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Quant Time: Apr 02 14:34:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 02 14:32:17 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.684	152	4593	0.40	ng	0.00
7) Naphthalene-d8	10.454	136	16502	0.40	ng	0.00
13) Acenaphthene-d10	14.321	164	9399	0.40	ng	0.00
19) Phenanthrene-d10	17.055	188	19796	0.40	ng	0.00
29) Chrysene-d12	21.247	240	21319	0.40	ng	0.00
36) Perylene-d12	23.466	264	20828	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.284	112	9506	0.81	ng	0.00
5) Phenol-d6	6.855	99	11971	0.80	ng	0.00
8) Nitrobenzene-d5	8.832	82	9743	0.87	ng	0.00
11) 2-Methylnaphthalene-d10	12.053	152	28272	1.13	ng	0.00
14) 2,4,6-Tribromophenol	15.805	330	2590	0.86	ng	0.00
15) 2-Fluorobiphenyl	12.938	172	28025	0.79	ng	0.00
27) Fluoranthene-d10	19.096	212	61865	1.19	ng	0.00
31) Terphenyl-d14	19.697	244	37508	0.76	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.231	88	4393	0.74	ng	97
3) n-Nitrosodimethylamine	3.561	42	3434	0.75	ng	# 91
6) bis(2-Chloroethyl)ether	7.112	93	9887	0.83	ng	98
9) Naphthalene	10.505	128	34887	0.86	ng	100
10) Hexachlorobutadiene	10.796	225	6471	0.87	ng	# 99
12) 2-Methylnaphthalene	12.124	142	23468	0.88	ng	99
16) Acenaphthylene	14.029	152	29982	0.83	ng	100
17) Acenaphthene	14.372	154	21524	0.83	ng	100
18) Fluorene	15.361	166	27091	0.86	ng	100
20) 4,6-Dinitro-2-methylph...	15.450	198	2061	0.84	ng	# 73
21) 4-Bromophenyl-phenylether	16.264	248	8718	0.86	ng	99
22) Hexachlorobenzene	16.373	284	9613	0.85	ng	99
23) Atrazine	16.532	200	5881	0.85	ng	98
24) Pentachlorophenol	16.714	266	1859	0.53	ng	97
25) Phenanthrene	17.104	178	45055	0.85	ng	100
26) Anthracene	17.189	178	38484	0.86	ng	100
28) Fluoranthene	19.126	202	53462	0.96	ng	100
30) Pyrene	19.488	202	53419	0.77	ng	100
32) Benzo(a)anthracene	21.237	228	53997	0.91	ng	100
33) Chrysene	21.279	228	55785	0.85	ng	99
34) Bis(2-ethylhexyl)phtha...	21.173	149	21349	1.18	ng	98
35) Indeno(1,2,3-cd)pyrene	25.687	276	67649	1.00	ng	100
37) Benzo(b)fluoranthene	22.799	252	60892	0.83	ng	98
38) Benzo(k)fluoranthene	22.843	252	57313	0.80	ng	98
39) Benzo(a)pyrene	23.367	252	53228	0.84	ng	98
40) Dibenzo(a,h)anthracene	25.705	278	57271	0.88	ng	99
41) Benzo(g,h,i)perylene	26.369	276	59444	0.86	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
Data File : BN014189.D
Acq On : 02 Apr 2021 13:24
Operator : CG/JU
Sample : SSTDICC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Quant Time: Apr 02 14:34:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 02 14:32:17 2021
Response via : Initial Calibration




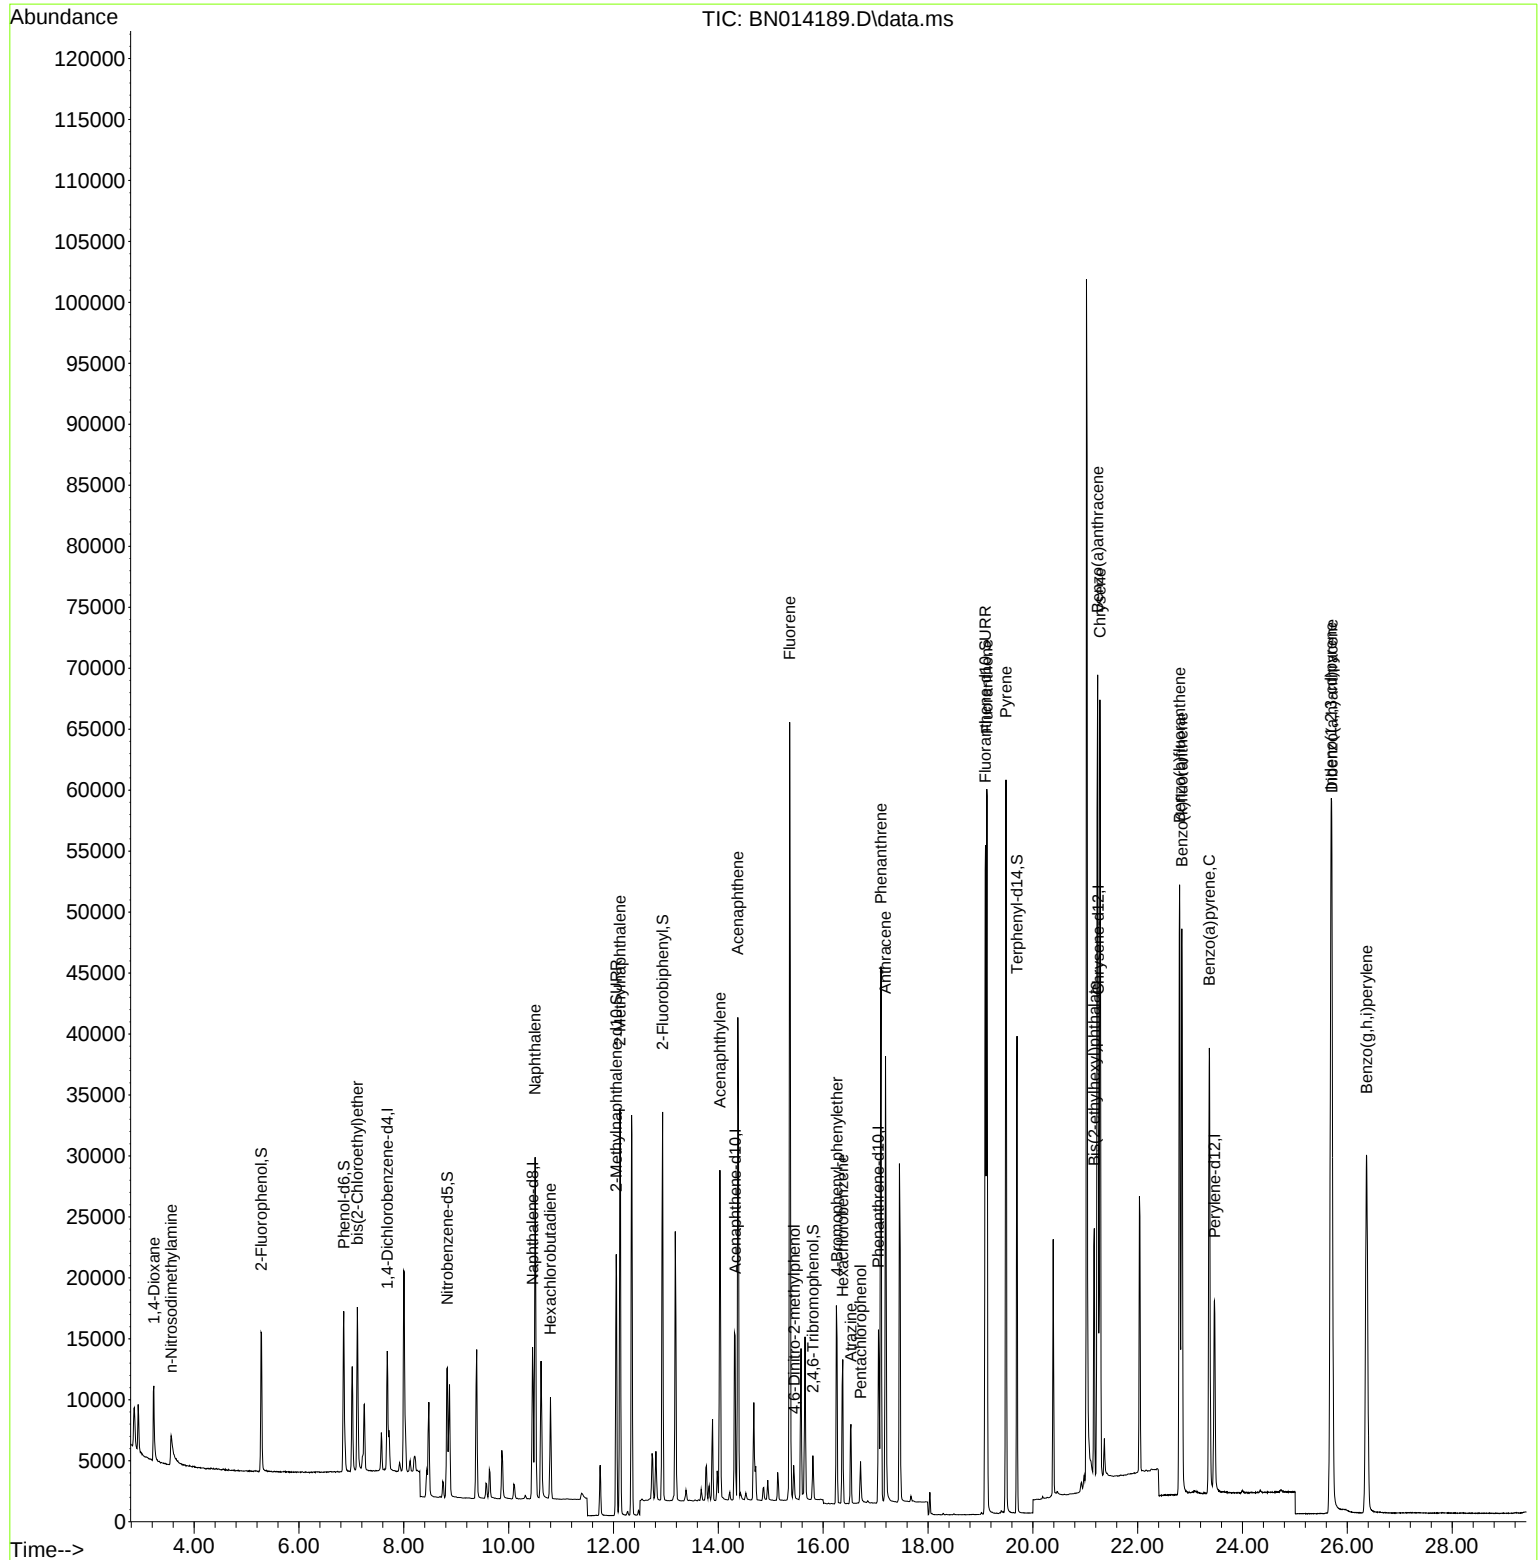




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.684 min Scan# 609
 Delta R.T. 0.000 min
 Lab File: BN014189.D
 Acq: 02 Apr 2021 13:24




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:152 Resp: 4593
 Ion Ratio Lower Upper
 152 100
 150 156.1 126.2 189.4
 115 60.1 49.8 74.6

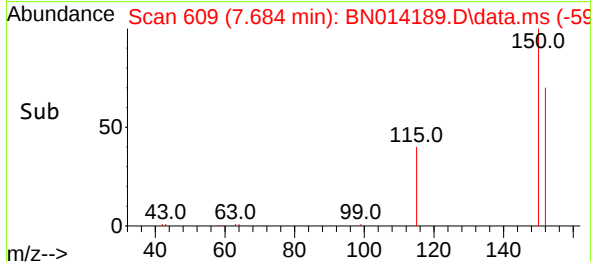

#2
 1,4-Dioxane
 Concen: 0.74 ng
 RT: 3.231 min Scan# 56
 Delta R.T. 0.000 min
 Lab File: BN014189.D
 Acq: 02 Apr 2021 13:24

Tgt Ion: 88 Resp: 4393
 Ion Ratio Lower Upper
 88 100
 58 81.2 63.2 94.8
 43 34.6 25.1 37.7




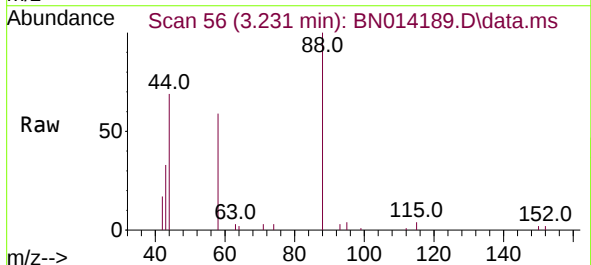


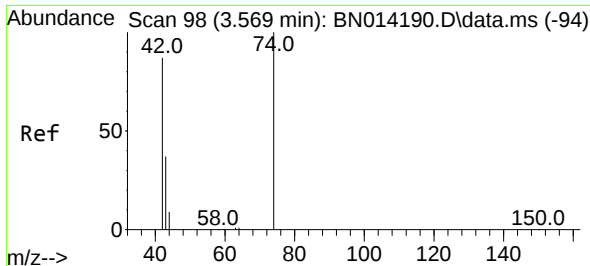

#3
n-Nitrosodimethylamine
Concen: 0.75 ng
RT: 3.561 min Scan# 97
Delta R.T. -0.008 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion: 42 Resp: 3434
Ion Ratio Lower Upper
42 100
74 113.6 98.8 148.2
44 7.1 0.0 0.0#

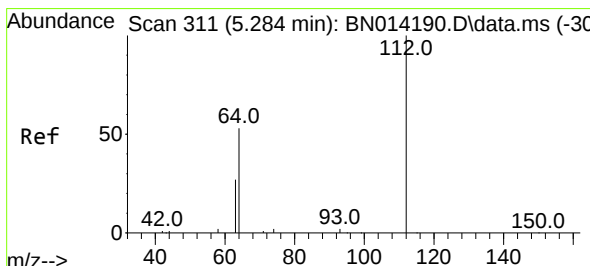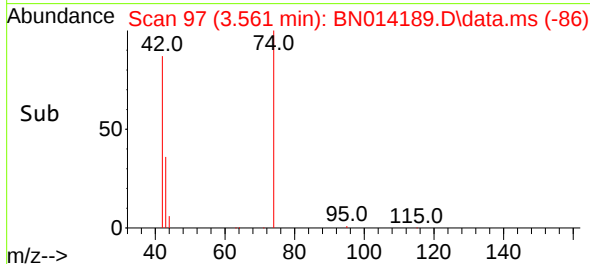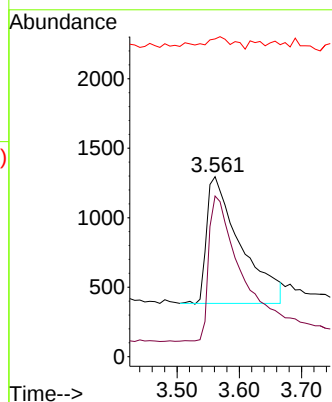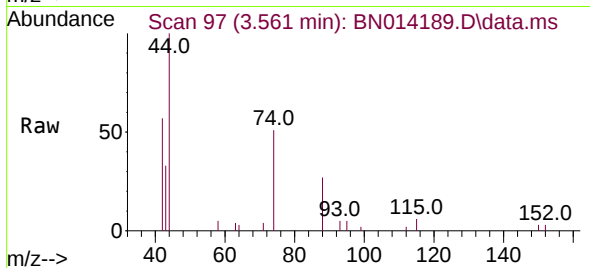

#4
2-Fluorophenol
Concen: 0.81 ng
RT: 5.284 min Scan# 311
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion: 112 Resp: 9506
Ion Ratio Lower Upper
112 100
64 60.0 48.3 72.5
63 31.3 25.8 38.6


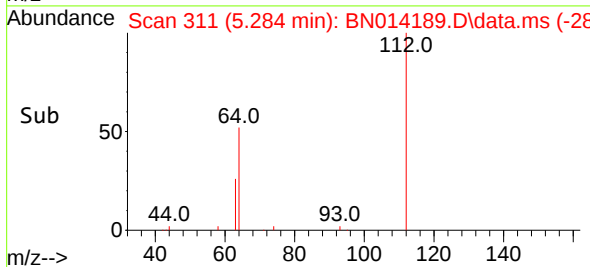

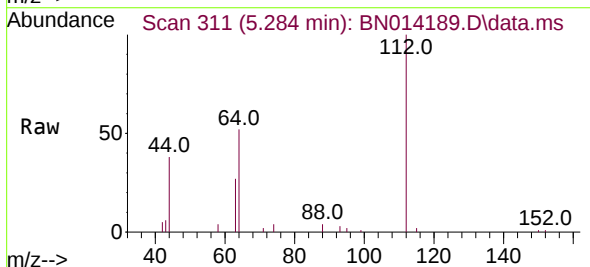


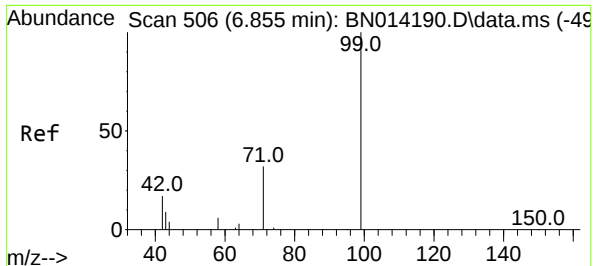

#5
Phenol-d6
Concen: 0.80 ng
RT: 6.855 min Scan# 506
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	99	Resp:	11971
Ion	Ratio	Lower	Upper
99	100		
42	21.6	17.8	26.6
71	33.3	26.6	40.0

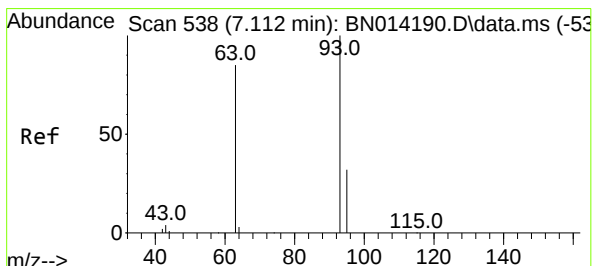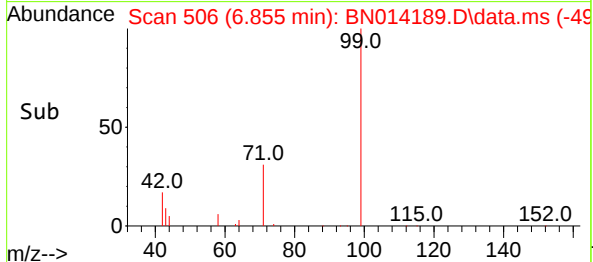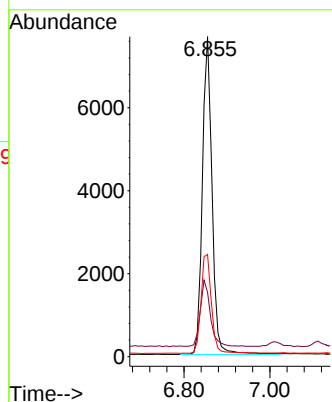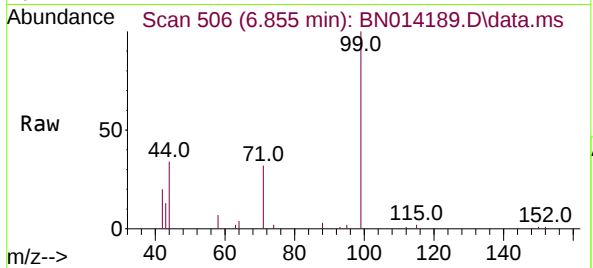

#6
bis(2-Chloroethyl)ether
Concen: 0.83 ng
RT: 7.112 min Scan# 538
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:	93	Resp:	9887
Ion	Ratio	Lower	Upper
93	100		
63	82.2	64.2	96.4
95	33.6	26.6	40.0


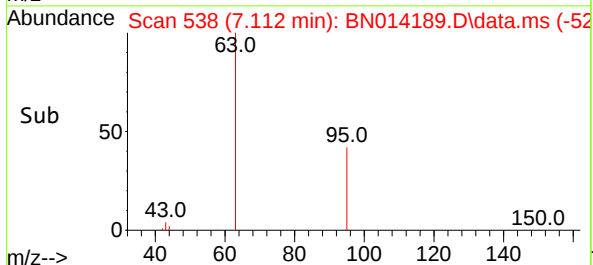

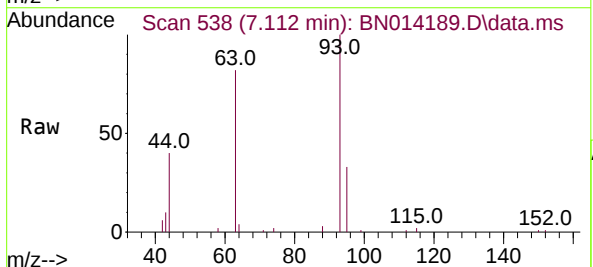




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.454 min Scan# 856
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	136	Resp:	16502
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.1	13.7
54	10.5	8.2	12.4
68	8.0	6.1	9.1

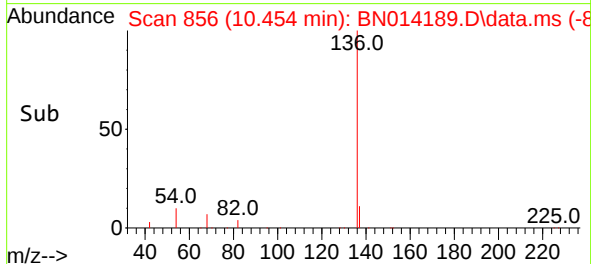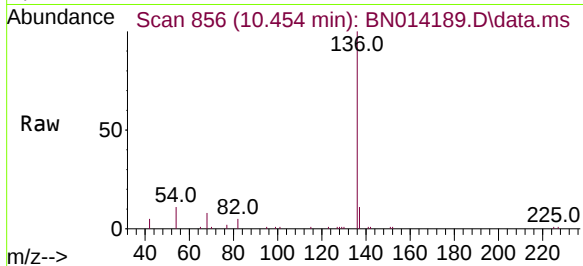

#8
Nitrobenzene-d5
Concen: 0.87 ng
RT: 8.832 min Scan# 728
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:	82	Resp:	9743
Ion	Ratio	Lower	Upper
82	100		
128	45.6	36.8	55.2
54	47.2	38.7	58.1




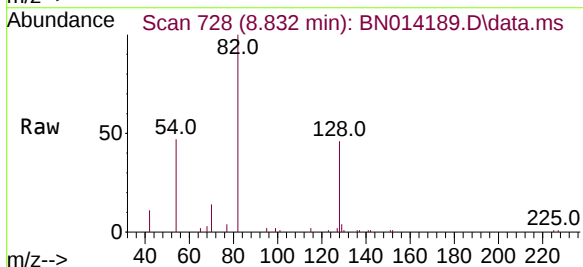




#9
Naphthalene
Concen: 0.86 ng
RT: 10.505 min Scan# 860
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:128 Resp: 34887
Ion Ratio Lower Upper
128 100
129 11.1 9.1 13.7
127 13.2 10.6 15.8

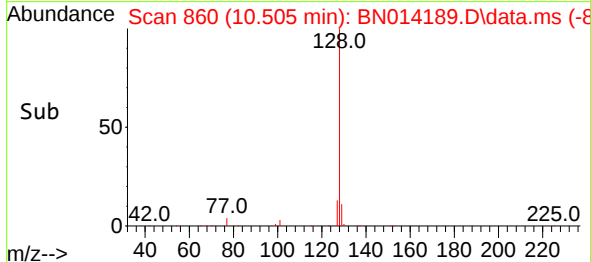

#10
Hexachlorobutadiene
Concen: 0.87 ng
RT: 10.796 min Scan# 883
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:225 Resp: 6471
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.1 50.8 76.2









#11
2-Methylnaphthalene-d10
Concen: 1.13 ng
RT: 12.053 min Scan# 1062
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:152 Resp: 28272
Ion Ratio Lower Upper
152 100
151 20.2 16.1 24.1

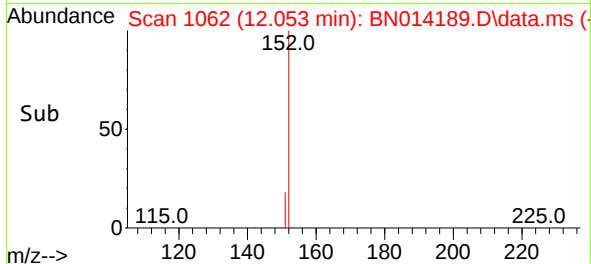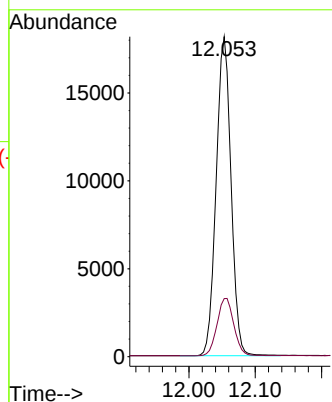

#12
2-Methylnaphthalene
Concen: 0.88 ng
RT: 12.124 min Scan# 1078
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:142 Resp: 23468
Ion Ratio Lower Upper
142 100
141 88.8 71.6 107.4
115 35.9 29.2 43.8



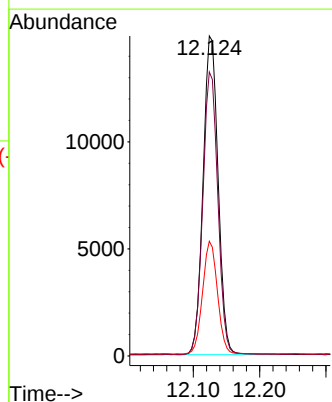





#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.321 min Scan# 1307
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:164 Resp: 9399
Ion Ratio Lower Upper
164 100
162 96.9 77.4 116.2
160 43.5 34.2 51.4

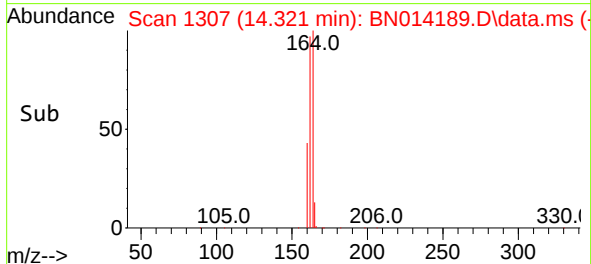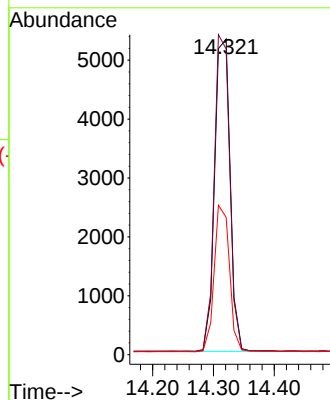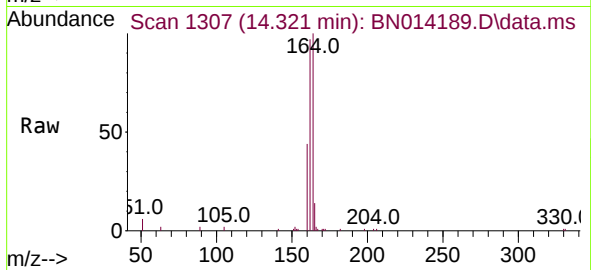

#14
2,4,6-Tribromophenol
Concen: 0.86 ng
RT: 15.805 min Scan# 1424
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:330 Resp: 2590
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 36.3 29.8 44.6


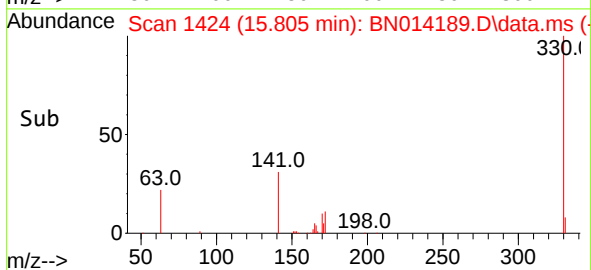
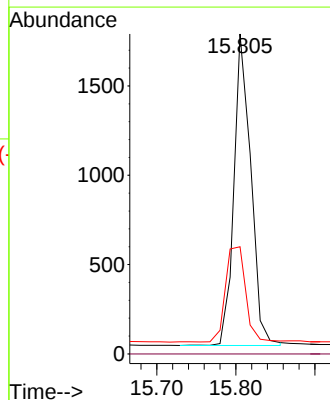





#15
2-Fluorobiphenyl
Concen: 0.79 ng
RT: 12.938 min Scan# 1198
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	172	Resp:	28025
Ion Ratio	Lower	Upper	
172	100		
171	33.7	27.3	40.9
170	22.3	18.1	27.1

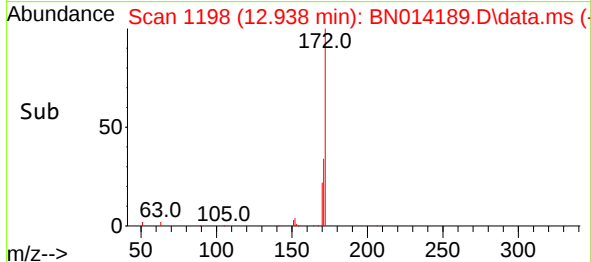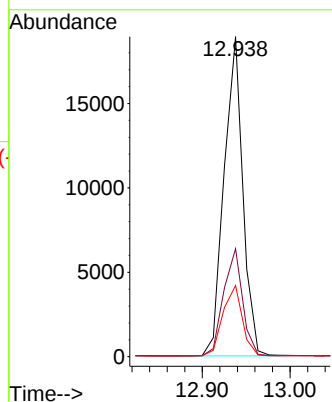

#16
Acenaphthylene
Concen: 0.83 ng
RT: 14.029 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:	152	Resp:	29982
Ion Ratio	Lower	Upper	
152	100		
151	19.3	15.1	22.7
153	13.1	10.5	15.7




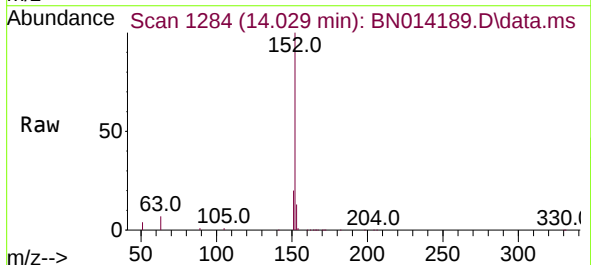




#17
Acenaphthene
Concen: 0.83 ng
RT: 14.372 min Scan# 1311
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:154 Resp: 21524
Ion Ratio Lower Upper
154 100
153 111.4 89.2 133.8
152 54.2 43.8 65.6

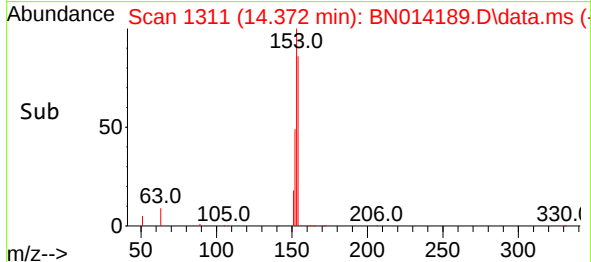

#18
Fluorene
Concen: 0.86 ng
RT: 15.361 min Scan# 1389
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:166 Resp: 27091
Ion Ratio Lower Upper
166 100
165 97.8 78.5 117.7
167 13.4 10.9 16.3




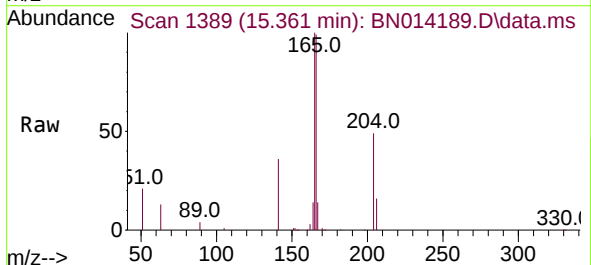


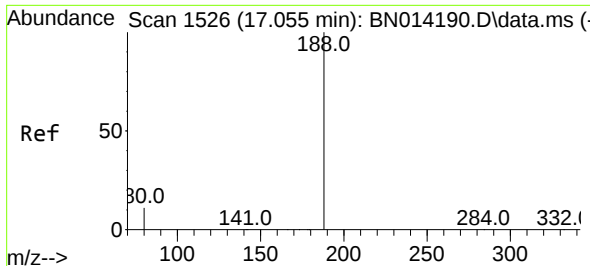

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.055 min Scan# 1526
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:188 Resp: 19796
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.1 9.5 14.3

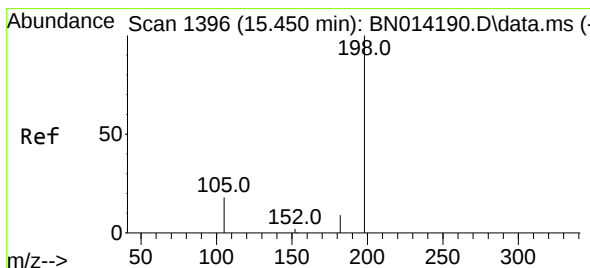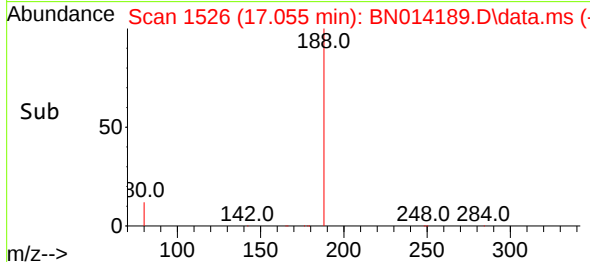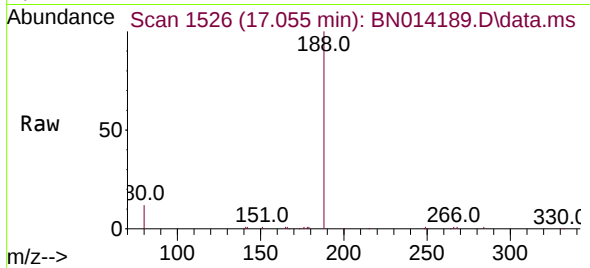

#20
4,6-Dinitro-2-methylphenol
Concen: 0.84 ng
RT: 15.450 min Scan# 1396
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:198 Resp: 2061
Ion Ratio Lower Upper
198 100
51 45.2 59.4 89.0#
105 30.4 29.8 44.6


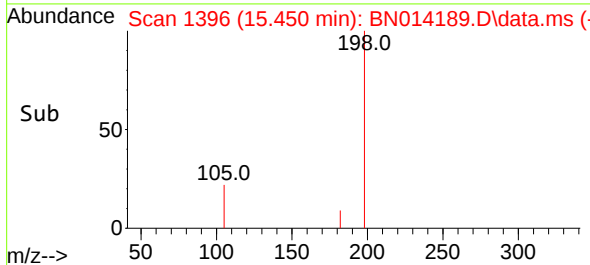

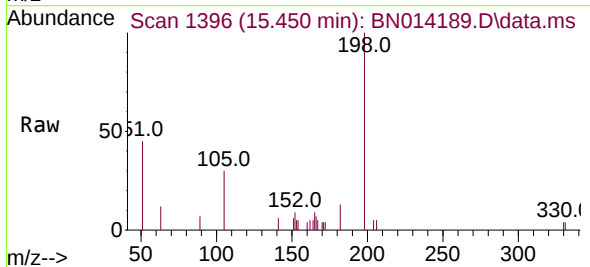


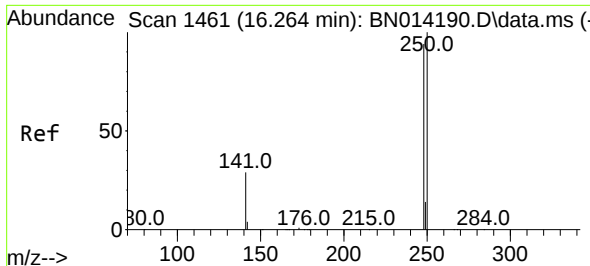

#21
4-Bromophenyl-phenylether
Concen: 0.86 ng
RT: 16.264 min Scan# 1461
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:248 Resp: 8718
Ion Ratio Lower Upper
248 100
250 107.2 85.6 128.4
141 30.4 26.1 39.1

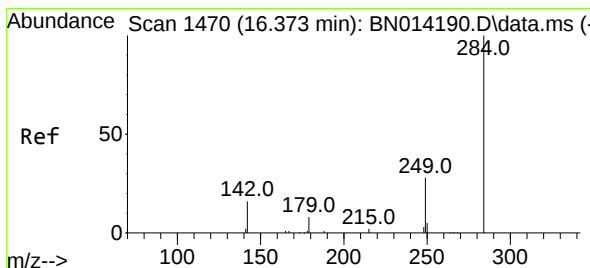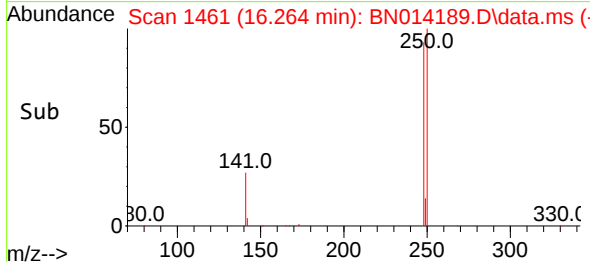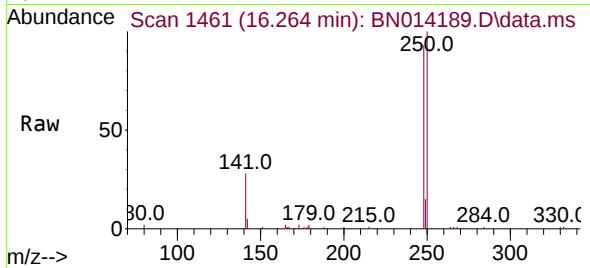

#22
Hexachlorobenzene
Concen: 0.85 ng
RT: 16.373 min Scan# 1470
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:284 Resp: 9613
Ion Ratio Lower Upper
284 100
142 35.3 28.6 42.8
249 31.2 25.3 37.9


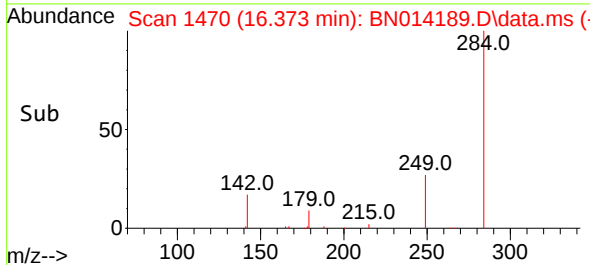

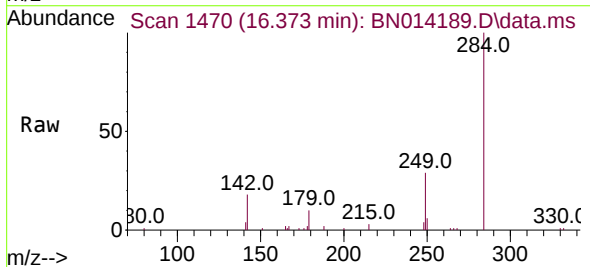




#23
Atrazine
Concen: 0.85 ng
RT: 16.532 min Scan# 1483
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:200 Resp: 5881
Ion Ratio Lower Upper
200 100
173 20.6 17.6 26.4
215 51.0 41.4 62.0

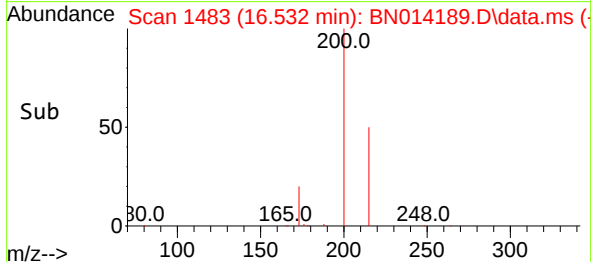

#24
Pentachlorophenol
Concen: 0.53 ng
RT: 16.714 min Scan# 1498
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:266 Resp: 1859
Ion Ratio Lower Upper
266 100
264 62.2 51.8 77.8
268 60.9 47.7 71.5




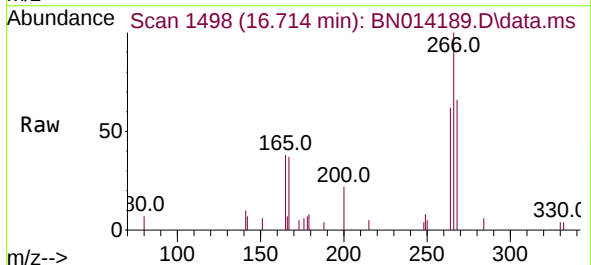


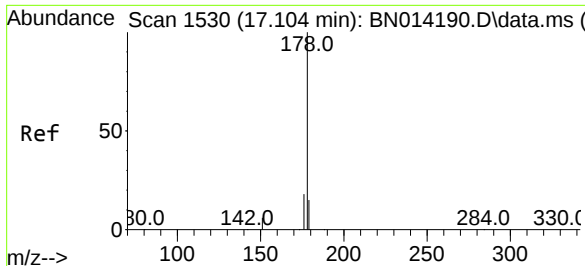

#25
Phenanthrene
Concen: 0.85 ng
RT: 17.104 min Scan# 1530
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:178 Resp: 45055
Ion Ratio Lower Upper
178 100
176 18.7 15.2 22.8
179 15.3 12.3 18.5

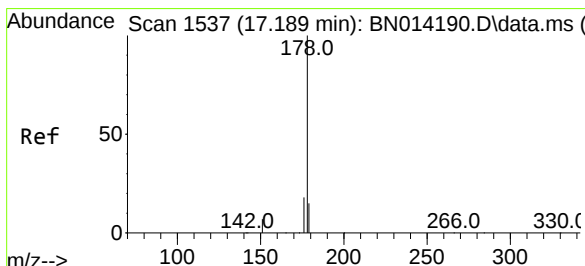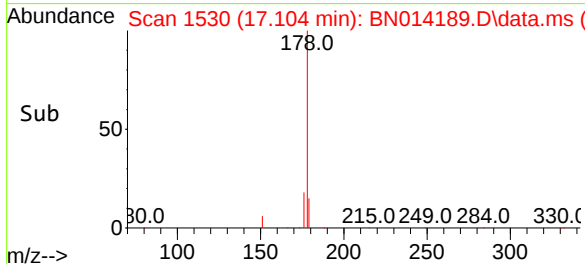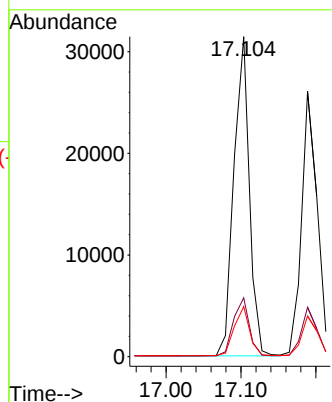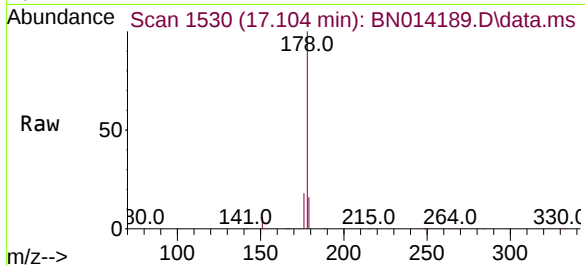

#26
Anthracene
Concen: 0.86 ng
RT: 17.189 min Scan# 1537
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:178 Resp: 38484
Ion Ratio Lower Upper
178 100
176 18.1 14.6 22.0
179 15.3 12.4 18.6


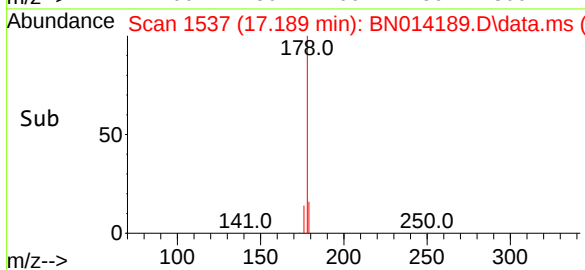

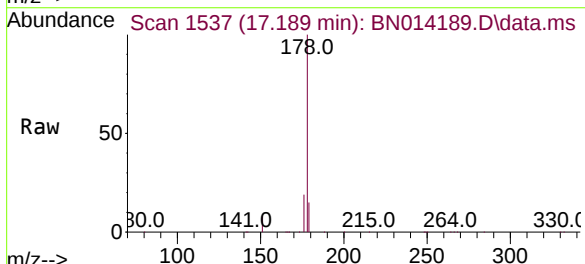




#27
Fluoranthene-d10
Concen: 1.19 ng
RT: 19.096 min Scan# 1824
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:212 Resp: 61865
Ion Ratio Lower Upper
212 100
106 12.4 9.9 14.9
104 6.9 5.6 8.4

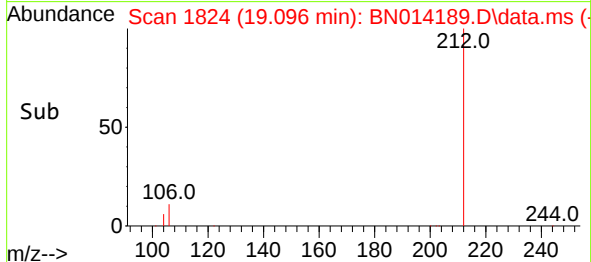

#28
Fluoranthene
Concen: 0.96 ng
RT: 19.126 min Scan# 1830
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:202 Resp: 53462
Ion Ratio Lower Upper
202 100
101 10.7 8.5 12.7
203 17.3 13.9 20.9

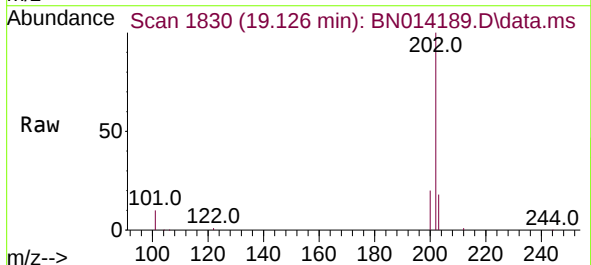



#29

Chrysene-d12

Concen: 0.40 ng

RT: 21.247 min Scan# 2124

Delta R.T. 0.000 min

Lab File: BN014189.D

Acq: 02 Apr 2021 13:24





Tgt Ion:240 Resp: 21319

Ion Ratio Lower Upper

240 100

120 8.8 7.3 10.9

236 26.2 20.8 31.2

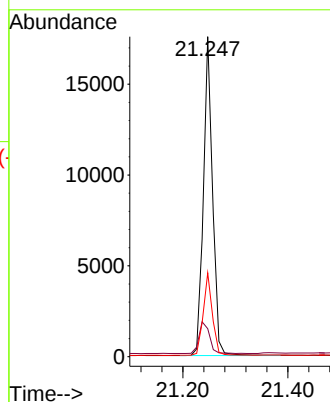

#30

Pyrene

Concen: 0.77 ng

RT: 19.488 min Scan# 1903

Delta R.T. 0.000 min

Lab File: BN014189.D

Acq: 02 Apr 2021 13:24




Tgt Ion:202 Resp: 53419


Ion Ratio Lower Upper

202 100

200 20.5 16.3 24.5

203 17.5 13.9 20.9


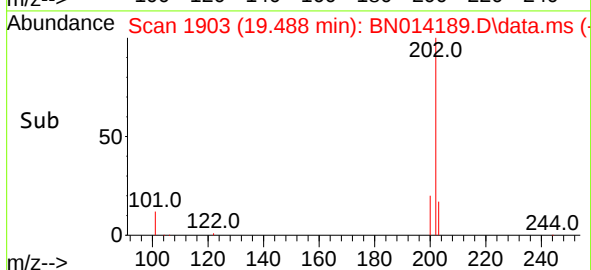
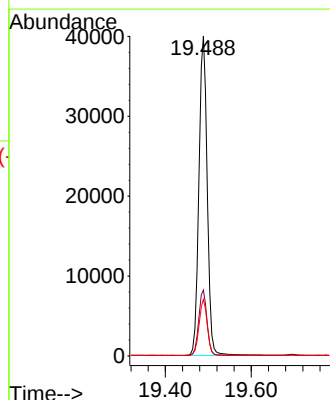





#31
 Terphenyl-d14
 Concen: 0.76 ng
 RT: 19.697 min Scan# 1945
 Delta R.T. 0.000 min
 Lab File: BN014189.D
 Acq: 02 Apr 2021 13:24




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:244 Resp: 37508
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.1 9.1
 122 11.1 9.0 13.4

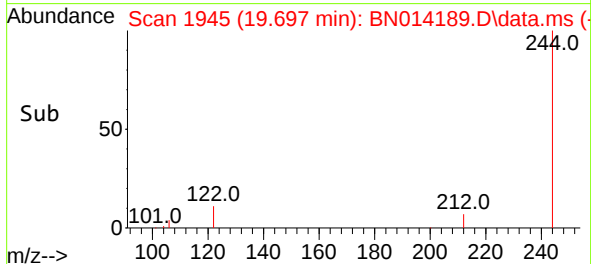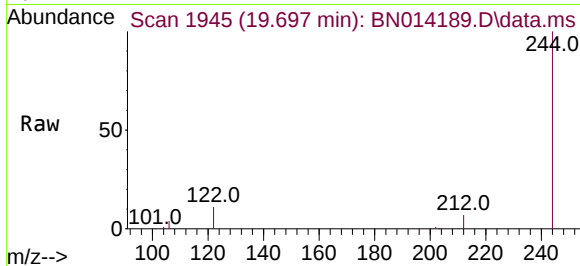

#32
 Benzo(a)anthracene
 Concen: 0.91 ng
 RT: 21.237 min Scan# 2123
 Delta R.T. 0.000 min
 Lab File: BN014189.D
 Acq: 02 Apr 2021 13:24

Tgt Ion:228 Resp: 53997
 Ion Ratio Lower Upper
 228 100
 226 25.5 20.6 30.8
 229 20.2 16.2 24.2


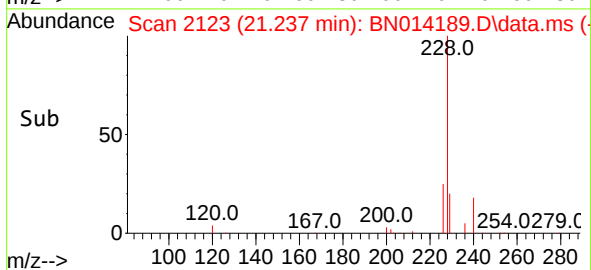

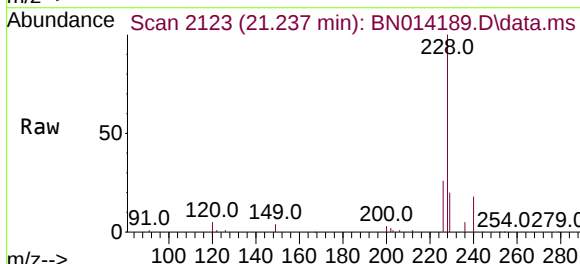


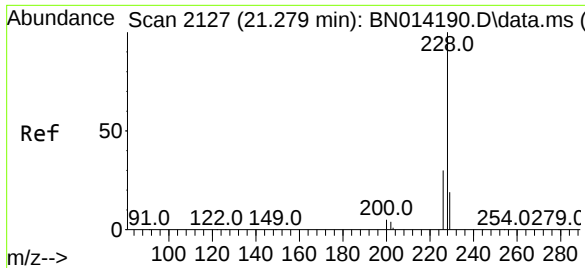

#33
Chrysene
Concen: 0.85 ng
RT: 21.279 min Scan# 2127
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	228	Resp:	55785
Ion Ratio	Lower	Upper	
228	100		
226	30.0	24.3	36.5
229	19.1	15.4	23.0

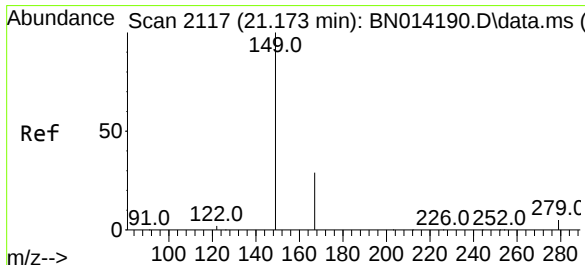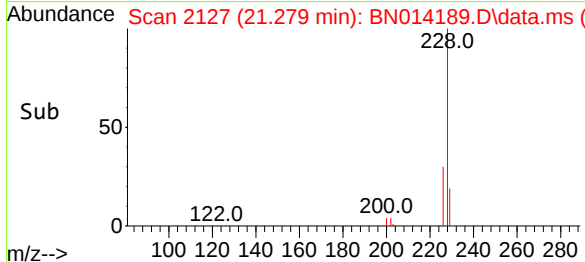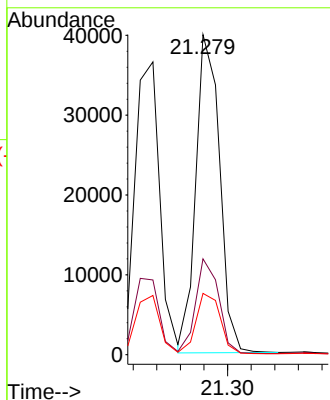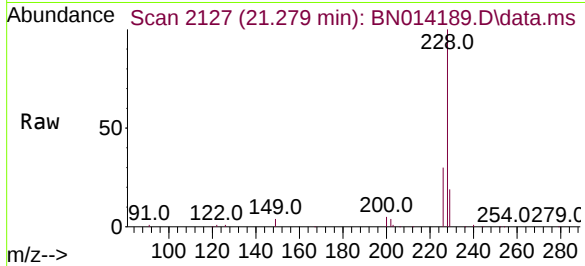

#34
Bis(2-ethylhexyl)phthalate
Concen: 1.18 ng
RT: 21.173 min Scan# 2117
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:	149	Resp:	21349
Ion Ratio	Lower	Upper	
149	100		
167	26.6	20.6	30.8
279	4.0	3.4	5.2


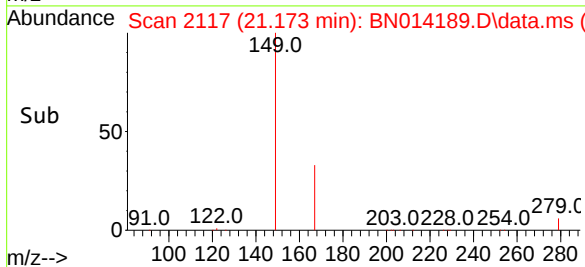
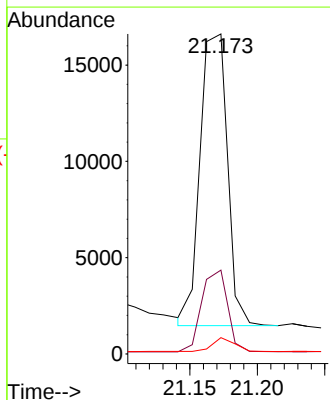
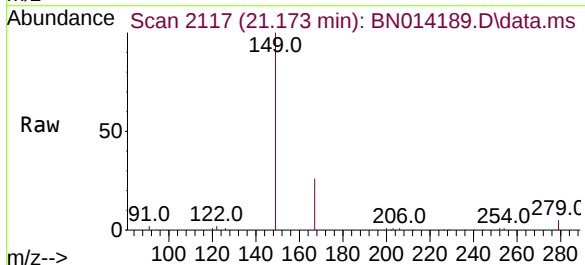


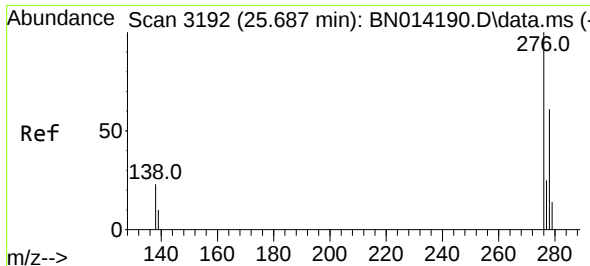

#35
Indeno(1,2,3-cd)pyrene
Concen: 1.00 ng
RT: 25.687 min Scan# 3192
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:276 Resp: 67649
Ion Ratio Lower Upper
276 100
138 23.6 19.0 28.4
277 24.9 19.9 29.9

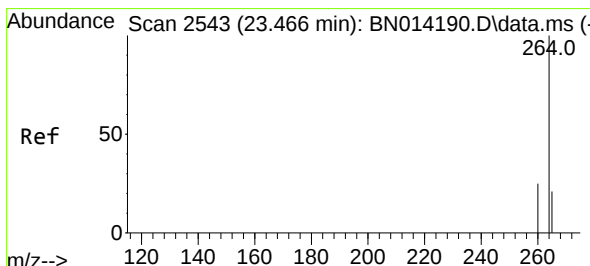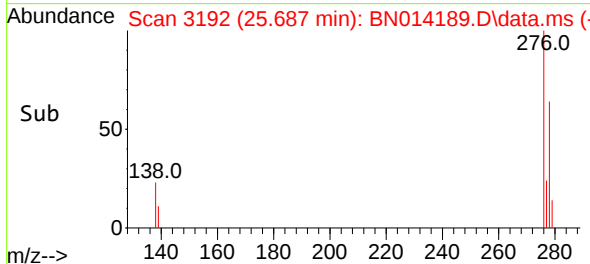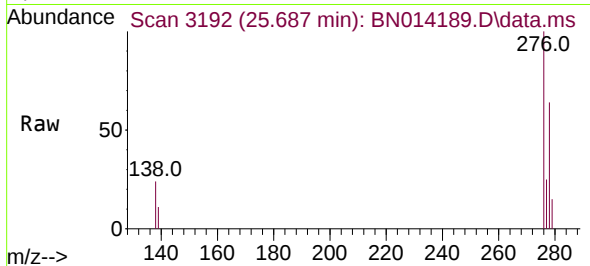

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.466 min Scan# 2543
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:264 Resp: 20828
Ion Ratio Lower Upper
264 100
260 24.3 20.1 30.1
265 31.2 25.0 37.4


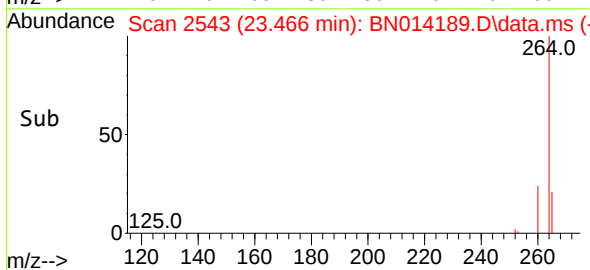

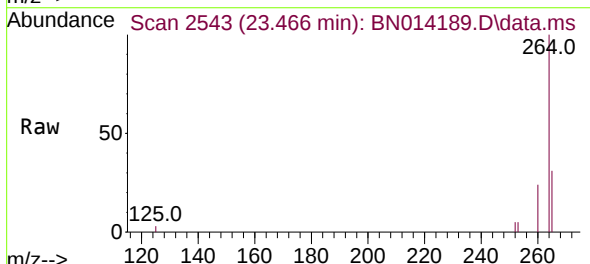




#37
Benzo(b)fluoranthene
Concen: 0.83 ng
RT: 22.799 min Scan# 2348
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:252 Resp: 60892
Ion Ratio Lower Upper
252 100
253 22.5 18.8 28.2
125 10.2 8.9 13.3

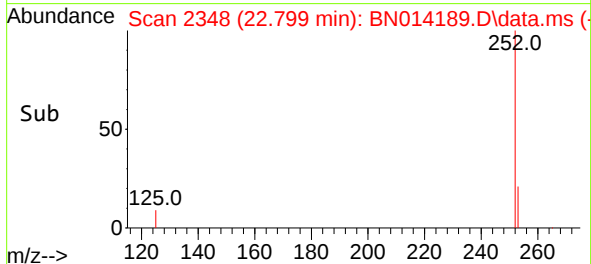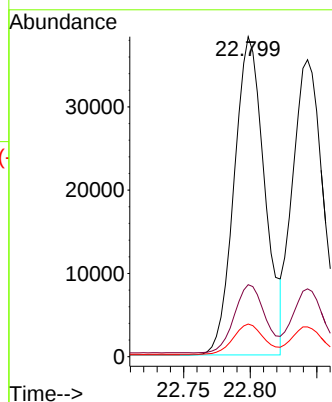

#38
Benzo(k)fluoranthene
Concen: 0.80 ng
RT: 22.843 min Scan# 2361
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:252 Resp: 57313
Ion Ratio Lower Upper
252 100
253 22.8 18.9 28.3
125 10.0 8.5 12.7


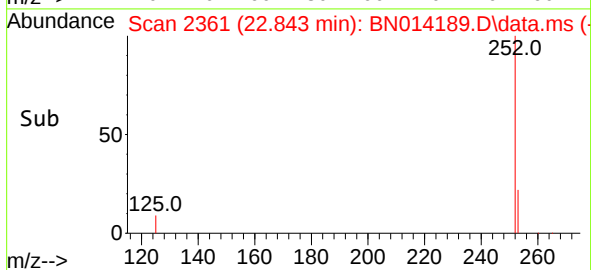

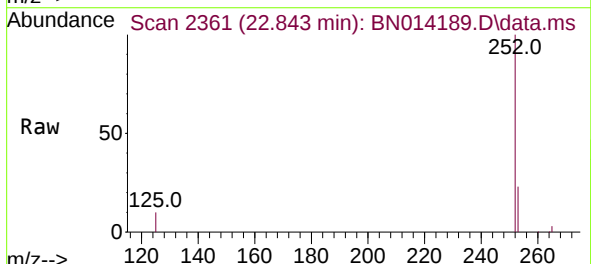




#39
Benzo(a)pyrene
Concen: 0.84 ng
RT: 23.367 min Scan# 2514
Delta R.T. 0.000 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:252 Resp: 53228
Ion Ratio Lower Upper
252 100
253 23.1 19.6 29.4
125 11.8 9.9 14.9

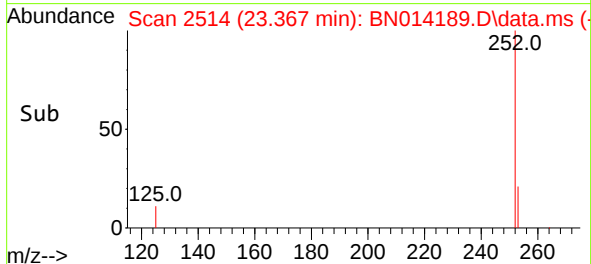

#40
Dibenzo(a,h)anthracene
Concen: 0.88 ng
RT: 25.705 min Scan# 3197
Delta R.T. 0.004 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Tgt Ion:278 Resp: 57271
Ion Ratio Lower Upper
278 100
139 15.7 13.1 19.7
279 24.6 19.9 29.9

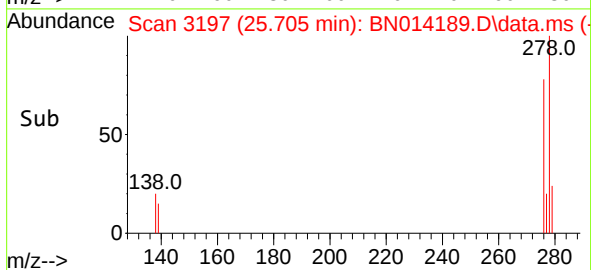

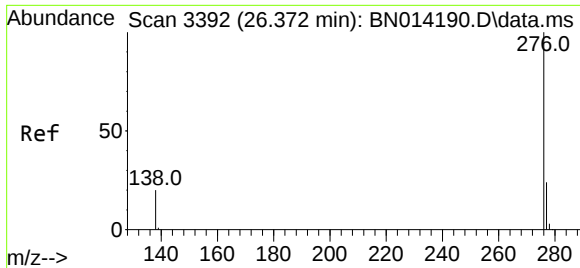

#41
Benzo(g,h,i)perylene
Concen: 0.86 ng
RT: 26.369 min Scan# 3391
Delta R.T. -0.003 min
Lab File: BN014189.D
Acq: 02 Apr 2021 13:24

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion:	276	Resp:	59444
Ion Ratio	Lower	Upper	
276	100		
277	24.2	19.9	29.9
138	20.3	16.4	24.6

