

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
 Data File : BN014193.D
 Acq On : 02 Apr 2021 15:48
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Apr 02 16:18:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 02 15:44:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.684	152	5385	0.40	ng	0.00
7) Naphthalene-d8	10.454	136	18185	0.40	ng	0.00
13) Acenaphthene-d10	14.308	164	10652	0.40	ng	-0.01
19) Phenanthrene-d10	17.055	188	22020	0.40	ng	0.00
29) Chrysene-d12	21.247	240	23781	0.40	ng	0.00
36) Perylene-d12	23.463	264	21620	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.284	112	62396	4.52	ng	0.00
5) Phenol-d6	6.855	99	82937	4.73	ng	0.00
8) Nitrobenzene-d5	8.819	82	69160	5.59	ng	-0.01
11) 2-Methylnaphthalene-d10	12.053	152	193354	7.00	ng	0.00
14) 2,4,6-Tribromophenol	15.805	330	22599	6.60	ng	0.00
15) 2-Fluorobiphenyl	12.938	172	188962	4.73	ng	0.00
27) Fluoranthene-d10	19.096	212	438458	7.61	ng	0.00
31) Terphenyl-d14	19.697	244	261503	4.77	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.223	88	28640	4.13	ng	98
3) n-Nitrosodimethylamine	3.537	42	27969	5.24	ng	# 92
6) bis(2-Chloroethyl)ether	7.112	93	66627	4.77	ng	100
9) Naphthalene	10.505	128	232084	5.17	ng	99
10) Hexachlorobutadiene	10.796	225	42360	5.15	ng	# 100
12) 2-Methylnaphthalene	12.124	142	158449	5.39	ng	99
16) Acenaphthylene	14.029	152	236520	5.80	ng	100
17) Acenaphthene	14.372	154	153716	5.21	ng	98
18) Fluorene	15.361	166	193355	5.43	ng	99
21) 4-Bromophenyl-phenylether	16.252	248	62968	5.56	ng	# 66
22) Hexachlorobenzene	16.373	284	66386	5.25	ng	99
23) Atrazine	16.532	200	48228	6.23	ng	97
25) Phenanthrene	17.104	178	312904	5.29	ng	100
26) Anthracene	17.189	178	288931	5.81	ng	100
28) Fluoranthene	19.126	202	370162	5.99	ng	100
30) Pyrene	19.488	202	375744	4.84	ng	100
32) Benzo(a)anthracene	21.237	228	386965	5.87	ng	99
33) Chrysene	21.279	228	386613	5.31	ng	100
34) Bis(2-ethylhexyl)phtha...	21.162	149	170268	8.47	ng	97
35) Indeno(1,2,3-cd)pyrene	25.687	276	440301	5.82	ng	100
37) Benzo(b)fluoranthene	22.798	252	395419	5.19	ng	96
38) Benzo(k)fluoranthene	22.843	252	391461	5.25	ng	97
39) Benzo(a)pyrene	23.367	252	355597	5.43	ng	95
40) Dibenzo(a,h)anthracene	25.701	278	370595	5.51	ng	97
41) Benzo(g,h,i)perylene	26.372	276	380549	5.32	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
Data File : BN014193.D
Acq On : 02 Apr 2021 15:48
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Apr 02 16:18:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 02 15:44:53 2021
Response via : Initial Calibration




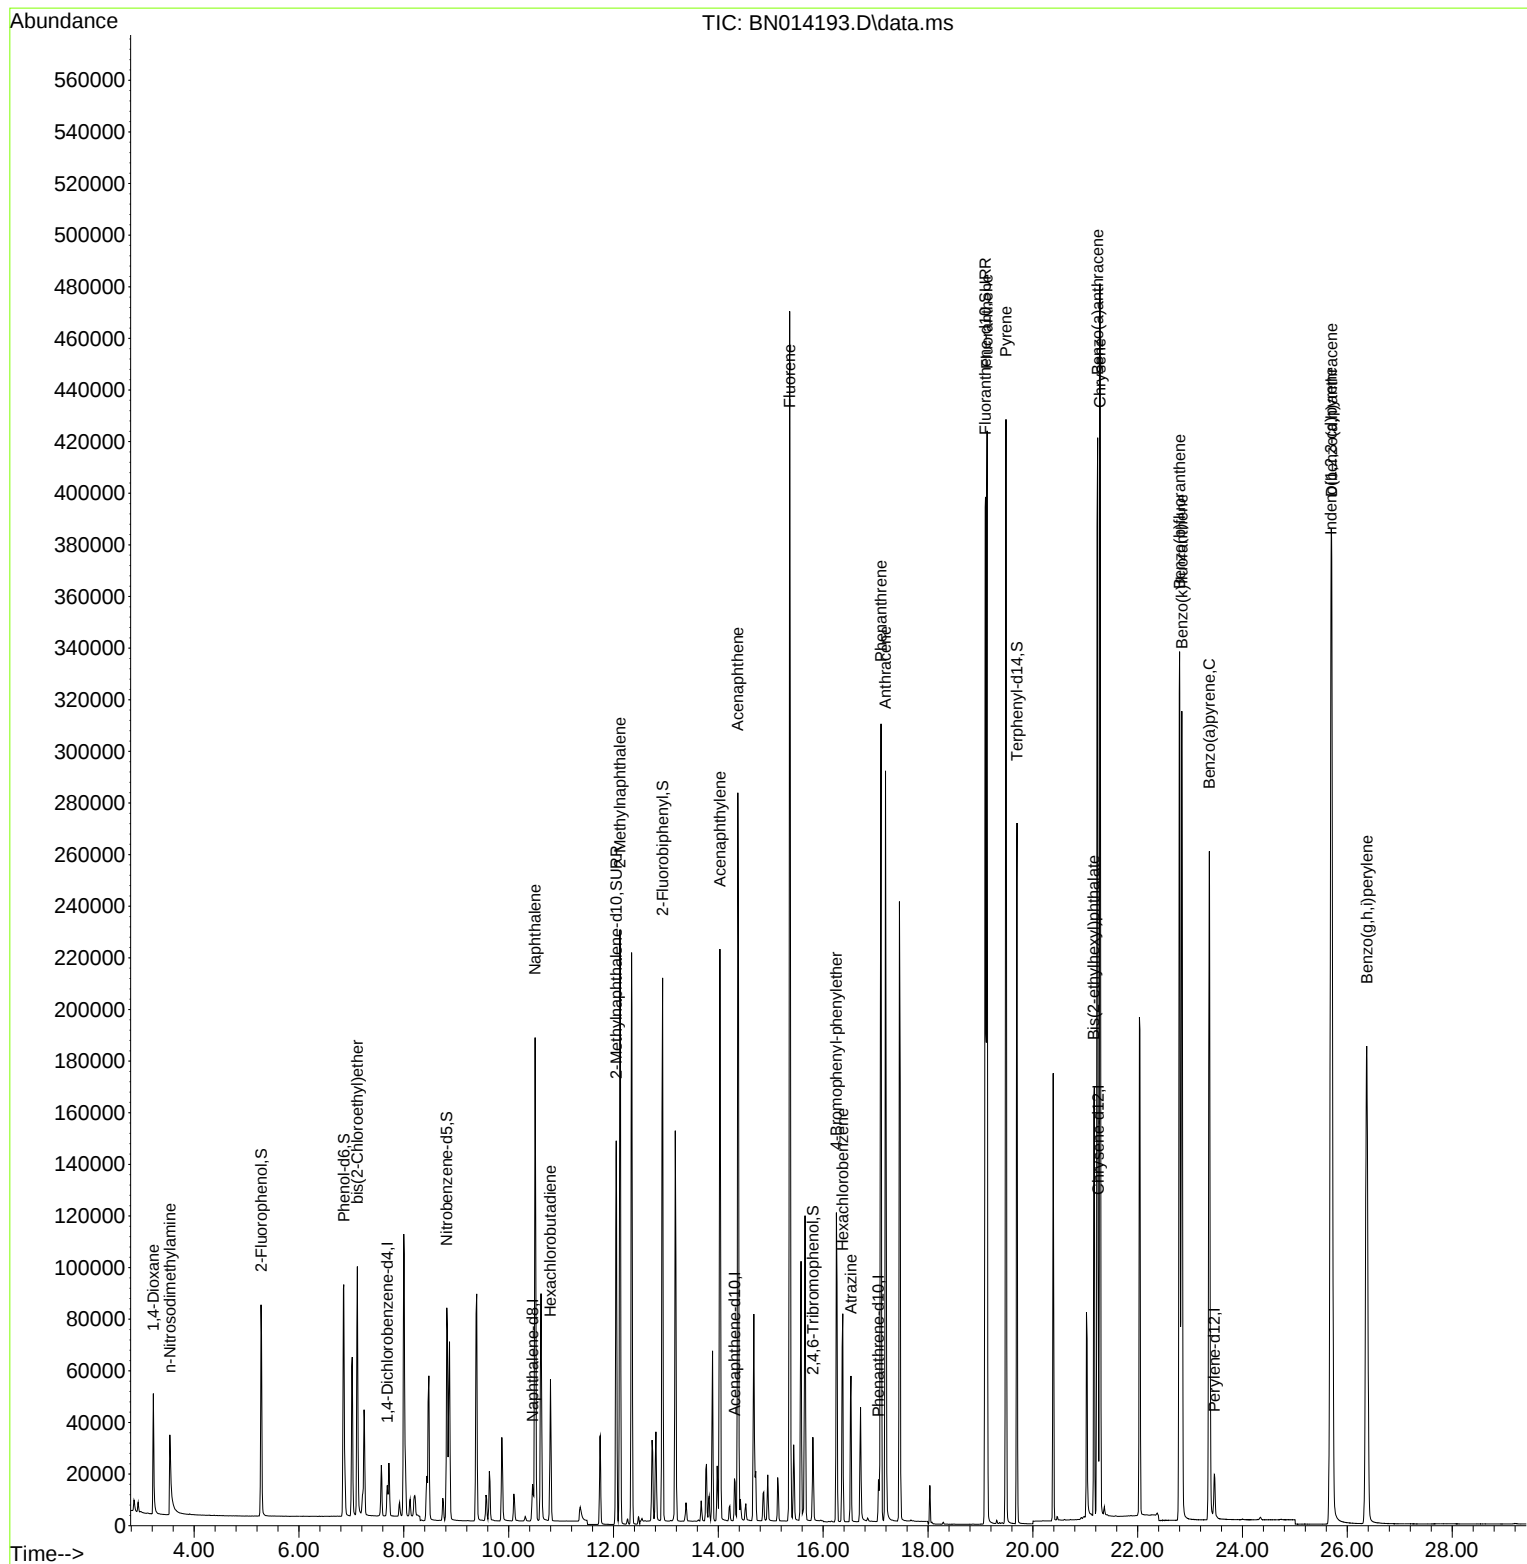




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.684 min Scan# 609
 Delta R.T. 0.000 min
 Lab File: BN014193.D
 Acq: 02 Apr 2021 15:48




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:152 Resp: 5385
 Ion Ratio Lower Upper
 152 100
 150 155.4 126.2 189.4
 115 59.8 49.8 74.6

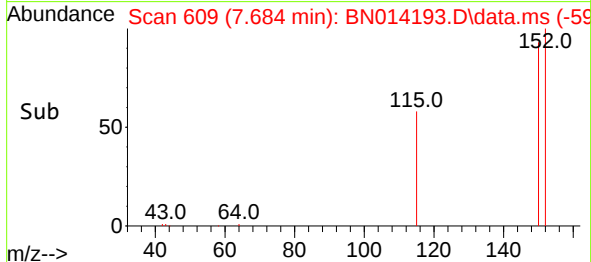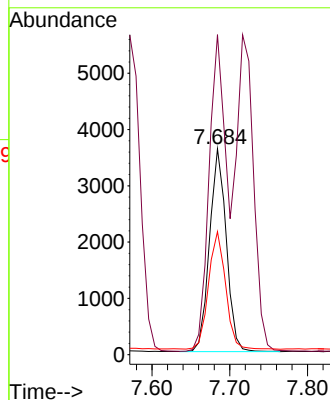

#2
 1,4-Dioxane
 Concen: 4.13 ng
 RT: 3.223 min Scan# 55
 Delta R.T. -0.008 min
 Lab File: BN014193.D
 Acq: 02 Apr 2021 15:48

Tgt Ion: 88 Resp: 28640
 Ion Ratio Lower Upper
 88 100
 58 79.9 63.2 94.8
 43 33.0 25.1 37.7


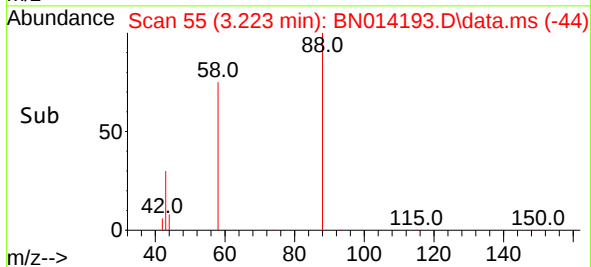
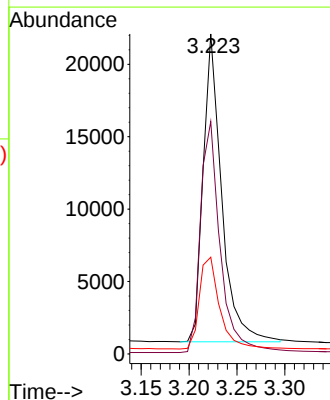
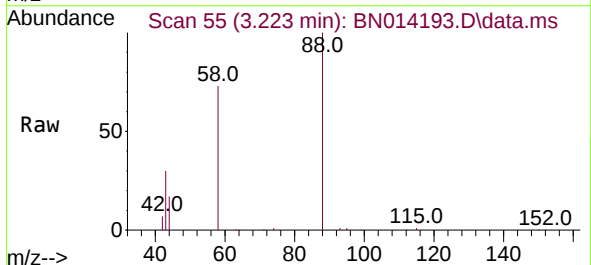


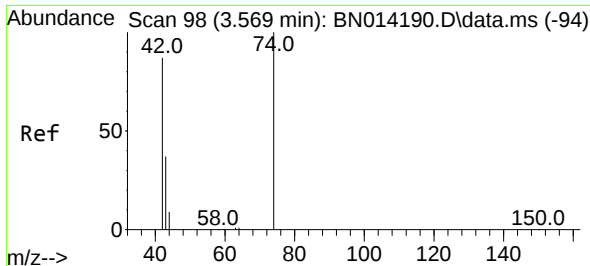

#3
n-Nitrosodimethylamine
Concen: 5.24 ng
RT: 3.537 min Scan# 94
Delta R.T. -0.032 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 27969
Ion Ratio Lower Upper
42 100
74 114.4 98.8 148.2
44 5.9 0.0 0.0#

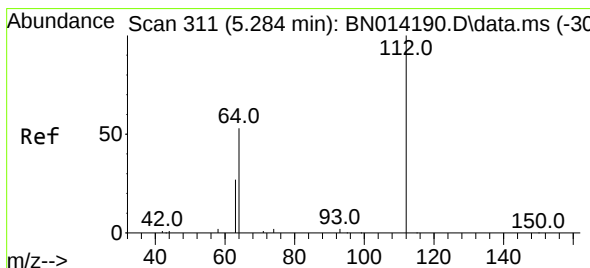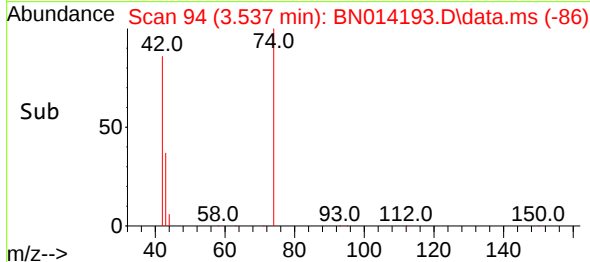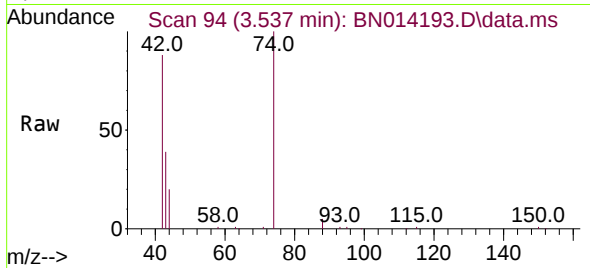

#4
2-Fluorophenol
Concen: 4.52 ng
RT: 5.284 min Scan# 311
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion: 112 Resp: 62396
Ion Ratio Lower Upper
112 100
64 60.0 48.3 72.5
63 31.7 25.8 38.6


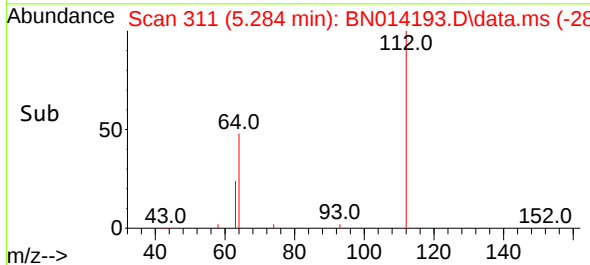

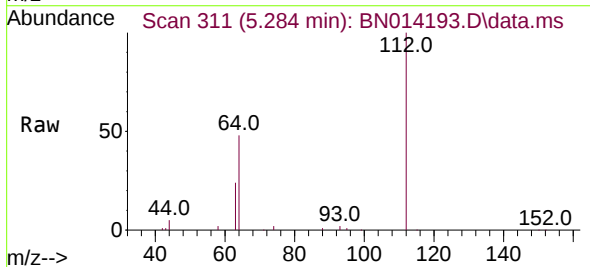


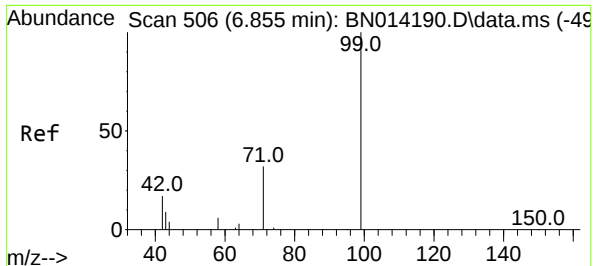

#5
Phenol-d6
Concen: 4.73 ng
RT: 6.855 min Scan# 506
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	99	Resp:	82937
Ion	Ratio	Lower	Upper
99	100		
42	21.9	17.8	26.6
71	33.5	26.6	40.0

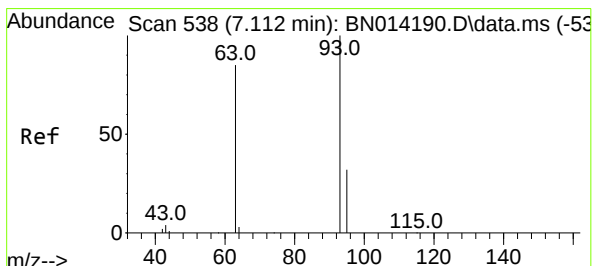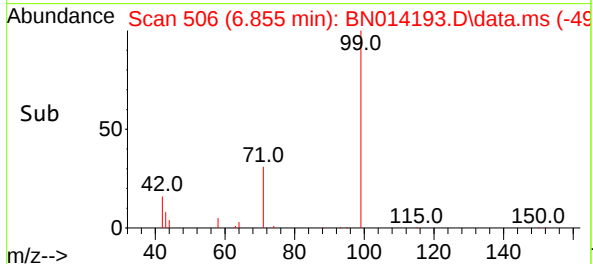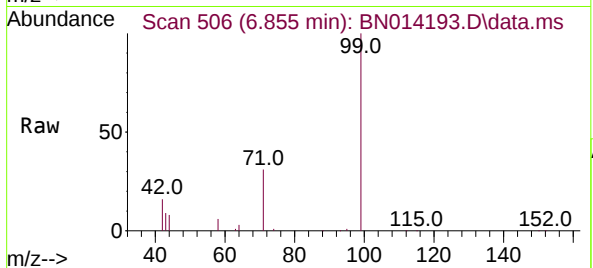

#6
bis(2-Chloroethyl)ether
Concen: 4.77 ng
RT: 7.112 min Scan# 538
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:	93	Resp:	66627
Ion	Ratio	Lower	Upper
93	100		
63	80.5	64.2	96.4
95	32.9	26.6	40.0


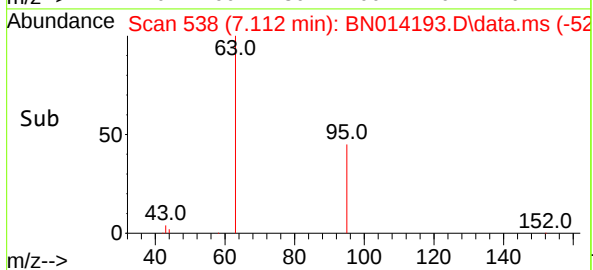

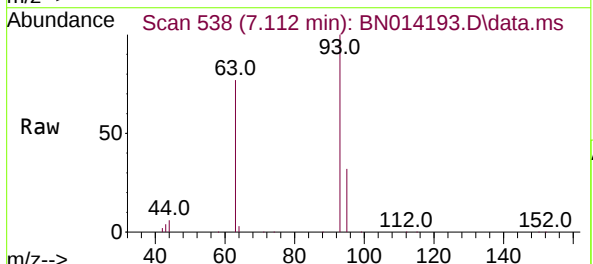




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.454 min Scan# 856
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	18185
Ion Ratio	Lower	Upper	
136	100		
137	11.4	9.1	13.7
54	9.6	8.2	12.4
68	7.2	6.1	9.1

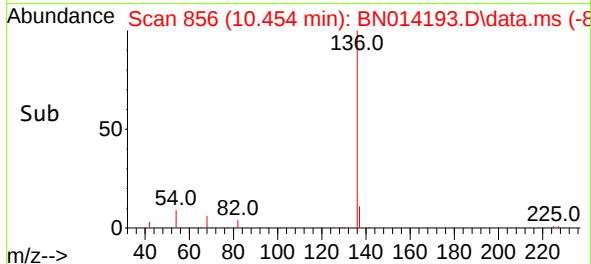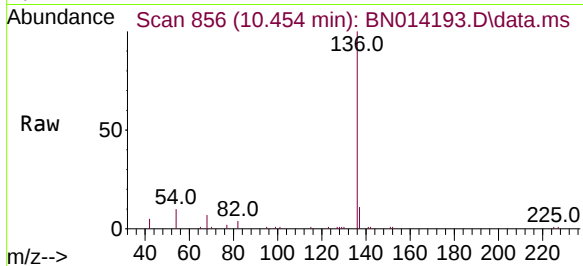

#8
Nitrobenzene-d5
Concen: 5.59 ng
RT: 8.819 min Scan# 727
Delta R.T. -0.013 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:	82	Resp:	69160
Ion Ratio	Lower	Upper	
82	100		
128	31.5	36.8	55.2#
54	60.9	38.7	58.1#


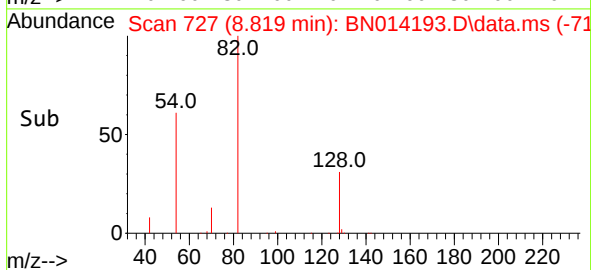

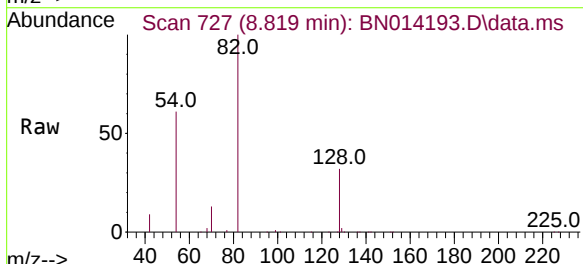


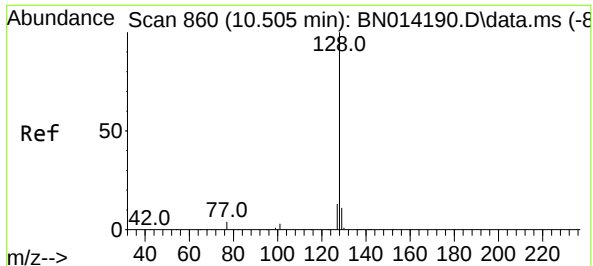

#9
Naphthalene
Concen: 5.17 ng
RT: 10.505 min Scan# 860
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 232084
Ion Ratio Lower Upper
128 100
129 10.9 9.1 13.7
127 13.0 10.6 15.8

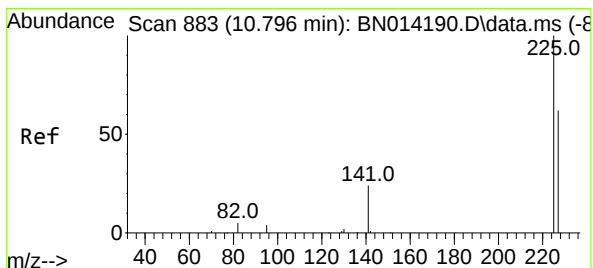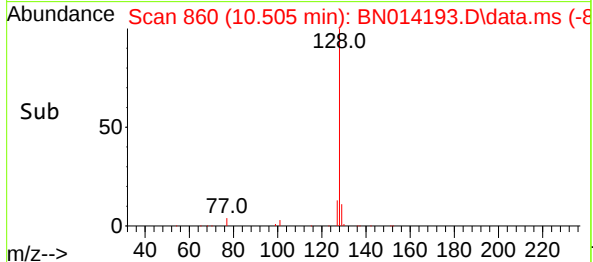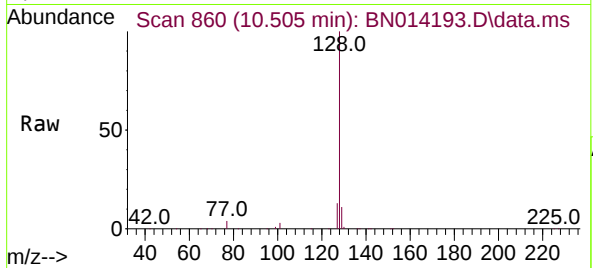

#10
Hexachlorobutadiene
Concen: 5.15 ng
RT: 10.796 min Scan# 883
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:225 Resp: 42360
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.9 50.8 76.2


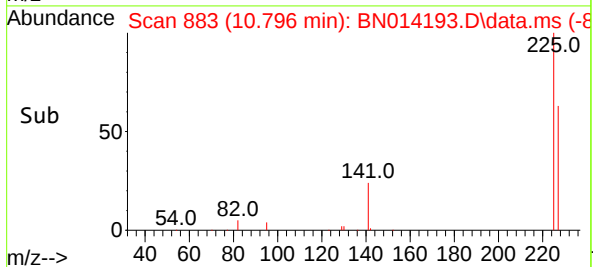

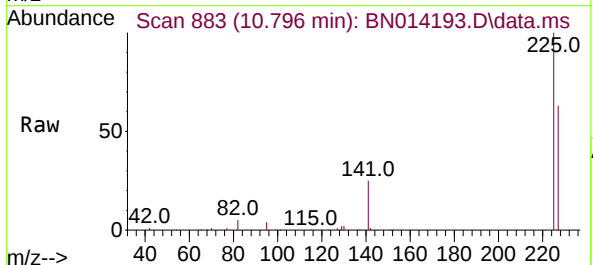


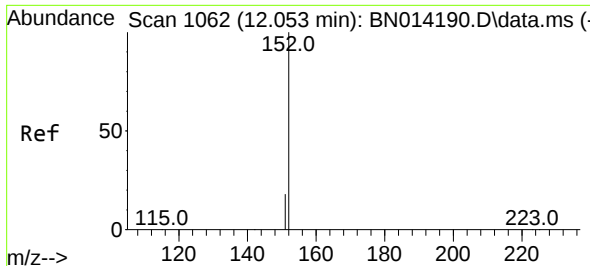

#11
2-Methylnaphthalene-d10
Concen: 7.00 ng
RT: 12.053 min Scan# 1062
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 193354
Ion Ratio Lower Upper
152 100
151 20.0 16.1 24.1

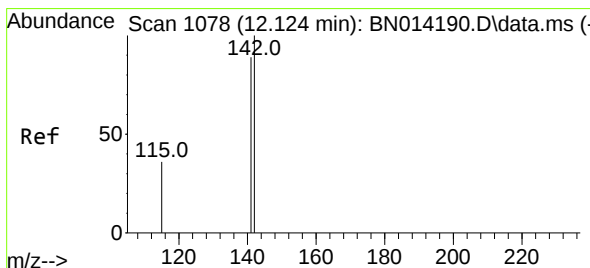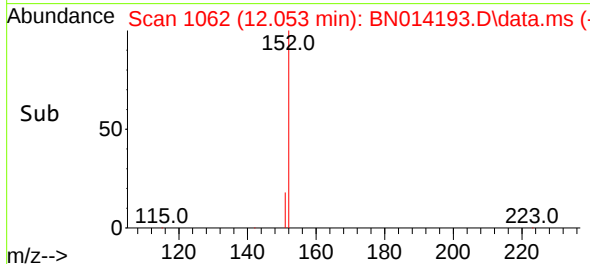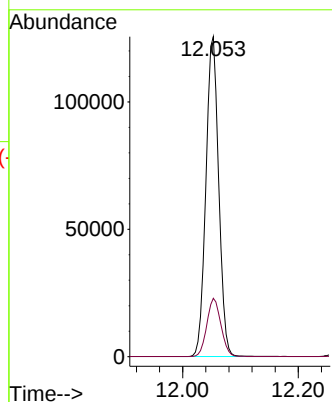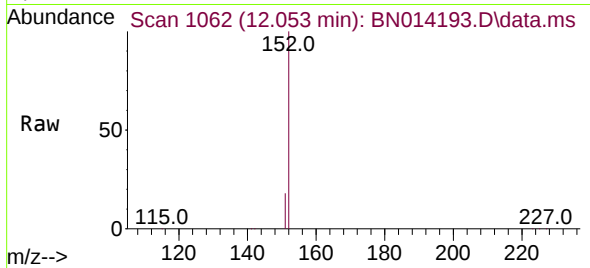

#12
2-Methylnaphthalene
Concen: 5.39 ng
RT: 12.124 min Scan# 1078
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:142 Resp: 158449
Ion Ratio Lower Upper
142 100
141 88.7 71.6 107.4
115 35.2 29.2 43.8


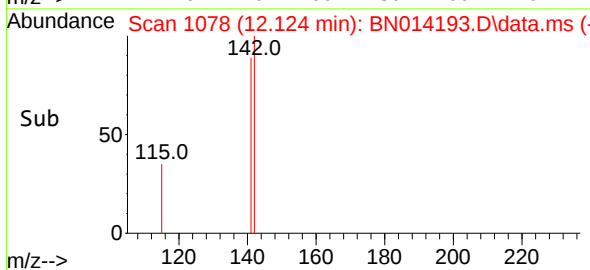

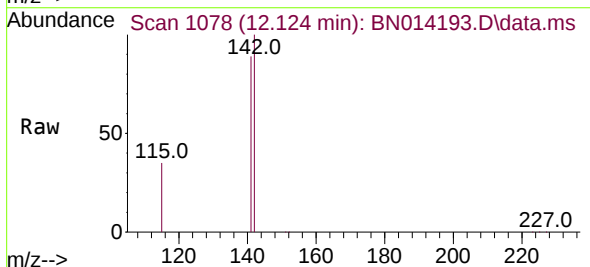




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.308 min Scan# 1306
Delta R.T. -0.013 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 10652
Ion Ratio Lower Upper
164 100
162 104.5 77.4 116.2
160 49.1 34.2 51.4

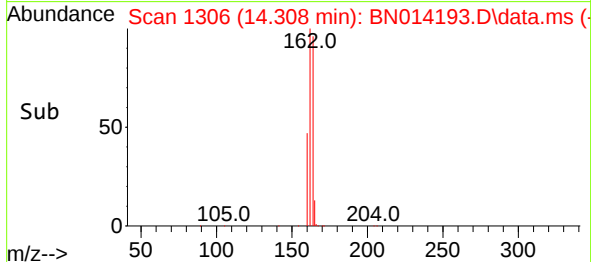

#14
2,4,6-Tribromophenol
Concen: 6.60 ng
RT: 15.805 min Scan# 1424
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:330 Resp: 22599
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 37.5 29.8 44.6


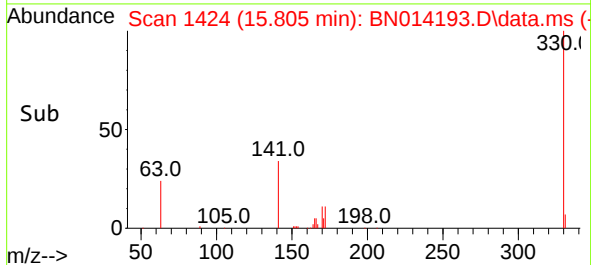

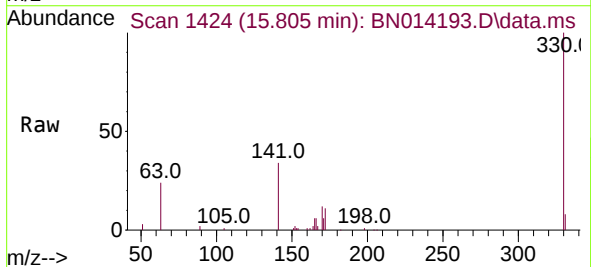




#15
2-Fluorobiphenyl
Concen: 4.73 ng
RT: 12.938 min Scan# 1198
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:172 Resp: 188962
Ion Ratio Lower Upper
172 100
171 33.6 27.3 40.9
170 22.0 18.1 27.1

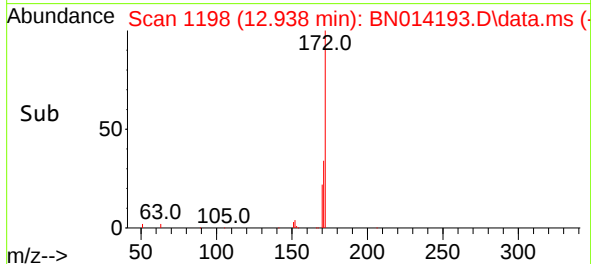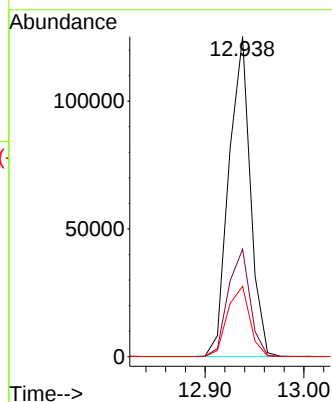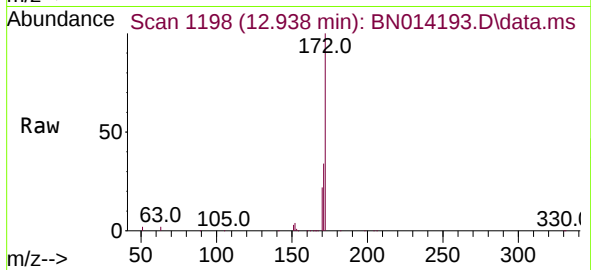

#16
Acenaphthylene
Concen: 5.80 ng
RT: 14.029 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:152 Resp: 236520
Ion Ratio Lower Upper
152 100
151 19.2 15.1 22.7
153 13.0 10.5 15.7


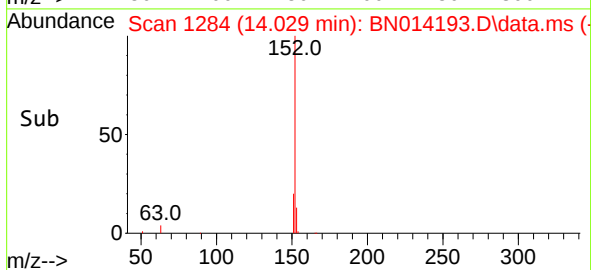
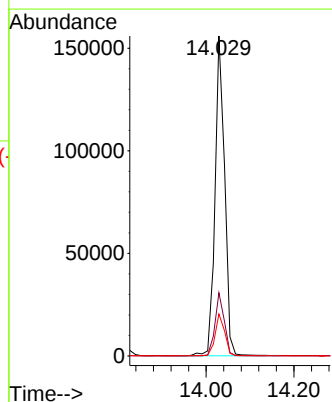
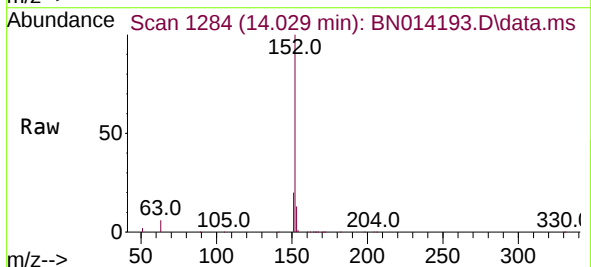




#17
Acenaphthene
Concen: 5.21 ng
RT: 14.372 min Scan# 1311
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 153716
Ion Ratio Lower Upper
154 100
153 109.5 89.2 133.8
152 52.7 43.8 65.6

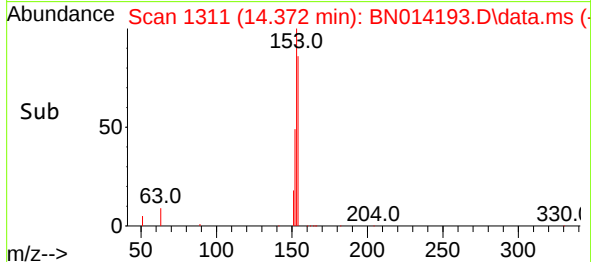

#18
Fluorene
Concen: 5.43 ng
RT: 15.361 min Scan# 1389
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:166 Resp: 193355
Ion Ratio Lower Upper
166 100
165 97.3 78.5 117.7
167 13.4 10.9 16.3


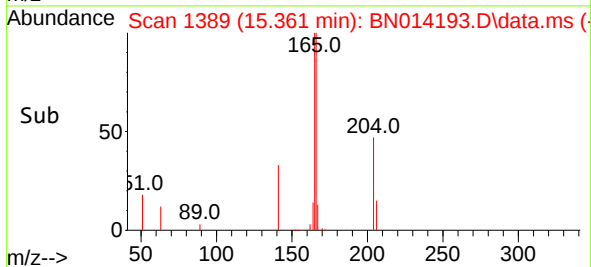

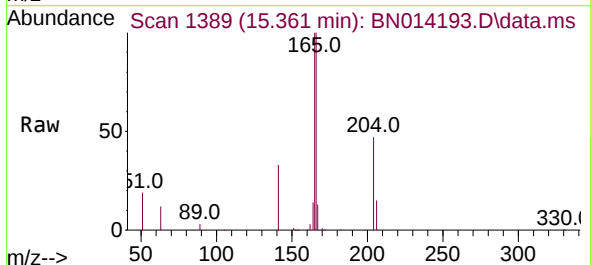


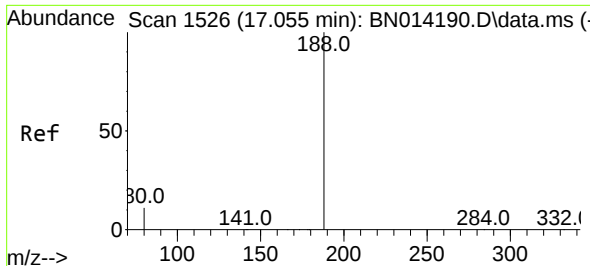

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.055 min Scan# 1526
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	188	Resp:	22020
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	11.8	9.5	14.3

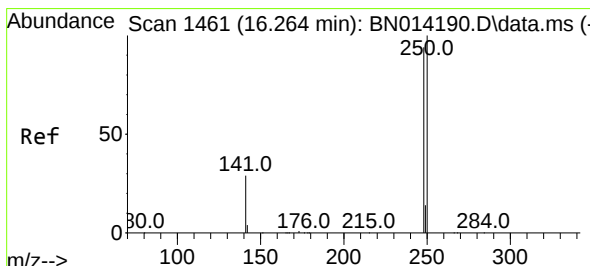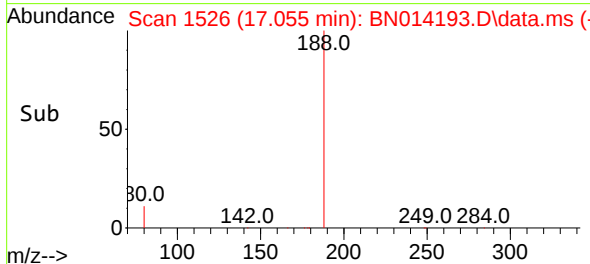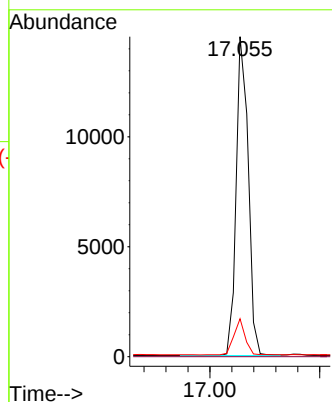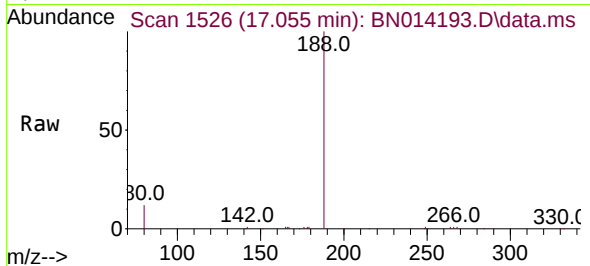

#21
4-Bromophenyl-phenylether
Concen: 5.56 ng
RT: 16.252 min Scan# 1460
Delta R.T. -0.012 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:	248	Resp:	62968
Ion Ratio	Lower	Upper	
248	100		
250	88.7	85.6	128.4
141	82.6	26.1	39.1#


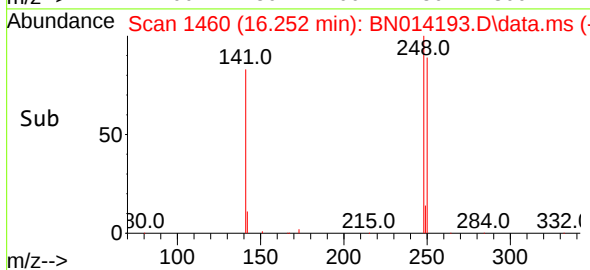

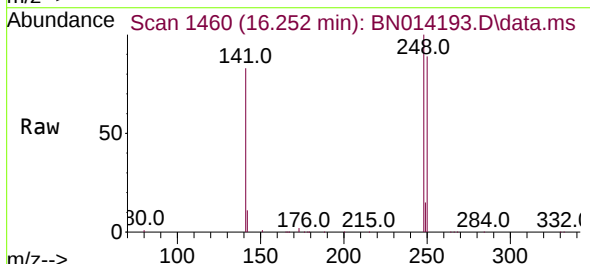




#22
Hexachlorobenzene
Concen: 5.25 ng
RT: 16.373 min Scan# 1470
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:284 Resp: 66386
Ion Ratio Lower Upper
284 100
142 35.2 28.6 42.8
249 31.1 25.3 37.9

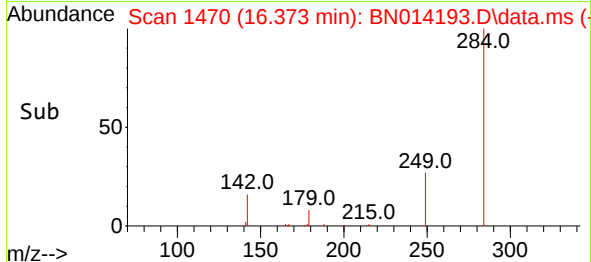

#23
Atrazine
Concen: 6.23 ng
RT: 16.532 min Scan# 1483
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:200 Resp: 48228
Ion Ratio Lower Upper
200 100
173 19.7 17.6 26.4
215 50.2 41.4 62.0


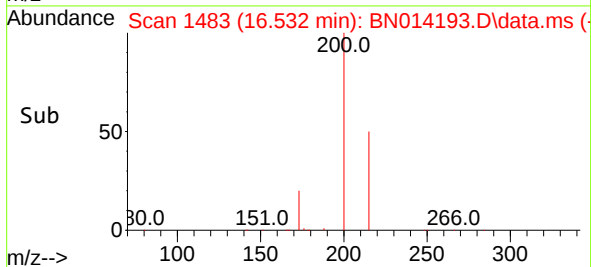

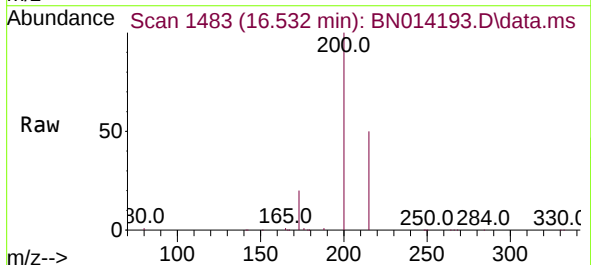


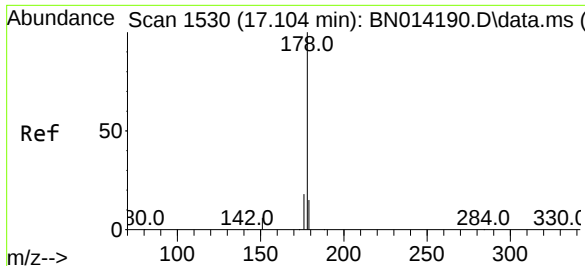

#25
Phenanthrene
Concen: 5.29 ng
RT: 17.104 min Scan# 1530
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 312904
Ion Ratio Lower Upper
178 100
176 18.8 15.2 22.8
179 15.4 12.3 18.5

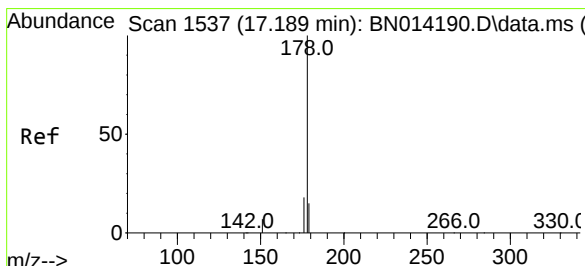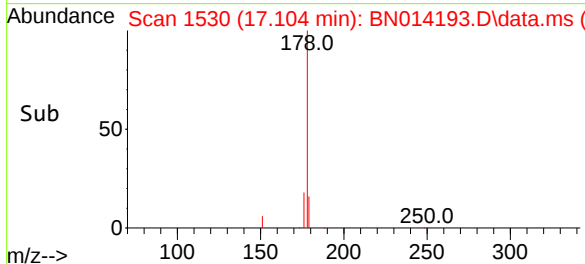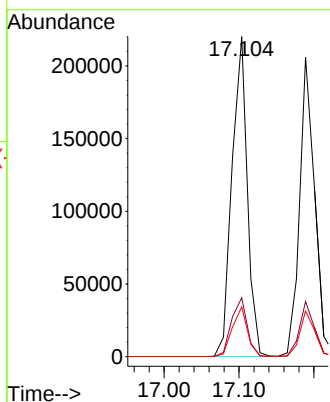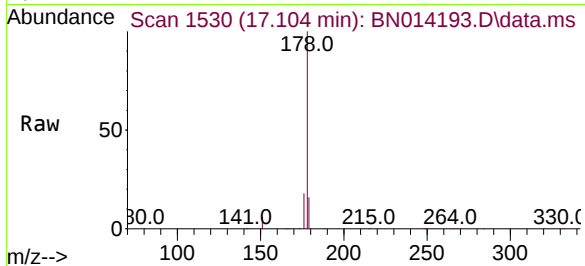

#26
Anthracene
Concen: 5.81 ng
RT: 17.189 min Scan# 1537
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:178 Resp: 288931
Ion Ratio Lower Upper
178 100
176 18.2 14.6 22.0
179 15.4 12.4 18.6


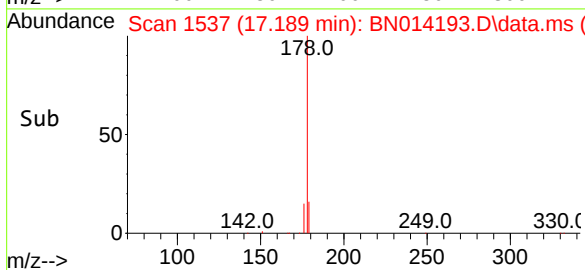
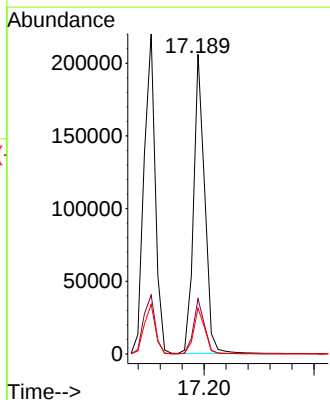
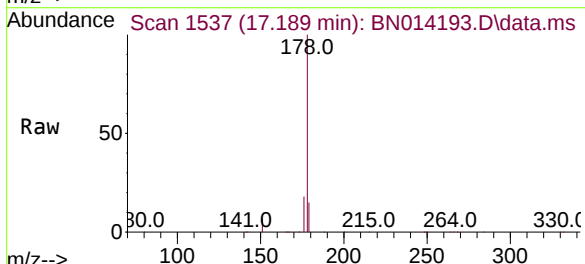




#27
Fluoranthene-d10
Concen: 7.61 ng
RT: 19.096 min Scan# 1824
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 438458
Ion Ratio Lower Upper
212 100
106 12.5 9.9 14.9
104 6.9 5.6 8.4

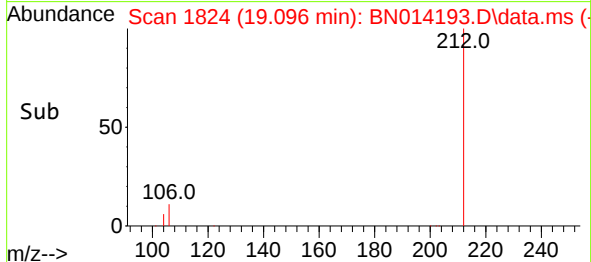

#28
Fluoranthene
Concen: 5.99 ng
RT: 19.126 min Scan# 1830
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:202 Resp: 370162
Ion Ratio Lower Upper
202 100
101 10.8 8.5 12.7
203 17.4 13.9 20.9


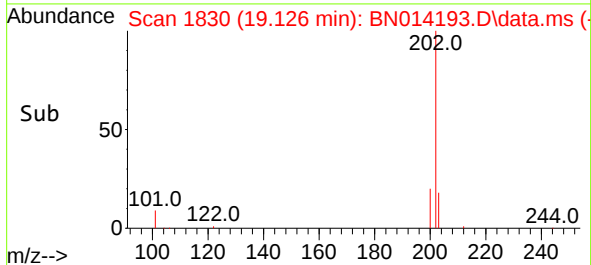

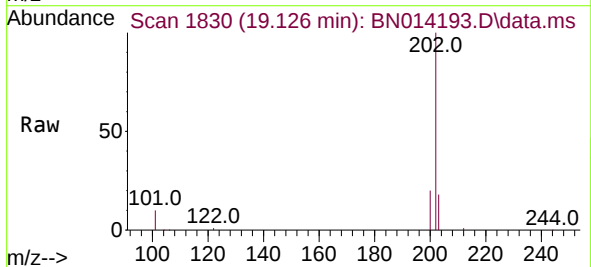


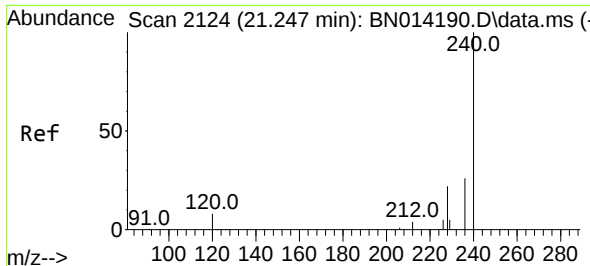

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.247 min Scan# 2124
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 23781
Ion Ratio Lower Upper
240 100
120 9.3 7.3 10.9
236 26.3 20.8 31.2

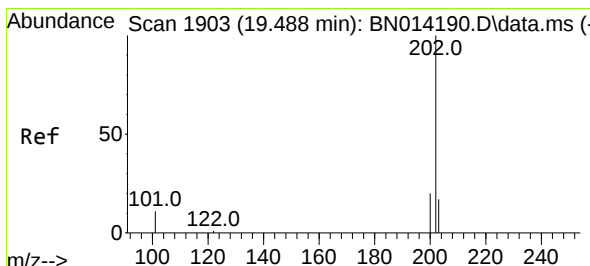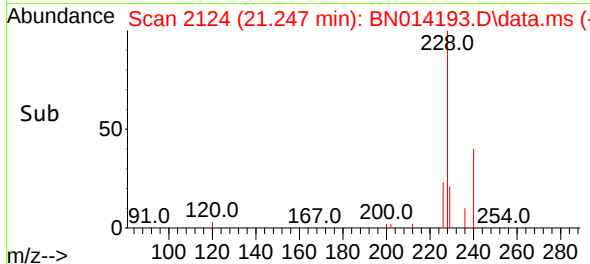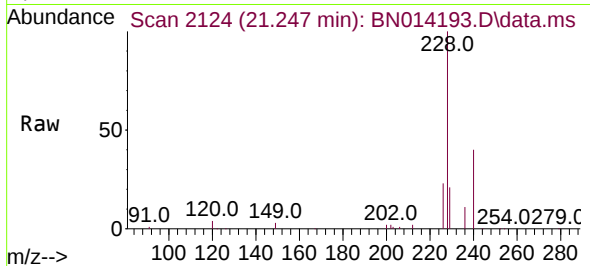

#30
Pyrene
Concen: 4.84 ng
RT: 19.488 min Scan# 1903
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:202 Resp: 375744
Ion Ratio Lower Upper
202 100
200 20.4 16.3 24.5
203 17.5 13.9 20.9


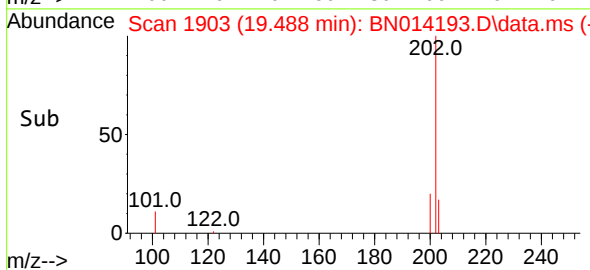

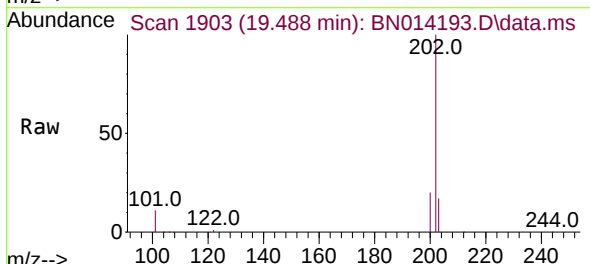




#31
 Terphenyl-d14
 Concen: 4.77 ng
 RT: 19.697 min Scan# 1945
 Delta R.T. 0.000 min
 Lab File: BN014193.D
 Acq: 02 Apr 2021 15:48




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:244 Resp: 261503
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.1 9.1
 122 10.3 9.0 13.4

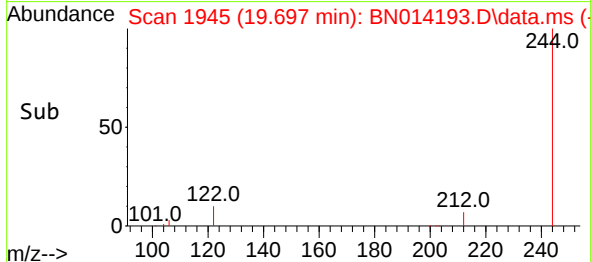

#32
 Benzo(a)anthracene
 Concen: 5.87 ng
 RT: 21.237 min Scan# 2123
 Delta R.T. 0.000 min
 Lab File: BN014193.D
 Acq: 02 Apr 2021 15:48

Tgt Ion:228 Resp: 386965
 Ion Ratio Lower Upper
 228 100
 226 25.2 20.6 30.8
 229 20.2 16.2 24.2

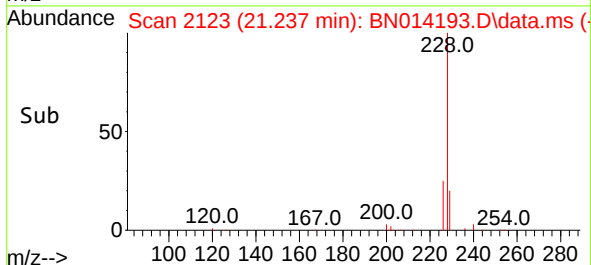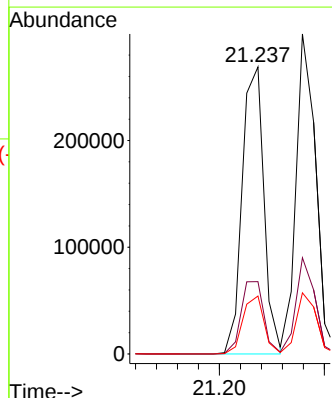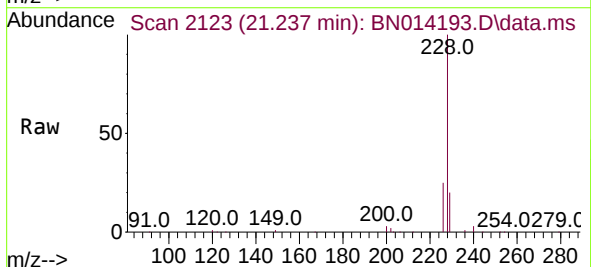

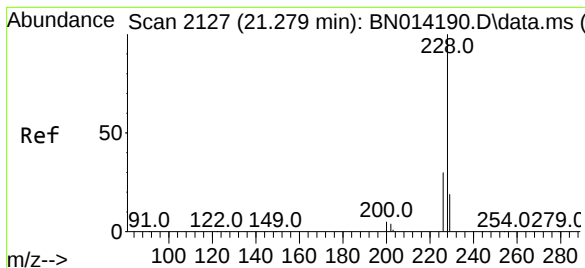

#33

Chrysene

Concen: 5.31 ng

RT: 21.279 min Scan# 2127

Delta R.T. 0.000 min

Lab File: BN014193.D

Acq: 02 Apr 2021 15:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:228 Resp: 386613

Ion Ratio Lower Upper

228 100

226 30.1 24.3 36.5

229 19.1 15.4 23.0

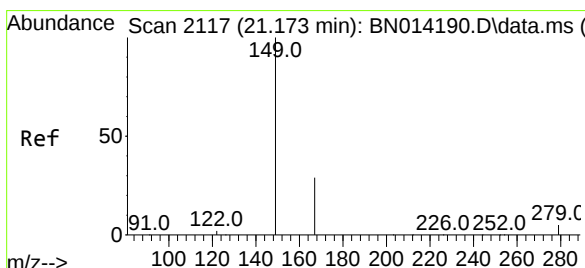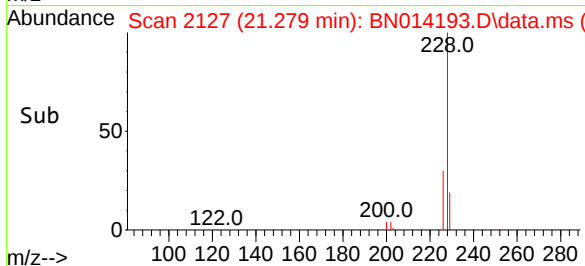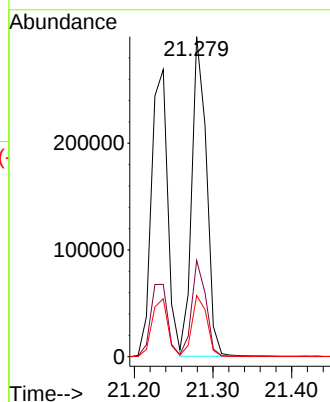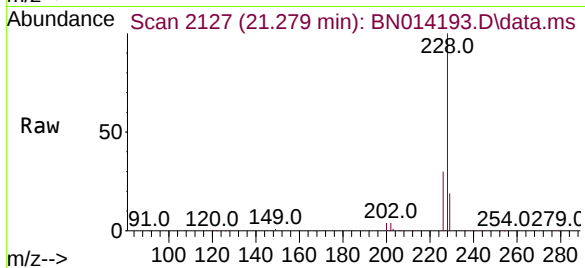

#34

Bis(2-ethylhexyl)phthalate

Concen: 8.47 ng

RT: 21.162 min Scan# 2116

Delta R.T. -0.011 min

Lab File: BN014193.D

Acq: 02 Apr 2021 15:48




Tgt Ion:149 Resp: 170268


Ion Ratio Lower Upper

149 100

167 27.3 20.6 30.8


279 4.0 3.4 5.2

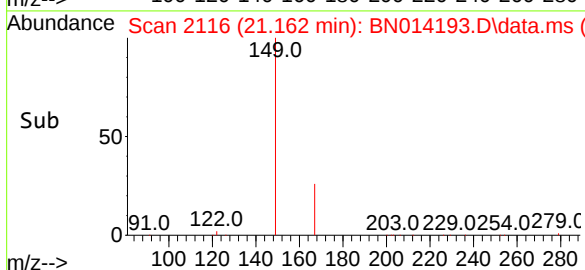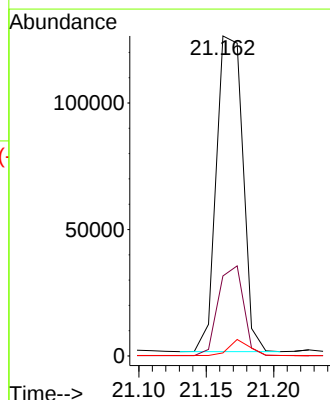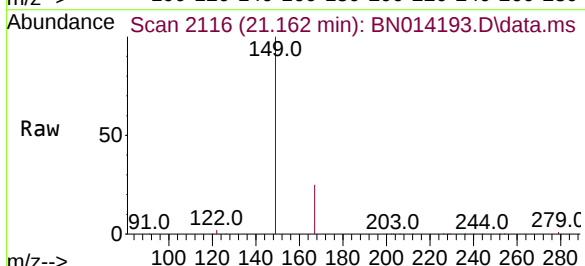






#35
Indeno(1,2,3-cd)pyrene
Concen: 5.82 ng
RT: 25.687 min Scan# 3192
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0





Tgt Ion:276 Resp: 440301
Ion Ratio Lower Upper
276 100
138 23.8 19.0 28.4
277 24.8 19.9 29.9

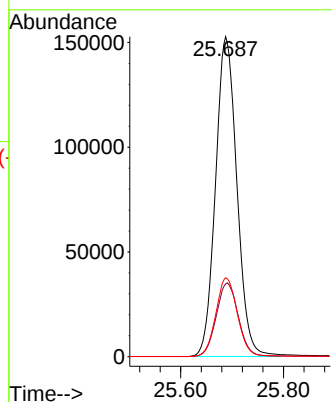


#36
Perylene-d12
Concen: 0.40 ng
RT: 23.463 min Scan# 2542
Delta R.T. -0.003 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48



Tgt Ion:264 Resp: 21620
Ion Ratio Lower Upper
264 100
260 24.5 20.1 30.1
265 30.0 25.0 37.4




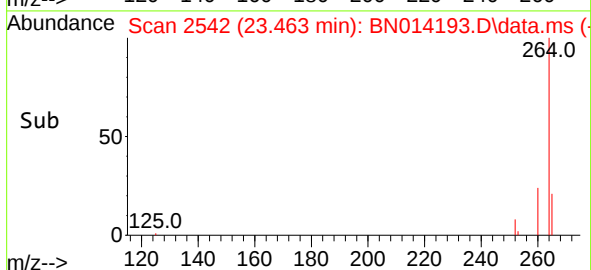




#37
Benzo(b)fluoranthene
Concen: 5.19 ng
RT: 22.798 min Scan# 2348
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 395419
Ion Ratio Lower Upper
252 100
253 21.8 18.8 28.2
125 9.4 8.9 13.3

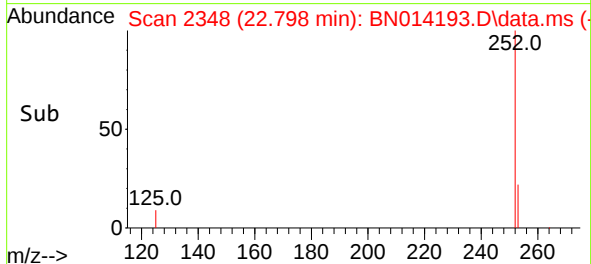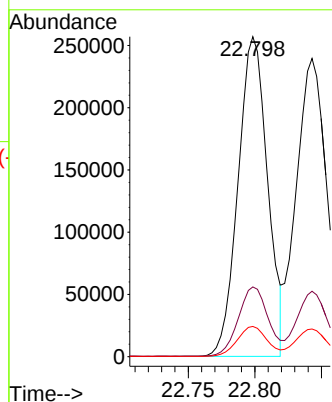

#38
Benzo(k)fluoranthene
Concen: 5.25 ng
RT: 22.843 min Scan# 2361
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Tgt Ion:252 Resp: 391461
Ion Ratio Lower Upper
252 100
253 21.9 18.9 28.3
125 9.3 8.5 12.7

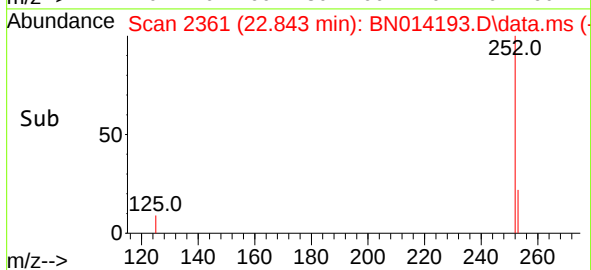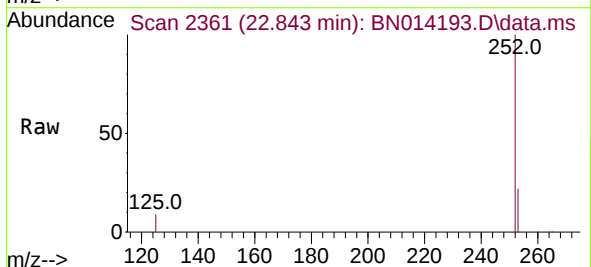



#39

Benzo(a)pyrene

Concen: 5.43 ng

RT: 23.367 min Scan# 2514

Delta R.T. 0.000 min

Lab File: BN014193.D

Acq: 02 Apr 2021 15:48





Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0

Tgt Ion:252	Resp:	355597
Ion Ratio	Lower	Upper
252	100	
253	21.7	19.6 29.4
125	10.5	9.9 14.9

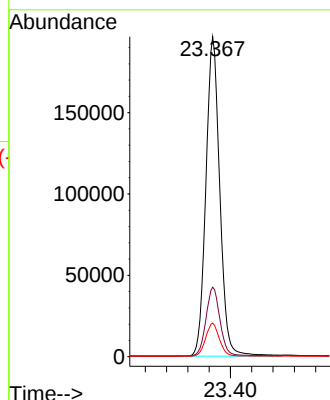

#40

Dibenzo(a,h)anthracene

Concen: 5.51 ng




RT: 25.701 min Scan# 3196


Delta R.T. 0.000 min

Lab File: BN014193.D

Acq: 02 Apr 2021 15:48

Tgt Ion:278	Resp:	370595
Ion Ratio	Lower	Upper
278	100	
139	15.6	13.1 19.7
279	23.2	19.9 29.9

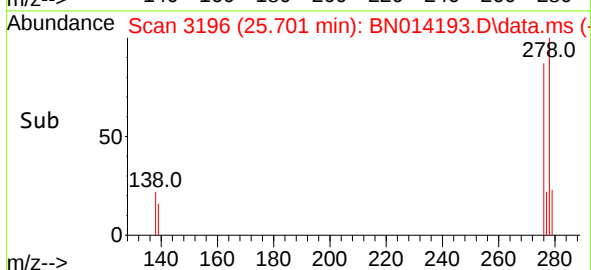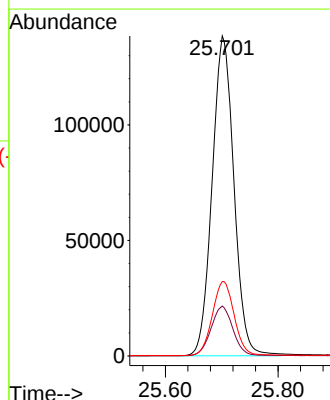

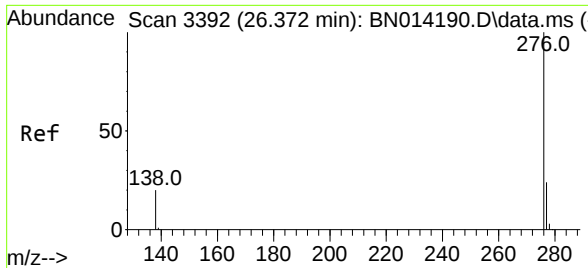

#41
Benzo(g,h,i)perylene
Concen: 5.32 ng
RT: 26.372 min Scan# 3392
Delta R.T. 0.000 min
Lab File: BN014193.D
Acq: 02 Apr 2021 15:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:276 Resp: 380549
Ion Ratio Lower Upper
276 100
277 23.7 19.9 29.9
138 20.2 16.4 24.6

