


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
 Data File : BN014185.D
 Acq On : 02 Apr 2021 10:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 02 18:54:36 2021

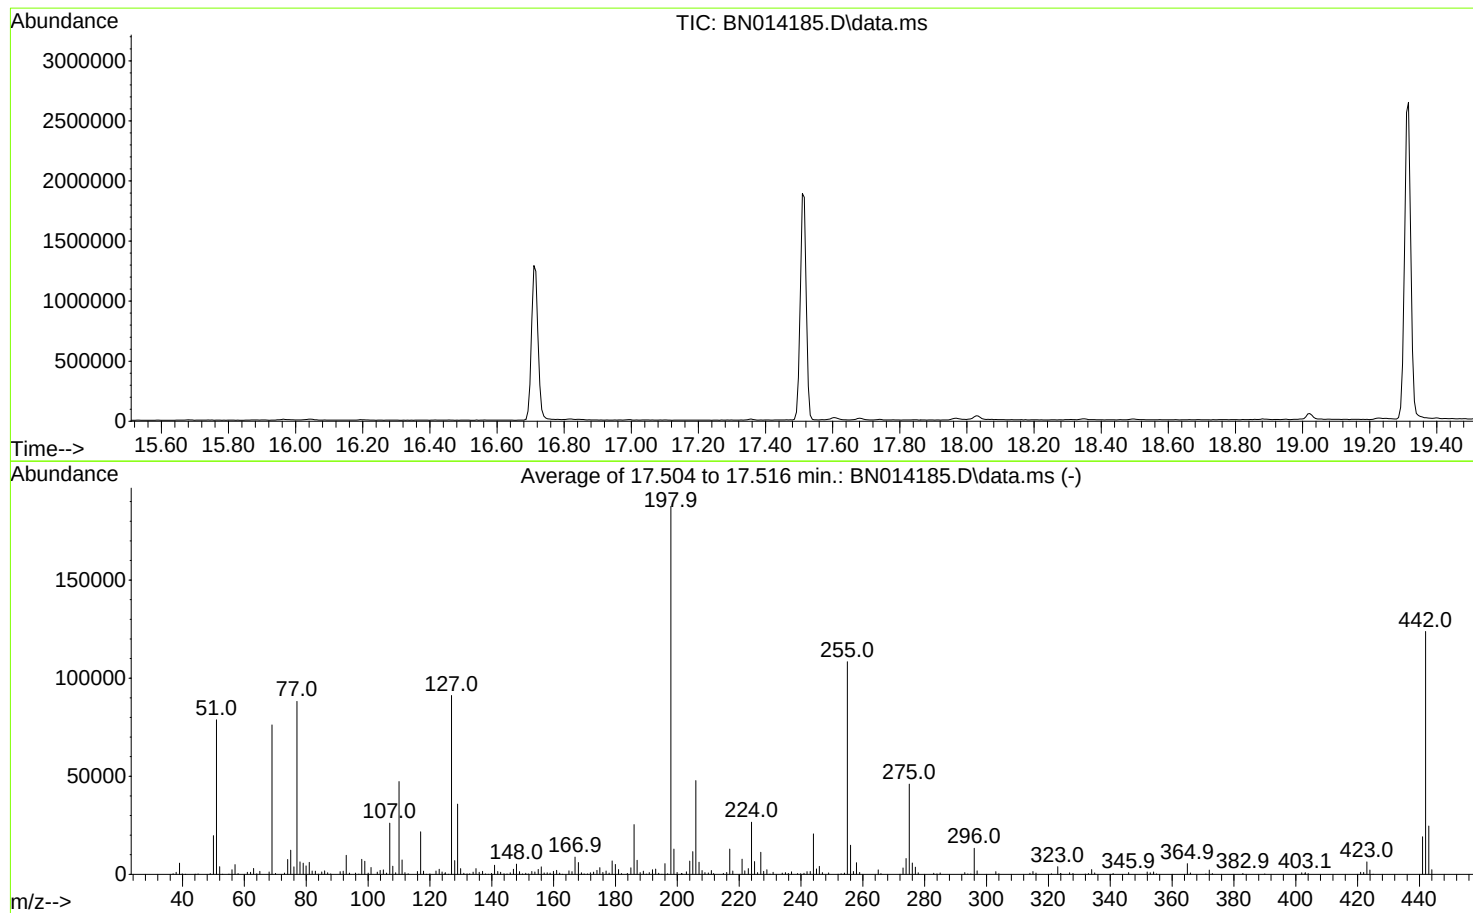

AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	78803	PASS
68	69	0.00	2	1.6	1253	PASS
69	198	0.00	100	40.6	76154	PASS
70	69	0.00	2	0.6	465	PASS
127	198	10	80	48.6	91176	PASS
197	198	0.00	2	0.2	299	PASS
198	198	100	100	100.0	187509	PASS
199	198	5	9	6.9	12860	PASS
275	198	10	60	24.5	45989	PASS
365	198	1	100	2.9	5487	PASS
441	198	0.01	100	10.2	19194	PASS
442	442	50	100	100.0	123795	PASS
443	442	15	24	19.9	24603	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/2/2021	BNA_N	<u>BN014185.D</u>
Compound Name	Response	Retention Time
DDT	701147	20.551
DDD	866	20.116
DDE	654	19.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1520	702667	0.22

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
Data File : BN014185.D
Acq On : 02 Apr 2021 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 03 02:22:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

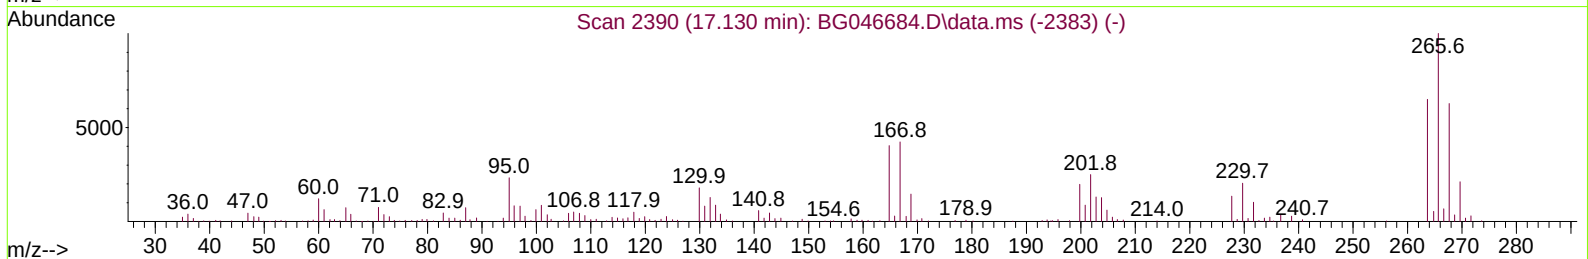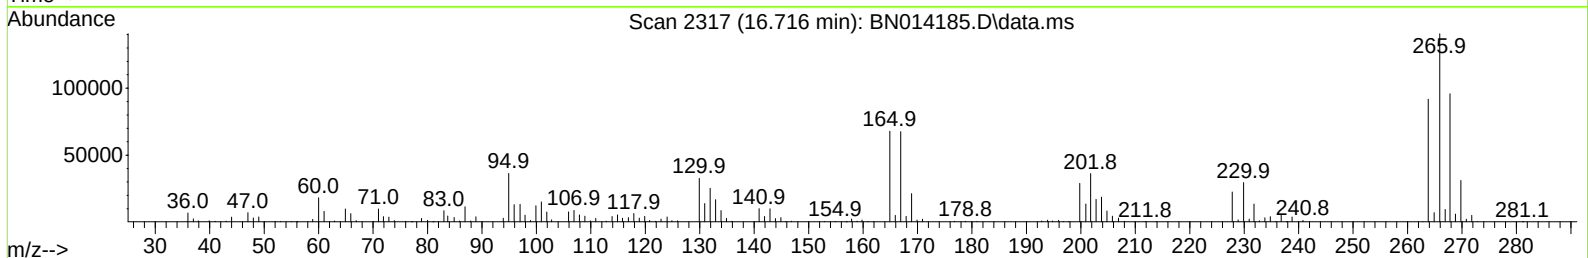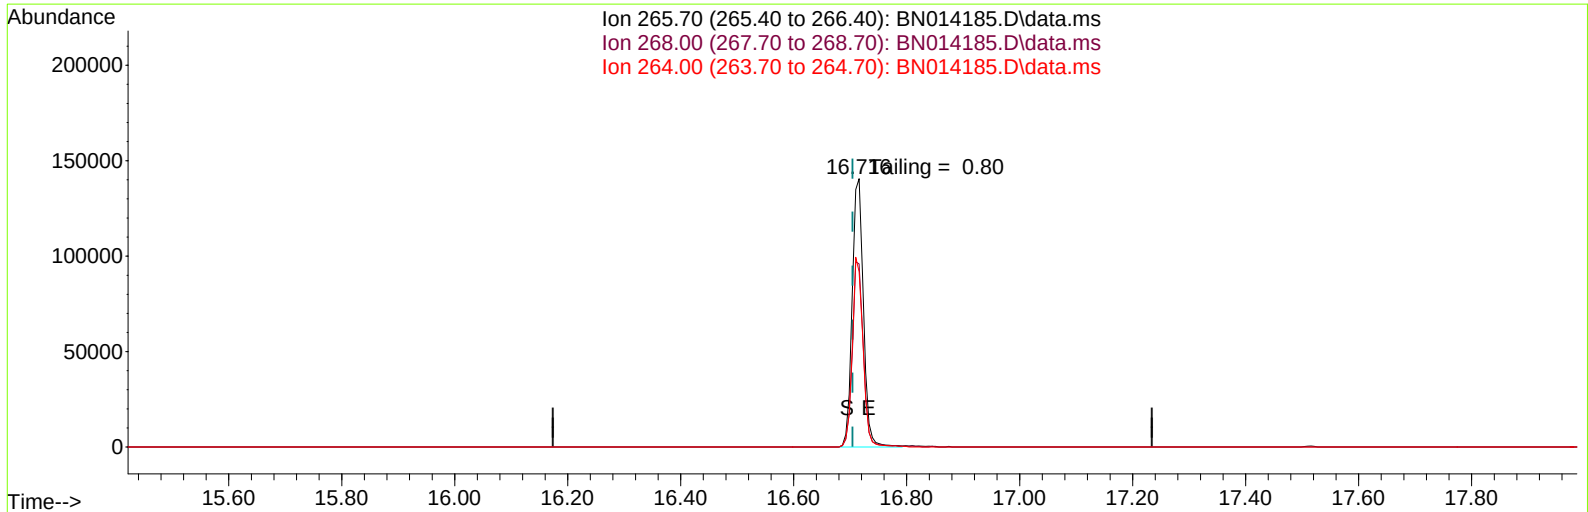

TIC: BN014185.D\data.ms

(70) Pentachlorophenol (C)

16.716min (+ 0.012) 23067.48 ng




response 195329

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.19
264.00	61.60	65.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040221\
Data File : BN014185.D
Acq On : 02 Apr 2021 10:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 03 02:22:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

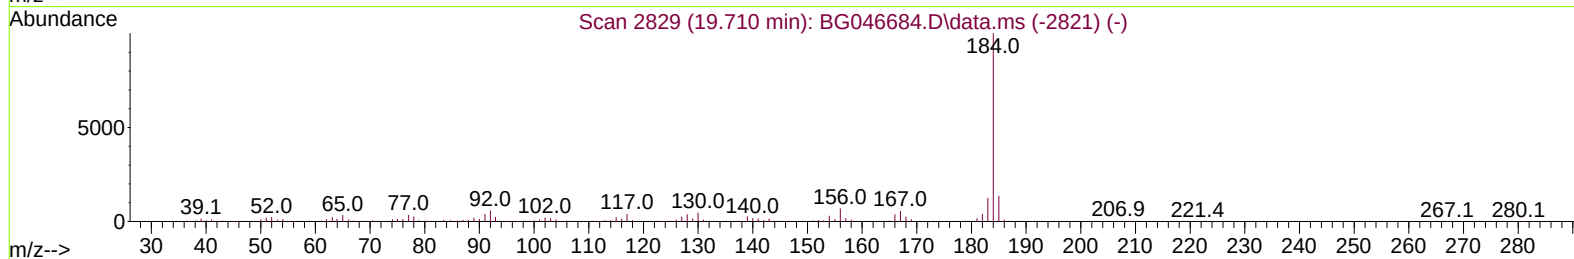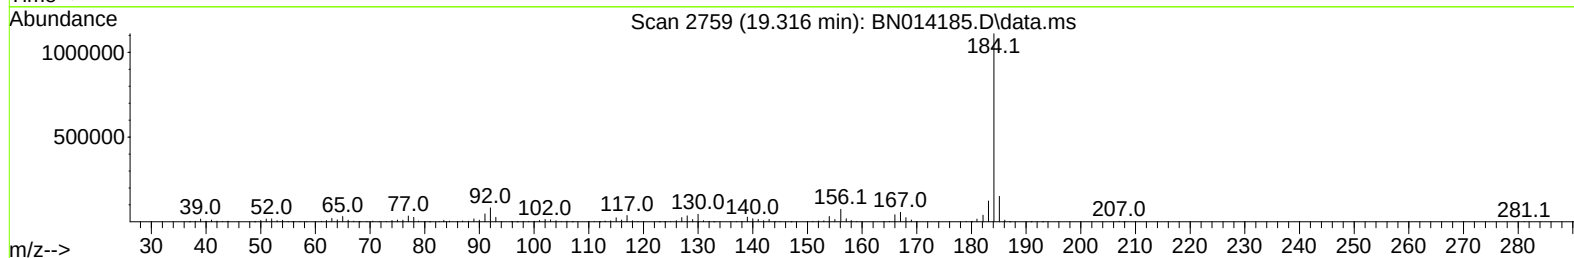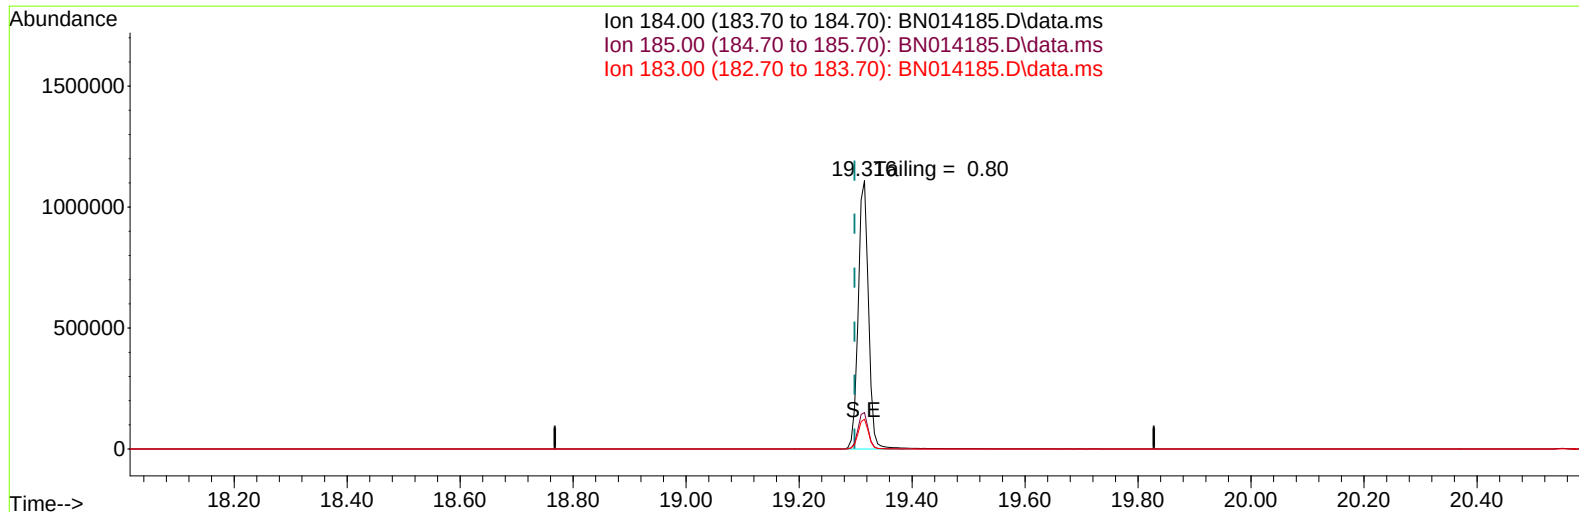

TIC: BN014185.D\data.ms

(77) Benzidine

19.316min (+ 0.018) 0.00 ng

response 1420920

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	11.11
0.00	0.00	0.00