

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
 Data File : BN030583.D
 Acq On : 01 Apr 2024 10:53
 Operator : MA/JU
 Sample : PB159896BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK896

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030583.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	33	36	47	rVB	81198	135128	1.26%	0.127%
2	3.605	101	105	134	rBV	1138857	2089315	19.47%	1.966%
3	3.928	156	160	165	rBV2	15352	23985	0.22%	0.023%
4	6.863	652	659	676	rBV	1517781	2507500	23.37%	2.360%
5	7.040	682	689	701	rBV	1259762	2052887	19.13%	1.932%
6	7.228	714	721	734	rBV	1556748	2521825	23.50%	2.373%
7	7.693	793	800	813	rBV	1425147	2422313	22.57%	2.280%
8	8.399	910	920	935	rBV	1916964	3169299	29.54%	2.983%
9	8.851	989	997	1009	rBV	1543594	2495838	23.26%	2.349%
10	9.569	1108	1119	1129	rBV	1182990	1978636	18.44%	1.862%
11	10.098	1201	1209	1224	rBV	1929760	3231873	30.12%	3.042%
12	10.481	1264	1274	1285	rBV	2223178	3691015	34.40%	3.474%
13	10.616	1290	1297	1311	rBV	1099137	1901878	17.72%	1.790%
14	12.069	1537	1544	1551	rBV	33513	58690	0.55%	0.055%
15	13.234	1738	1742	1747	rBV	21128	32827	0.31%	0.031%
16	13.757	1823	1831	1843	rBV	3353996	4835444	45.06%	4.551%
17	14.034	1870	1878	1889	rBV	3987296	6000731	55.92%	5.648%
18	14.339	1922	1930	1939	rBV	3461612	5048084	47.04%	4.751%
19	14.428	1942	1945	1952	rVB9	6285	11294	0.11%	0.011%
20	14.534	1957	1963	1988	rBV	1712419	2648082	24.68%	2.492%
21	15.333	2092	2099	2112	rBV	5065996	7387408	68.84%	6.953%
22	15.451	2112	2119	2133	rVV	1403538	1988569	18.53%	1.872%
23	15.575	2136	2140	2149	rVB2	24416	44588	0.42%	0.042%
24	16.116	2227	2232	2238	rVB4	18218	26493	0.25%	0.025%
25	16.763	2339	2342	2347	rVB6	9122	12125	0.11%	0.011%
26	16.875	2357	2361	2366	rBV3	10751	17058	0.16%	0.016%
27	17.086	2390	2397	2407	rBV	4247864	6123293	57.06%	5.763%
28	17.186	2407	2414	2432	rVB	5716578	8366343	77.97%	7.874%
29	17.986	2545	2550	2556	rBV8	14834	23351	0.22%	0.022%
30	19.045	2725	2730	2737	rBV2	75229	105915	0.99%	0.100%
31	19.116	2737	2742	2748	rBV	67660	94312	0.88%	0.089%
32	19.274	2766	2769	2775	rBV8	12486	15482	0.14%	0.015%
33	19.433	2793	2796	2798	rBV3	13350	12334	0.11%	0.012%
34	19.486	2798	2805	2821	rBV	7263002	9791534	91.25%	9.215%
35	21.321	3111	3117	3131	rVB	4640045	7024083	65.46%	6.611%
36	24.068	3574	3584	3599	rBV2	4431542	10730517	100.00%	10.099%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030583.D
Acq On : 01 Apr 2024 10:53
Operator : MA/JU
Sample : PB159896BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK896

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	24.274	3609	3619	3640	rVB	2946820	7633976	71.14%	7.185%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 106254025

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030583.D
Acq On : 01 Apr 2024 10:53
Operator : MA/JU
Sample : PB159896BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK896

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

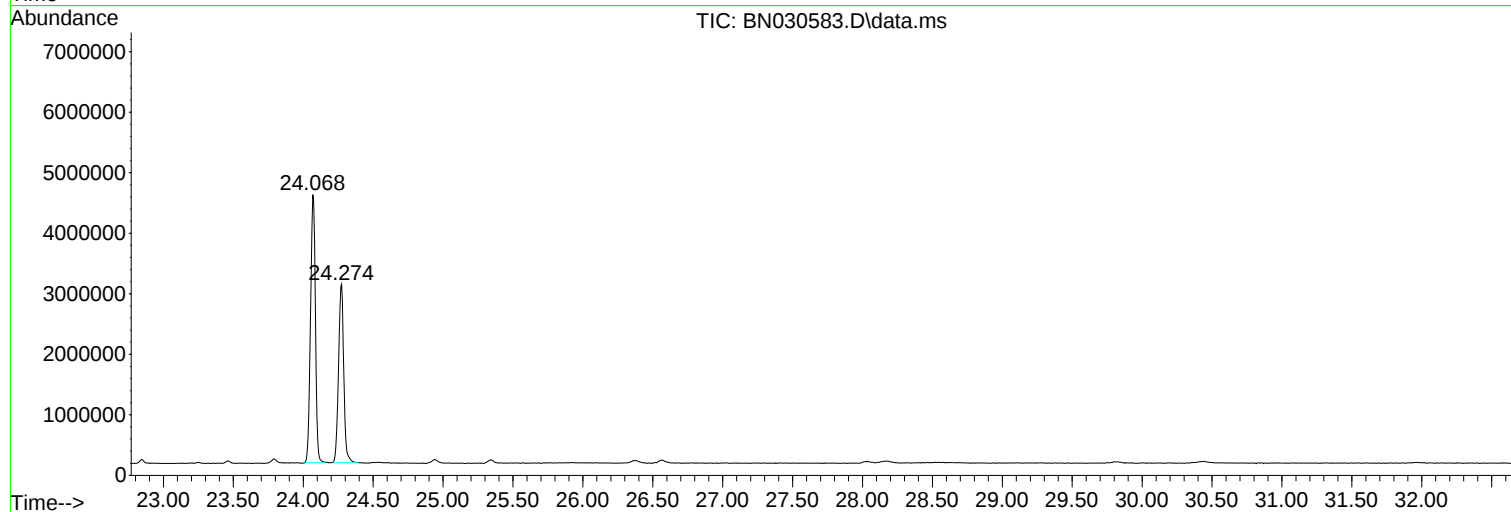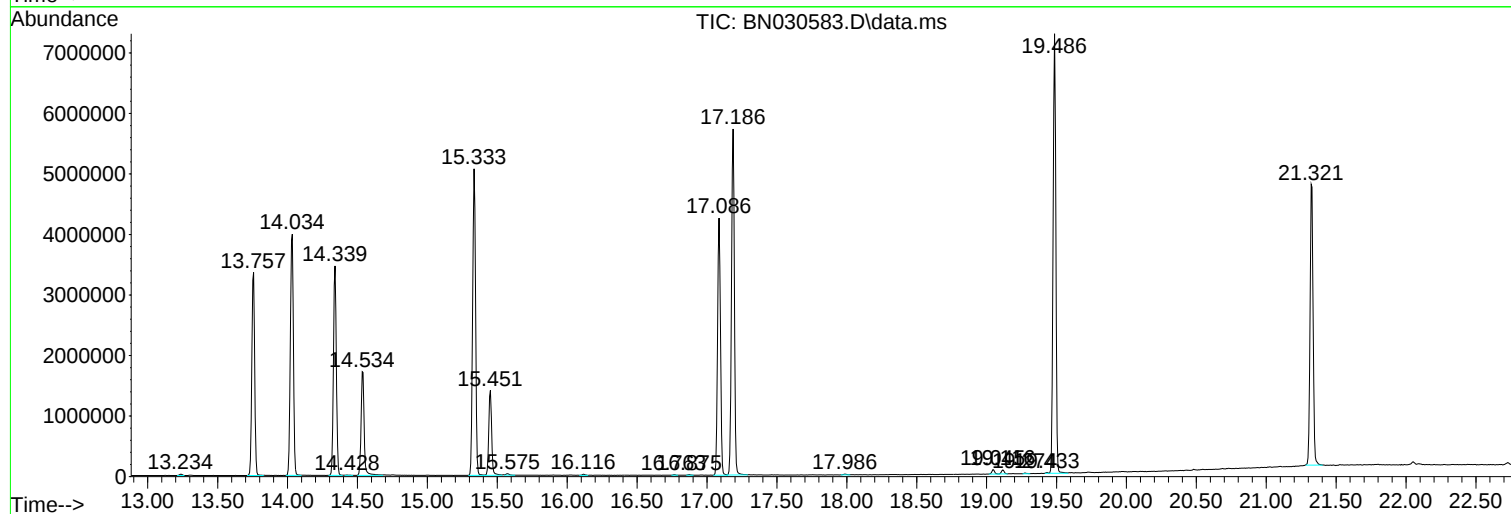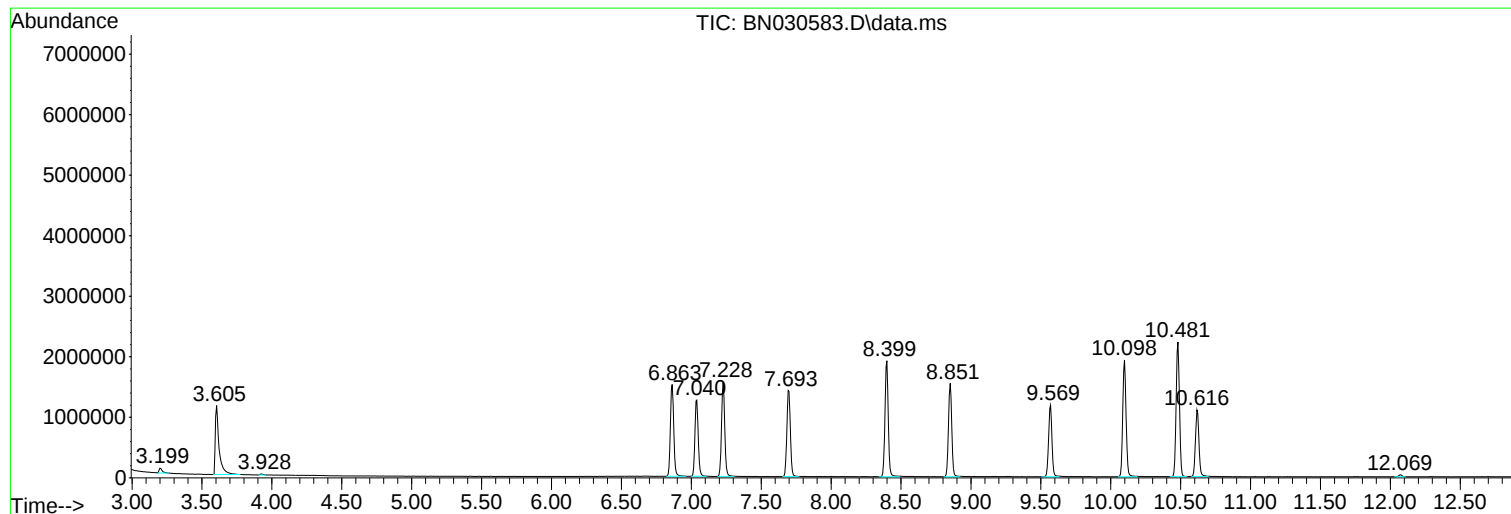

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030583.D
Acq On : 01 Apr 2024 10:53
Operator : MA/JU
Sample : PB159896BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK896

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030583.D
Acq On : 01 Apr 2024 10:53
Operator : MA/JU
Sample : PB159896BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK896

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------