

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
 Data File : BN030587.D
 Acq On : 01 Apr 2024 13:43
 Operator : MA/JU
 Sample : P1925-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 FB(20240327)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030587.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	46	rVB	43301	68575	0.90%	0.108%
2	3.534	90	93	100	rVB	10572	15178	0.20%	0.024%
3	3.605	102	105	127	rVB	163937	285969	3.76%	0.450%
4	3.922	156	159	165	rVB2	9395	13688	0.18%	0.022%
5	6.352	567	572	577	rBV7	6168	12393	0.16%	0.020%
6	6.863	651	659	669	rBV	220667	377206	4.96%	0.594%
7	7.034	682	688	701	rBV	889624	1398566	18.40%	2.201%
8	7.228	713	721	731	rBV	833176	1339602	17.63%	2.109%
9	7.316	733	736	741	rVB5	7297	11078	0.15%	0.017%
10	7.693	792	800	808	rBV	736492	1165690	15.34%	1.835%
11	7.758	808	811	815	rVB3	10090	15299	0.20%	0.024%
12	8.393	912	919	931	rBV	642437	1036153	13.63%	1.631%
13	8.516	934	940	946	rVB	13882	24348	0.32%	0.038%
14	8.852	987	997	1011	rBV	1041982	1749403	23.02%	2.754%
15	9.016	1020	1025	1030	rVB8	6655	9016	0.12%	0.014%
16	9.263	1061	1067	1073	rVB7	6887	15289	0.20%	0.024%
17	9.569	1111	1119	1133	rBV	757003	1274116	16.77%	2.006%
18	10.099	1201	1209	1221	rBV	1221944	1997469	26.29%	3.144%
19	10.340	1244	1250	1255	rVB6	5638	8940	0.12%	0.014%
20	10.481	1266	1274	1286	rBV	1057513	1795860	23.63%	2.827%
21	10.616	1286	1297	1309	rBV	1088218	1830616	24.09%	2.881%
22	11.022	1356	1366	1370	rBV	44497	70387	0.93%	0.111%
23	11.081	1371	1376	1381	rVB	56975	86327	1.14%	0.136%
24	11.257	1401	1406	1410	rBV7	5055	8224	0.11%	0.013%
25	12.069	1534	1544	1550	rBV	24609	44251	0.58%	0.070%
26	13.240	1738	1743	1749	rBV	26277	39402	0.52%	0.062%
27	13.751	1823	1830	1844	rBV	2448189	3408097	44.85%	5.364%
28	14.028	1870	1877	1887	rBV	2878786	4260126	56.06%	6.706%
29	14.340	1923	1930	1937	rBV	1688327	2505435	32.97%	3.944%
30	14.534	1957	1963	1976	rBV	193865	315854	4.16%	0.497%
31	14.757	1997	2001	2006	rVV7	8627	12278	0.16%	0.019%
32	15.334	2092	2099	2112	rBV	3836631	5287240	69.58%	8.322%
33	15.445	2112	2118	2132	rVV	962171	1308122	17.21%	2.059%
34	15.569	2135	2139	2145	rVB2	16495	27252	0.36%	0.043%
35	16.116	2226	2232	2239	rVB4	13588	22479	0.30%	0.035%
36	16.763	2339	2342	2347	rBV4	5346	7961	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030587.D
Acq On : 01 Apr 2024 13:43
Operator : MA/JU
Sample : P1925-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
FB(20240327)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	17.086	2390	2397	2403	rBV	2196577	3064191	40.32%	4.823%
38	17.186	2407	2414	2425	rBV	4152095	6068906	79.86%	9.553%
39	17.481	2460	2464	2472	rVB6	12262	19596	0.26%	0.031%
40	17.763	2509	2512	2519	rVB9	5426	8025	0.11%	0.013%
41	17.986	2545	2550	2556	rBV3	57462	84655	1.11%	0.133%
42	18.428	2620	2625	2629	rVB2	27222	32765	0.43%	0.052%
43	19.045	2726	2730	2735	rBV2	57301	76873	1.01%	0.121%
44	19.116	2738	2742	2745	rBV2	52571	72782	0.96%	0.115%
45	19.157	2745	2749	2754	rVB2	71717	86129	1.13%	0.136%
46	19.275	2766	2769	2776	rBV4	41314	56048	0.74%	0.088%
47	19.486	2798	2805	2812	rBV	5322657	7382666	97.15%	11.621%
48	21.322	3111	3117	3127	rBV2	2358765	3478740	45.78%	5.476%
49	24.068	3574	3584	3603	rVB2	3205880	7599263	100.00%	11.962%
50	24.268	3609	3618	3637	rVB	1437986	3652123	48.06%	5.749%




Sum of corrected areas: 63530651

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030587.D
Acq On : 01 Apr 2024 13:43
Operator : MA/JU
Sample : P1925-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
FB(20240327)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

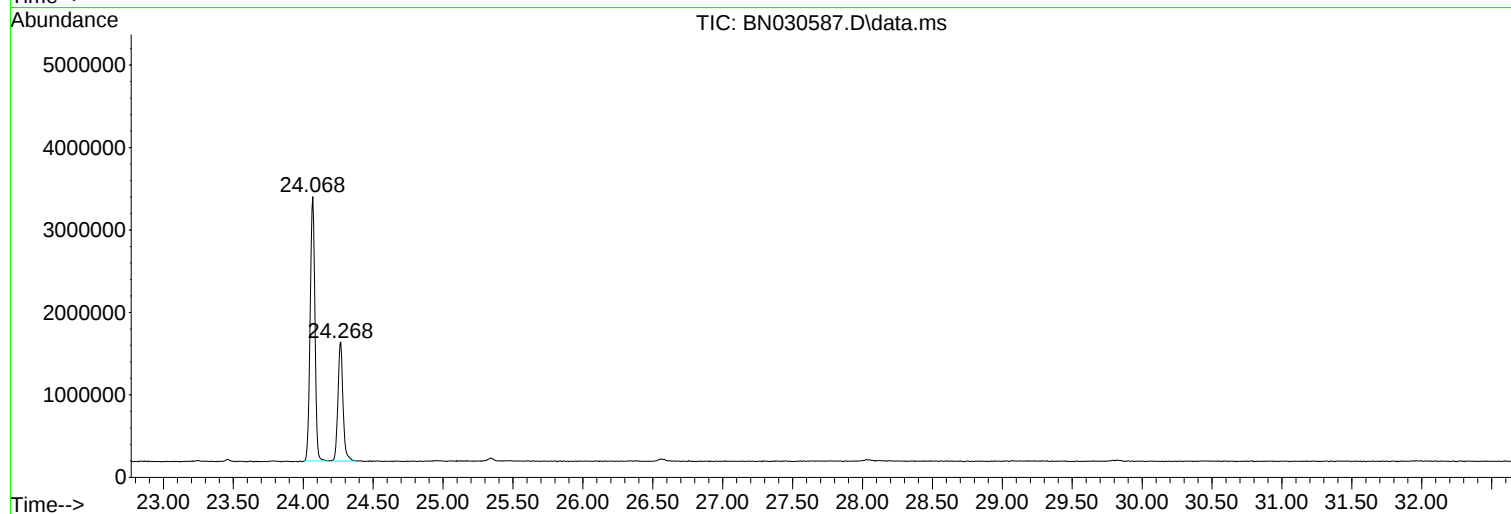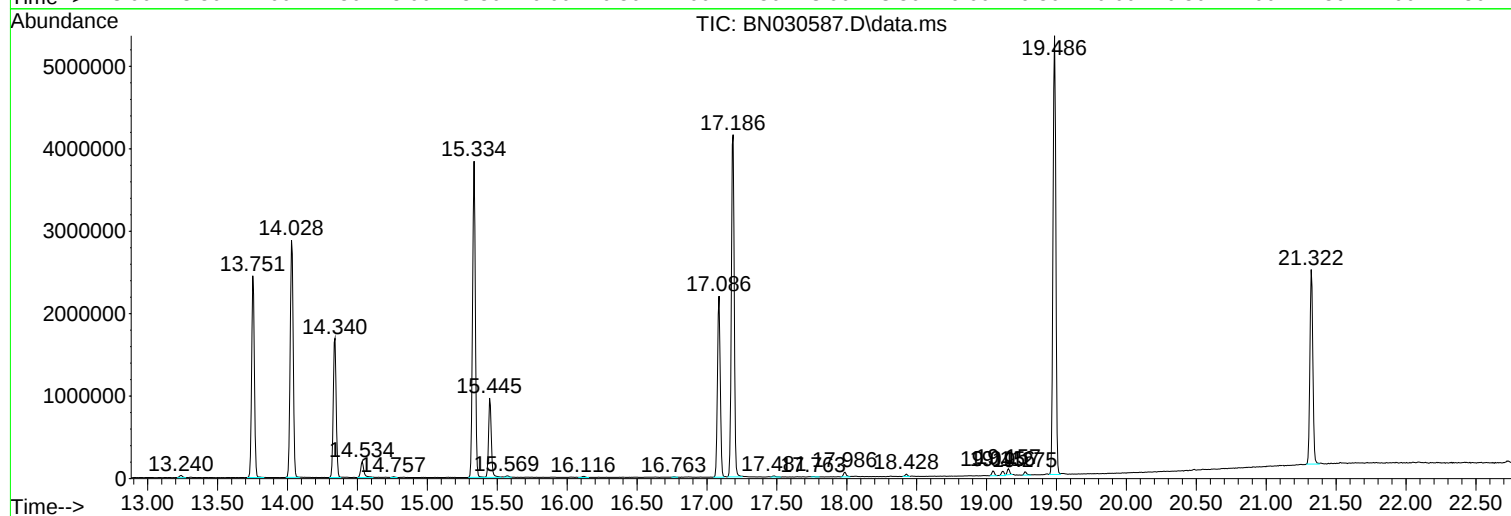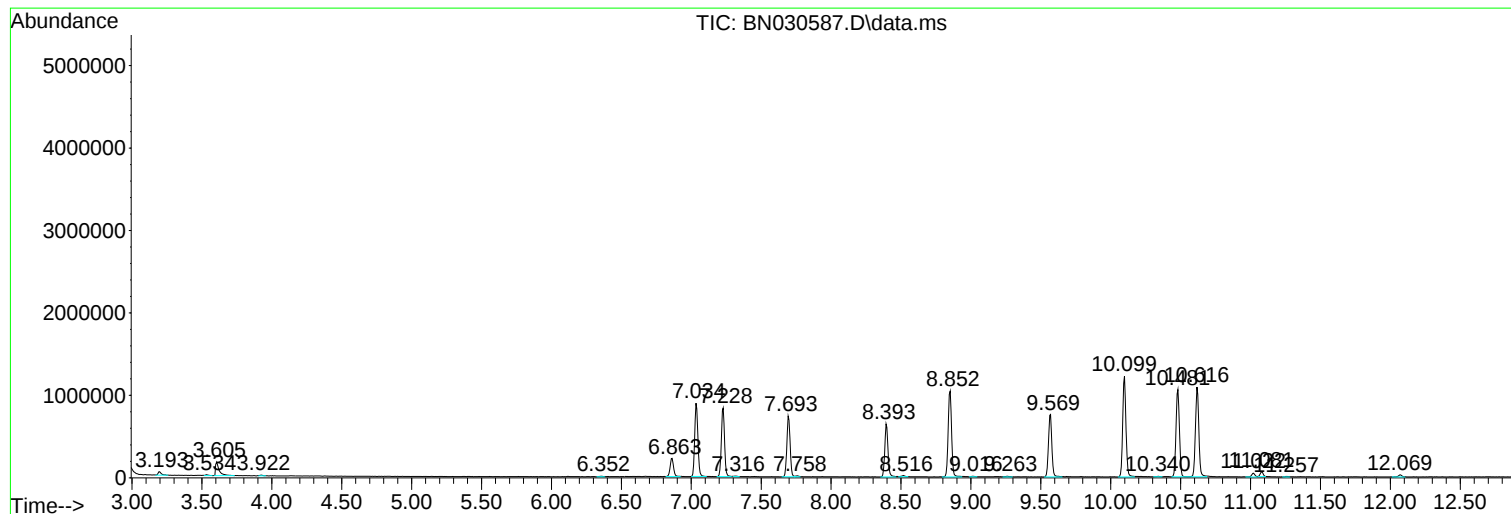

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030587.D
Acq On : 01 Apr 2024 13:43
Operator : MA/JU
Sample : P1925-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
FB(20240327)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030587.D
Acq On : 01 Apr 2024 13:43
Operator : MA/JU
Sample : P1925-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
FB(20240327)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc