

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
 Data File : BN030592.D
 Acq On : 01 Apr 2024 17:00
 Operator : MA/JU
 Sample : PB159926BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK926

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	47	rVB	83177	118758	1.53%	0.148%
2	3.599	101	104	124	rBV	1179200	1771665	22.81%	2.205%
3	3.922	156	159	165	rVB3	13459	22900	0.29%	0.028%
4	6.864	652	659	669	rBV	1274151	1978621	25.47%	2.462%
5	7.034	682	688	700	rBV	1012231	1621694	20.88%	2.018%
6	7.228	713	721	732	rBV	1264922	1998371	25.73%	2.487%
7	7.699	793	801	813	rBV	1053323	1724687	22.20%	2.146%
8	8.399	912	920	930	rBV	1584841	2530036	32.57%	3.148%
9	8.852	989	997	1011	rBV	1240315	1999019	25.74%	2.488%
10	9.569	1110	1119	1129	rBV	972482	1575022	20.28%	1.960%
11	10.099	1202	1209	1224	rBV	1609117	2616132	33.68%	3.255%
12	10.481	1266	1274	1286	rBV	1608493	2655984	34.19%	3.305%
13	10.622	1289	1298	1313	rBV	1328765	2272731	29.26%	2.828%
14	12.075	1539	1545	1553	rBV2	26309	47799	0.62%	0.059%
15	13.240	1738	1743	1748	rBV2	16600	27069	0.35%	0.034%
16	13.751	1824	1830	1839	rBV	2752246	3959915	50.98%	4.928%
17	14.028	1871	1877	1892	rBV	3298477	4951489	63.75%	6.161%
18	14.340	1923	1930	1941	rBV	2501505	3695494	47.58%	4.599%
19	14.534	1956	1963	1980	rBV	1400001	2086162	26.86%	2.596%
20	15.334	2092	2099	2110	rBV	4258484	6075866	78.22%	7.561%
21	15.451	2112	2119	2135	rVV	1087640	1512666	19.47%	1.882%
22	15.575	2135	2140	2145	rVB2	20389	31584	0.41%	0.039%
23	15.904	2190	2196	2201	rBV2	4043	8971	0.12%	0.011%
24	16.116	2229	2232	2239	rVB5	15512	21957	0.28%	0.027%
25	16.769	2338	2343	2348	rBV7	6897	10514	0.14%	0.013%
26	16.869	2356	2360	2365	rVB4	5752	8863	0.11%	0.011%
27	17.086	2390	2397	2407	rBV	3223127	4487444	57.77%	5.584%
28	17.186	2407	2414	2430	rVV	4714211	6623910	85.28%	8.243%
29	17.986	2546	2550	2556	rBV7	8421	14405	0.19%	0.018%
30	19.045	2726	2730	2736	rBV2	58703	80954	1.04%	0.101%
31	19.116	2738	2742	2747	rVV	52027	67259	0.87%	0.084%
32	19.428	2793	2795	2798	rBV3	11895	13389	0.17%	0.017%
33	19.486	2799	2805	2813	rVV	5680058	7767287	100.00%	9.665%
34	19.728	2843	2846	2853	rVB5	25530	55950	0.72%	0.070%
35	21.322	3111	3117	3133	rVB	3417819	4865316	62.64%	6.054%
36	24.063	3574	3583	3597	rVB2	2779151	6717964	86.49%	8.360%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030592.D
Acq On : 01 Apr 2024 17:00
Operator : MA/JU
Sample : PB159926BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK926

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	24.268	3609	3618	3634	rVB	1767710	4344262	55.93%	5.406%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 80362109

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030592.D
Acq On : 01 Apr 2024 17:00
Operator : MA/JU
Sample : PB159926BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK926

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

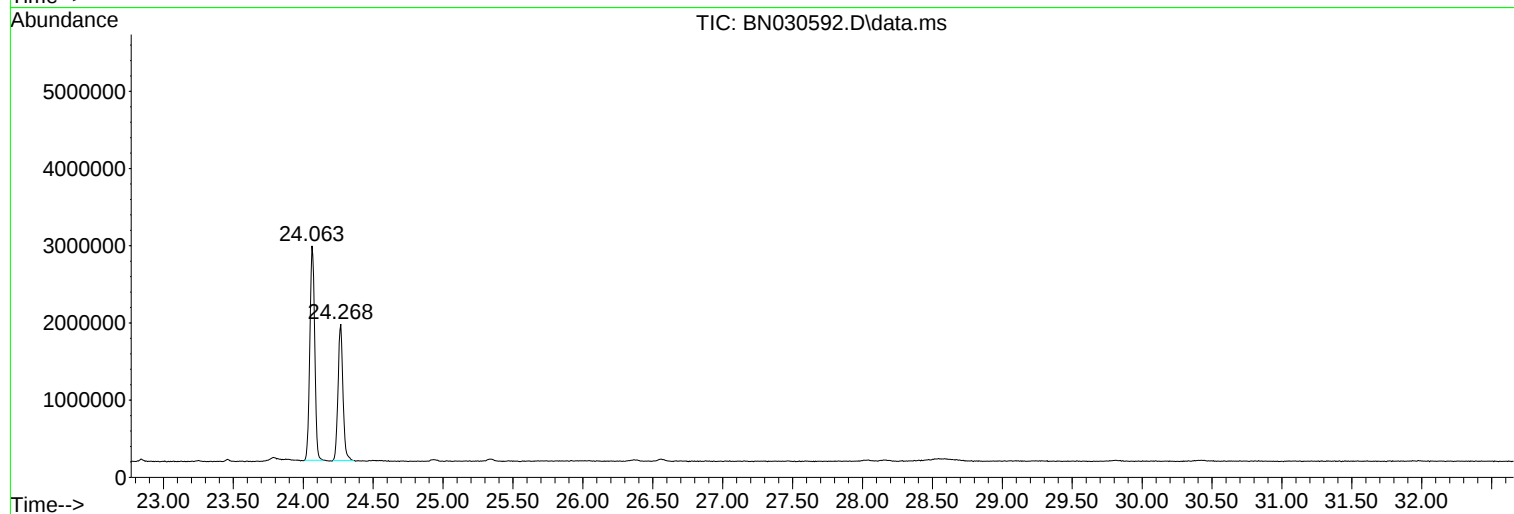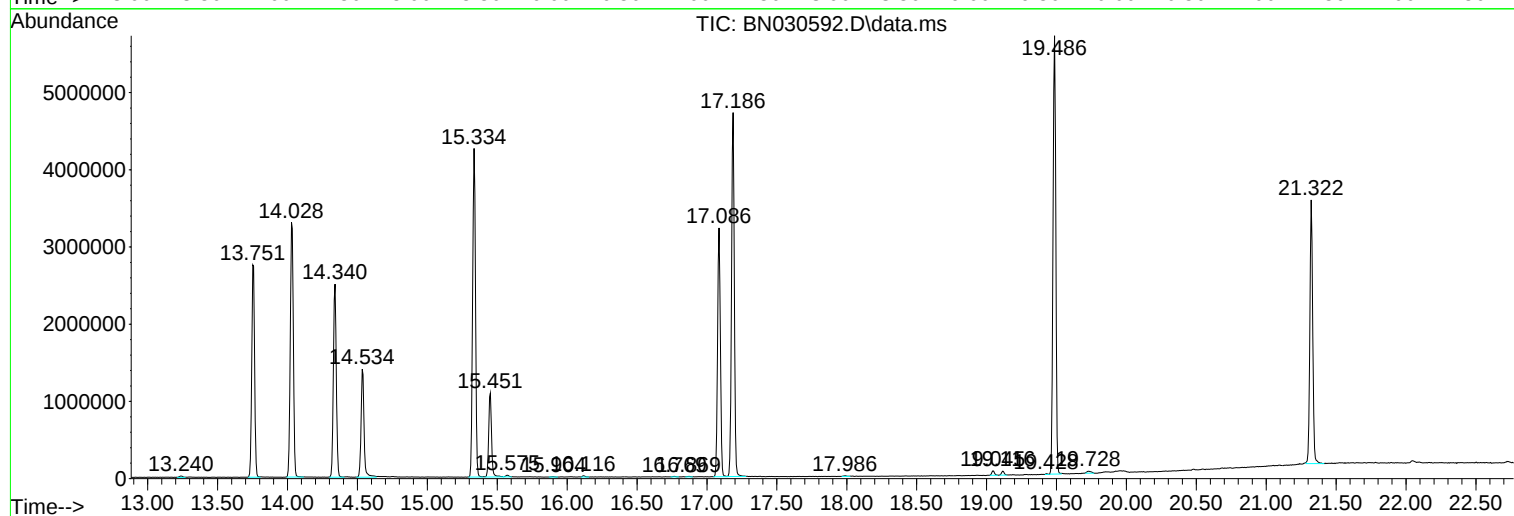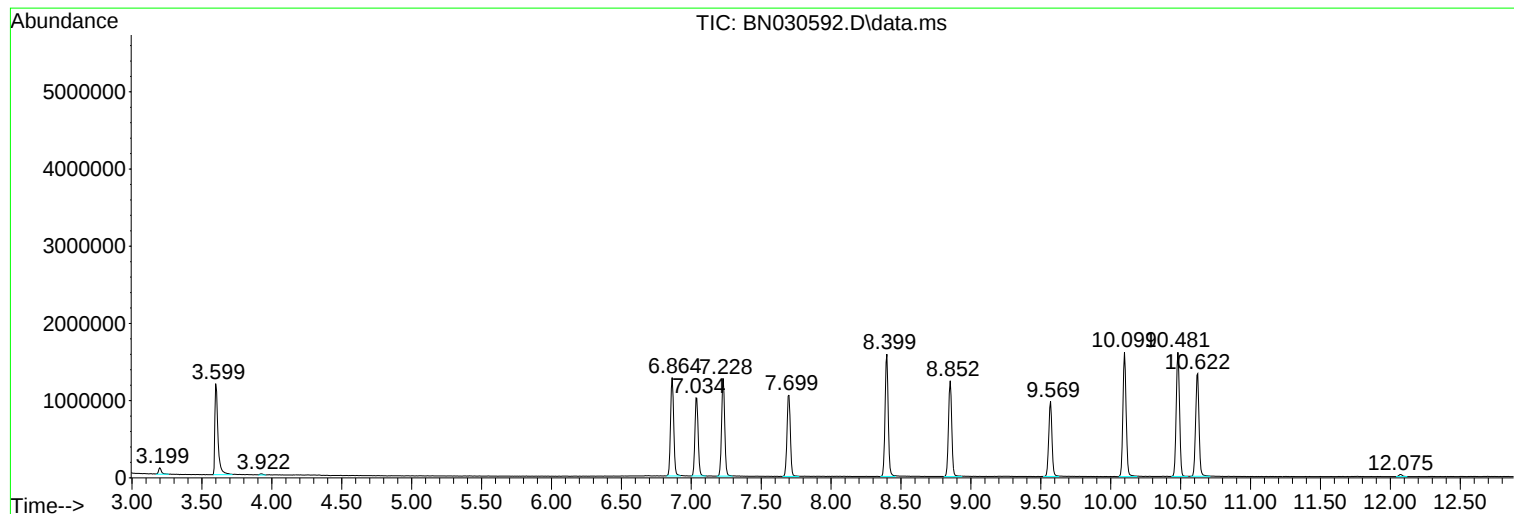

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030592.D
Acq On : 01 Apr 2024 17:00
Operator : MA/JU
Sample : PB159926BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK926

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030592.D
Acq On : 01 Apr 2024 17:00
Operator : MA/JU
Sample : PB159926BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK926

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc