

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
 Data File : BN030593.D
 Acq On : 01 Apr 2024 17:39
 Operator : MA/JU
 Sample : P1929-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	47	rVB	50779	76258	0.92%	0.112%
2	3.605	102	105	120	rBV	236835	397631	4.78%	0.586%
3	3.922	156	159	165	rVB3	9977	14621	0.18%	0.022%
4	6.863	651	659	672	rVB	226472	373725	4.49%	0.551%
5	7.034	682	688	702	rBV	899294	1424853	17.13%	2.099%
6	7.228	714	721	732	rBV	848361	1326803	15.95%	1.955%
7	7.693	793	800	810	rBV	731314	1195383	14.37%	1.761%
8	8.393	912	919	934	rBV	668875	1117115	13.43%	1.646%
9	8.852	989	997	1009	rBV	1090589	1757700	21.13%	2.590%
10	8.957	1010	1015	1020	rVV3	15421	28677	0.34%	0.042%
11	9.263	1060	1067	1073	rVB3	14621	26080	0.31%	0.038%
12	9.428	1090	1095	1101	rBV6	6708	12446	0.15%	0.018%
13	9.569	1111	1119	1132	rBV	785088	1302714	15.66%	1.919%
14	10.099	1201	1209	1223	rBV	1254170	2062485	24.79%	3.039%
15	10.269	1234	1238	1247	rVB8	6141	10636	0.13%	0.016%
16	10.481	1267	1274	1284	rBV	1095743	1828874	21.98%	2.694%
17	10.616	1290	1297	1319	rVB	1255996	2172478	26.11%	3.201%
18	11.228	1394	1401	1404	rBV4	8552	15864	0.19%	0.023%
19	12.069	1540	1544	1551	rVB2	24352	38023	0.46%	0.056%
20	12.816	1666	1671	1677	rVB7	6978	11669	0.14%	0.017%
21	13.169	1726	1731	1737	rVB6	7802	11871	0.14%	0.017%
22	13.240	1737	1743	1748	rBV3	13781	23403	0.28%	0.034%
23	13.751	1824	1830	1837	rBV	2630905	3803444	45.72%	5.603%
24	14.028	1867	1877	1889	rBV	3063693	4595084	55.23%	6.770%
25	14.245	1911	1914	1918	rVB5	5968	8837	0.11%	0.013%
26	14.340	1923	1930	1940	rVV	1708680	2529558	30.40%	3.727%
27	14.534	1957	1963	1975	rBV2	226851	385115	4.63%	0.567%
28	14.757	1996	2001	2007	rVB10	8782	13515	0.16%	0.020%
29	15.145	2063	2067	2074	rBV2	17950	29109	0.35%	0.043%
30	15.334	2092	2099	2107	rBV	4086433	5961737	71.66%	8.783%
31	15.445	2112	2118	2133	rVV	1015981	1457265	17.52%	2.147%
32	15.575	2136	2140	2150	rVB3	20757	40962	0.49%	0.060%
33	16.116	2227	2232	2237	rVB4	15927	22729	0.27%	0.033%
34	16.763	2339	2342	2346	rBV6	7117	9044	0.11%	0.013%
35	17.022	2381	2386	2389	rBV5	12803	17327	0.21%	0.026%
36	17.086	2390	2397	2407	rBV	2200394	3066389	36.86%	4.518%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
 Data File : BN030593.D
 Acq On : 01 Apr 2024 17:39
 Operator : MA/JU
 Sample : P1929-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	17.186	2407	2414	2425	rBV	5029544	6922914	83.21%	10.199%
38	17.475	2457	2463	2470	rBV	8278	20454	0.25%	0.030%
39	17.986	2546	2550	2556	rBV2	54418	76521	0.92%	0.113%
40	18.063	2561	2563	2567	rVB2	10813	12245	0.15%	0.018%
41	18.428	2621	2625	2629	rBV5	13436	17997	0.22%	0.027%
42	18.851	2694	2697	2701	rBV6	15563	22650	0.27%	0.033%
43	19.045	2726	2730	2735	rBV	64314	86494	1.04%	0.127%
44	19.116	2738	2742	2746	rBV2	57306	76615	0.92%	0.113%
45	19.275	2765	2769	2775	rBV5	27808	40020	0.48%	0.059%
46	19.433	2793	2796	2798	rBV3	9536	9697	0.12%	0.014%
47	19.486	2798	2805	2819	rVV	5923016	8208020	98.66%	12.092%
48	19.722	2843	2845	2850	rVB3	14133	14492	0.17%	0.021%
49	21.016	3062	3065	3070	rVB4	46706	65795	0.79%	0.097%
50	21.321	3111	3117	3128	rBV2	2262645	3432944	41.26%	5.058%
51	24.068	3574	3584	3603	rVB	3519881	8319759	100.00%	12.257%
52	24.263	3609	3617	3632	rVB2	1363056	3381827	40.65%	4.982%




Sum of corrected areas: 67877868

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030593.D
Acq On : 01 Apr 2024 17:39
Operator : MA/JU
Sample : P1929-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAM0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

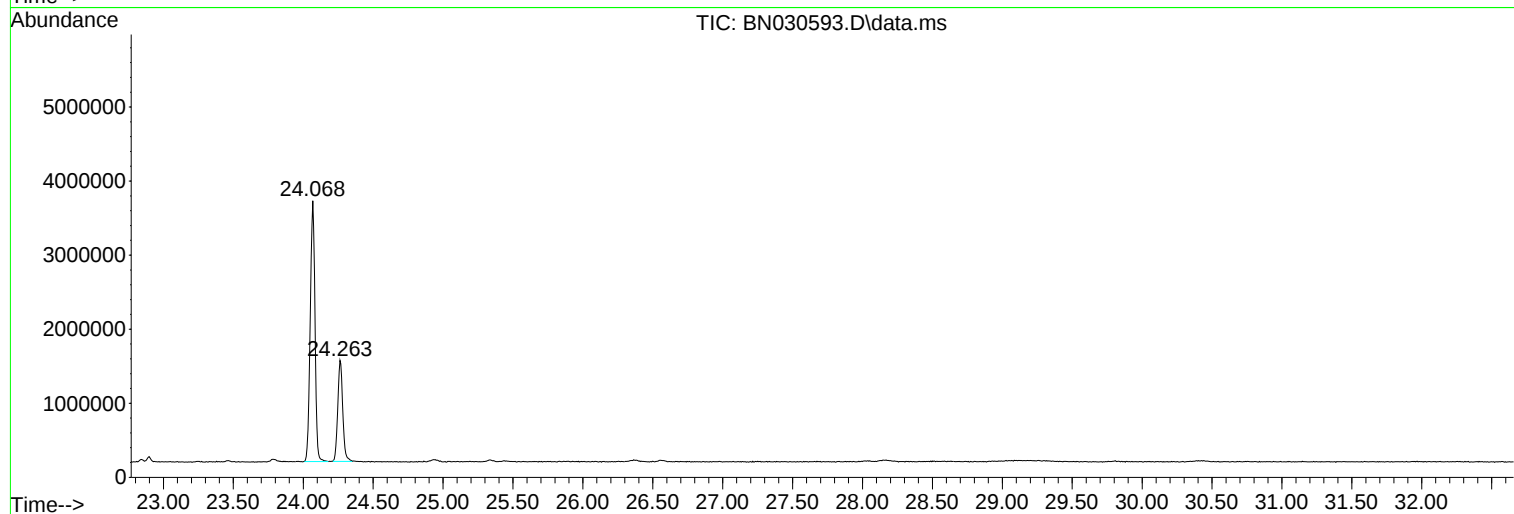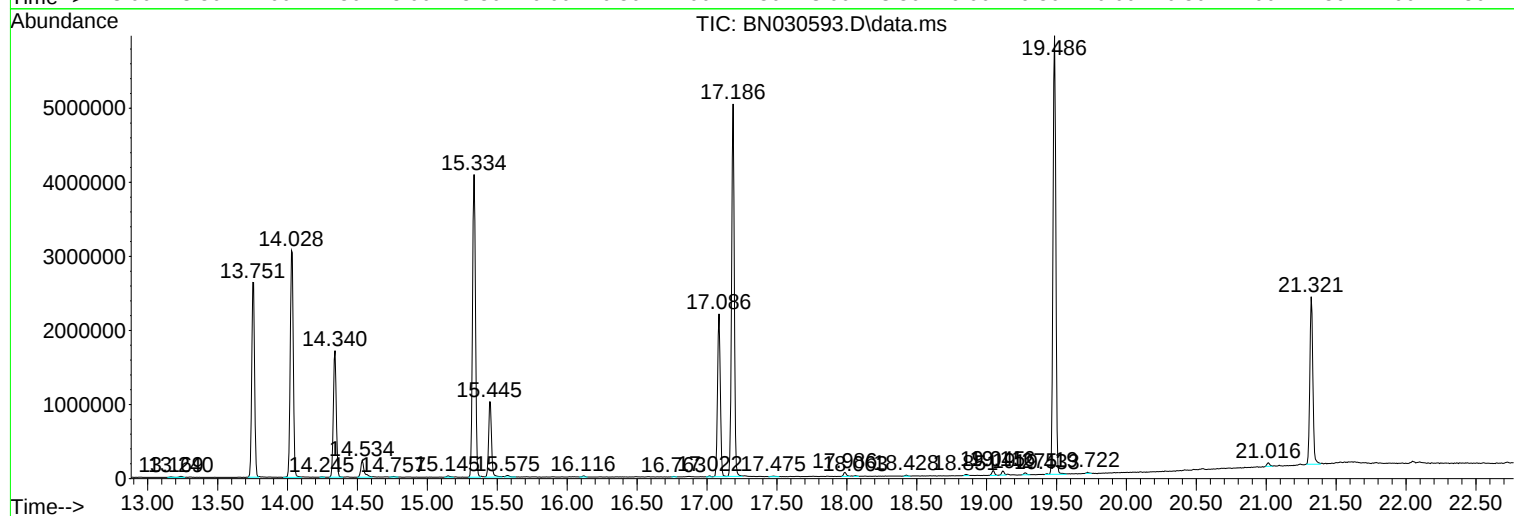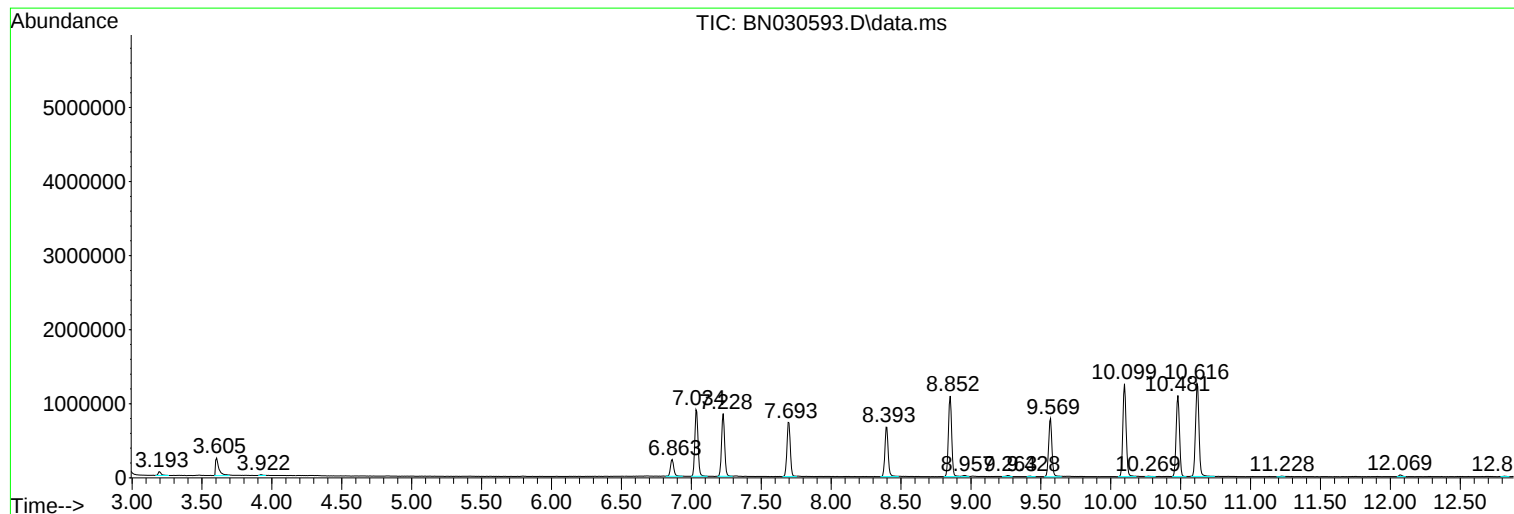

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030593.D
Acq On : 01 Apr 2024 17:39
Operator : MA/JU
Sample : P1929-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AM0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040224\
Data File : BN030593.D
Acq On : 01 Apr 2024 17:39
Operator : MA/JU
Sample : P1929-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AM0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------