
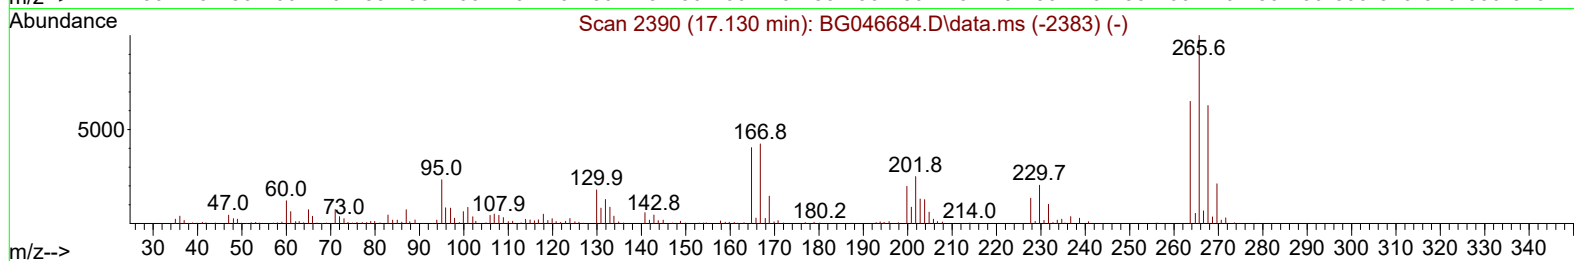
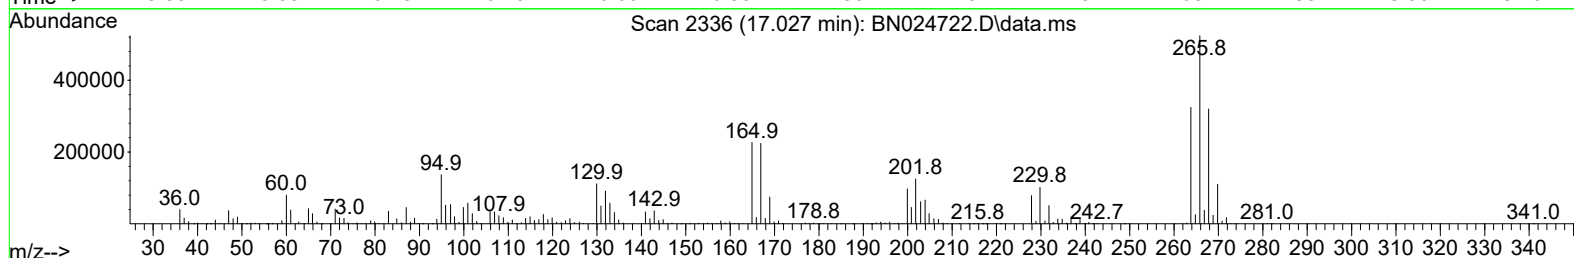


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040323\
Data File : BN024722.D
Acq On : 03 Apr 2023 09:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 06:27:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 04 06:27:46 2023
Response via : Initial Calibration

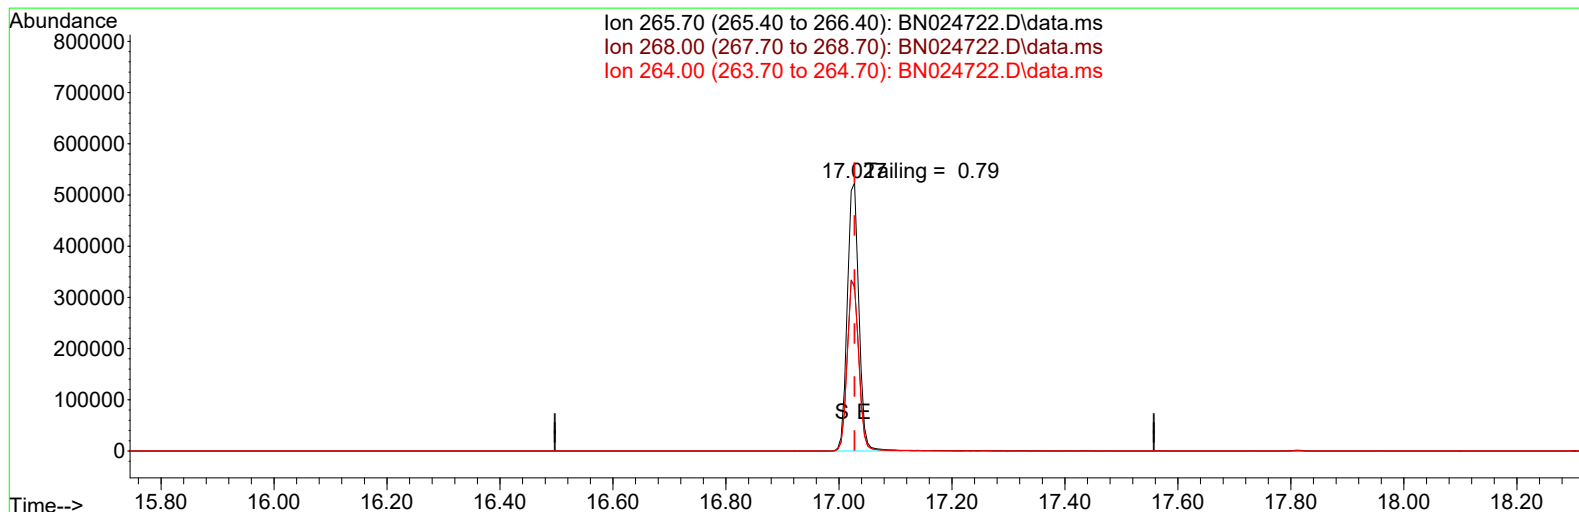

TIC: BN024722.D\data.ms

(70) Pentachlorophenol (C)




17.027min (0.000) 20848.03 ng

response 749498

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.07
264.00	61.60	61.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040323\
 Data File : BN024722.D
 Acq On : 03 Apr 2023 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 06:27:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 04 06:27:46 2023
 Response via : Initial Calibration

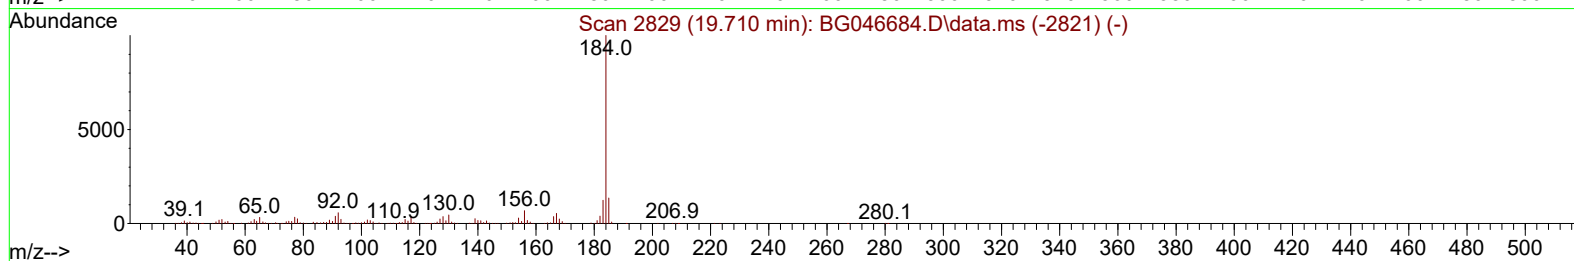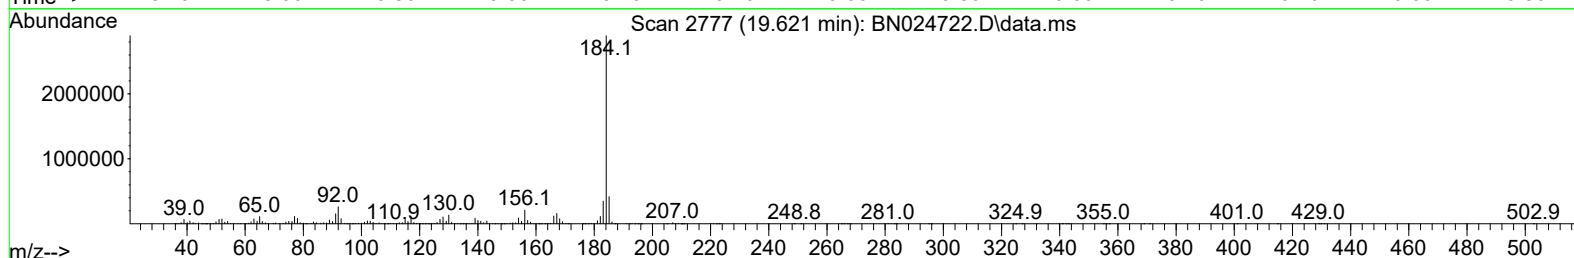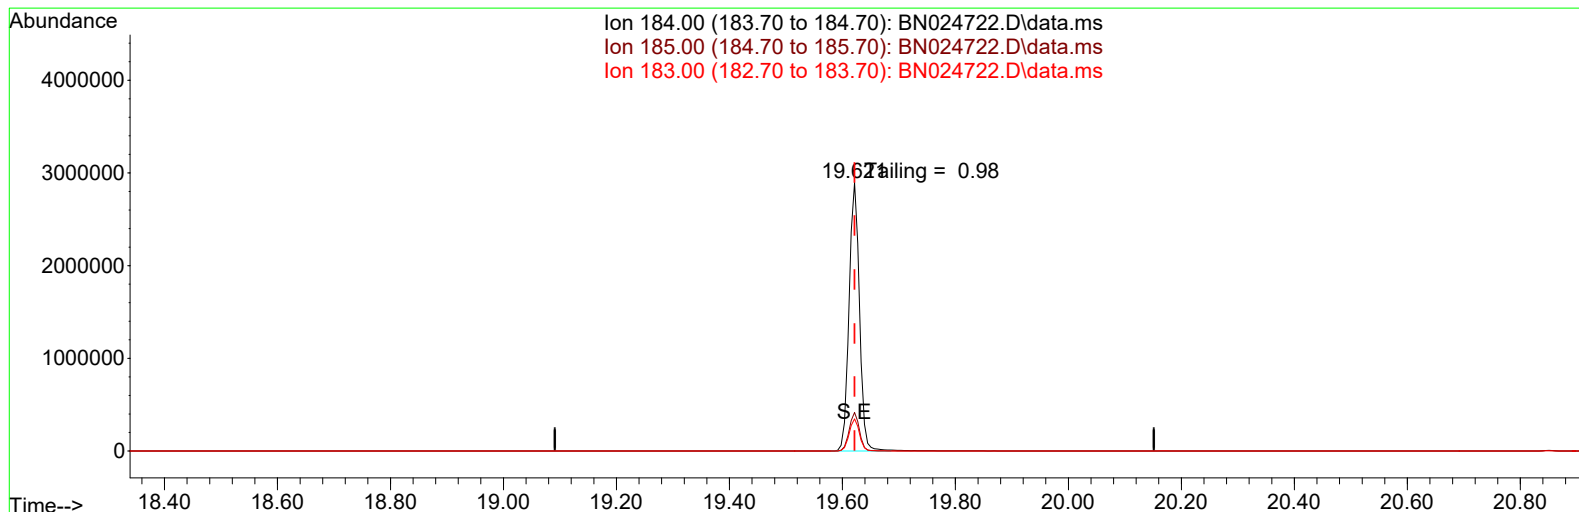

TIC: BN024722.D\data.ms

(77) Benzidine**19.621min (0.000) 861552.51 ng****response 3691517**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.36
183.00	13.20	12.03
0.00	0.00	0.00