
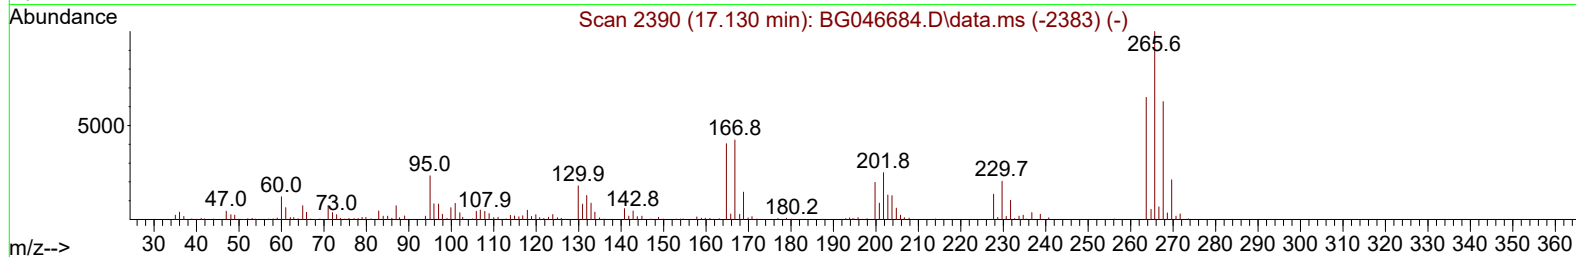
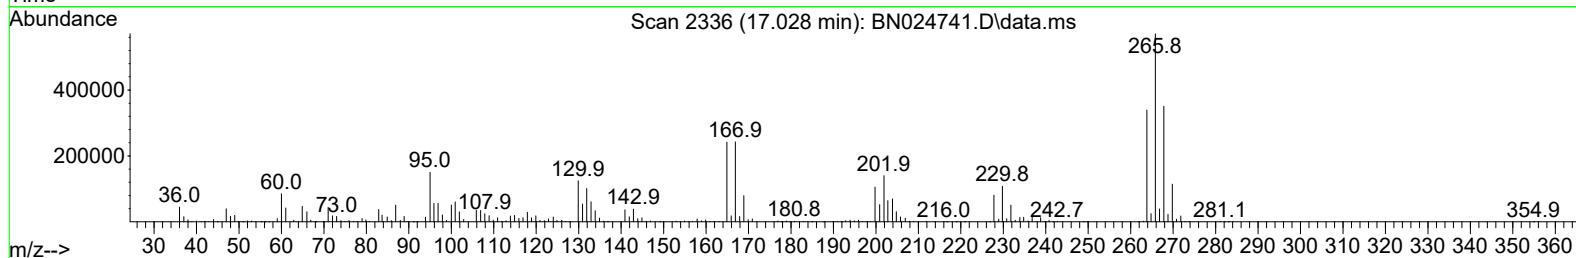


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040323\
Data File : BN024741.D
Acq On : 03 Apr 2023 22:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 06:32:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 04 06:27:46 2023
Response via : Initial Calibration

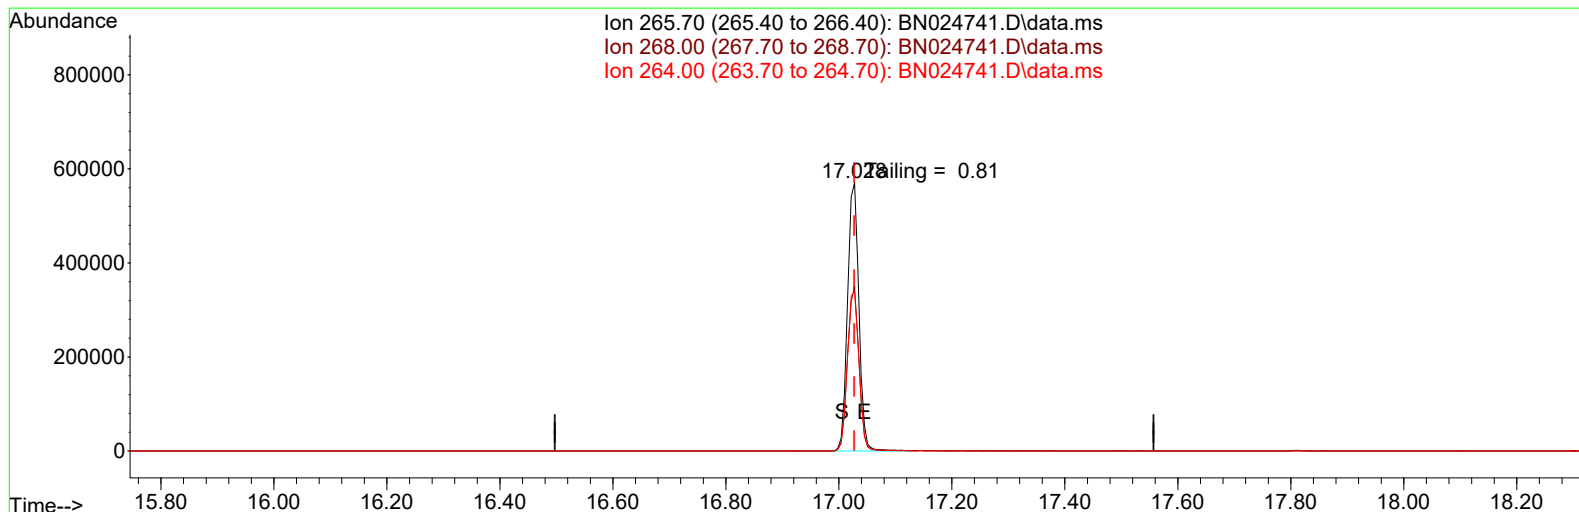

TIC: BN024741.D\data.ms

(70) Pentachlorophenol (C)




17.028min (+ 0.000) 23290.76 ng

response 798566

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.44
264.00	61.60	59.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040323\
Data File : BN024741.D
Acq On : 03 Apr 2023 22:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 06:32:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 04 06:27:46 2023
Response via : Initial Calibration

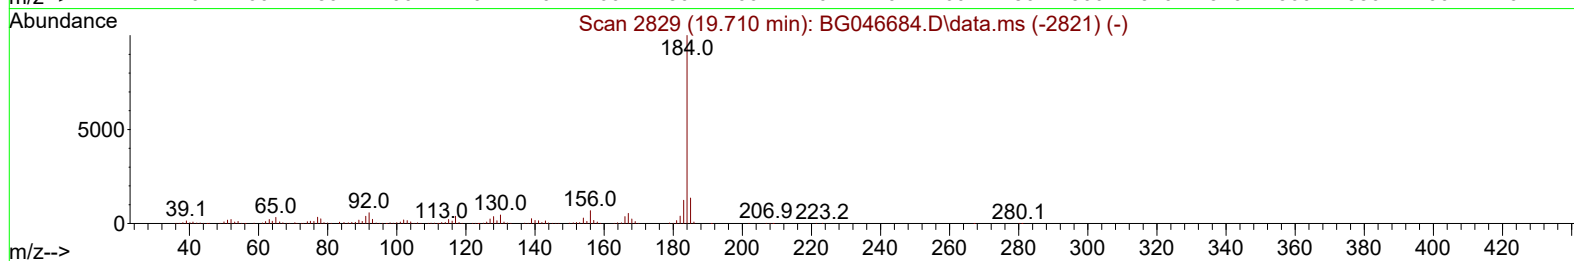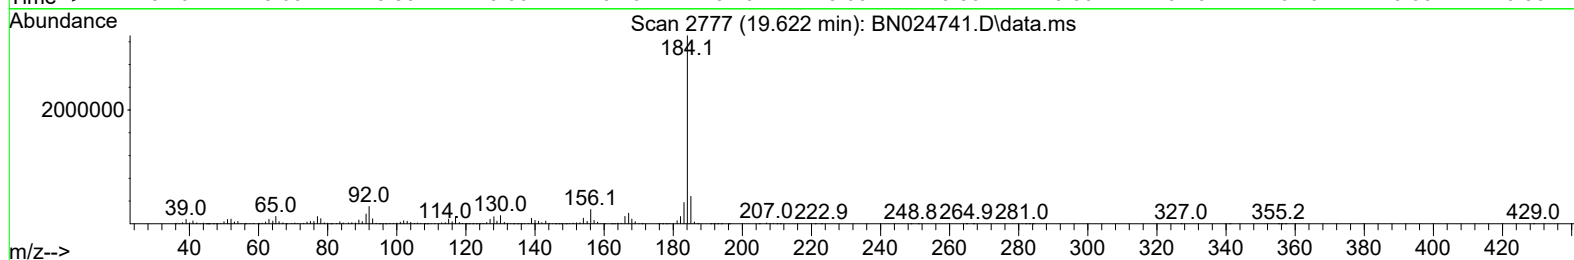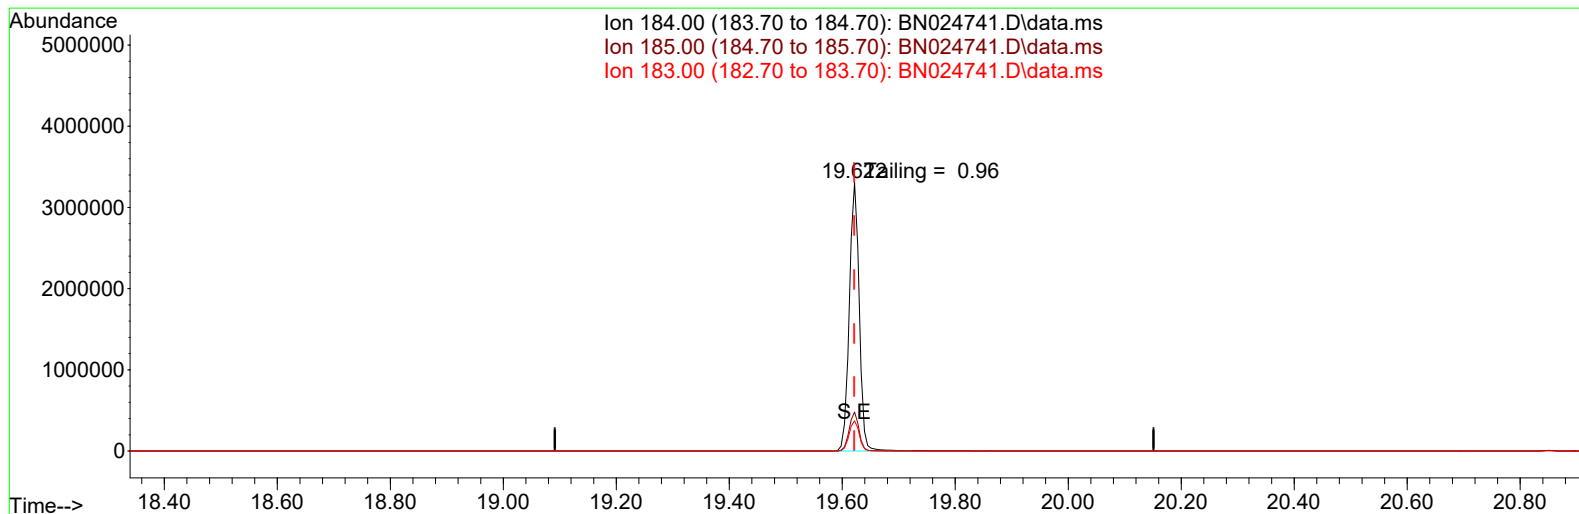

TIC: BN024741.D\data.ms

(77) Benzidine**19.622min (+ 0.000) 753629.81 ng****response 4018949**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.58
183.00	13.20	11.30
0.00	0.00	0.00