

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040323\
 Data File : BN024727.D
 Acq On : 03 Apr 2023 12:59
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Apr 04 03:06:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN040323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 03 15:20:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.997	152	10554	0.400	ng	0.00
7) Naphthalene-d8	10.802	136	29634	0.400	ng	0.00
13) Acenaphthene-d10	14.633	164	16333	0.400	ng	0.00
19) Phenanthrene-d10	17.376	188	32764	0.400	ng	0.00
29) Chrysene-d12	21.565	240	24847	0.400	ng	0.00
35) Perylene-d12	24.050	264	16138	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.541	112	42022	1.750	ng	0.00
5) Phenol-d6	7.152	99	54896	1.817	ng	0.00
8) Nitrobenzene-d5	9.158	82	42593	1.842	ng	0.00
11) 2-Methylnaphthalene-d10	12.391	152	68393	1.800	ng	0.00
14) 2,4,6-Tribromophenol	16.122	330	13307	1.893	ng	0.00
15) 2-Fluorobiphenyl	13.254	172	112985	1.773	ng	0.00
27) Fluoranthene-d10	19.404	212	126048	1.817	ng	0.00
31) Terphenyl-d14	19.998	244	125201	1.744	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.403	88	19521	1.791	ng	97
3) n-Nitrosodimethylamine	3.728	42	34275	1.876	ng	# 97
6) bis(2-Chloroethyl)ether	7.412	93	53051	1.788	ng	99
9) Naphthalene	10.856	128	137443	1.793	ng	99
10) Hexachlorobutadiene	11.144	225	27449	1.803	ng	# 100
12) 2-Methylnaphthalene	12.463	142	93362	1.814	ng	99
16) Acenaphthylene	14.355	152	127591	1.876	ng	100
17) Acenaphthene	14.697	154	85540	1.818	ng	96
18) Fluorene	15.680	166	116938	1.808	ng	100
20) 4,6-Dinitro-2-methylph...	15.750	198	5977	1.541	ng	# 41
21) 4-Bromophenyl-phenylether	16.569	248	35477	1.807	ng	98
22) Hexachlorobenzene	16.681	284	41304	1.788	ng	100
23) Atrazine	16.830	200	22289	1.864	ng	97
24) Pentachlorophenol	17.028	266	15465	1.896	ng	99
25) Phenanthrene	17.413	178	171586	1.813	ng	100
26) Anthracene	17.512	178	151897	1.852	ng	99
28) Fluoranthene	19.438	202	187725	1.865	ng	100
30) Pyrene	19.796	202	184769	1.768	ng	100
32) Benzo(a)anthracene	21.547	228	141854	1.781	ng	99
33) Chrysene	21.601	228	154933	1.762	ng	100
34) Bis(2-ethylhexyl)phtha...	21.467	149	60626	1.699	ng	99
36) Indeno(1,2,3-cd)pyrene	26.640	276	113286	1.850	ng	100
37) Benzo(b)fluoranthene	23.287	252	121468	1.852	ng	# 93
38) Benzo(k)fluoranthene	23.340	252	121069	1.863	ng	# 92
39) Benzo(a)pyrene	23.939	252	103250	1.854	ng	# 89
40) Dibenzo(a,h)anthracene	26.658	278	90816	1.882	ng	95
41) Benzo(g,h,i)perylene	27.439	276	102438	1.814	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040323\
Data File : BN024727.D
Acq On : 03 Apr 2023 12:59
Operator : CG/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Quant Time: Apr 04 03:06:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN040323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 03 15:20:44 2023
Response via : Initial Calibration

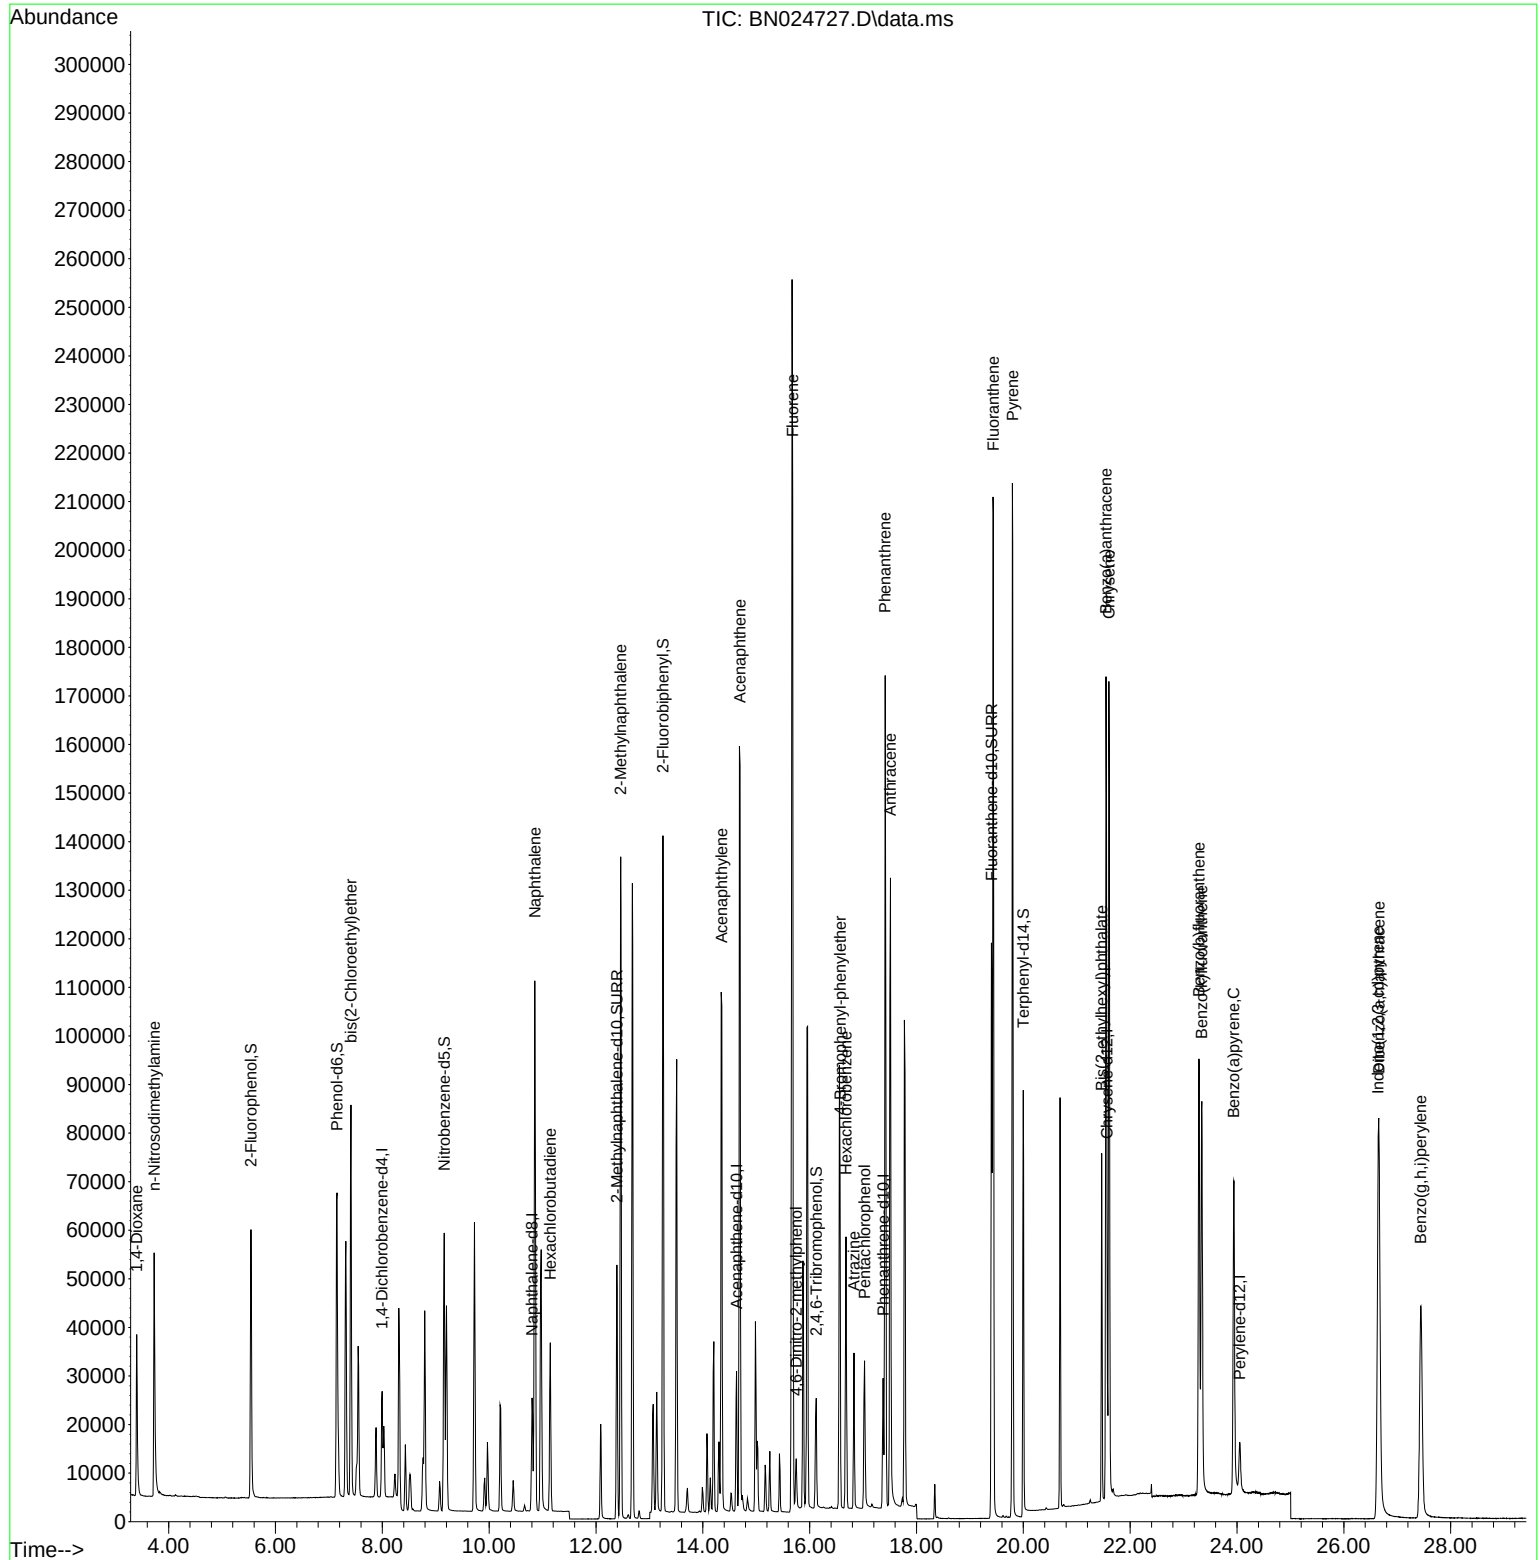






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.997 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN024727.D
 Acq: 03 Apr 2023 12:59


Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

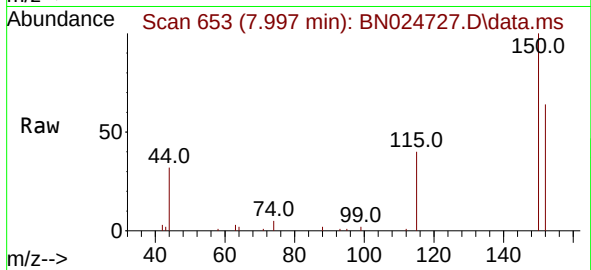



Tgt Ion:152 Resp: 10554
 Ion Ratio Lower Upper
 152 100
 150 155.4 123.0 184.4
 115 61.5 48.7 73.1

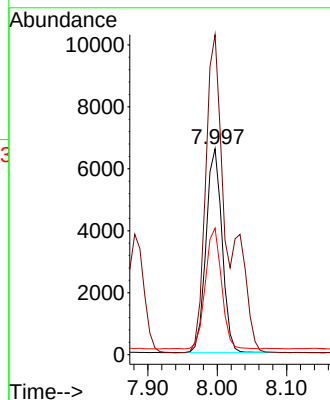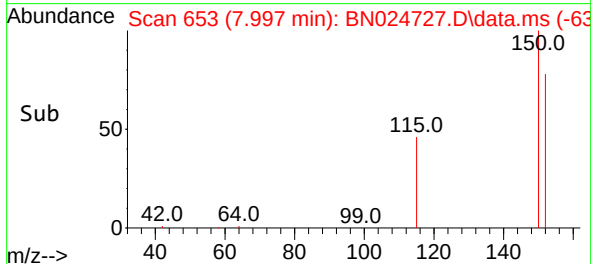


#2
 1,4-Dioxane
 Concen: 1.791 ng
 RT: 3.403 min Scan# 17
 Delta R.T. 0.000 min
 Lab File: BN024727.D
 Acq: 03 Apr 2023 12:59

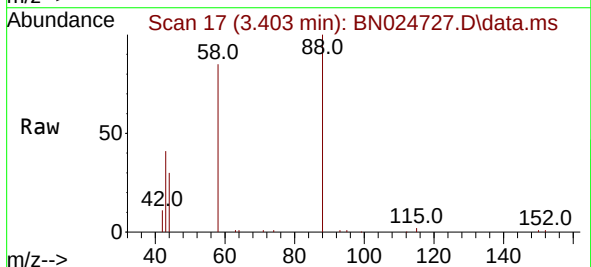

Tgt Ion: 88 Resp: 19521
 Ion Ratio Lower Upper
 88 100
 43 40.4 32.8 49.2
 58 88.0 73.0 109.6



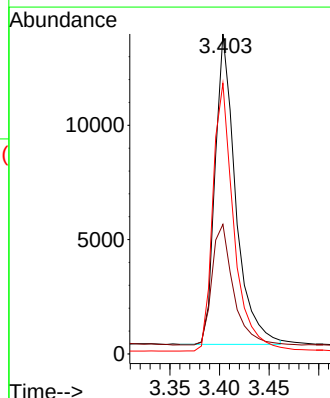



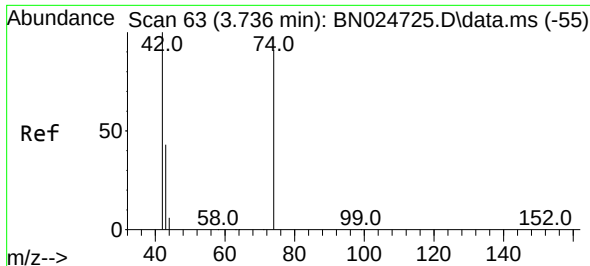

#3
n-Nitrosodimethylamine
Concen: 1.876 ng
RT: 3.728 min Scan# 61
Delta R.T. -0.007 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 34275
Ion Ratio Lower Upper
42 100
74 90.4 73.9 110.9
44 6.5 7.6 11.4#

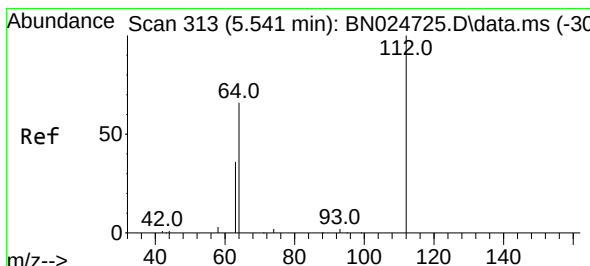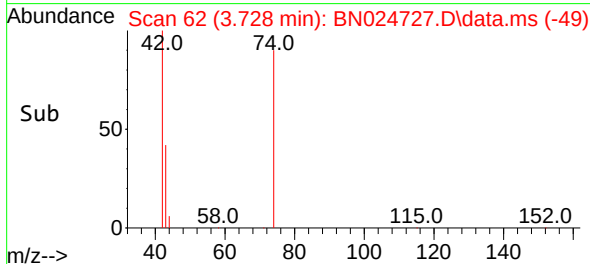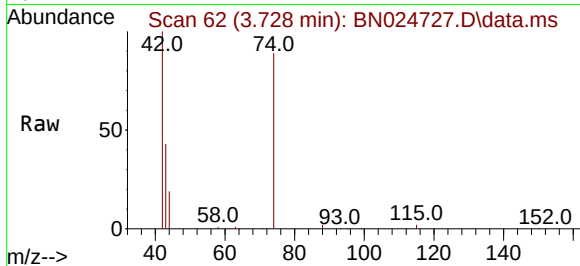

#4
2-Fluorophenol
Concen: 1.750 ng
RT: 5.541 min Scan# 313
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion: 112 Resp: 42022
Ion Ratio Lower Upper
112 100
64 65.4 52.1 78.1
63 35.2 28.7 43.1


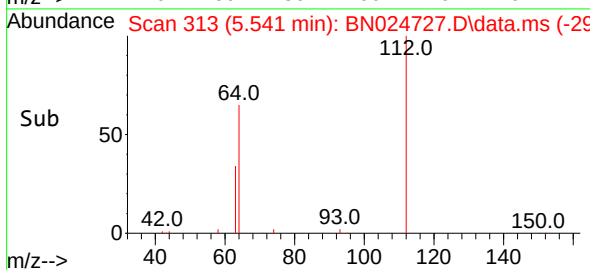

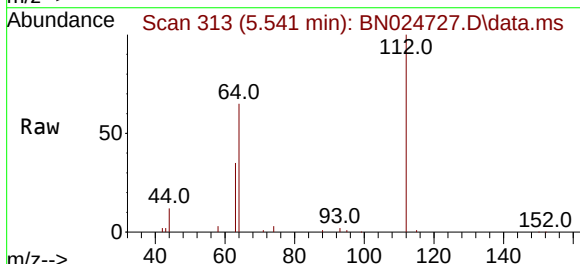




#5
Phenol-d6
Concen: 1.817 ng
RT: 7.152 min Scan# 511
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 54896
Ion Ratio Lower Upper
99 100
42 28.9 23.7 35.5
71 35.0 28.2 42.4

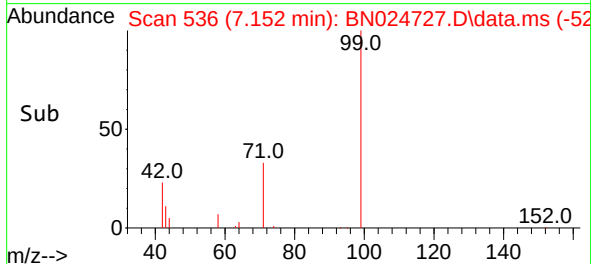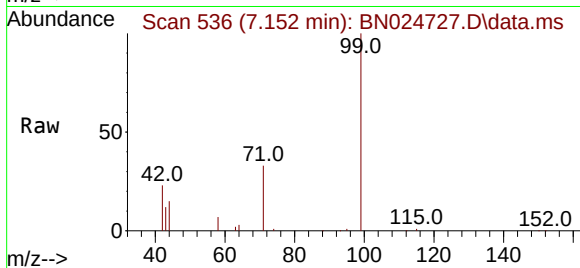

#6
bis(2-Chloroethyl)ether
Concen: 1.788 ng
RT: 7.412 min Scan# 572
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion: 93 Resp: 53051
Ion Ratio Lower Upper
93 100
63 86.9 69.0 103.6
95 32.5 26.1 39.1


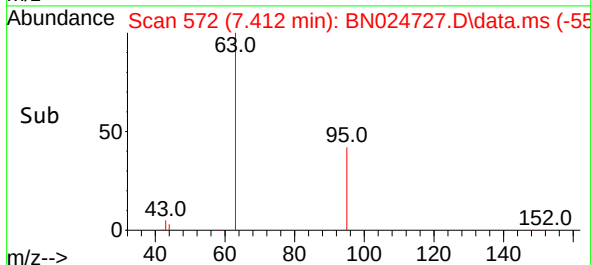

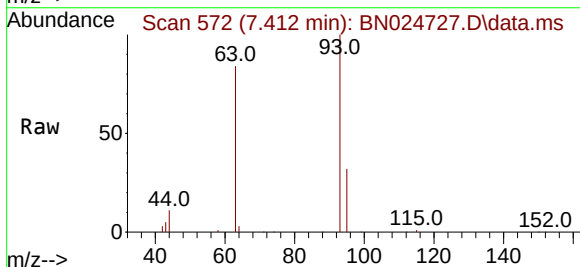




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.802 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	136	Resp:	29634
Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.0	13.6
54	13.6	11.4	17.0
68	8.8	7.0	10.6

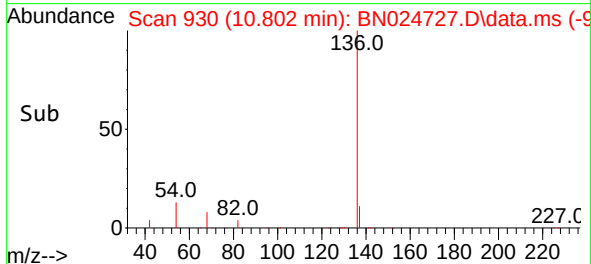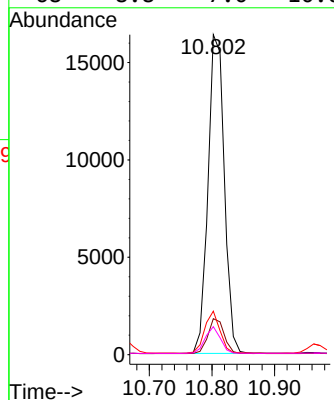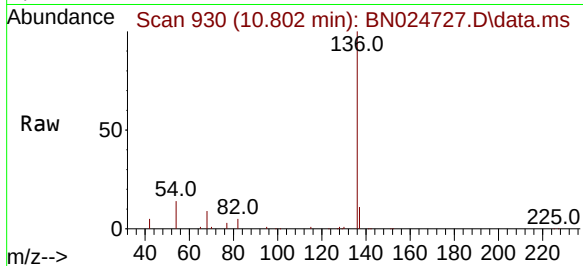

#8
Nitrobenzene-d5
Concen: 1.842 ng
RT: 9.158 min Scan# 776
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion:	82	Resp:	42593
Ion	Ratio	Lower	Upper
82	100		
128	37.7	29.4	44.2
54	62.3	51.3	76.9

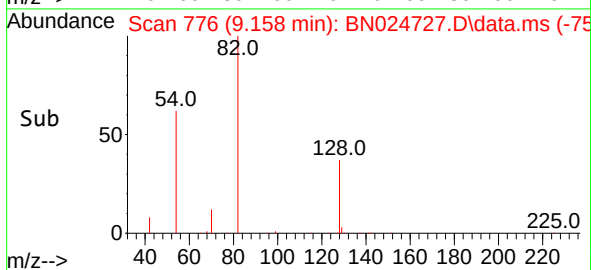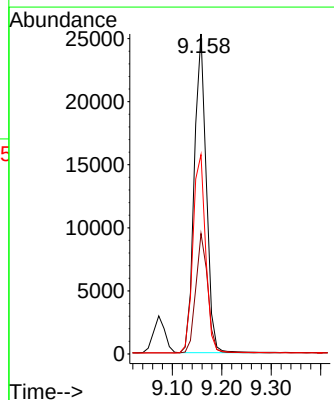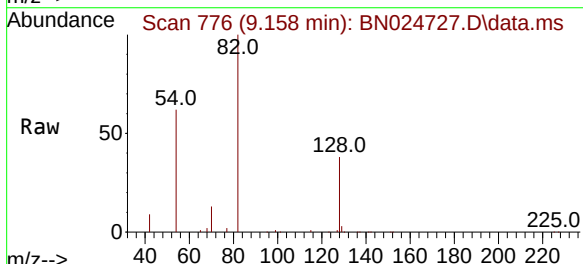

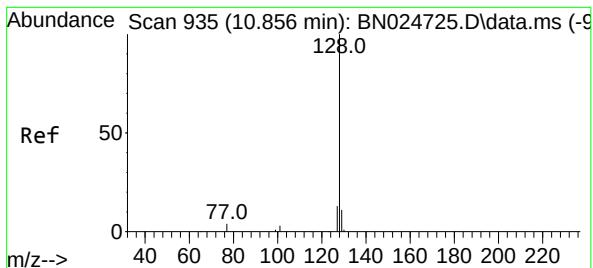

#9

Naphthalene

Concen: 1.793 ng

RT: 10.856 min Scan# 91

Delta R.T. 0.000 min

Lab File: BN024727.D

Acq: 03 Apr 2023 12:59

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:128 Resp: 137443

Ion Ratio Lower Upper

128 100

129 10.8 9.0 13.6

127 13.0 10.6 15.8

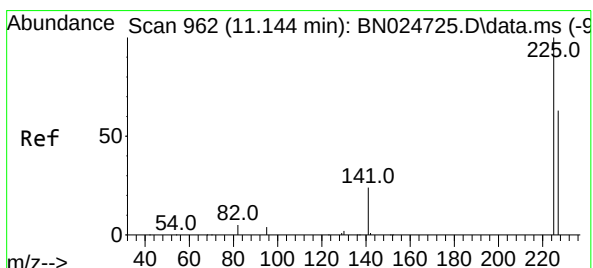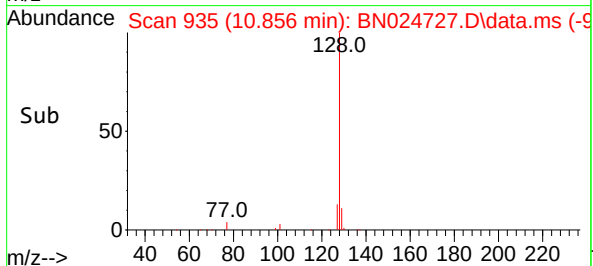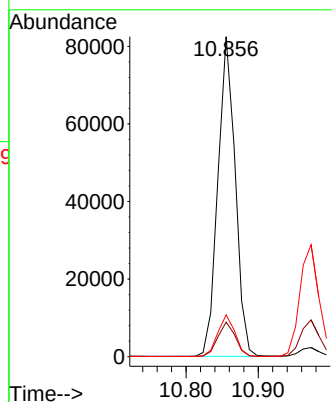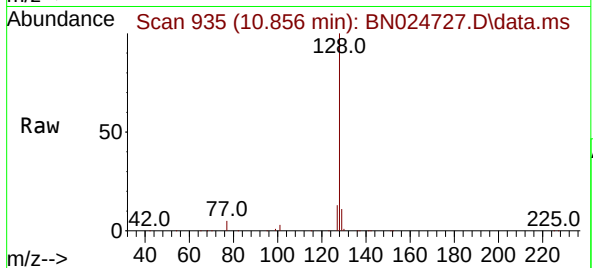

#10

Hexachlorobutadiene

Concen: 1.803 ng

RT: 11.144 min Scan# 962

Delta R.T. 0.000 min

Lab File: BN024727.D

Acq: 03 Apr 2023 12:59




Tgt Ion:225 Resp: 27449


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.2 50.5 75.7


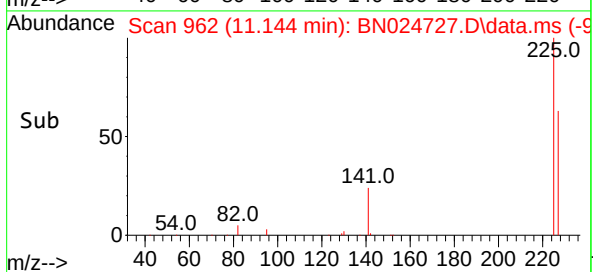
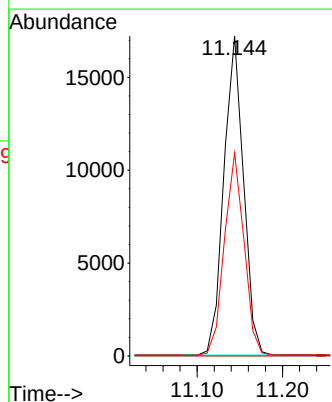
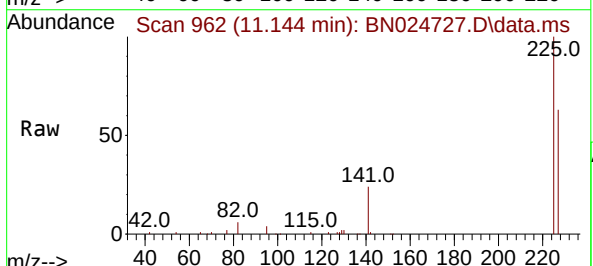


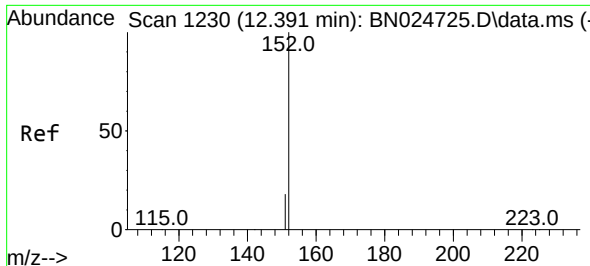

#11
2-Methylnaphthalene-d10
Concen: 1.800 ng
RT: 12.391 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 68393
Ion Ratio Lower Upper
152 100
151 20.9 16.6 25.0

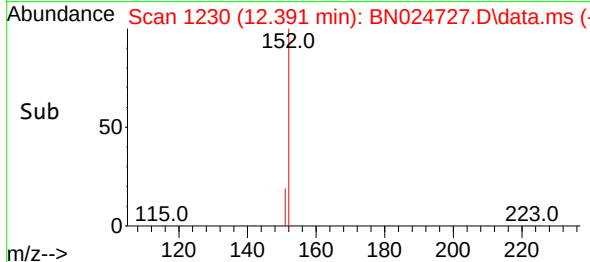

#12
2-Methylnaphthalene
Concen: 1.814 ng
RT: 12.463 min Scan# 1249
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion:142 Resp: 93362
Ion Ratio Lower Upper
142 100
141 88.3 70.5 105.7
115 37.6 30.9 46.3


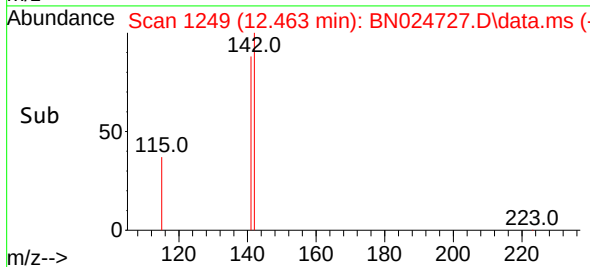

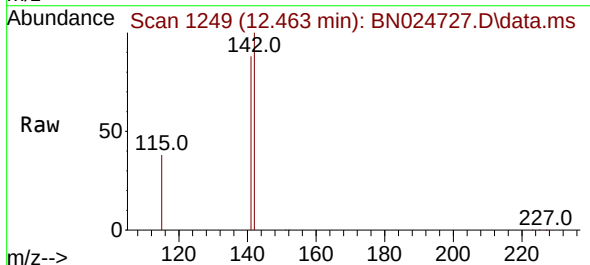




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.633 min Scan# 1545
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 16333
Ion Ratio Lower Upper
164 100
162 101.9 82.2 123.4
160 49.2 39.4 59.0

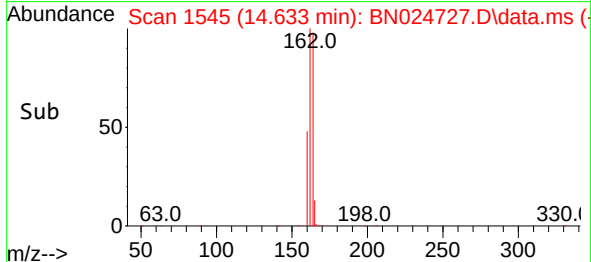

#14
2,4,6-Tribromophenol
Concen: 1.893 ng
RT: 16.122 min Scan# 1679
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion:330 Resp: 13307
Ion Ratio Lower Upper
330 100
332 96.9 77.6 116.4
141 38.0 29.6 44.4


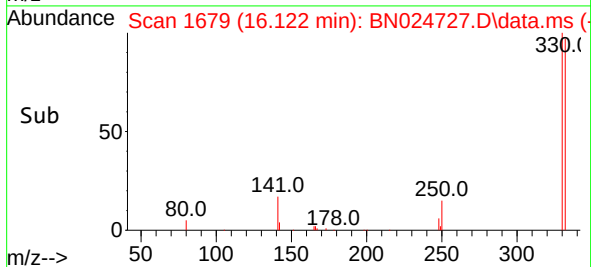

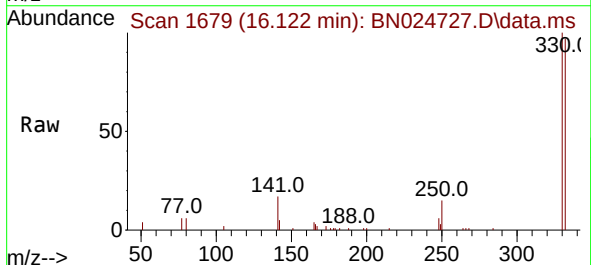




#15
2-Fluorobiphenyl
Concen: 1.773 ng
RT: 13.254 min Scan# 1416
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:172 Resp: 112985
Ion Ratio Lower Upper
172 100
171 34.9 28.8 43.2
170 23.7 19.5 29.3

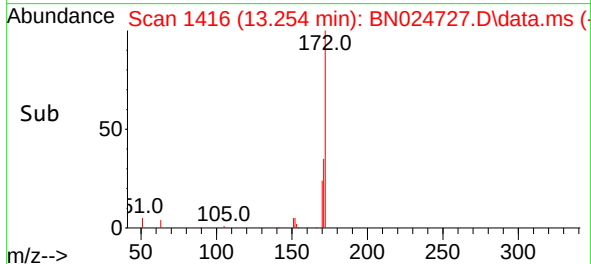

#16
Acenaphthylene
Concen: 1.876 ng
RT: 14.355 min Scan# 1519
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion:152 Resp: 127591
Ion Ratio Lower Upper
152 100
151 19.2 15.2 22.8
153 13.0 10.4 15.6


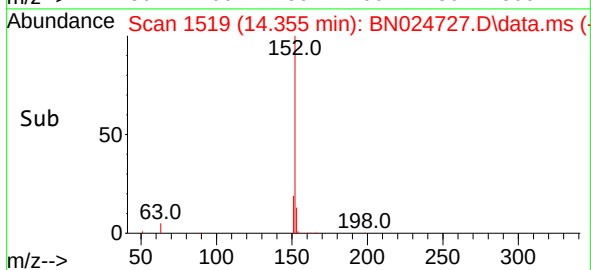

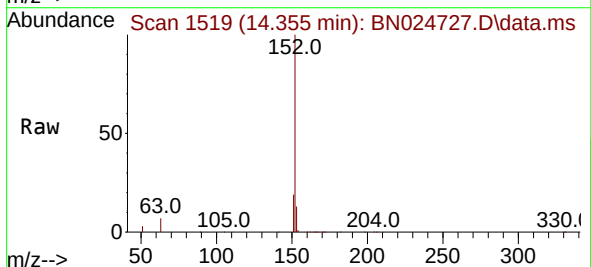




#17
Acenaphthene
Concen: 1.818 ng
RT: 14.697 min Scan# 1551
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:154 Resp: 85540
Ion Ratio Lower Upper
154 100
153 110.9 92.5 138.7
152 56.3 47.2 70.8

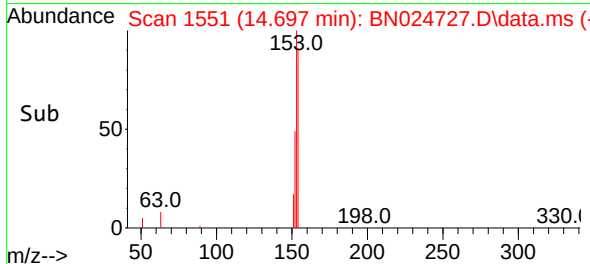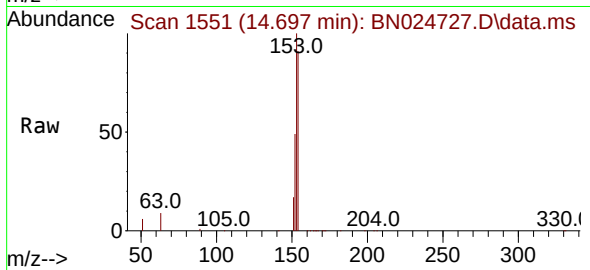

#18
Fluorene
Concen: 1.808 ng
RT: 15.680 min Scan# 1643
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion:166 Resp: 116938
Ion Ratio Lower Upper
166 100
165 98.7 79.1 118.7
167 13.4 10.6 16.0


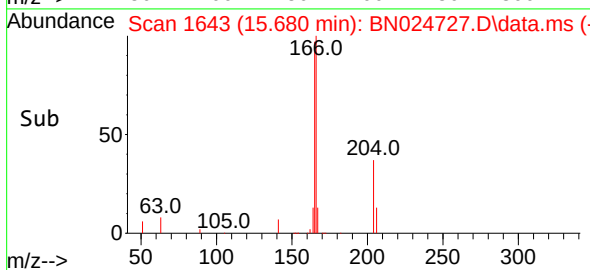

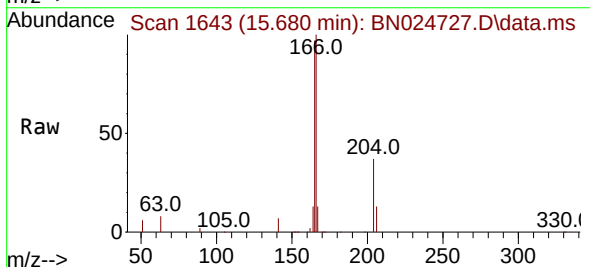


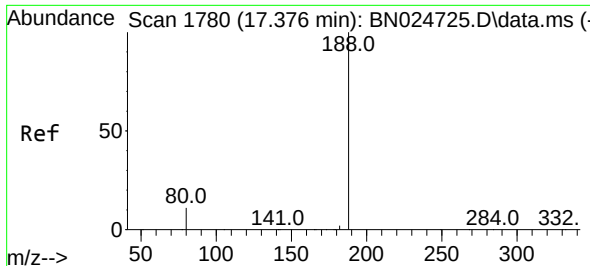

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.376 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:188 Resp: 32764
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.1 9.2 13.8

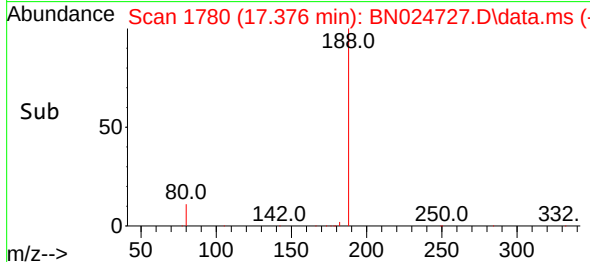

#20
4,6-Dinitro-2-methylphenol
Concen: 1.541 ng
RT: 15.750 min Scan# 1649
Delta R.T. -0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion:198 Resp: 5977
Ion Ratio Lower Upper
198 100
51 62.1 118.9 178.3#
105 44.8 64.6 97.0#


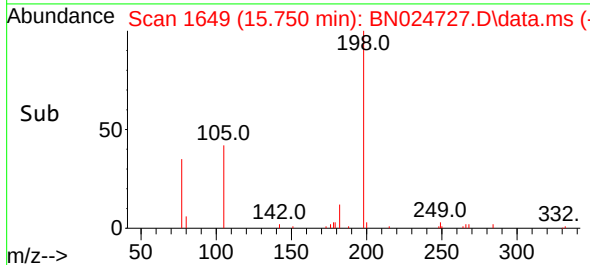

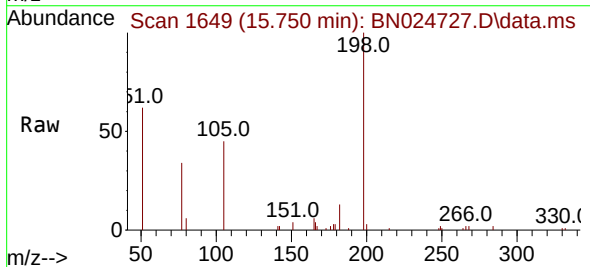


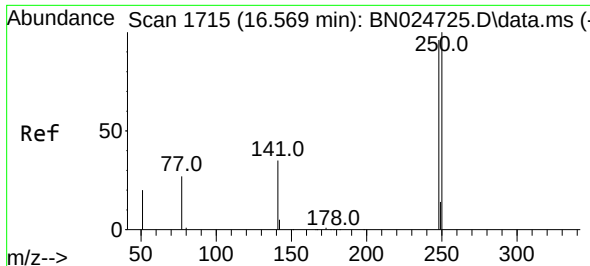

#21
4-Bromophenyl-phenylether
Concen: 1.807 ng
RT: 16.569 min Scan# 1715
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:248 Resp: 35477
Ion Ratio Lower Upper
248 100
250 102.8 83.6 125.4
141 35.2 30.3 45.5

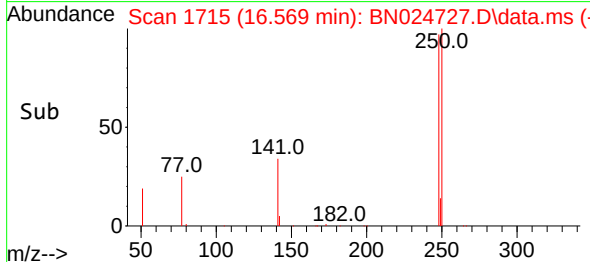

#22
Hexachlorobenzene
Concen: 1.788 ng
RT: 16.681 min Scan# 1724
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion:284 Resp: 41304
Ion Ratio Lower Upper
284 100
142 36.6 29.4 44.2
249 30.9 24.8 37.2


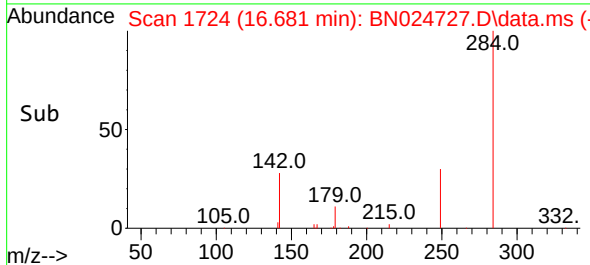

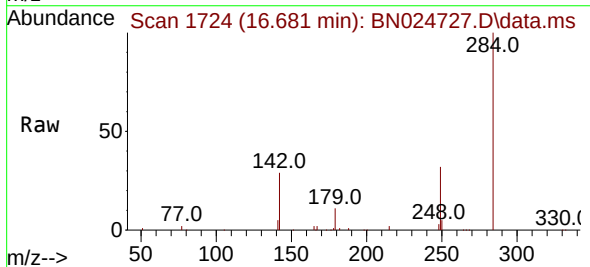


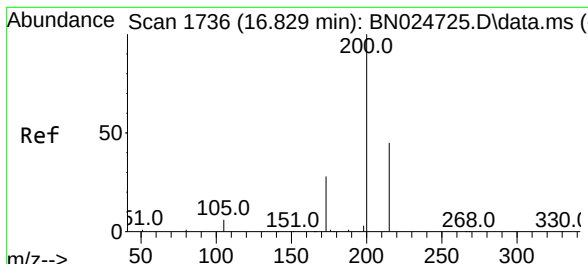

#23
 Atrazine
 Concen: 1.864 ng
 RT: 16.830 min Scan# 1736
 Delta R.T. 0.000 min
 Lab File: BN024727.D
 Acq: 03 Apr 2023 12:59




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:	200	Resp:	22289
Ion Ratio	Lower	Upper	
200	100		
173	26.1	23.7	35.5
215	45.6	37.0	55.4

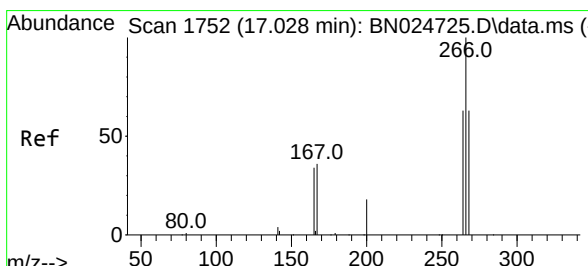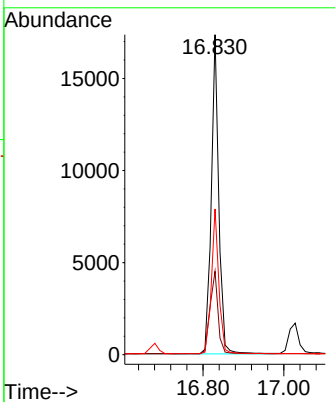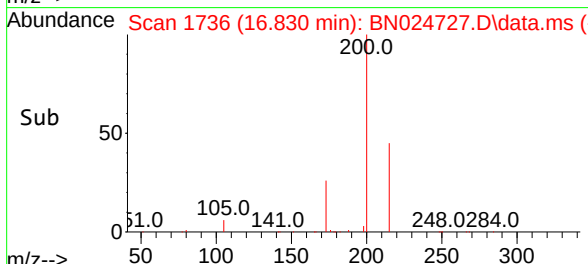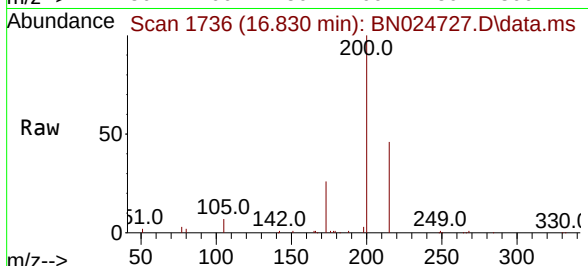

#24
 Pentachlorophenol
 Concen: 1.896 ng
 RT: 17.028 min Scan# 1752
 Delta R.T. 0.000 min
 Lab File: BN024727.D
 Acq: 03 Apr 2023 12:59

Tgt Ion:	266	Resp:	15465
Ion Ratio	Lower	Upper	
266	100		
264	63.1	49.4	74.0
268	64.0	51.0	76.4


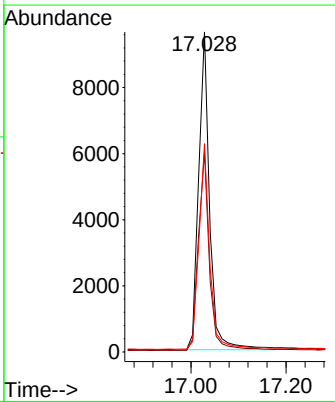
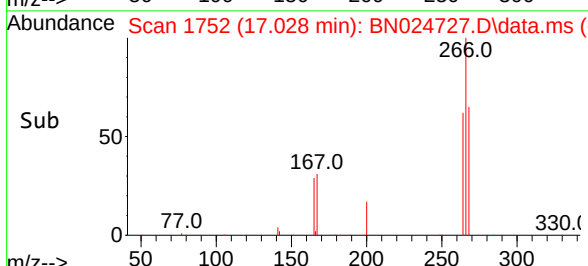
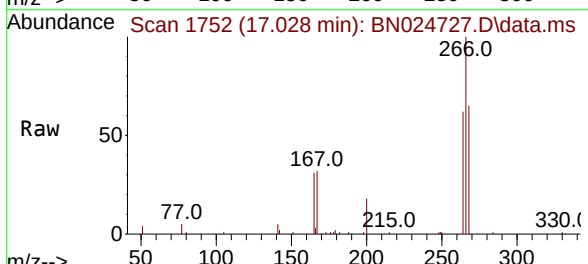


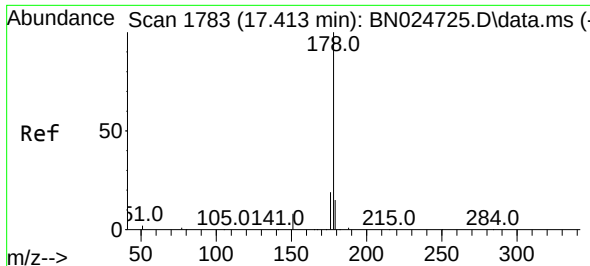

#25
 Phenanthrene
 Concen: 1.813 ng
 RT: 17.413 min Scan# 1783
 Delta R.T. 0.000 min
 Lab File: BN024727.D
 Acq: 03 Apr 2023 12:59




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:178 Resp: 171586
 Ion Ratio Lower Upper
 178 100
 176 19.4 15.4 23.2
 179 15.1 12.2 18.4

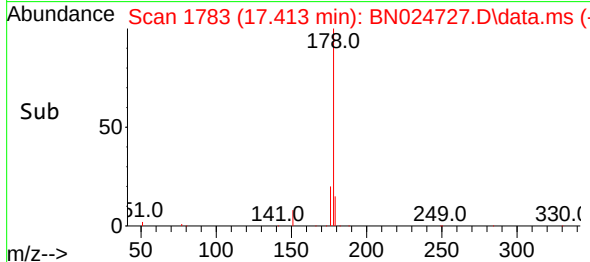

#26
 Anthracene
 Concen: 1.852 ng
 RT: 17.512 min Scan# 1791
 Delta R.T. 0.000 min
 Lab File: BN024727.D
 Acq: 03 Apr 2023 12:59

Tgt Ion:178 Resp: 151897
 Ion Ratio Lower Upper
 178 100
 176 18.6 14.6 21.8
 179 15.3 12.0 18.0


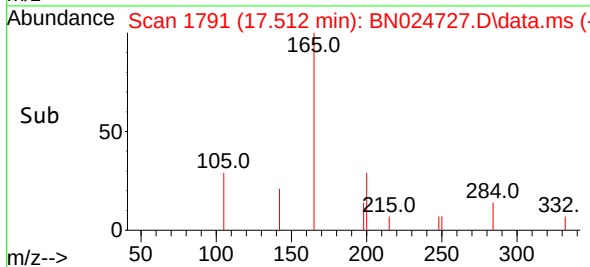

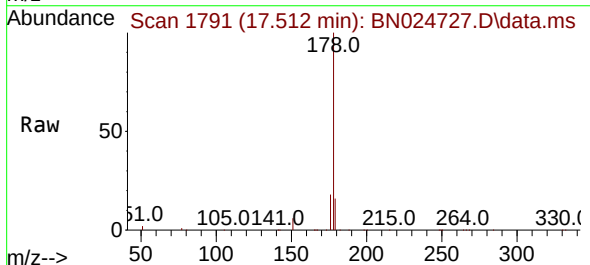


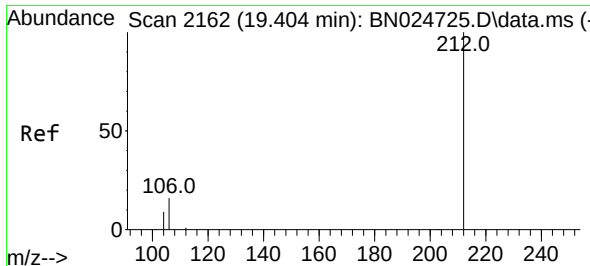

#27
Fluoranthene-d10
Concen: 1.817 ng
RT: 19.404 min Scan# 2162
Delta R.T. 0.000 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:212 Resp: 126048
Ion Ratio Lower Upper
212 100
106 16.5 13.0 19.4
104 9.3 7.4 11.0

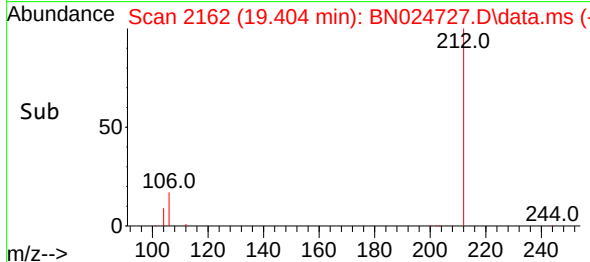

#28
Fluoranthene
Concen: 1.865 ng
RT: 19.438 min Scan# 2170
Delta R.T. 0.004 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion:202 Resp: 187725
Ion Ratio Lower Upper
202 100
101 12.5 10.1 15.1
203 17.2 13.6 20.4

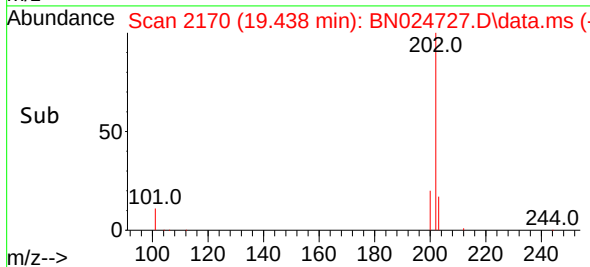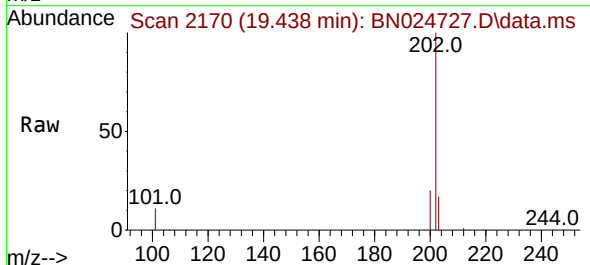

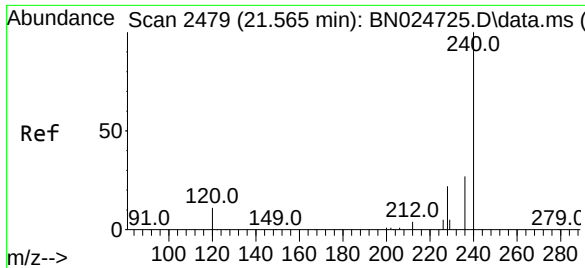

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.565 min Scan# 2479

Delta R.T. 0.000 min

Lab File: BN024727.D

Acq: 03 Apr 2023 12:59

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:240 Resp: 24847

Ion Ratio Lower Upper

240 100

120 14.6 10.6 16.0

236 28.1 22.3 33.5

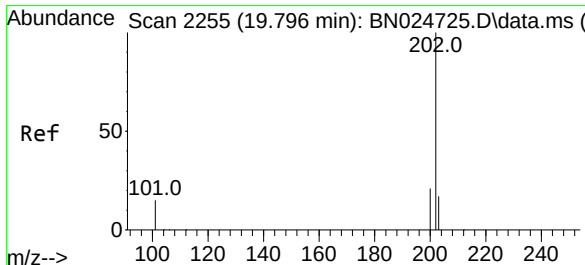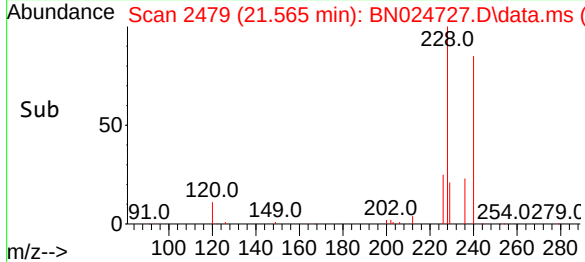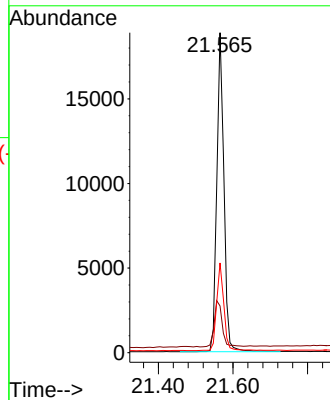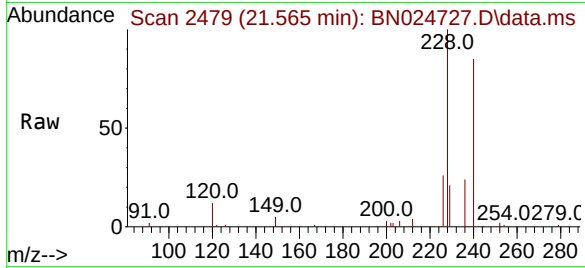

#30

Pyrene

Concen: 1.768 ng

RT: 19.796 min Scan# 2255

Delta R.T. 0.000 min

Lab File: BN024727.D

Acq: 03 Apr 2023 12:59




Tgt Ion:202 Resp: 184769


Ion Ratio Lower Upper

202 100

200 20.9 16.6 25.0

203 17.7 14.2 21.2


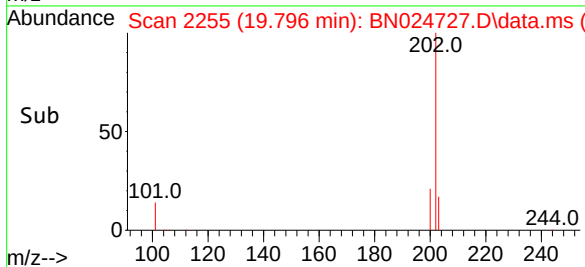
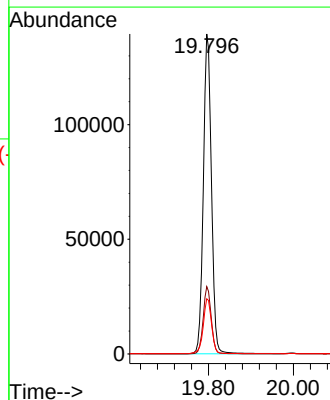
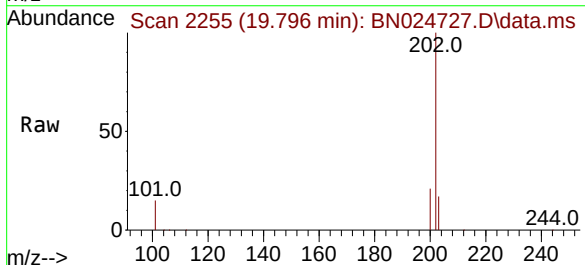




#31
 Terphenyl-d14
 Concen: 1.744 ng
 RT: 19.998 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN024727.D
 Acq: 03 Apr 2023 12:59




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion:244 Resp: 125201
 Ion Ratio Lower Upper
 244 100
 212 8.7 7.4 11.0
 122 0.0 0.0 0.0

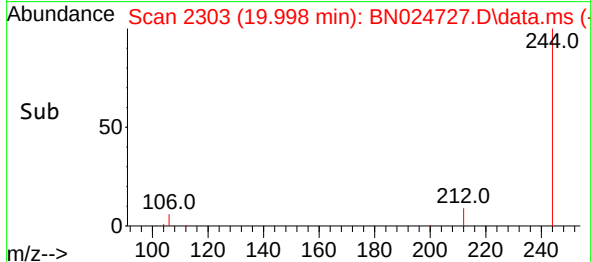

#32
 Benzo(a)anthracene
 Concen: 1.781 ng
 RT: 21.547 min Scan# 2477
 Delta R.T. 0.000 min
 Lab File: BN024727.D
 Acq: 03 Apr 2023 12:59

Tgt Ion:228 Resp: 141854
 Ion Ratio Lower Upper
 228 100
 226 28.1 22.2 33.2
 229 19.7 15.8 23.8

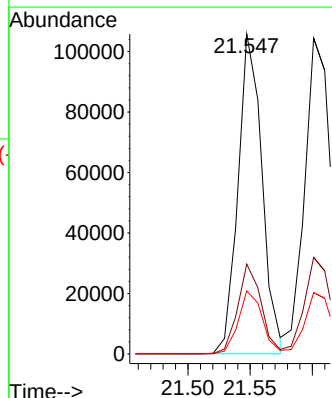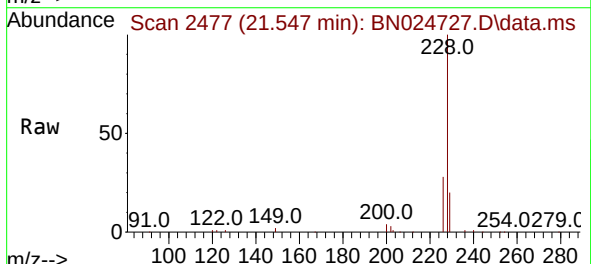

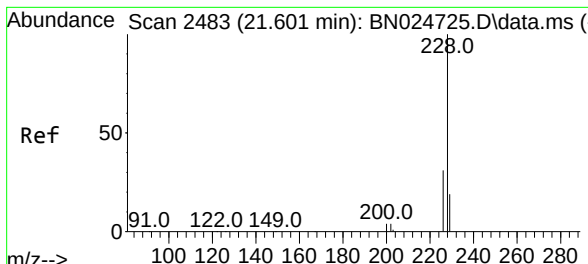

#33

Chrysene

Concen: 1.762 ng

RT: 21.601 min Scan# 2483

Delta R.T. 0.000 min

Lab File: BN024727.D

Acq: 03 Apr 2023 12:59

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:228 Resp: 154933

Ion Ratio Lower Upper

228 100

226 30.6 24.7 37.1

229 19.4 15.6 23.4

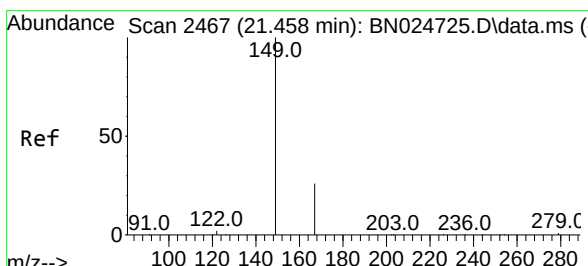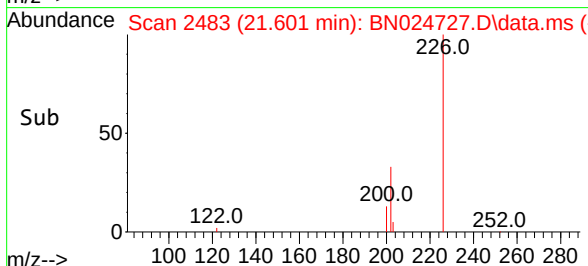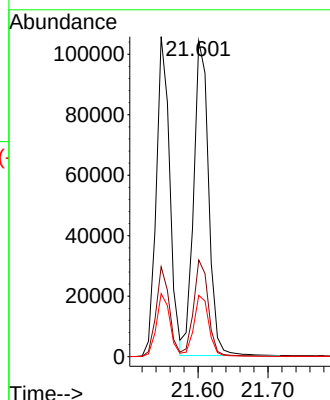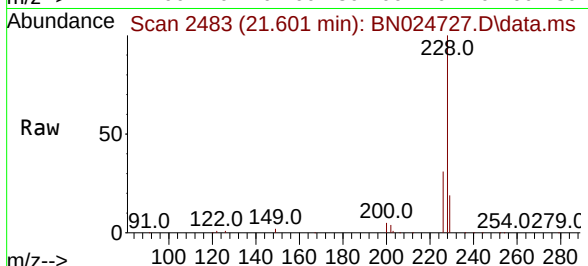

#34

Bis(2-ethylhexyl)phthalate

Concen: 1.699 ng

RT: 21.467 min Scan# 2468

Delta R.T. 0.009 min

Lab File: BN024727.D

Acq: 03 Apr 2023 12:59




Tgt Ion:149 Resp: 60626


Ion Ratio Lower Upper

149 100

167 26.5 21.0 31.6

279 2.9 2.8 4.2


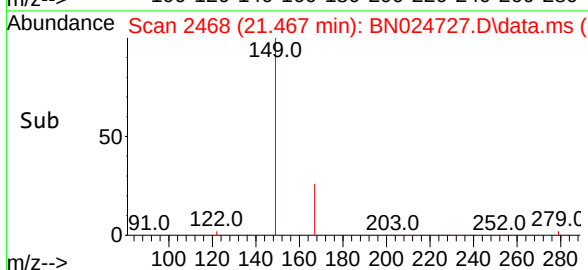
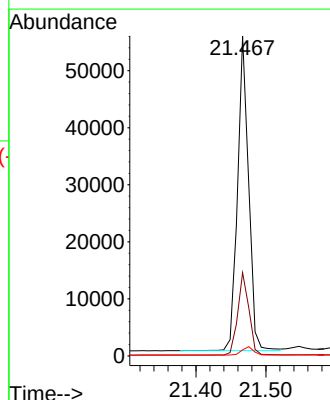
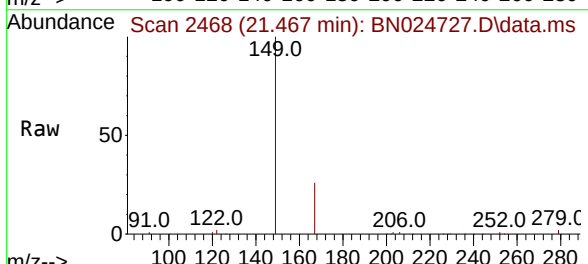




#35
Perylene-d12
Concen: 0.400 ng
RT: 24.050 min Scan# 3133
Delta R.T. 0.006 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:264 Resp: 16138
Ion Ratio Lower Upper
264 100
260 26.3 20.6 31.0
265 72.6 62.5 93.7

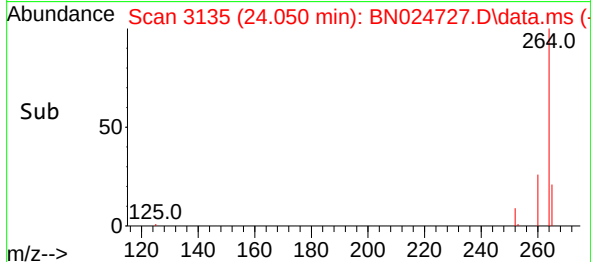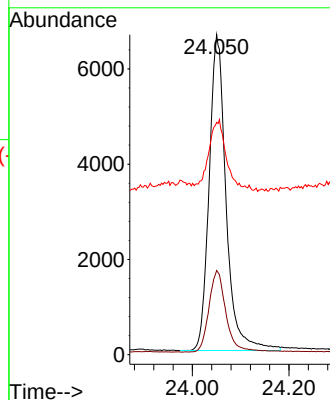

#36
Indeno(1,2,3-cd)pyrene
Concen: 1.850 ng
RT: 26.640 min Scan# 4021
Delta R.T. 0.003 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion:276 Resp: 113286
Ion Ratio Lower Upper
276 100
138 29.4 23.5 35.3
277 25.2 19.9 29.9


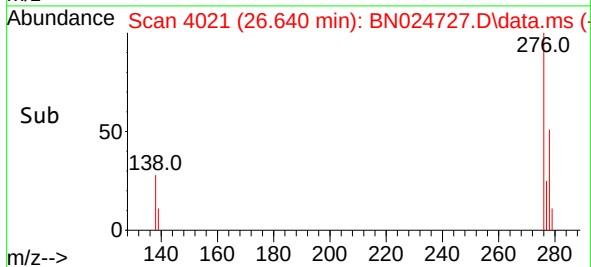
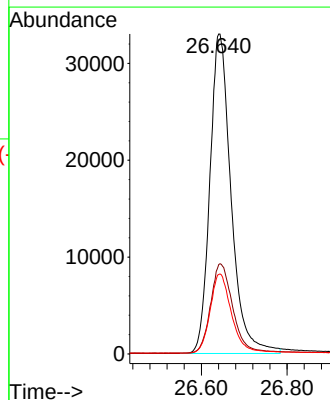
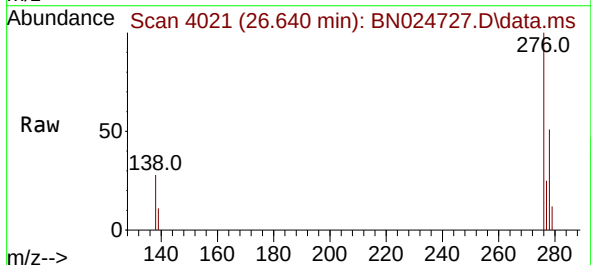




#37
Benzo(b)fluoranthene
Concen: 1.852 ng
RT: 23.287 min Scan# 2873
Delta R.T. 0.003 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 121468
Ion Ratio Lower Upper
252 100
253 22.6 20.4 30.6
125 12.4 13.4 20.0#

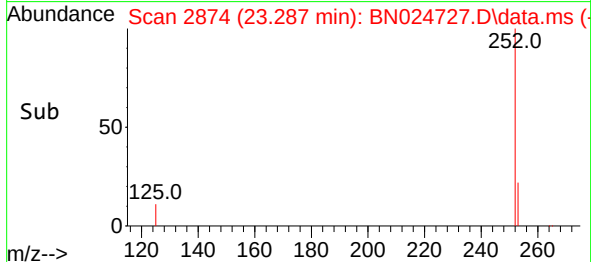

#38
Benzo(k)fluoranthene
Concen: 1.863 ng
RT: 23.340 min Scan# 2892
Delta R.T. 0.009 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion:252 Resp: 121069
Ion Ratio Lower Upper
252 100
253 22.5 21.0 31.4
125 12.6 13.3 19.9#


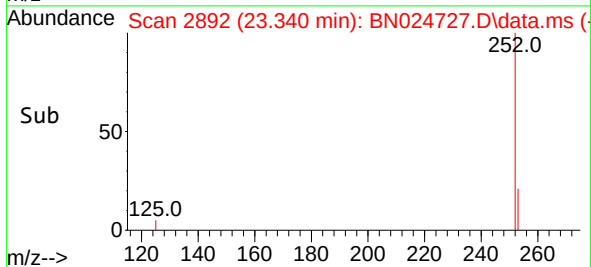

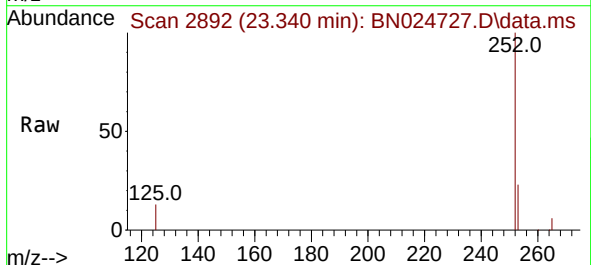




#39
Benzo(a)pyrene
Concen: 1.854 ng
RT: 23.939 min Scan# 3097
Delta R.T. 0.003 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 103250
Ion Ratio Lower Upper
252 100
253 23.1 22.5 33.7
125 14.3 16.5 24.7#

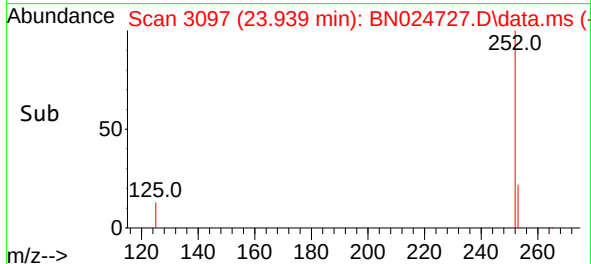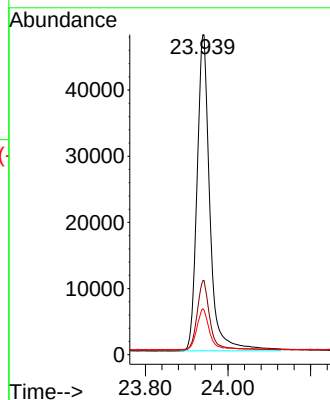

#40
Dibenzo(a,h)anthracene
Concen: 1.882 ng
RT: 26.658 min Scan# 4027
Delta R.T. 0.006 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Tgt Ion:278 Resp: 90816
Ion Ratio Lower Upper
278 100
139 19.6 16.9 25.3
279 24.0 21.7 32.5

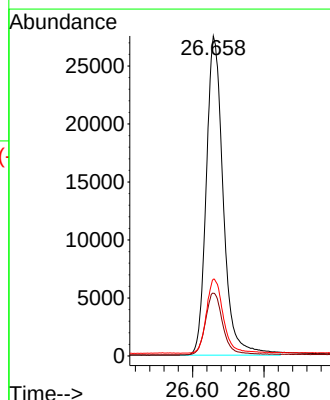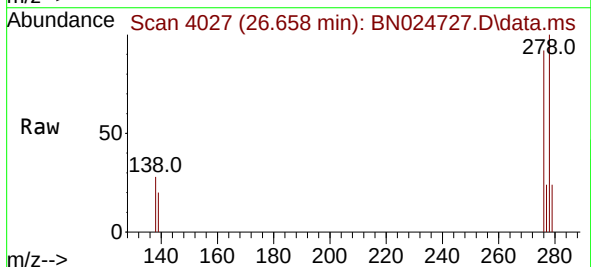

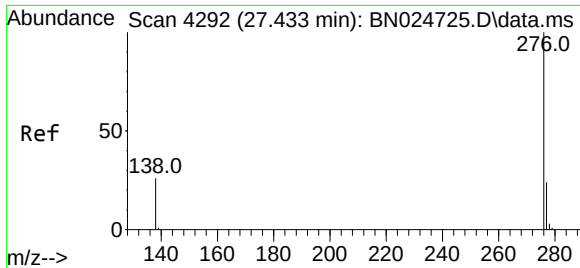

#41
Benzo(g,h,i)perylene
Concen: 1.814 ng
RT: 27.439 min Scan# 41
Delta R.T. 0.006 min
Lab File: BN024727.D
Acq: 03 Apr 2023 12:59

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:276 Resp: 102438
Ion Ratio Lower Upper
276 100
277 23.7 20.0 30.0
138 25.5 21.6 32.4

