
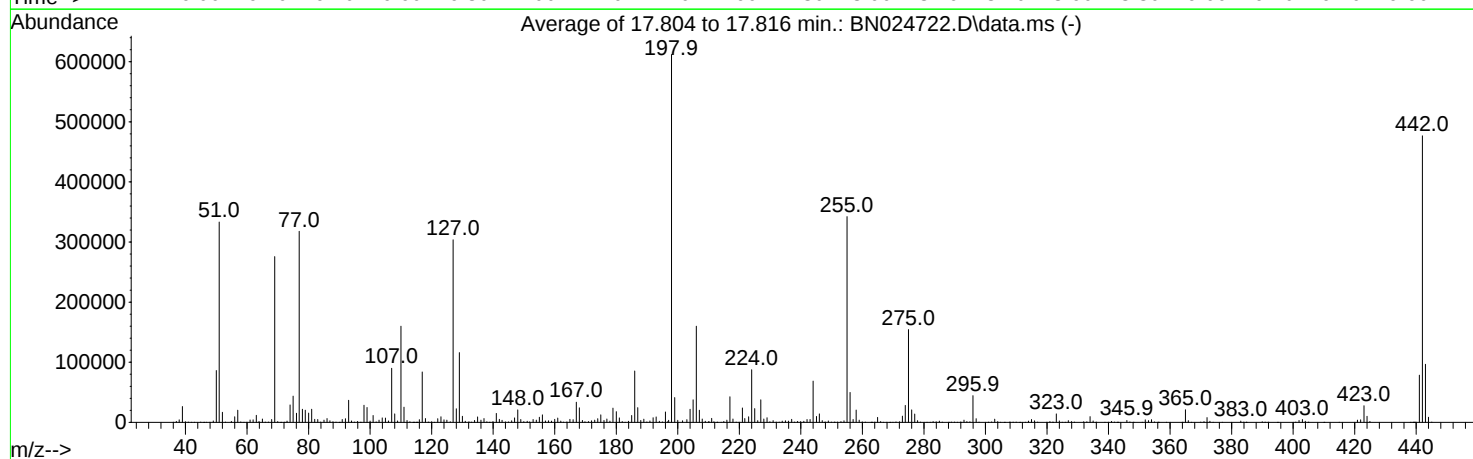


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040323\
 Data File : BN024722.D
 Acq On : 03 Apr 2023 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN040323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 04 03:11:39 2023

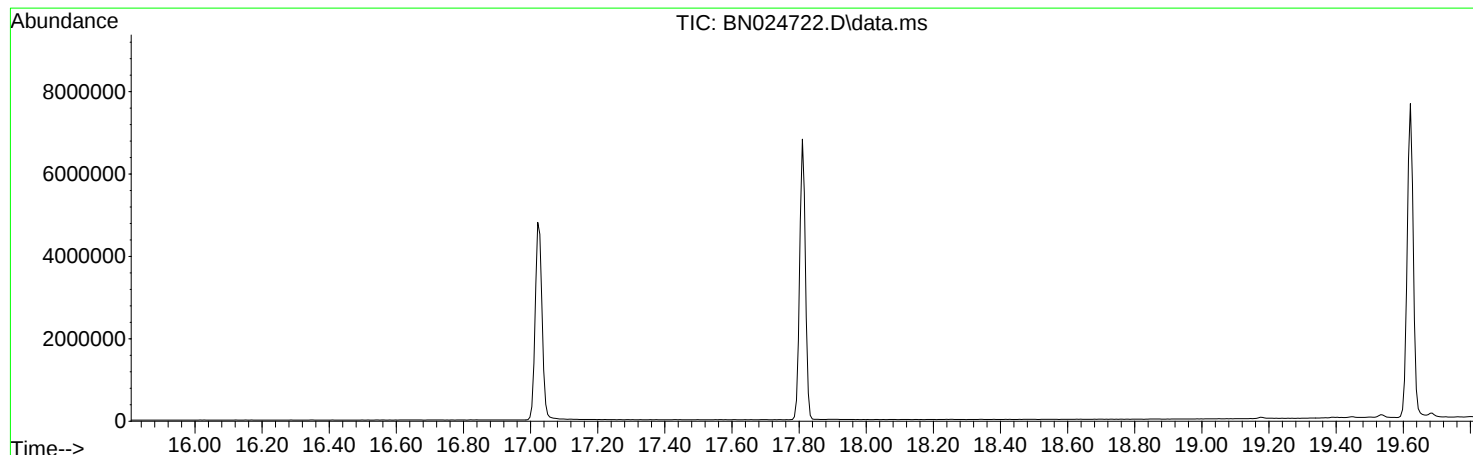




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.5	333279	PASS
68	69	0.00	2	1.7	4679	PASS
69	198	0.00	100	45.1	275797	PASS
70	69	0.00	2	0.5	1298	PASS
127	198	10	80	49.6	303701	PASS
197	198	0.00	2	0.6	3515	PASS
198	198	100	100	100.0	611968	PASS
199	198	5	9	6.7	41219	PASS
275	198	10	60	25.2	154429	PASS
365	198	1	100	3.4	20934	PASS
441	198	0.01	100	12.8	78424	PASS
442	442	50	100	100.0	476715	PASS
443	442	15	24	20.3	96661	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040323\
 Data File : BN024722.D
 Acq On : 03 Apr 2023 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 04 06:27:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 04 06:27:46 2023
 Response via : Initial Calibration

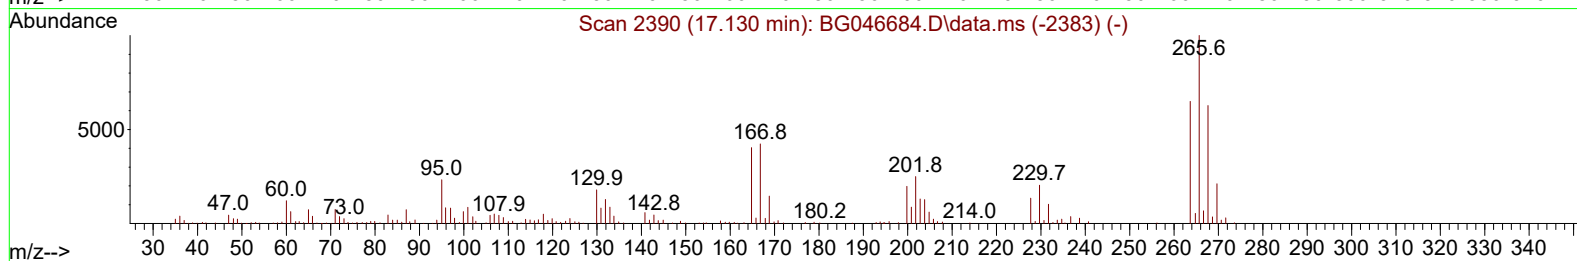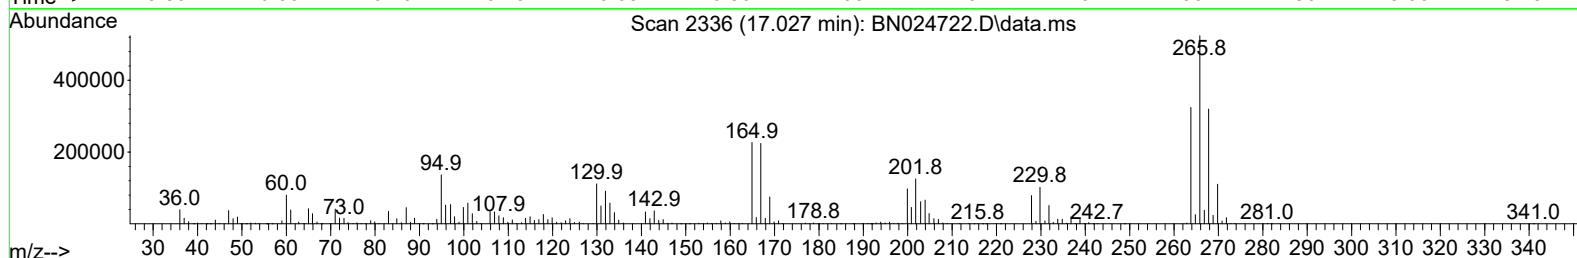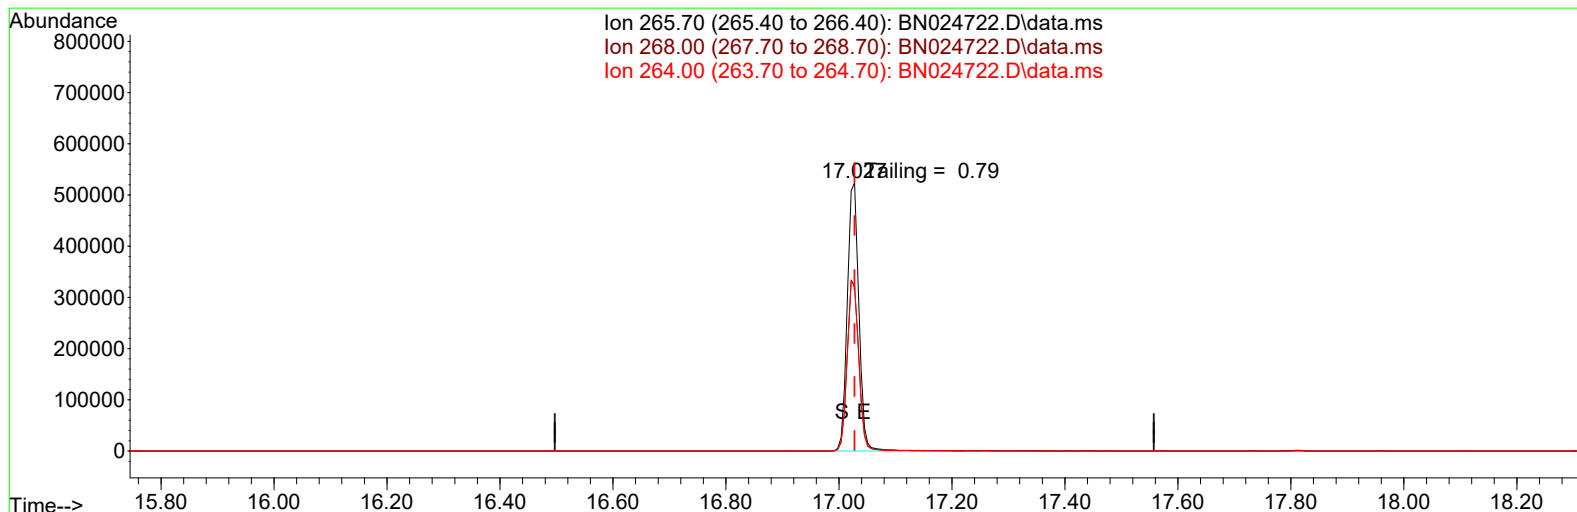

TIC: BN024722.D\data.ms

(70) Pentachlorophenol (C)

17.027min (0.000) 20848.03 ng




response 749498

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.07
264.00	61.60	61.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040323\
Data File : BN024722.D
Acq On : 03 Apr 2023 09:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 04 06:27:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 04 06:27:46 2023
Response via : Initial Calibration

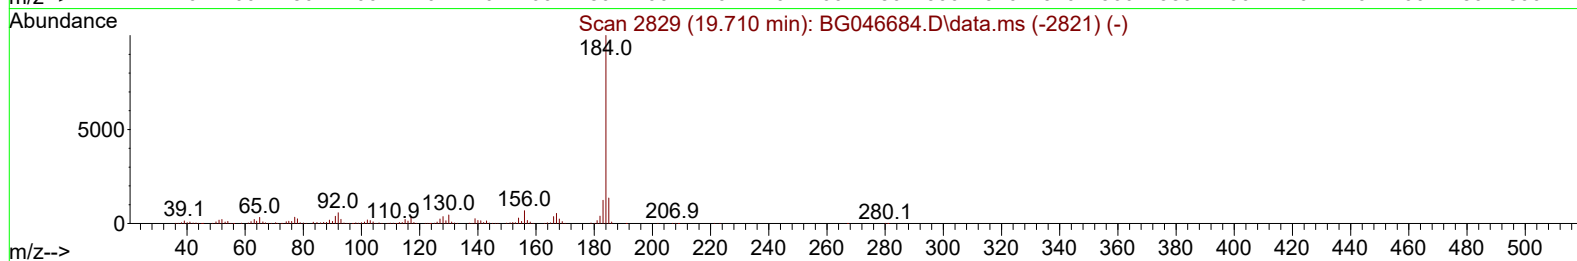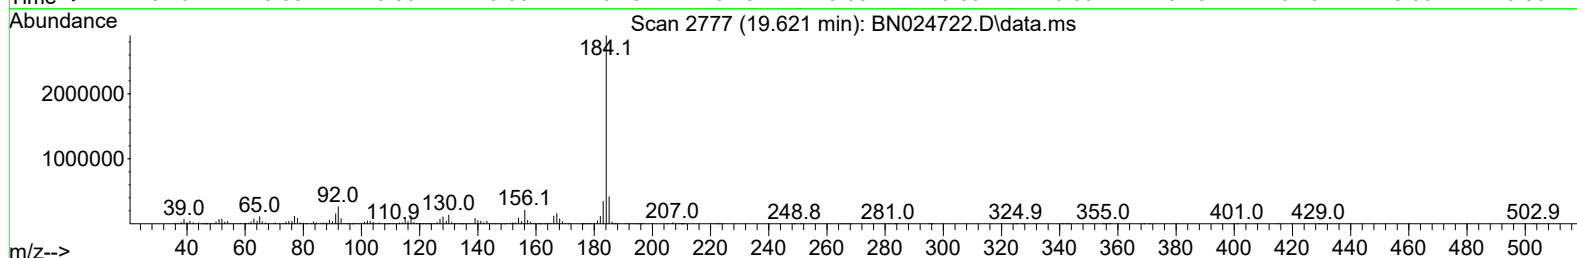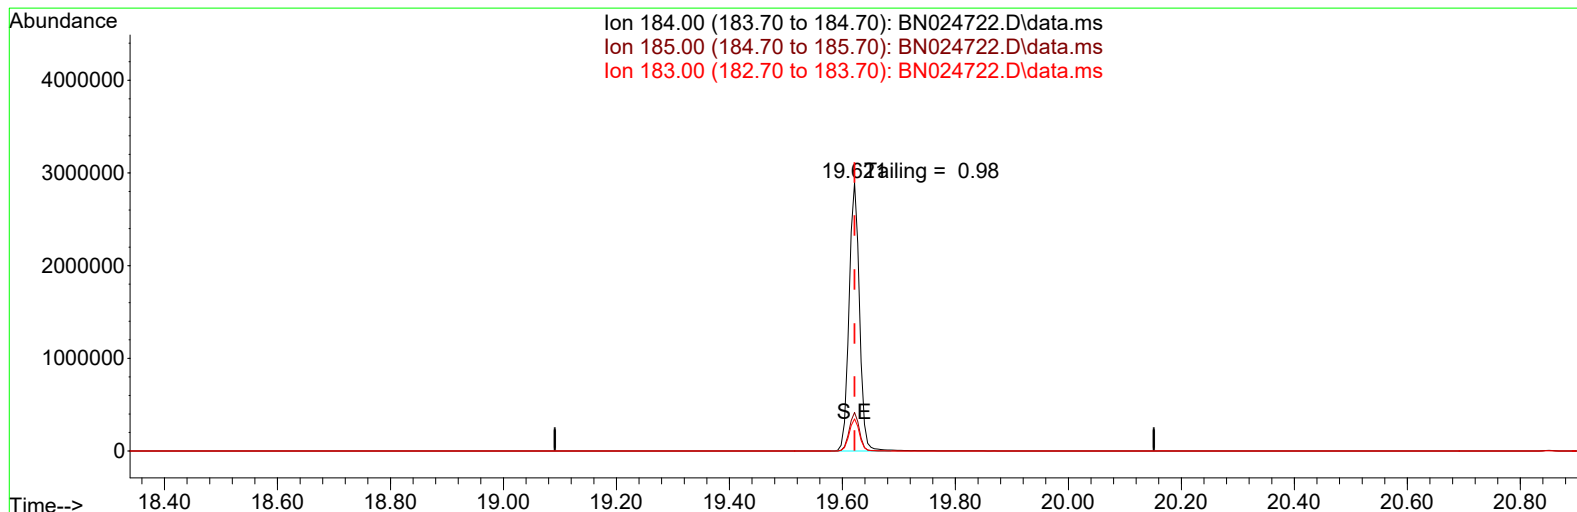

TIC: BN024722.D\data.ms

(77) Benzidine

19.621min (0.000) 861552.51 ng

response 3691517

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.36
183.00	13.20	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/3/2023	BNA_N	<u>BN024722.D</u>
Compound Name	Response	Retention Time
DDT	1882192	20.851
DDD	110583	20.41
DDE	7523	19.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
118106	2000298	5.90

Instrument :
BNA_N
ClientSampleId :
DFTPP