




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040324\
Data File : BN030603.D
Acq On : 02 Apr 2024 01:30
Operator : MA/JU
Sample : PB159927BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK927

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:10:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 02 02:09:33 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

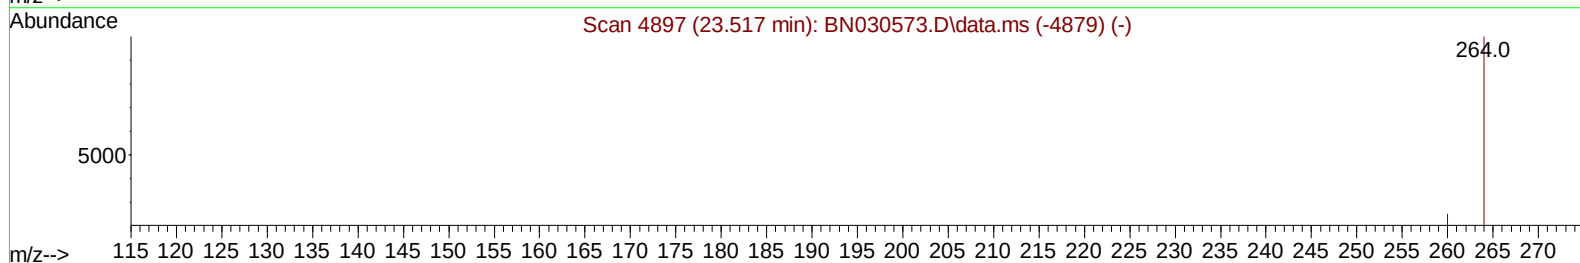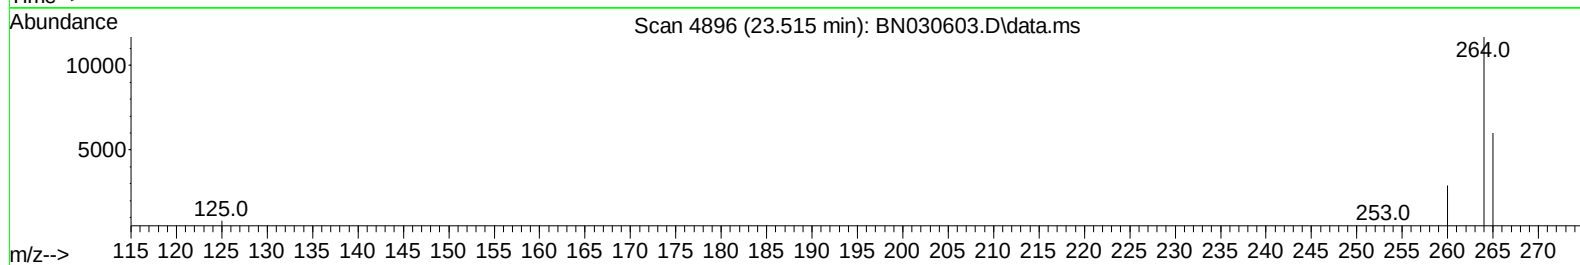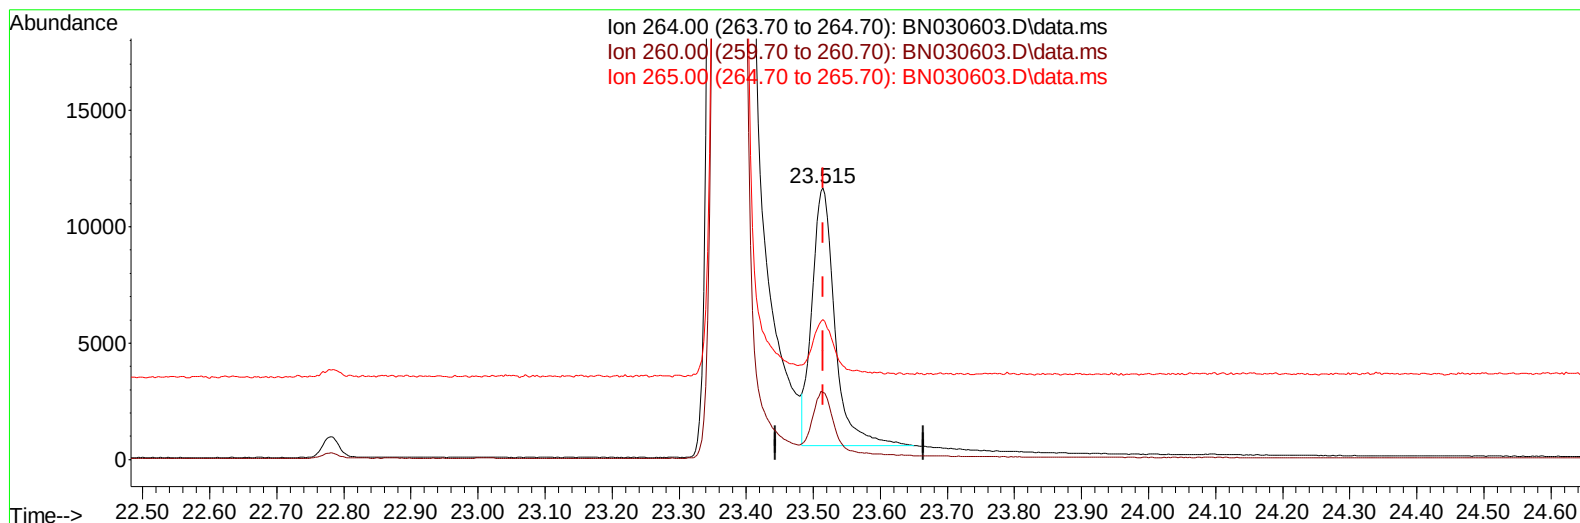

TIC: BN030603.D\data.ms

(23) Perylene-d12 (I)

23.515min (+ 0.000) 0.40 ng/ul

response 26265

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	24.69
265.00	52.70	51.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040324\
Data File : BN030603.D
Acq On : 02 Apr 2024 01:30
Operator : MA/JU
Sample : PB159927BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK927

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 02 02:10:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 02 02:09:33 2024
Response via : Initial Calibration

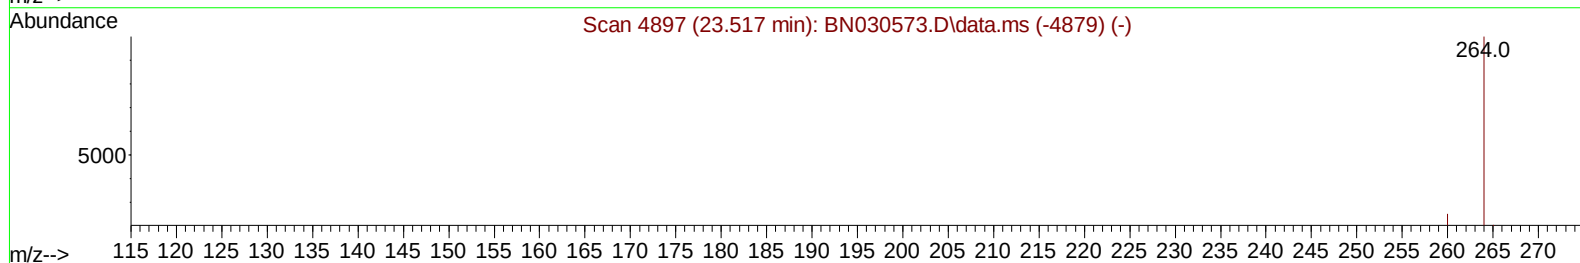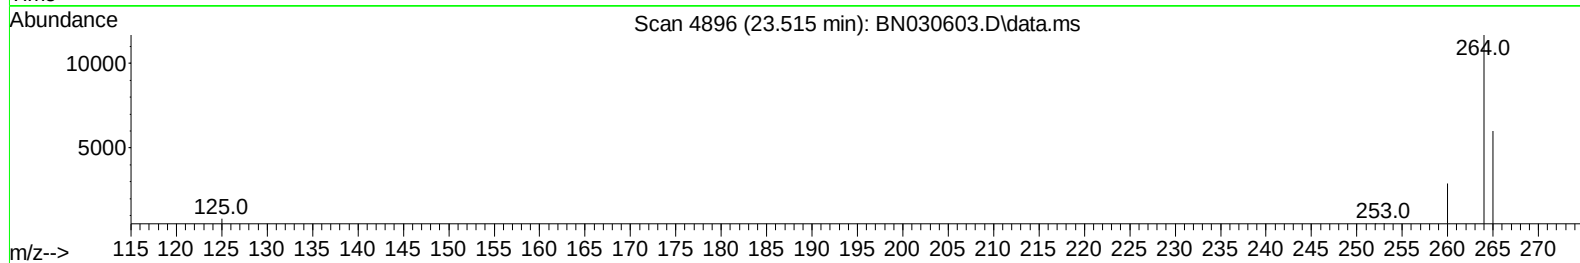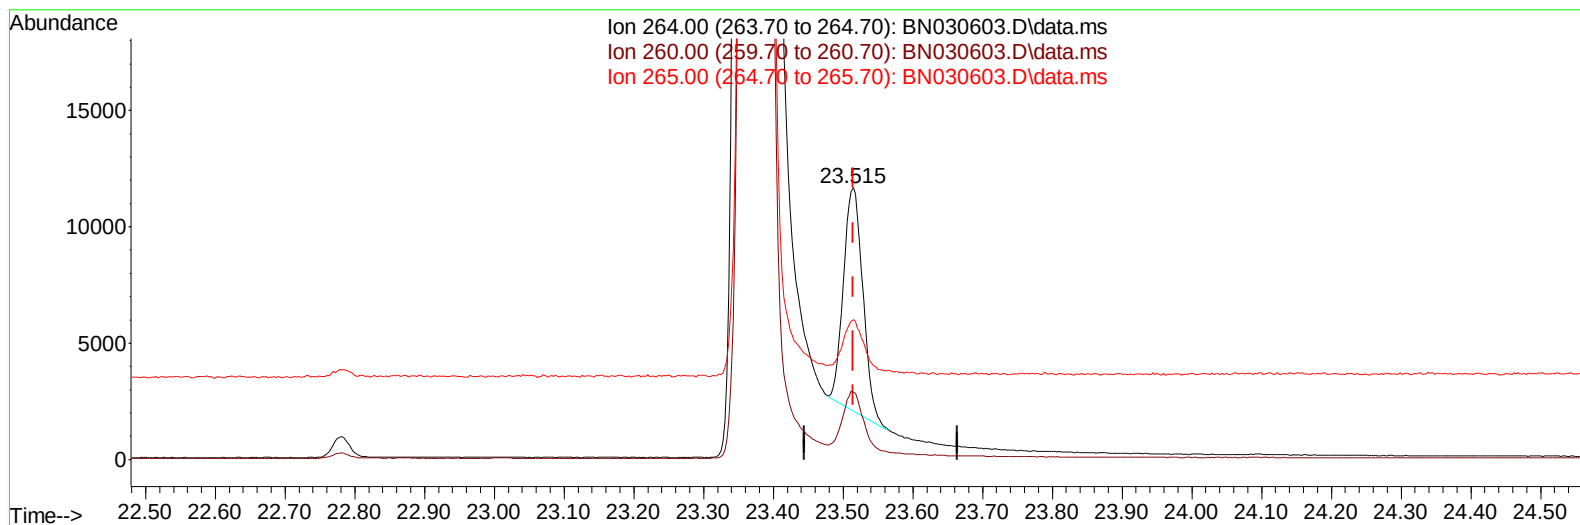

TIC: BN030603.D\data.ms

(23) Perylene-d12 (I)

23.515min (+ 0.000) 0.40 ng/ul m

response 18520

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	24.69
265.00	52.70	51.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040324\
 Data File : BN030603.D
 Acq On : 02 Apr 2024 01:30
 Operator : MA/JU
 Sample : PB159927BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK927

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 02 02:10:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 02 02:09:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	8187	0.400	ng/ul	0.00
4) Naphthalene-d8	10.481	136	25893	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.336	164	14655	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.084	188	32445	0.400	ng/ul	0.00
17) Chrysene-d12	21.279	240	24535	0.400	ng/ul	0.00
23) Perylene-d12	23.515	264	18520m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.198	96	49124	5.476	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.076	152	10870	0.279	ng/ul	0.00
18) Fluoranthene-d10	19.115	212	23397	0.309	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040324\
Data File : BN030603.D
Acq On : 02 Apr 2024 01:30
Operator : MA/JU
Sample : PB159927BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK927

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:10:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 02 02:09:33 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

