




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040324\
Data File : BN030604.D
Acq On : 02 Apr 2024 02:06
Operator : MA/JU
Sample : P1929-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAM0

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:54:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 02 02:09:33 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

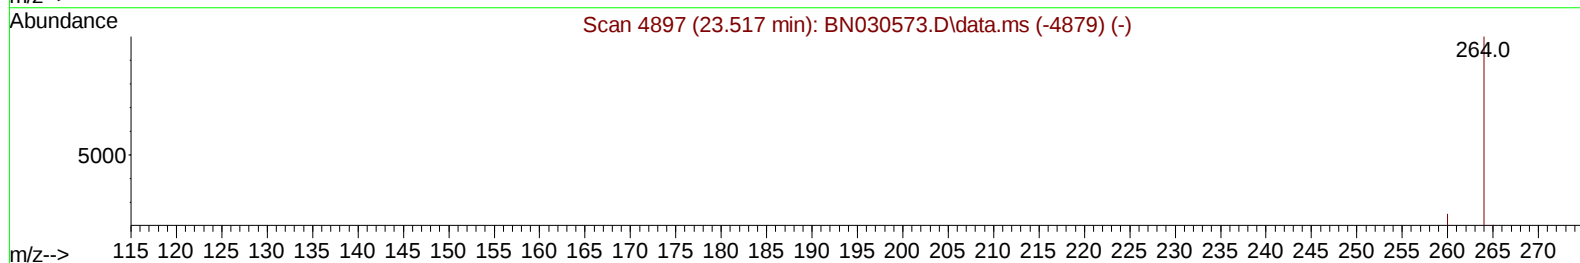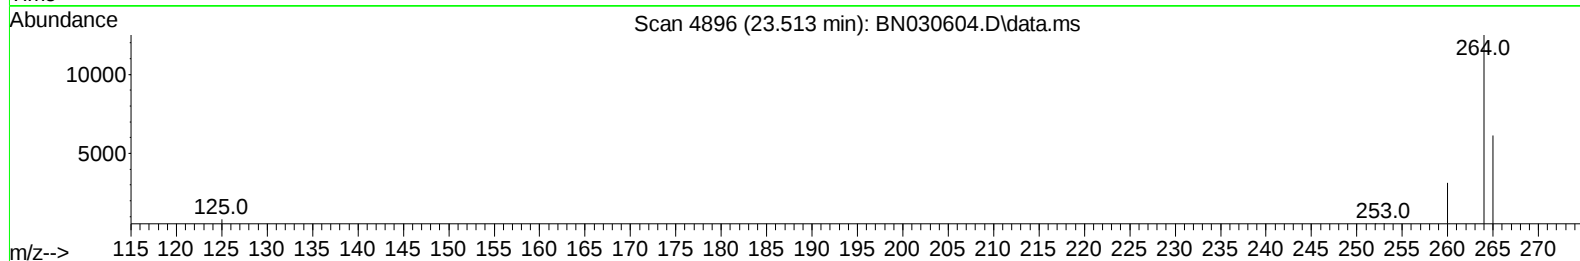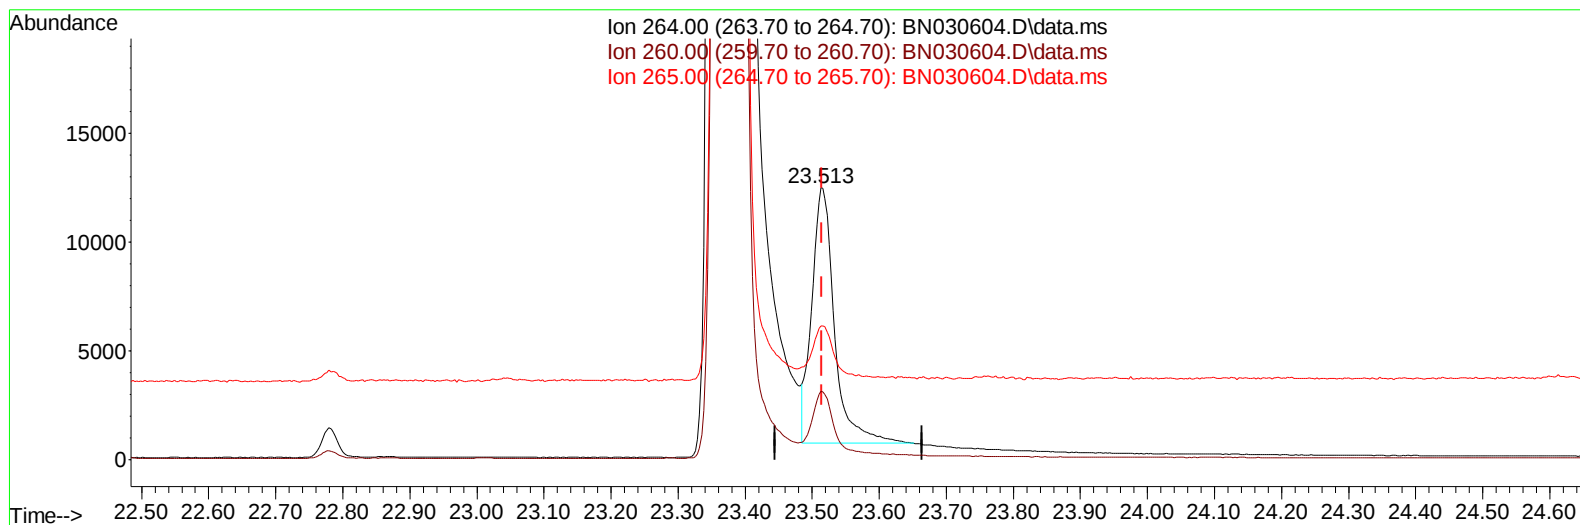

TIC: BN030604.D\data.ms

(23) Perylene-d12 (I)

23.513min (-0.001) 0.40 ng/u1

response 27568

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	25.24
265.00	52.70	49.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040324\
Data File : BN030604.D
Acq On : 02 Apr 2024 02:06
Operator : MA/JU
Sample : P1929-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAM0

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:54:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 02 02:09:33 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

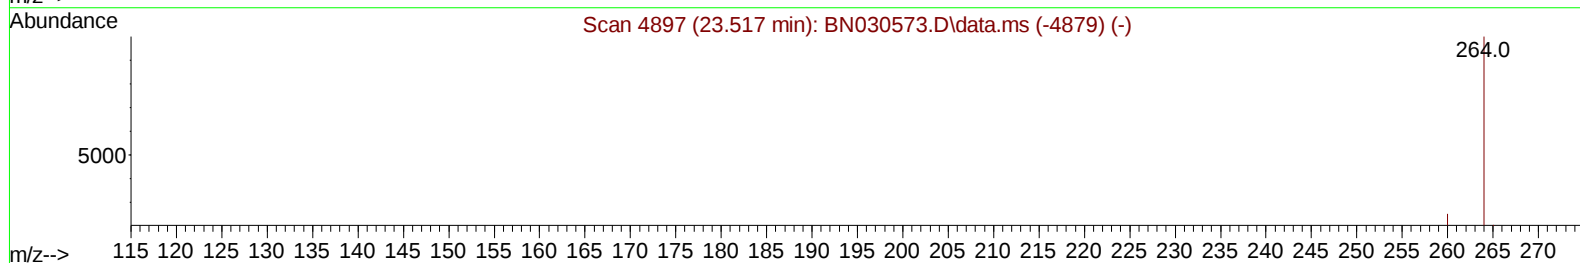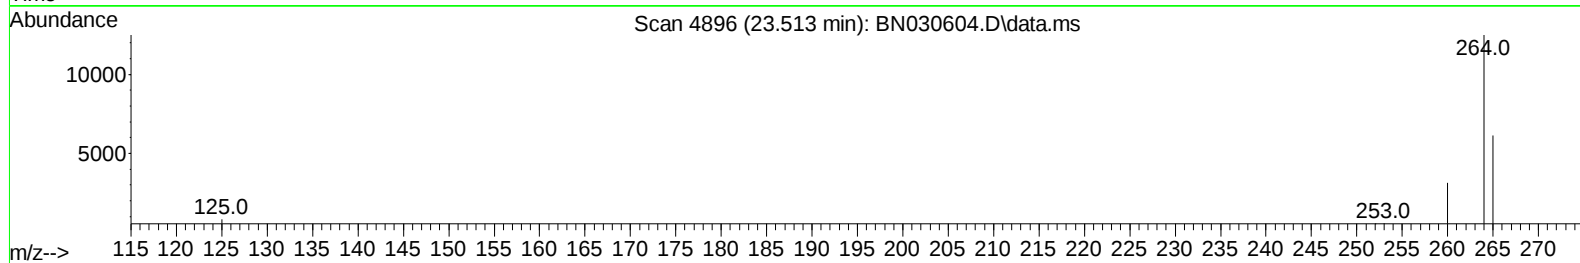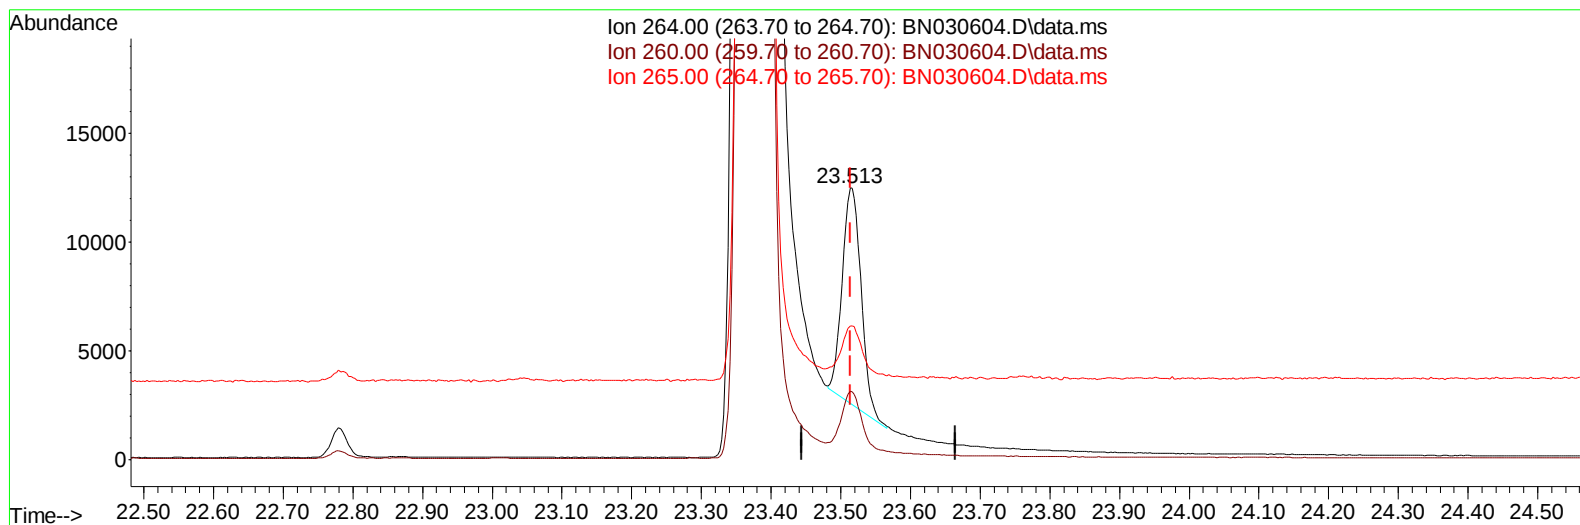

TIC: BN030604.D\data.ms

(23) Perylene-d12 (I)

23.513min (-0.001) 0.40 ng/ul m

response 18525

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.40	25.24
265.00	52.70	49.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040324\
 Data File : BN030604.D
 Acq On : 02 Apr 2024 02:06
 Operator : MA/JU
 Sample : P1929-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AM0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/02/2024
 Supervised By :mohammad ahmed 04/02/2024

Quant Time: Apr 02 02:54:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 02 02:09:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.700	152	7294	0.400	ng/ul	0.00
4) Naphthalene-d8	10.480	136	23014	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.335	164	13174	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.087	188	30056	0.400	ng/ul	0.00
17) Chrysene-d12	21.277	240	24376	0.400	ng/ul	0.00
23) Perylene-d12	23.513	264	18525m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.198	96	38695	4.842	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.074	152	11459	0.331	ng/ul	0.00
18) Fluoranthene-d10	19.119	212	31342	0.416	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040324\
Data File : BN030604.D
Acq On : 02 Apr 2024 02:06
Operator : MA/JU
Sample : P1929-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AM0

Manual IntegrationsAPPROVED

Quant Time: Apr 02 02:54:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN032724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 02 02:09:33 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/02/2024
Supervised By :mohammad ahmed 04/02/2024

