
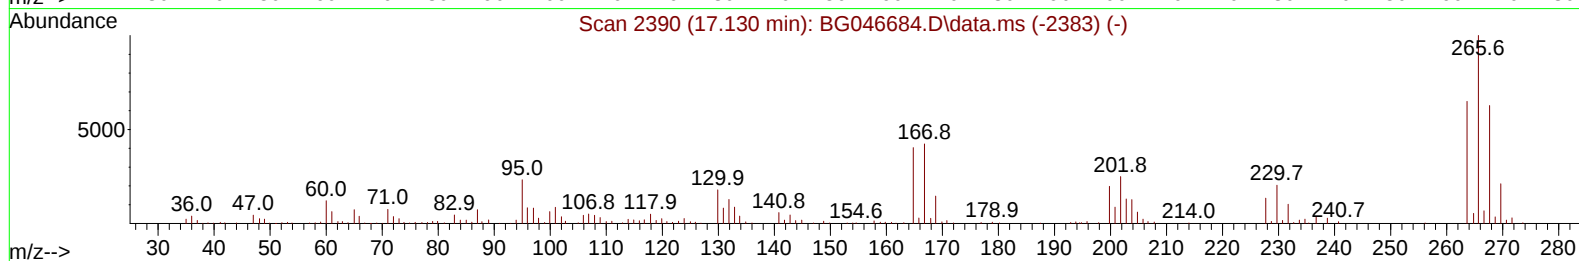
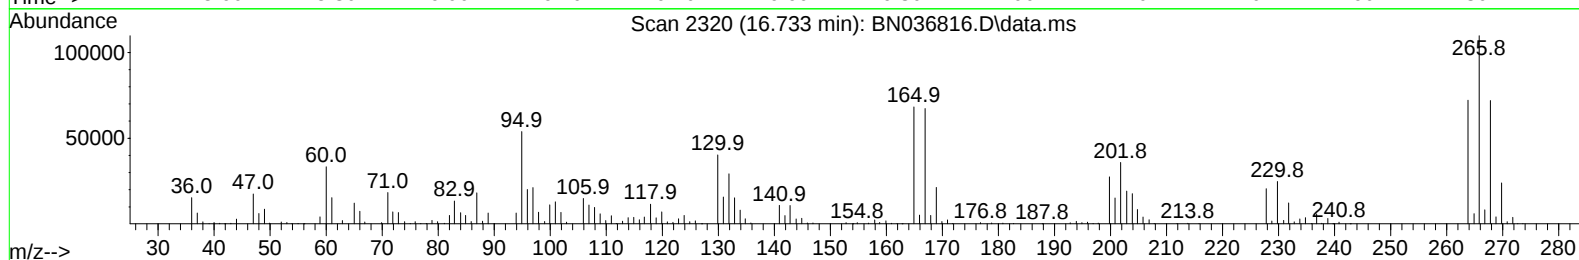


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040325\
Data File : BN036816.D
Acq On : 03 Apr 2025 11:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 14:18:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 03 14:16:27 2025
Response via : Initial Calibration

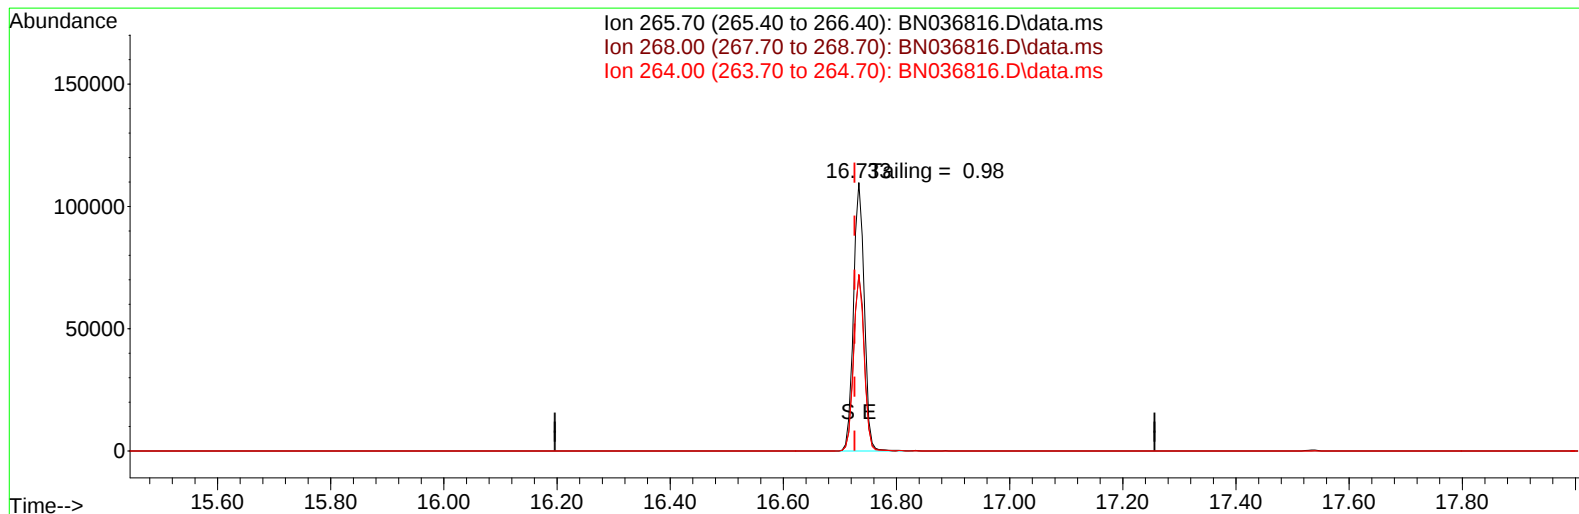

TIC: BN036816.D\data.ms

(70) Pentachlorophenol (C)




16.733min (+ 0.007) 15766.87 ng

response 145132

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.56
264.00	61.60	65.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040325\
Data File : BN036816.D
Acq On : 03 Apr 2025 11:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 14:25:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 03 14:16:27 2025
Response via : Initial Calibration

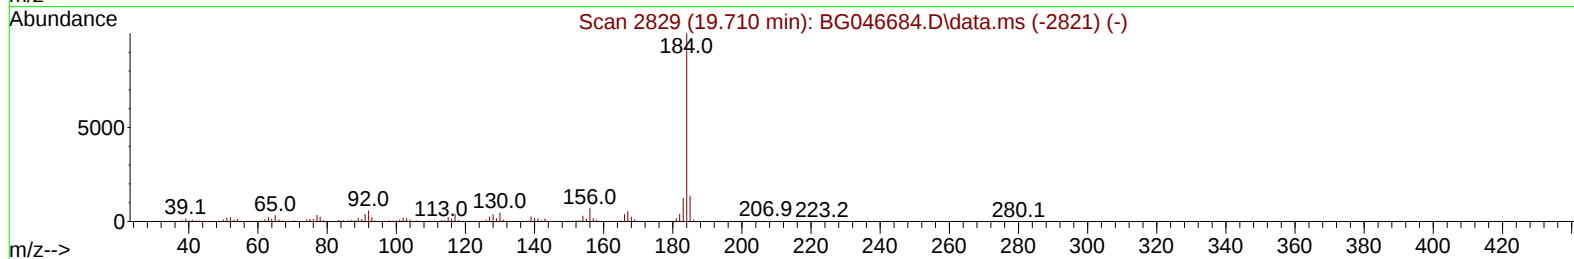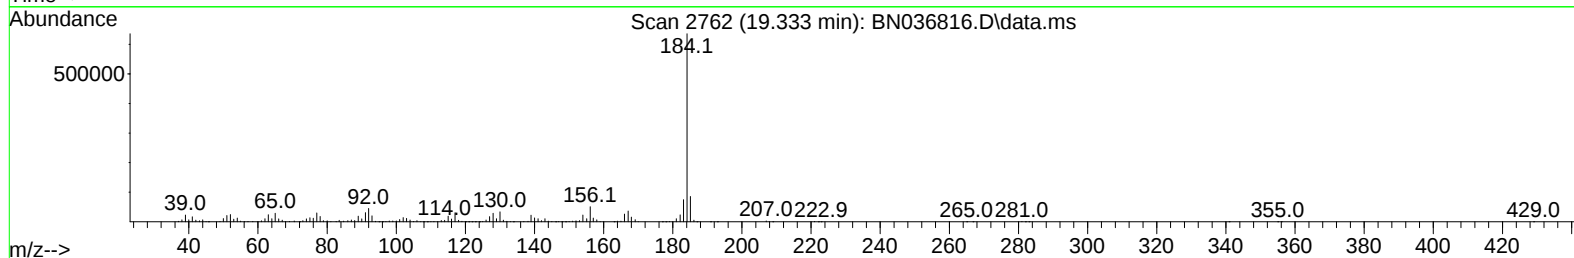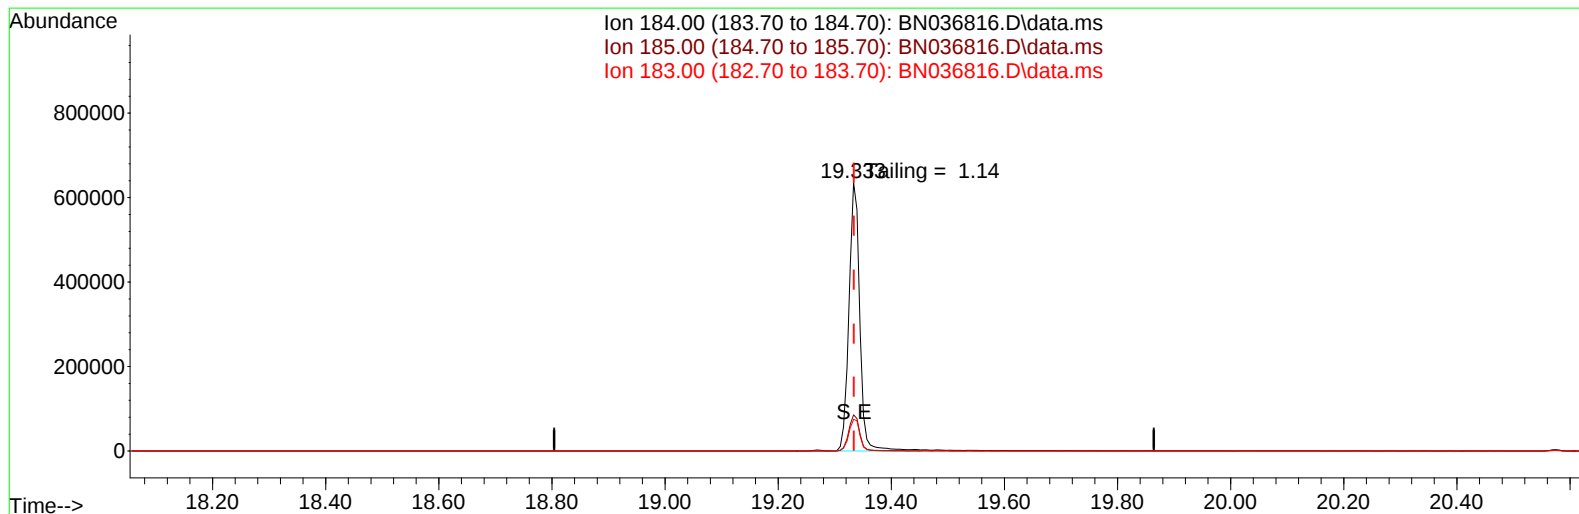

TIC: BN036816.D\data.ms

(77) Benzidine**19.333min (-0.001) 0.00 ng****response 839528**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.48
183.00	13.20	11.75
0.00	0.00	0.00