
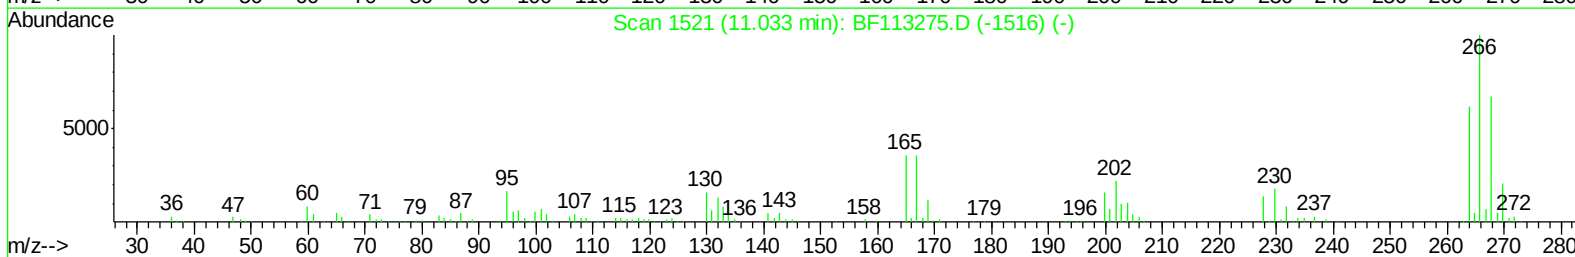
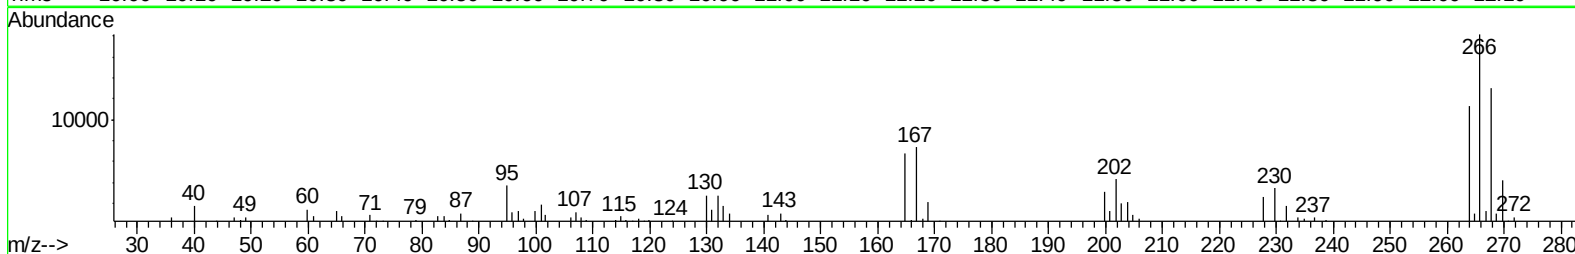


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF032819\
Data File : BF113393.D
Acq On : 29 Mar 2019 1:17
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 09:44:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 26 03:32:08 2019
Response via : Initial Calibration

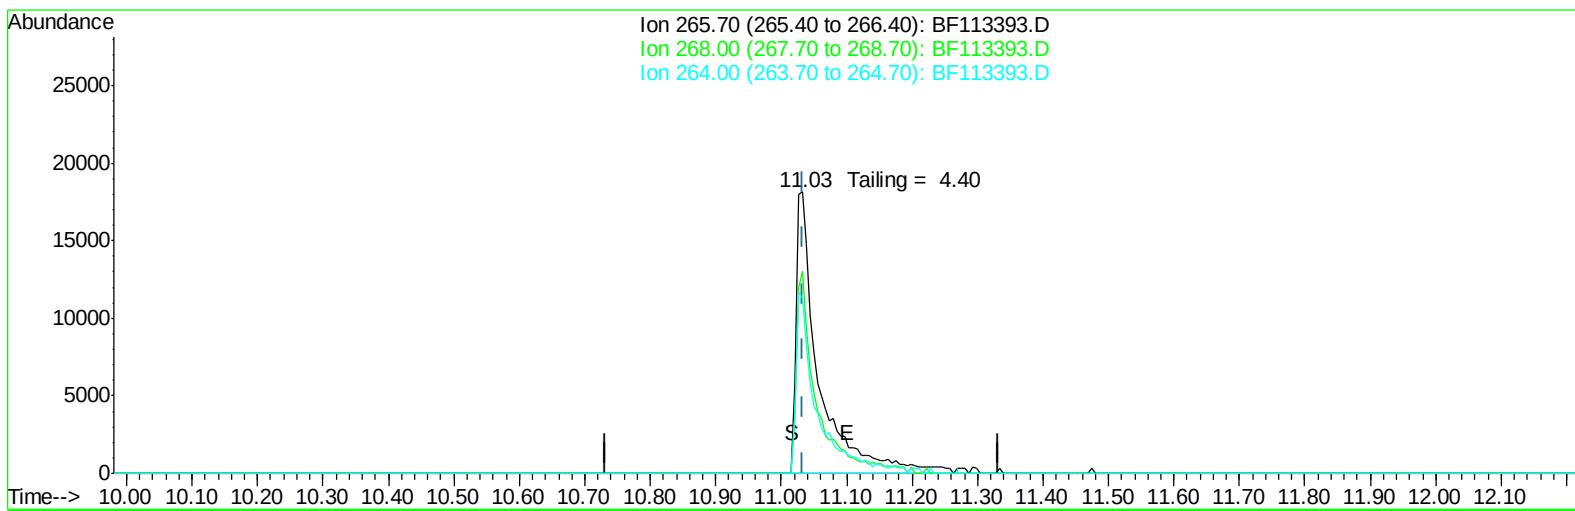

TIC: BF113393.D

(70) Pentachlorophenol (C)




11.033min (+0.000) 54982.96ng m

response 43489

Ion	Exp%	Act%
265.70	100	100
268.00	67.20	72.00
264.00	61.50	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF032819\
Data File : BF113369.D
Acq On : 28 Mar 2019 12:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 09:40:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 26 03:32:08 2019
Response via : Initial Calibration

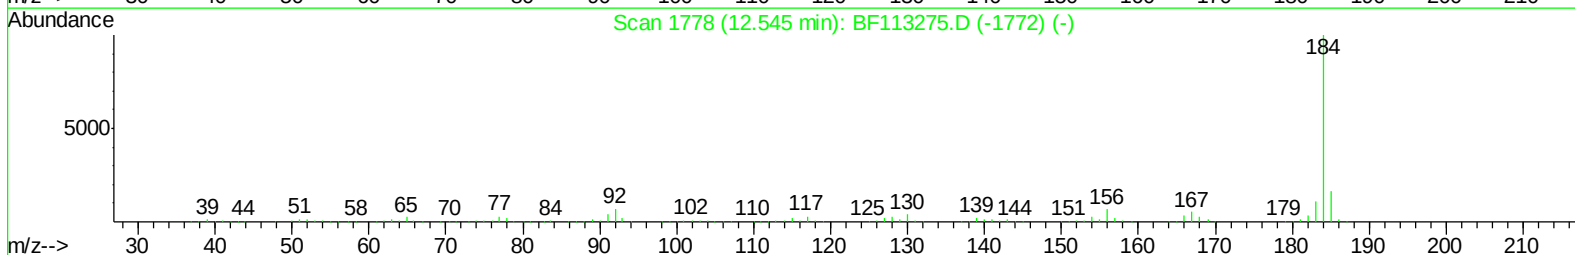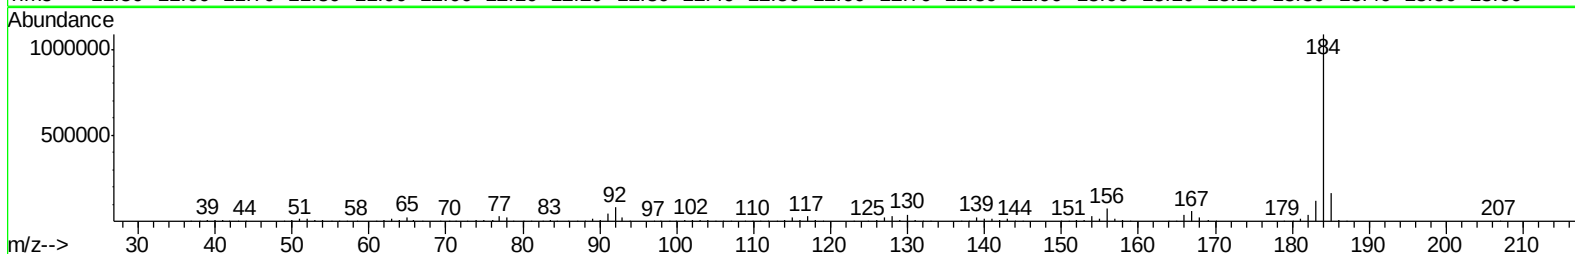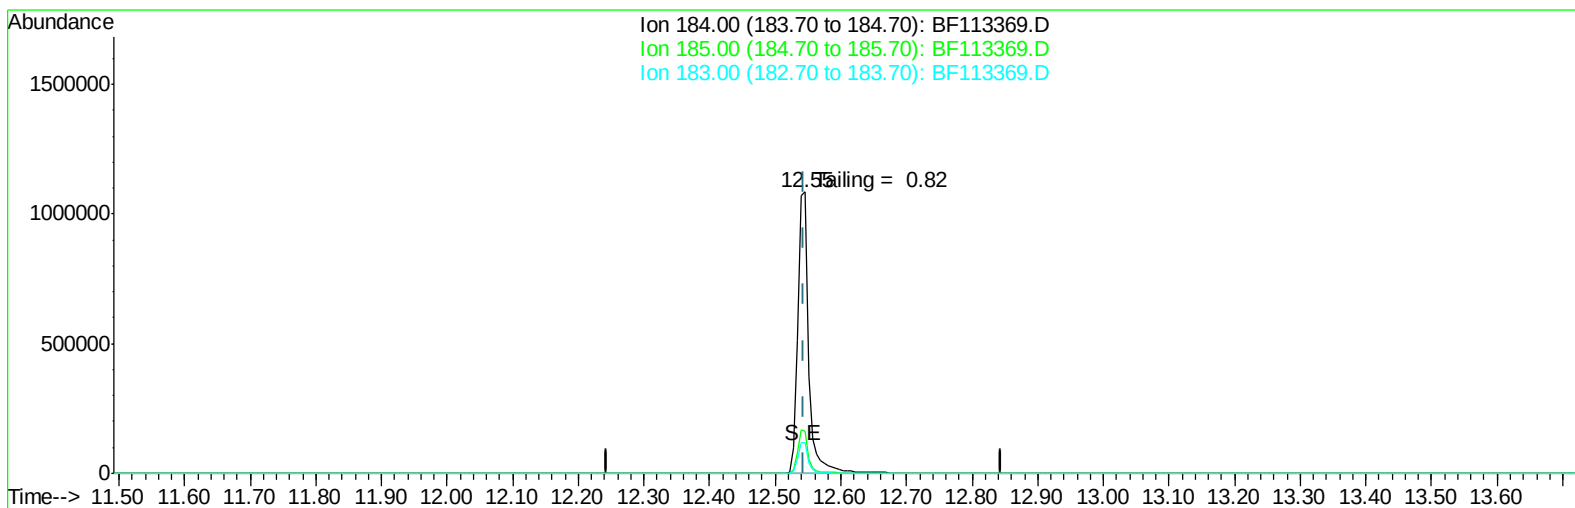

TIC: BF113369.D

(77) Benzidine

12.545min (+0.001) 0.00ng

response 1275783

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.92
183.00	11.20	10.93
0.00	0.00	0.00