

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040419\
 Data File : BN005099.D
 Acq On : 04 Apr 2019 18:42
 Operator : JU/SJ
 Sample : K2245-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TP-1D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.240	378	383	390	rBB	113125	159561	39.21%	7.121%
2	6.828	647	653	659	rBV	112483	173502	42.64%	7.743%
3	7.187	708	714	720	rBB	125353	188875	46.42%	8.429%
4	7.652	788	793	798	rBB	28066	40212	9.88%	1.795%
5	7.969	841	847	852	rBB	89662	135821	33.38%	6.062%
6	8.816	985	991	997	rBB	67512	102777	25.26%	4.587%
7	10.434	1260	1266	1273	rBB	39002	60716	14.92%	2.710%
8	12.916	1681	1688	1694	rBB	195316	281082	69.08%	12.544%
9	13.757	1827	1831	1836	rBB	15353	19045	4.68%	0.850%
10	14.298	1918	1923	1929	rBB2	60933	87014	21.38%	3.883%
11	15.798	2173	2178	2185	rBB	169278	223219	54.86%	9.962%
12	17.051	2385	2391	2397	rBB	78315	104557	25.70%	4.666%
13	19.686	2833	2839	2844	rBV	351873	406909	100.00%	18.160%
14	20.945	3050	3053	3060	rBV	13003	19004	4.67%	0.848%
15	21.251	3100	3105	3111	rBB	103007	118832	29.20%	5.303%
16	22.269	3274	3278	3281	rBV	4231	4648	1.14%	0.207%
17	22.763	3358	3362	3366	rBV	4469	5252	1.29%	0.234%
18	23.321	3453	3457	3461	rVB	3359	4588	1.13%	0.205%
19	23.480	3477	3484	3491	rVB2	58474	105074	25.82%	4.689%


Sum of corrected areas: 2240688

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040419\
Data File : BN005099.D
Acq On : 04 Apr 2019 18:42
Operator : JU/SJ
Sample : K2245-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TP-1D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

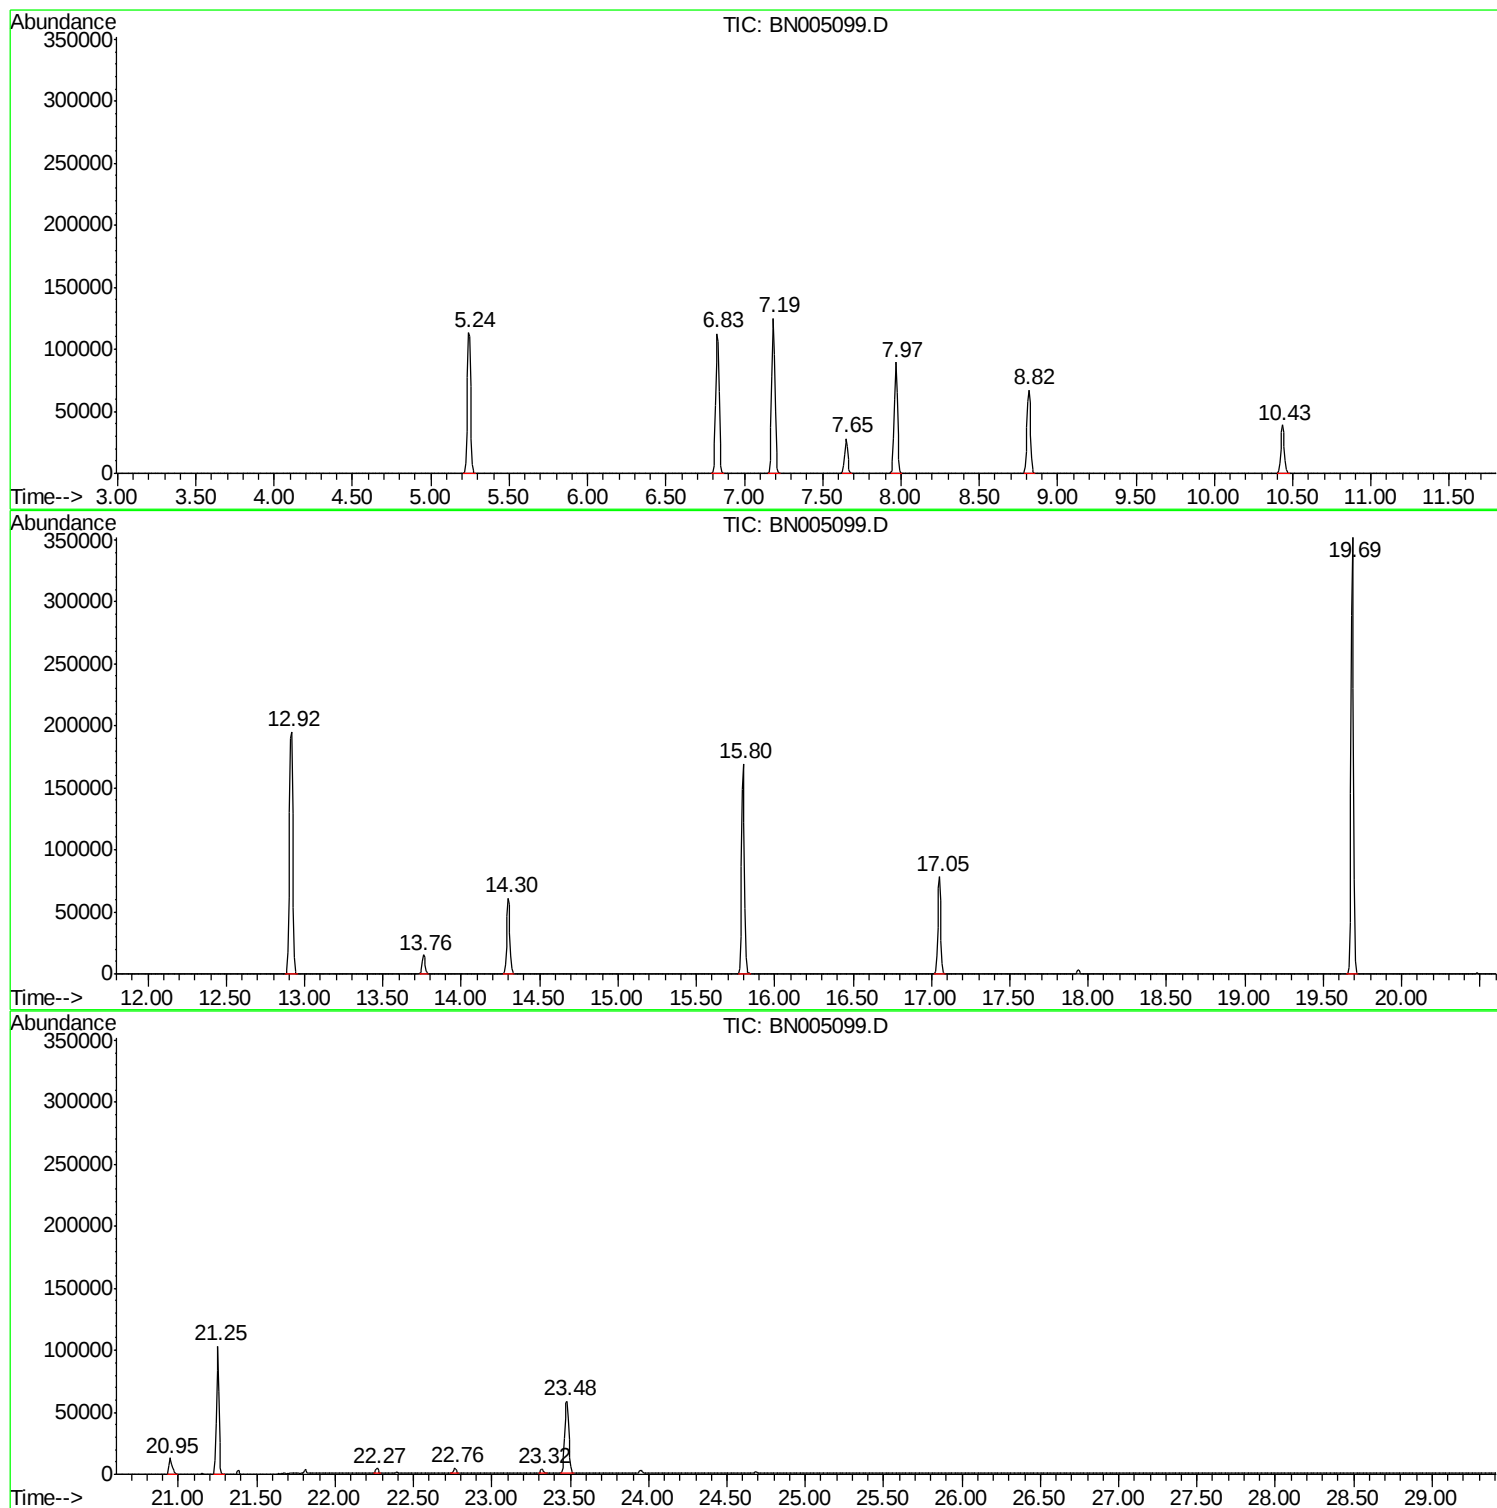

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040419\
Data File : BN005099.D
Acq On : 04 Apr 2019 18:42
Operator : JU/SJ
Sample : K2245-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TP-1D










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.19 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	93.94 ng	188875	1,4-Dichlorobenzene-d4	7.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

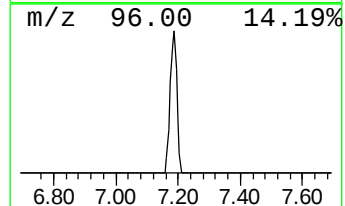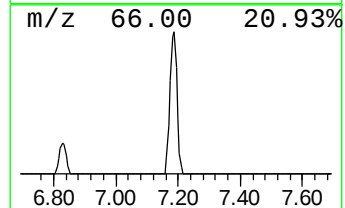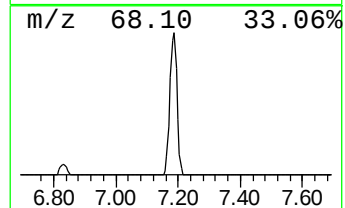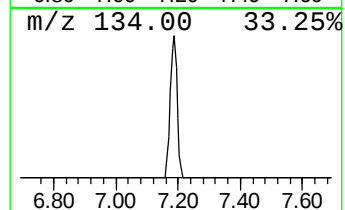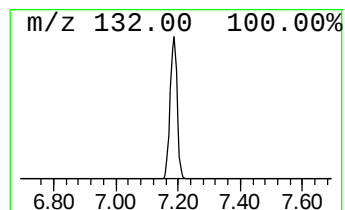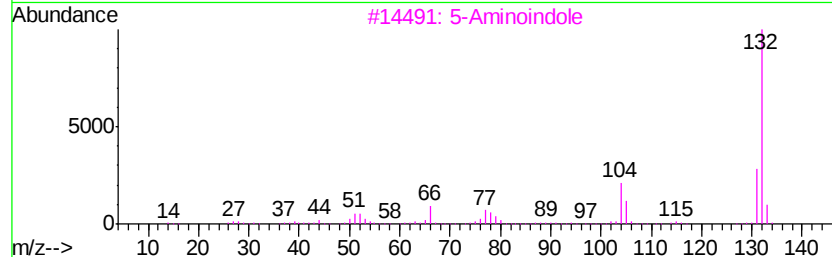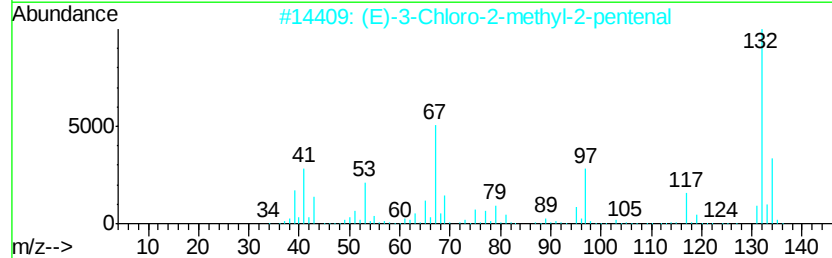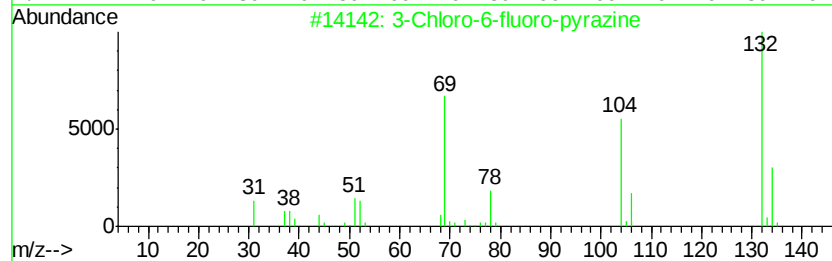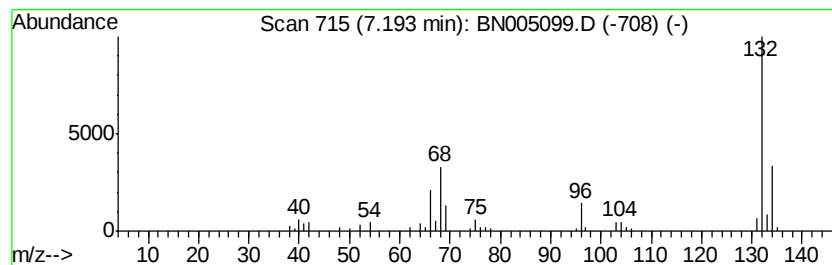

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040419\
Data File : BN005099.D
Acq On : 04 Apr 2019 18:42
Operator : JU/SJ
Sample : K2245-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TP-1D










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 17-Pentatriacontene Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.95	3.20 ng	19004	Chrysene-d12	21.25

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	17-Pentatriacontene	491	C35H70	006971-40-0	90
2		Octacosyl trifluoroacetate	506	C30H57F3O2	1000351-74-9	80
3		Docosyl pentafluoropropionate	472	C25H45F5O2	1000351-80-9	80
4		Hexatriacontyl pentafluoropropio...	669	C39H73F5O2	1000351-89-0	72
5		Isobutyl tetradecyl carbonate	314	C19H38O3	959275-58-2	72

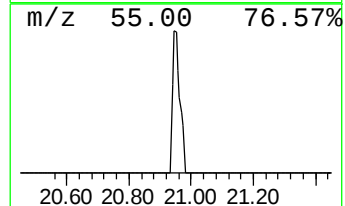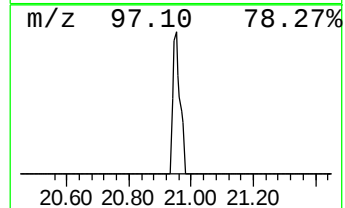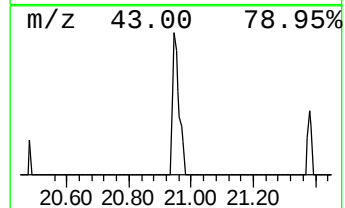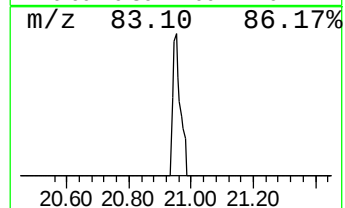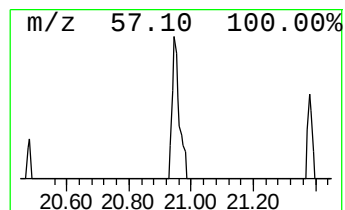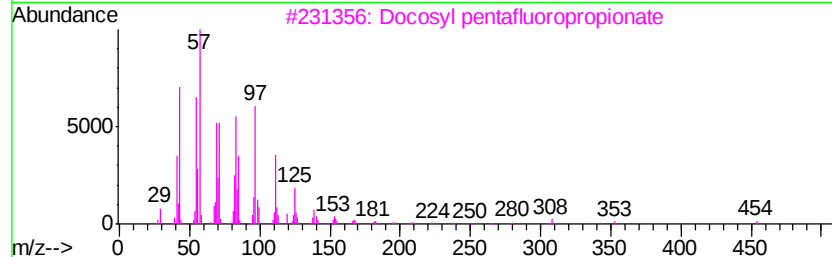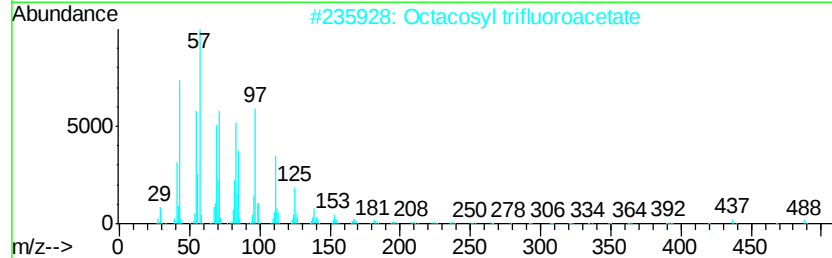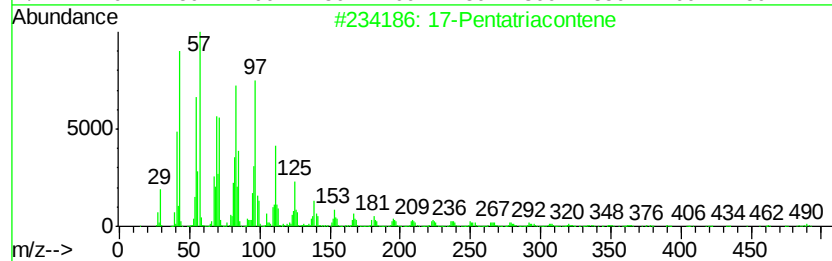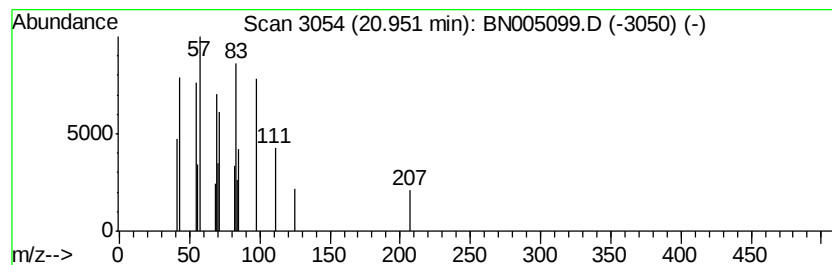

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040419\
Data File : BN005099.D
Acq On : 04 Apr 2019 18:42
Operator : JU/SJ
Sample : K2245-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TP-1D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.19	7.19	93.9	ng	188875	1	7.65	40212	20.0
17-Pentatriacontene	20.95	3.2	ng	19004	5	21.25	118832	20.0