

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040419\
 Data File : BN005100.D
 Acq On : 04 Apr 2019 19:17
 Operator : JU/SJ
 Sample : K2245-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TP-3S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.240	378	383	390	rBB	71146	95534	36.66%	6.242%
2	6.828	647	653	660	rBB	71447	104987	40.28%	6.860%
3	7.181	708	713	720	rBB	75135	114610	43.97%	7.488%
4	7.652	788	793	798	rBB	24657	36059	13.84%	2.356%
5	7.969	841	847	852	rBB	56052	84840	32.55%	5.543%
6	8.816	985	991	997	rBB	38828	61134	23.46%	3.994%
7	10.434	1260	1266	1273	rBB	36245	56496	21.68%	3.691%
8	12.910	1682	1687	1693	rBB	126682	176434	67.70%	11.528%
9	13.757	1827	1831	1836	rBB	9426	11348	4.35%	0.741%
10	14.298	1918	1923	1929	rBB2	56727	80712	30.97%	5.274%
11	15.798	2173	2178	2184	rBB	97480	129066	49.52%	8.433%
12	17.051	2386	2391	2396	rBV2	72817	97483	37.40%	6.369%
13	19.116	2739	2742	2746	rBB	3874	4493	1.72%	0.294%
14	19.486	2801	2805	2808	rBB	3682	4181	1.60%	0.273%
15	19.686	2834	2839	2844	rBB	228631	260630	100.00%	17.029%
16	21.251	3098	3105	3110	rBV	92419	109285	41.93%	7.141%
17	22.268	3275	3278	3282	rVB	2903	2839	1.09%	0.185%
18	22.768	3359	3363	3366	rBV	2703	3197	1.23%	0.209%
19	23.321	3454	3457	3460	rBV	2431	2962	1.14%	0.194%
20	23.480	3477	3484	3493	rVB	51777	94198	36.14%	6.155%


Sum of corrected areas: 1530488

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040419\
Data File : BN005100.D
Acq On : 04 Apr 2019 19:17
Operator : JU/SJ
Sample : K2245-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TP-3S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

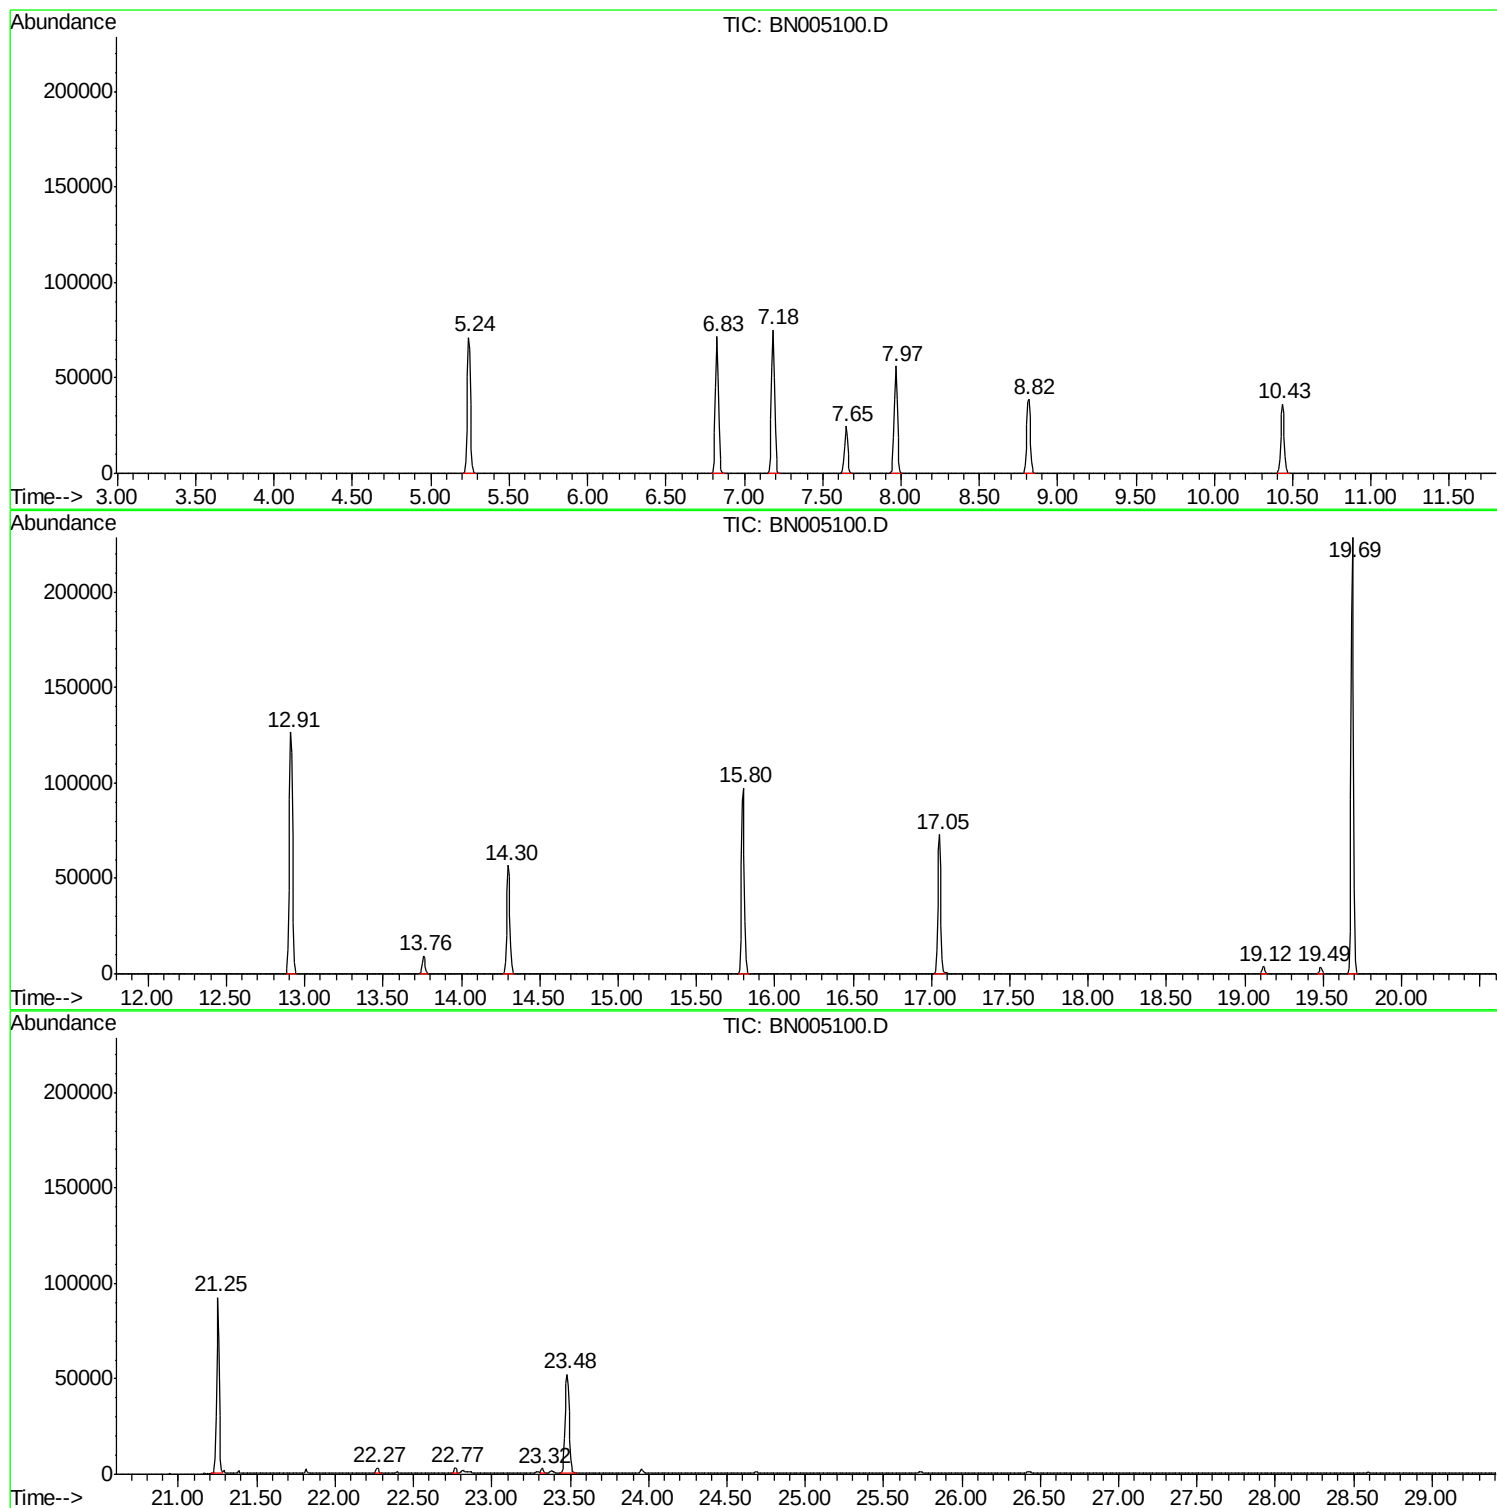

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040419\
Data File : BN005100.D
Acq On : 04 Apr 2019 19:17
Operator : JU/SJ
Sample : K2245-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TP-3S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.18 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.18	63.57 ng	114610	1,4-Dichlorobenzene-d4	7.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

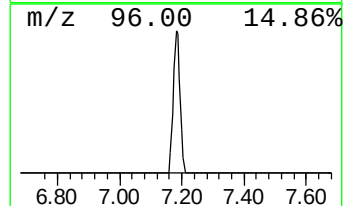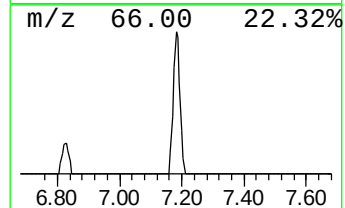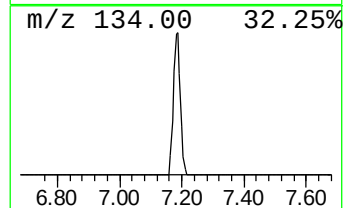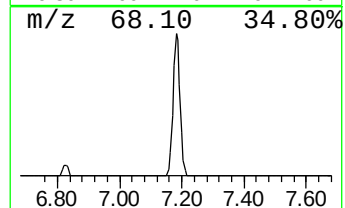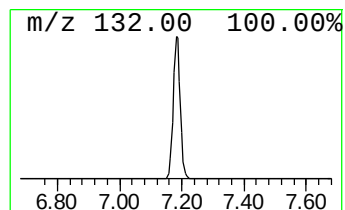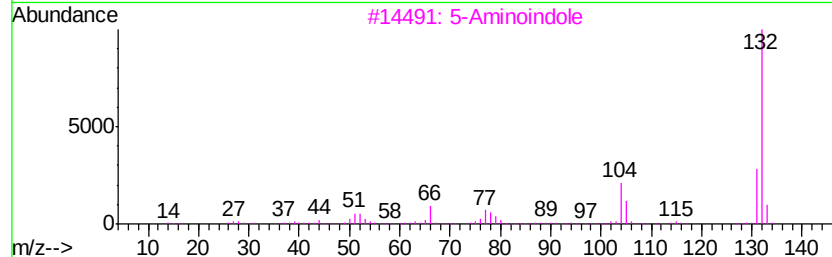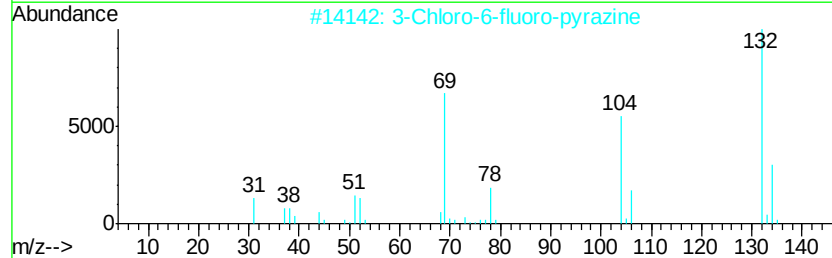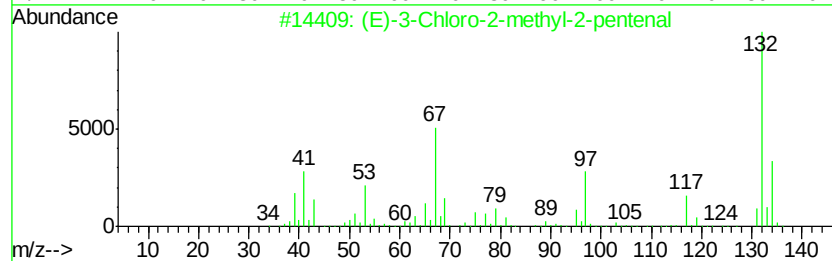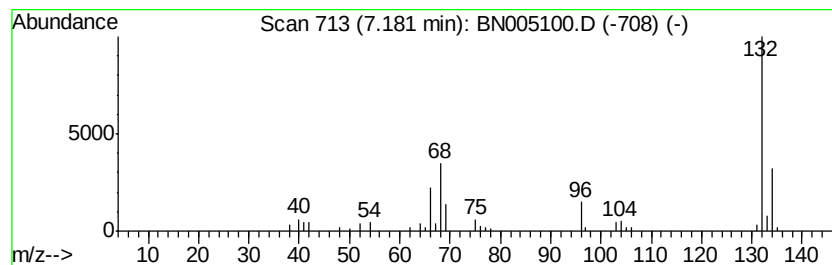

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040419\
Data File : BN005100.D
Acq On : 04 Apr 2019 19:17
Operator : JU/SJ
Sample : K2245-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TP-3S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.18	7.18	63.6	ng	114610	1	7.65	36059	20.0