
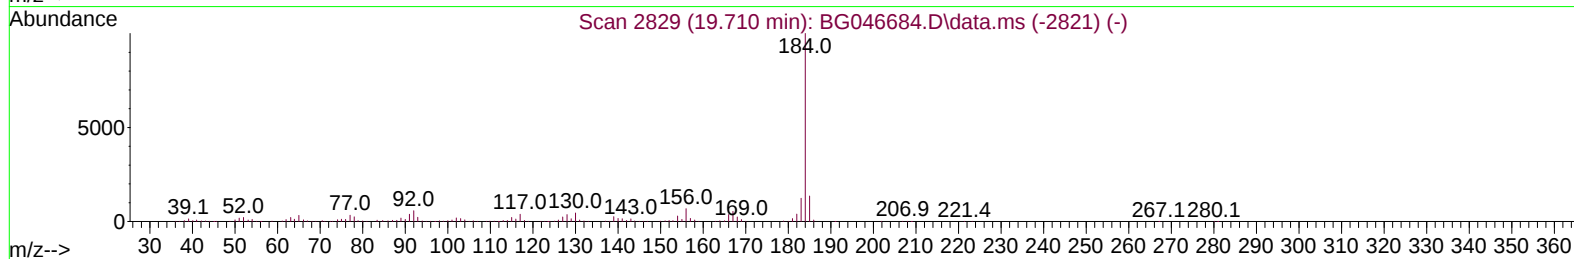
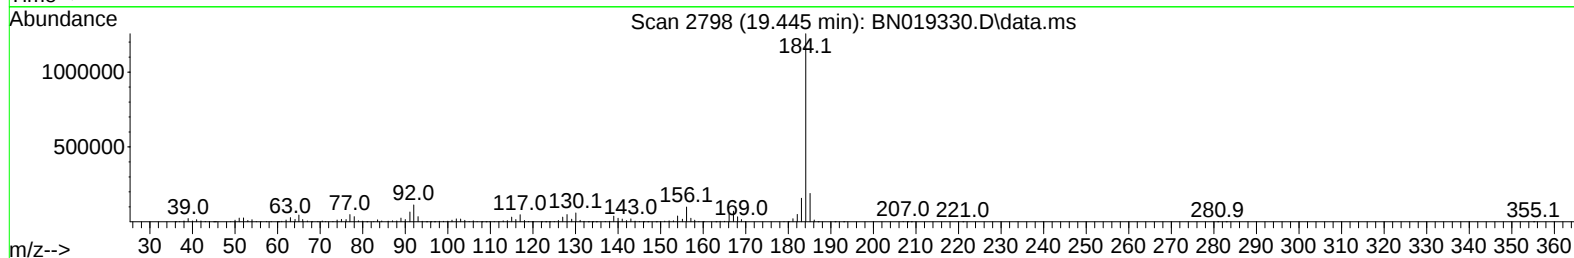


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040422\
Data File : BN019330.D
Acq On : 04 Apr 2022 23:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 17:41:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

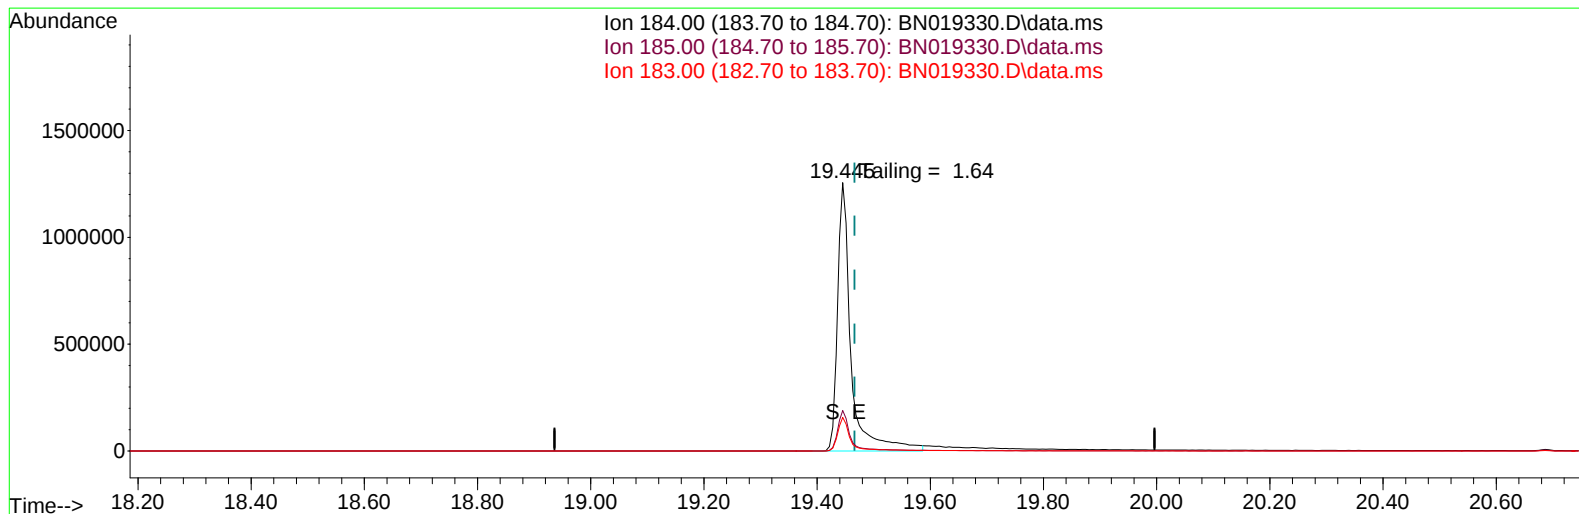

TIC: BN019330.D\data.ms

(77) Benzidine




19.445min (-0.021) 0.00 ng

response 2180330

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.07
183.00	13.20	12.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040422\
Data File : BN019330.D
Acq On : 04 Apr 2022 23:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 17:41:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

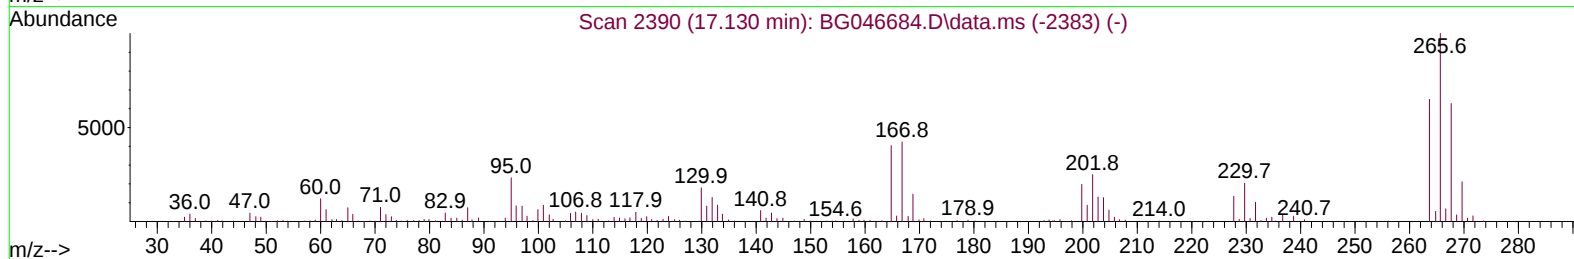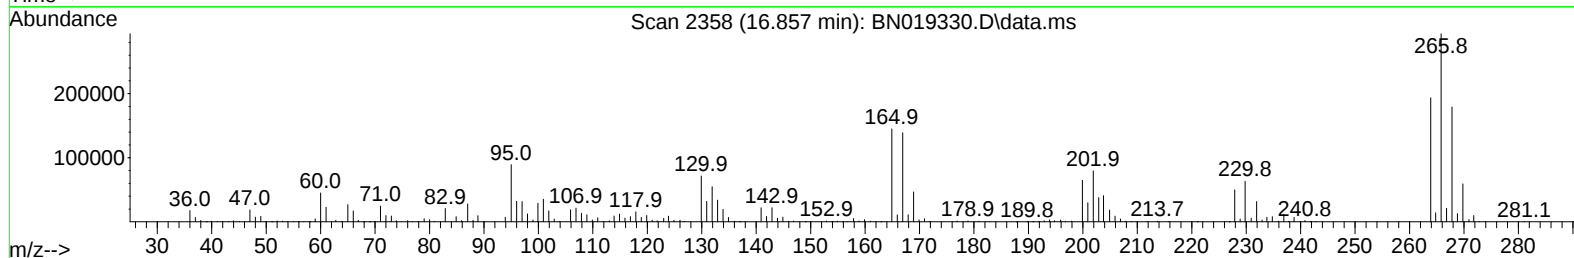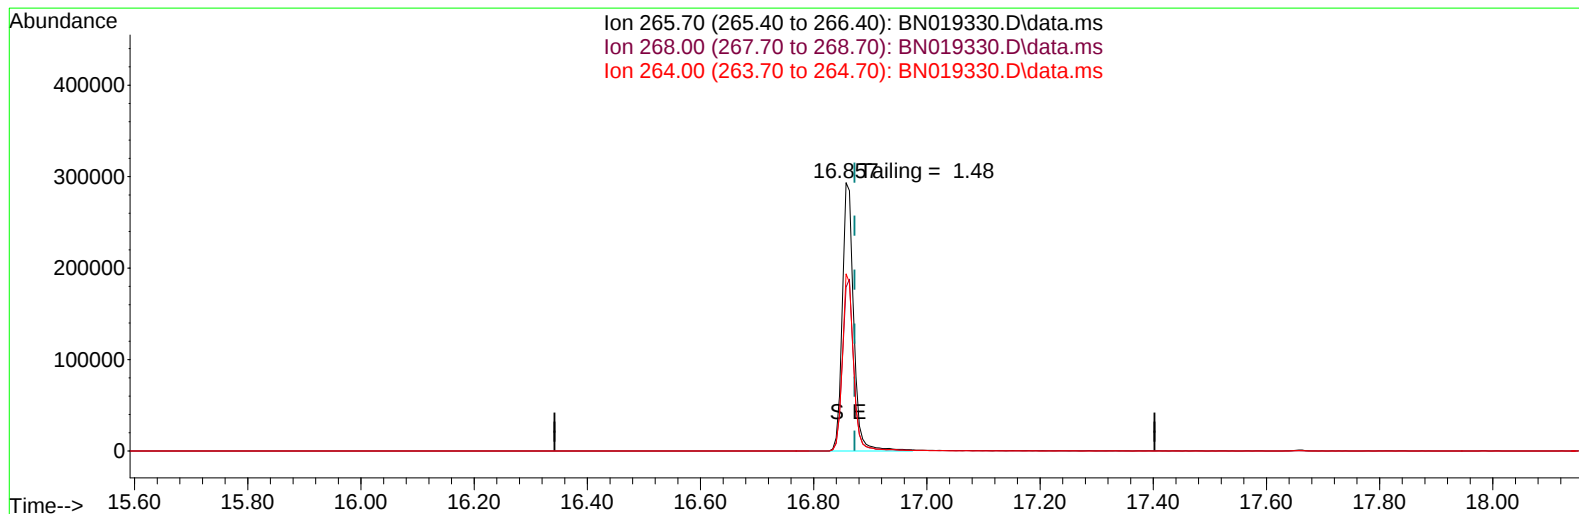

TIC: BN019330.D\data.ms

(70) Pentachlorophenol (C)

16.857min (-0.015) 17309.63 ng

response 415132

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.05
264.00	61.60	66.00
0.00	0.00	0.00