
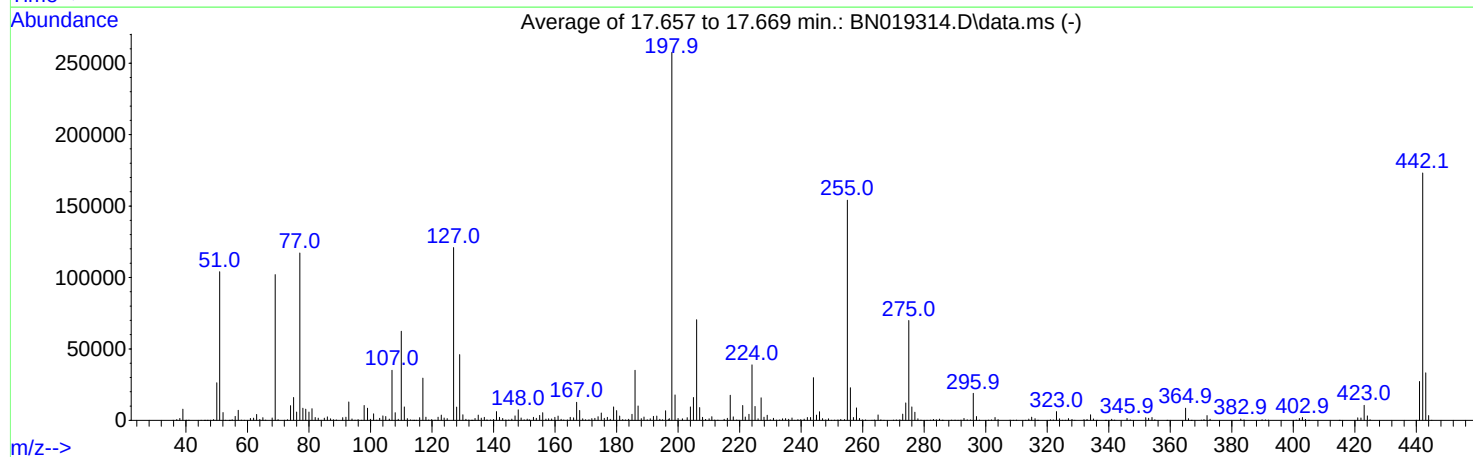


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040422\
 Data File : BN019314.D
 Acq On : 04 Apr 2022 11:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 04 17:40:00 2022

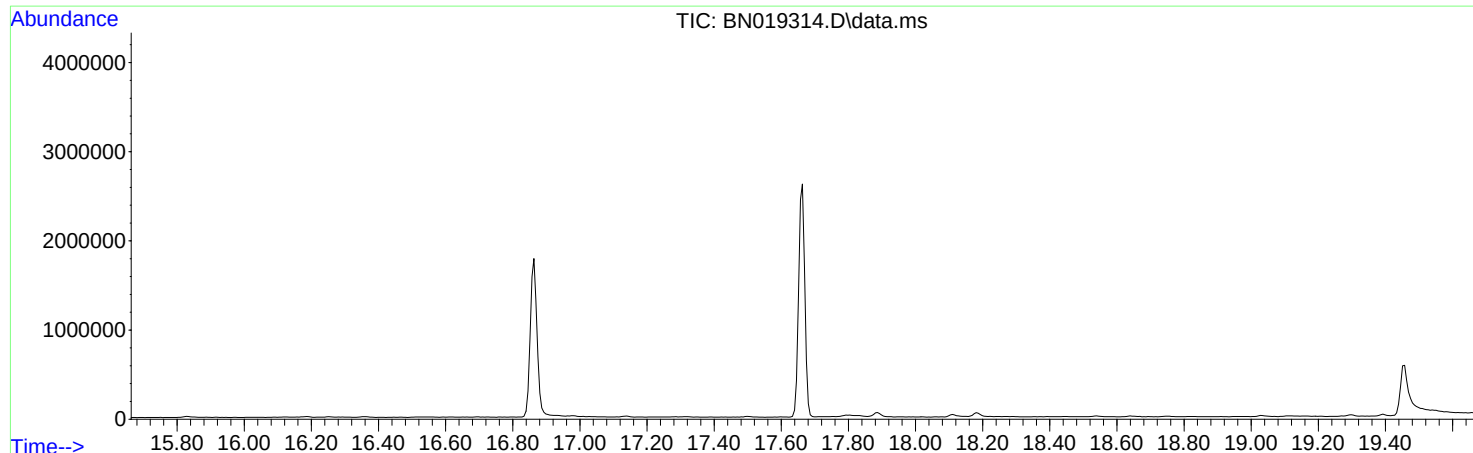




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	103988	PASS
68	69	0.00	2	1.7	1723	PASS
69	198	0.00	100	39.6	101987	PASS
70	69	0.00	2	0.6	617	PASS
127	198	10	80	47.0	120963	PASS
197	198	0.00	2	0.5	1204	PASS
198	198	100	100	100.0	257472	PASS
199	198	5	9	6.9	17776	PASS
275	198	10	60	27.1	69899	PASS
365	198	1	100	3.3	8518	PASS
441	198	0.01	100	10.6	27184	PASS
442	442	50	100	100.0	173120	PASS
443	442	15	24	19.2	33315	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040422\
Data File : BN019314.D
Acq On : 04 Apr 2022 11:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 04 15:15:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

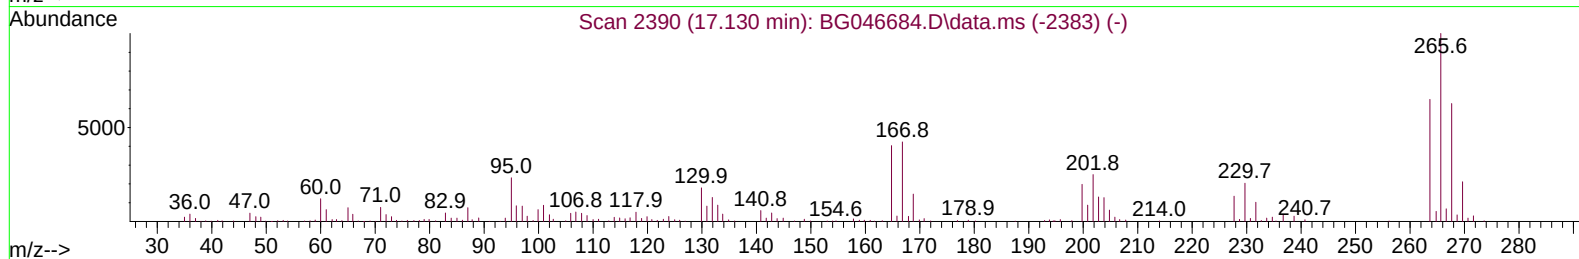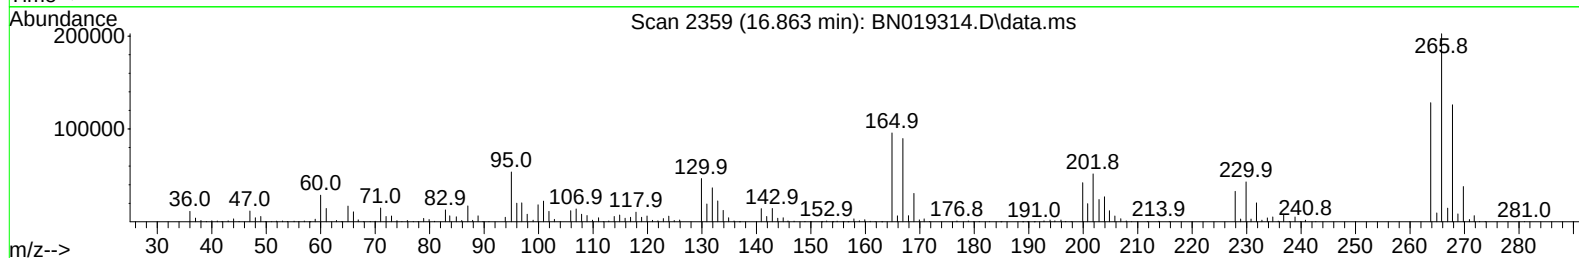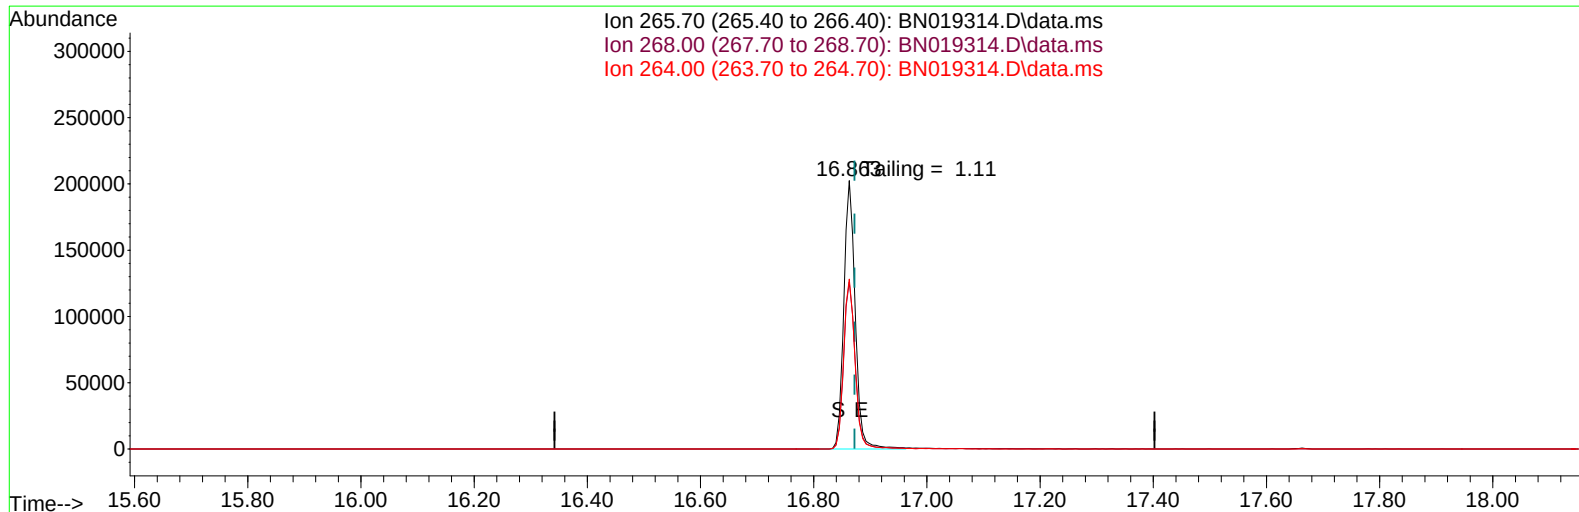

TIC: BN019314.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.009) 20123.03 ng




response 285994

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.22
264.00	61.60	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040422\
Data File : BN019314.D
Acq On : 04 Apr 2022 11:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 04 15:15:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

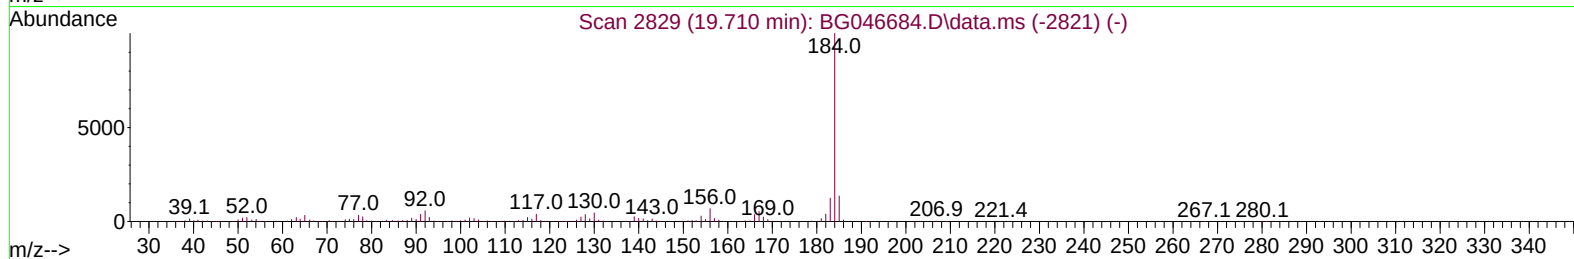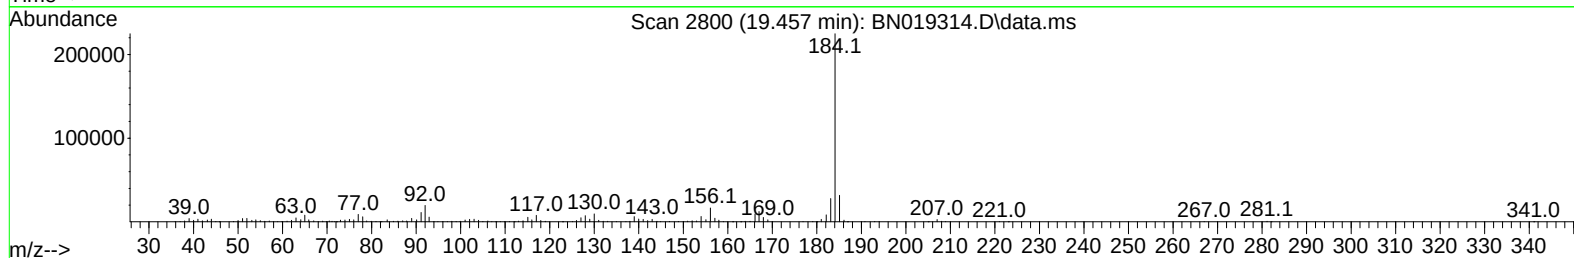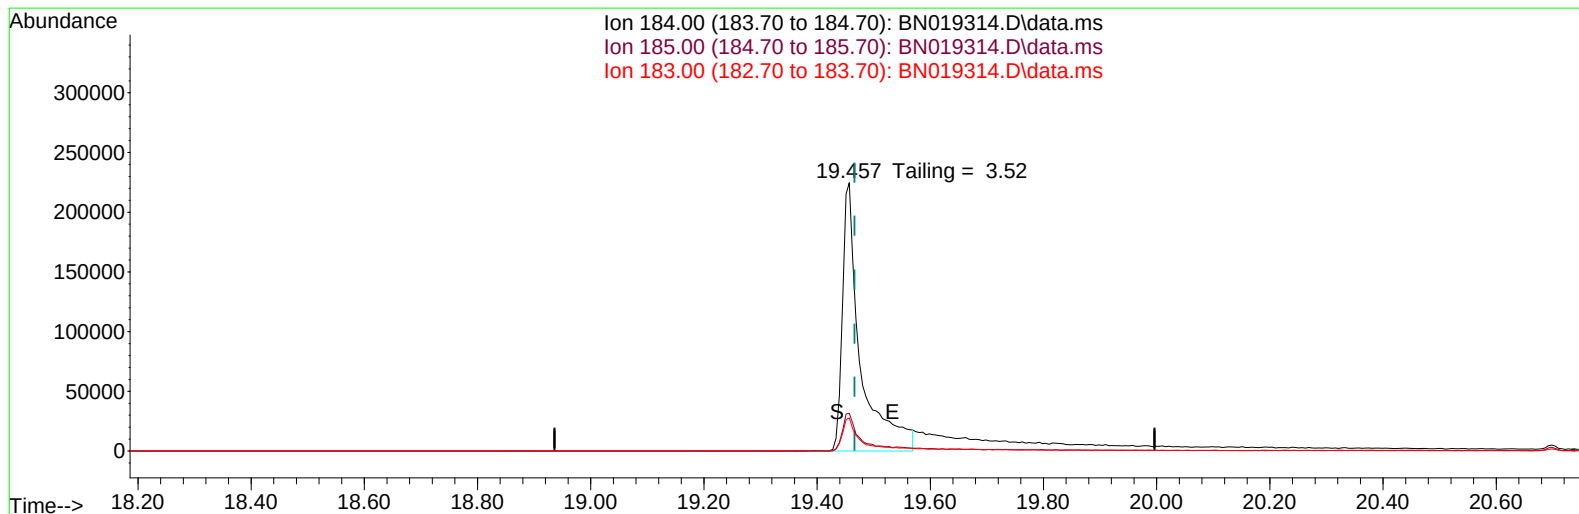

TIC: BN019314.D\data.ms

(77) Benzidine

19.457min (-0.009) 0.00 ng

response 564253

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	12.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/4/2022	BNA_N	<u>BN019314.D</u>
Compound Name	Response	Retention Time
DDT	906172	20.69
DDD	9909	20.25
DDE	265	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10174	916346	1.11

Instrument :
BNA_N
ClientSampleId :
DFTPP