
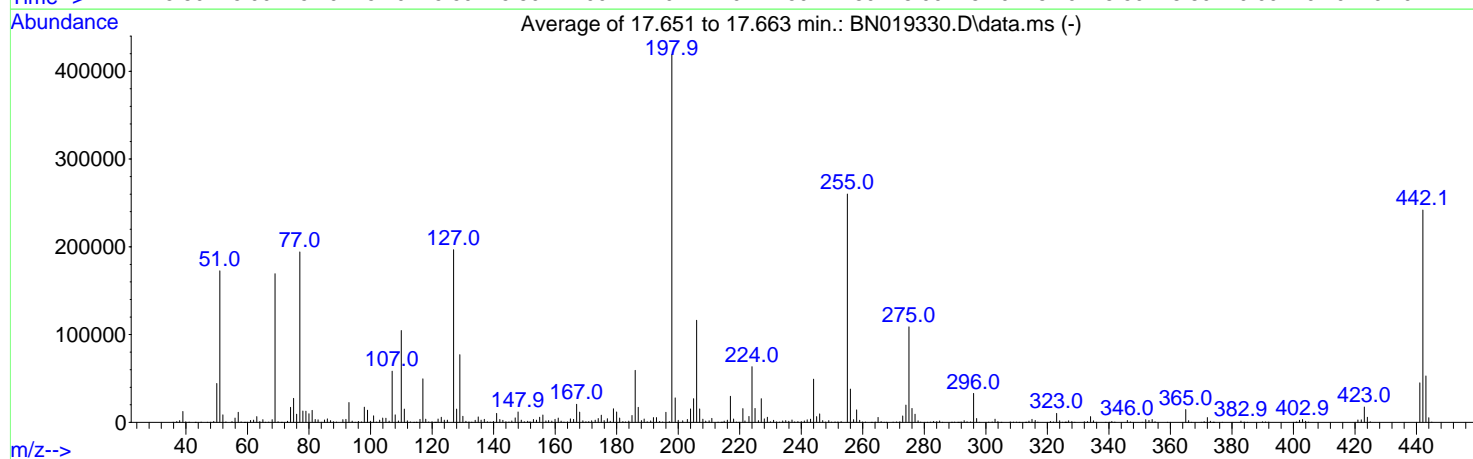


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN040422\  
 Data File : BN019330.D  
 Acq On : 04 Apr 2022 23:25  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN040422.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Apr 04 17:40:00 2022

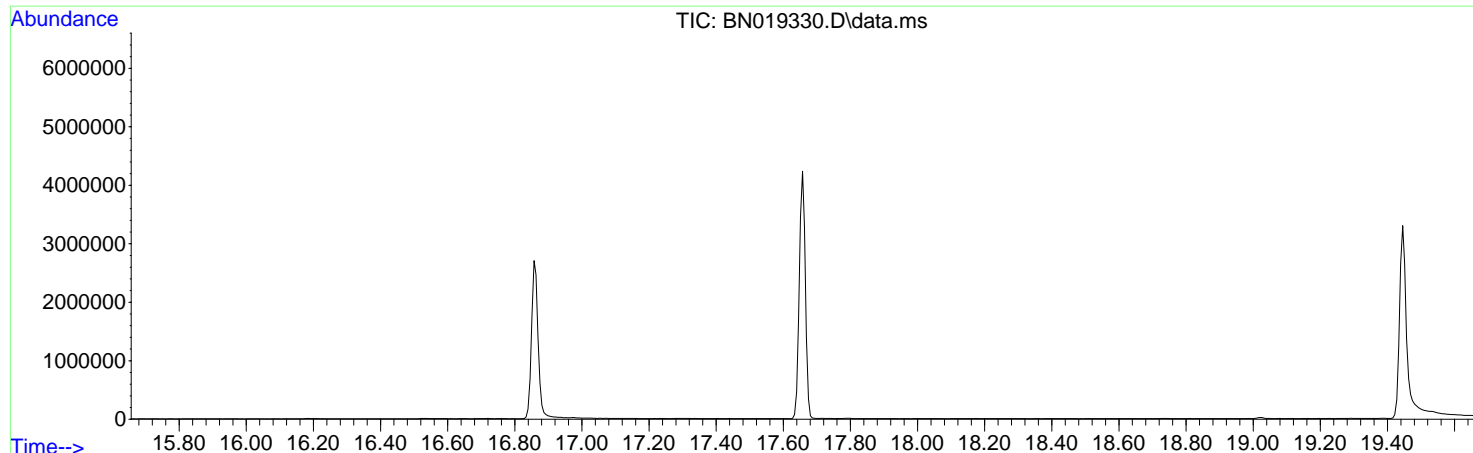




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	172651	PASS
68	69	0.00	2	1.8	3074	PASS
69	198	0.00	100	40.4	169275	PASS
70	69	0.00	2	0.5	813	PASS
127	198	10	80	46.9	196693	PASS
197	198	0.00	2	0.2	965	PASS
198	198	100	100	100.0	419093	PASS
199	198	5	9	6.7	27915	PASS
275	198	10	60	26.0	108896	PASS
365	198	1	100	3.5	14542	PASS
441	198	0.01	100	10.7	45051	PASS
442	442	50	100	100.0	241920	PASS
443	442	15	24	21.8	52795	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN040422\  
 Data File : BN019330.D  
 Acq On : 04 Apr 2022 23:25  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_N  
**ClientSampleId :**  
 DFTPP

Quant Time: Apr 05 17:41:22 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Mar 23 16:56:32 2022  
 Response via : Initial Calibration

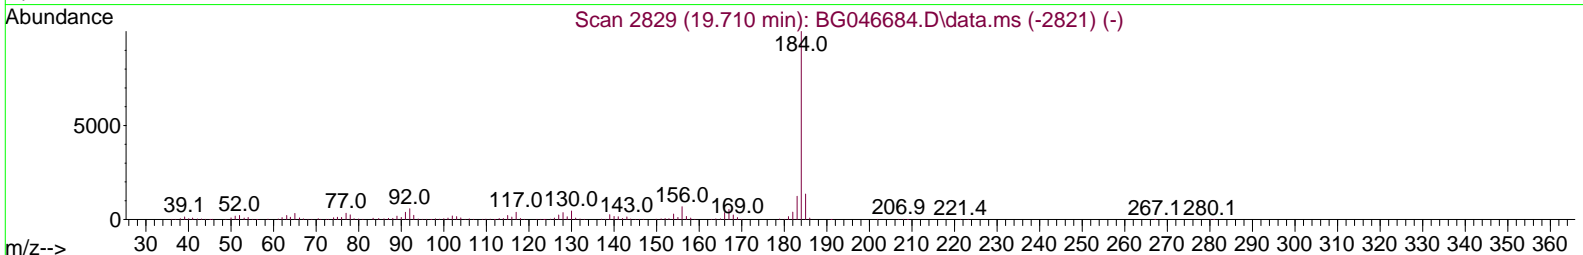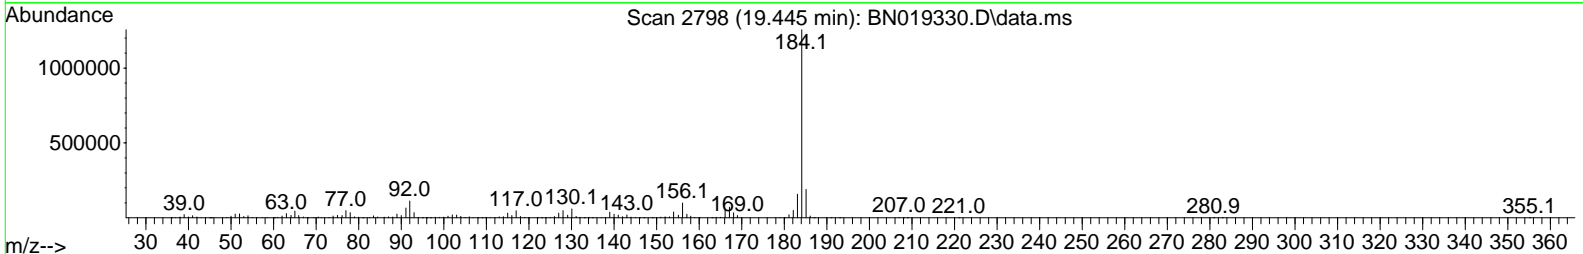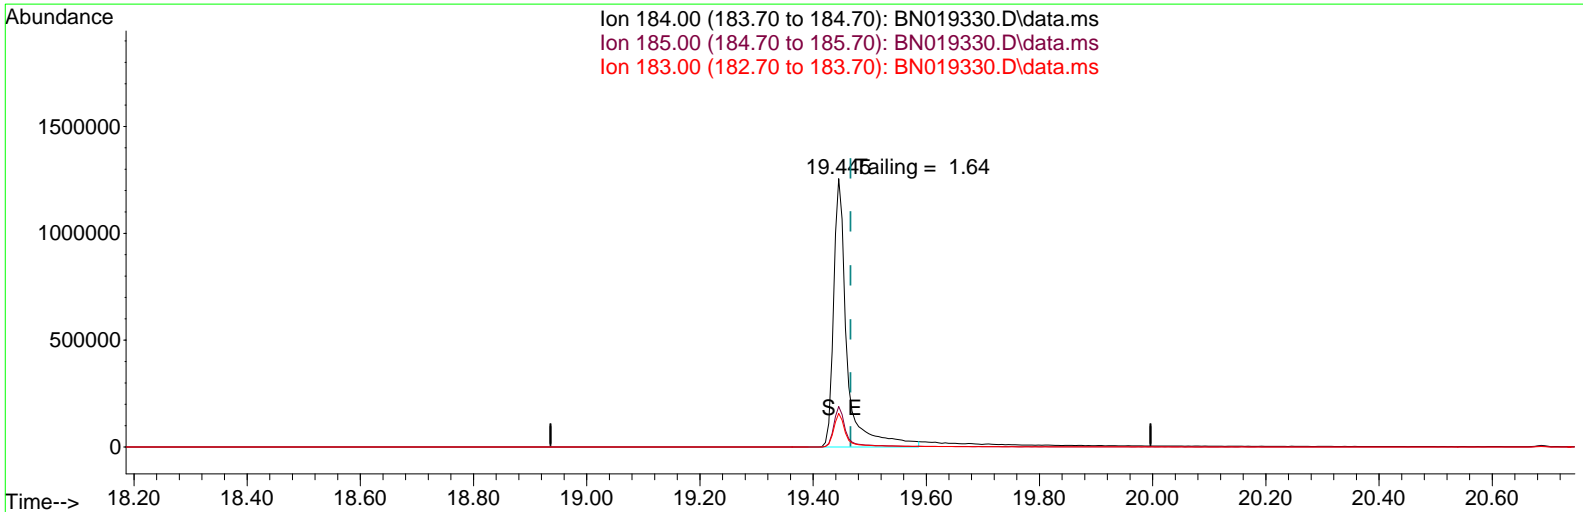

TIC: BN019330.D\data.ms

(77) Benzidine

19.445min (-0.021) 0.00 ng




response 2180330

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.07
183.00	13.20	12.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN040422\  
 Data File : BN019330.D  
 Acq On : 04 Apr 2022 23:25  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Quant Time: Apr 05 17:41:22 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Mar 23 16:56:32 2022  
 Response via : Initial Calibration

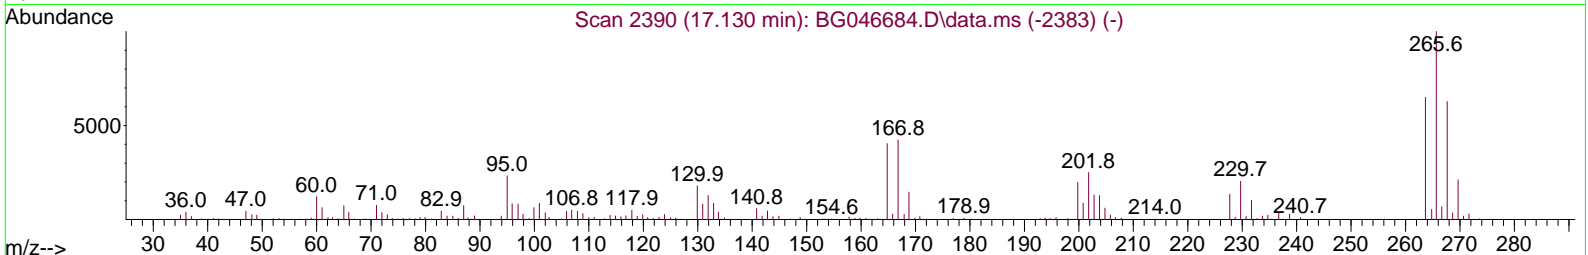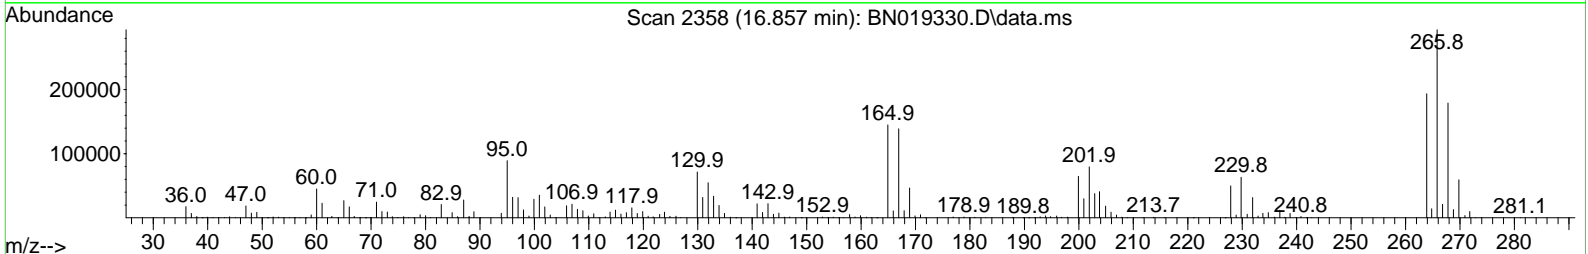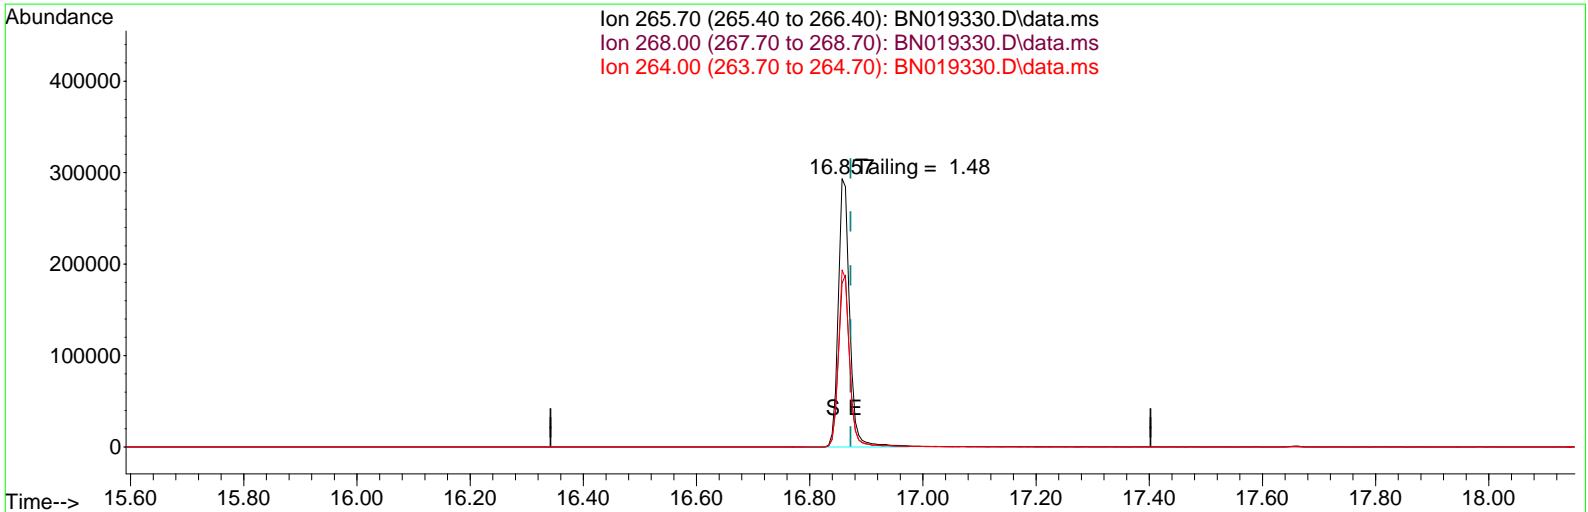

TIC: BN019330.D\data.ms

(70) Pentachlorophenol (C)

16.857min (-0.015) 17309.63 ng

response 415132

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.05
264.00	61.60	66.00
0.00	0.00	0.00

**DDT Breakdown**

Date	Instrument Name	DFTPP Data File
4/4/2022	BNA_N	<u>BN019330.D</u>
Compound Name	Response	Retention Time
DDT	1446901	20.686
DDD	52882	20.245
DDE	655	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
53537	1500438	3.57

Instrument :  
 BNA\_N  
 ClientSampled :  
 DFTPP