
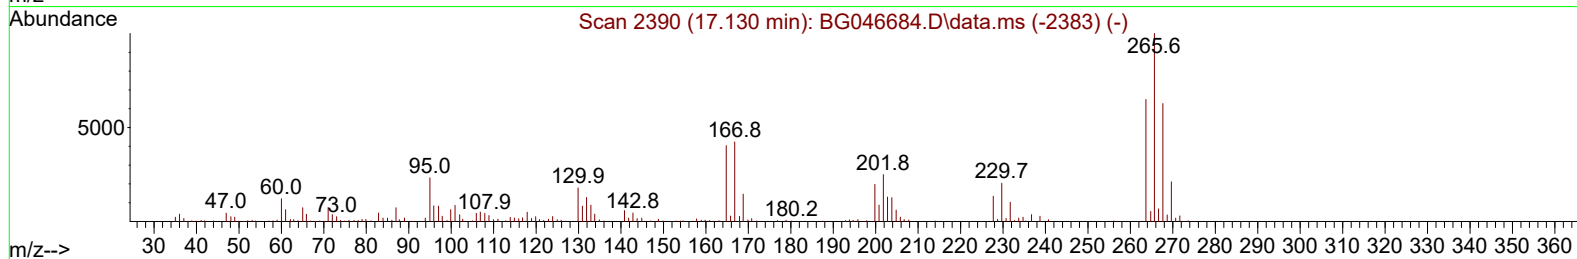
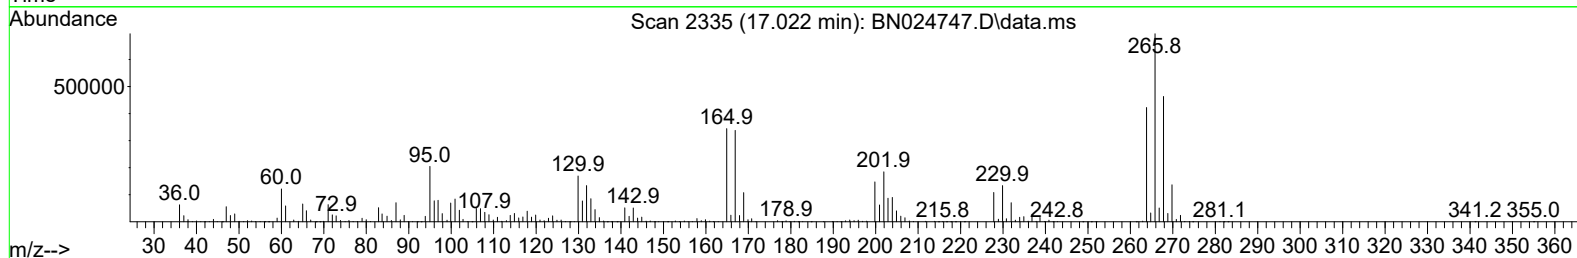


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040423\
Data File : BN024747.D
Acq On : 04 Apr 2023 09:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 00:42:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 05 00:41:59 2023
Response via : Initial Calibration

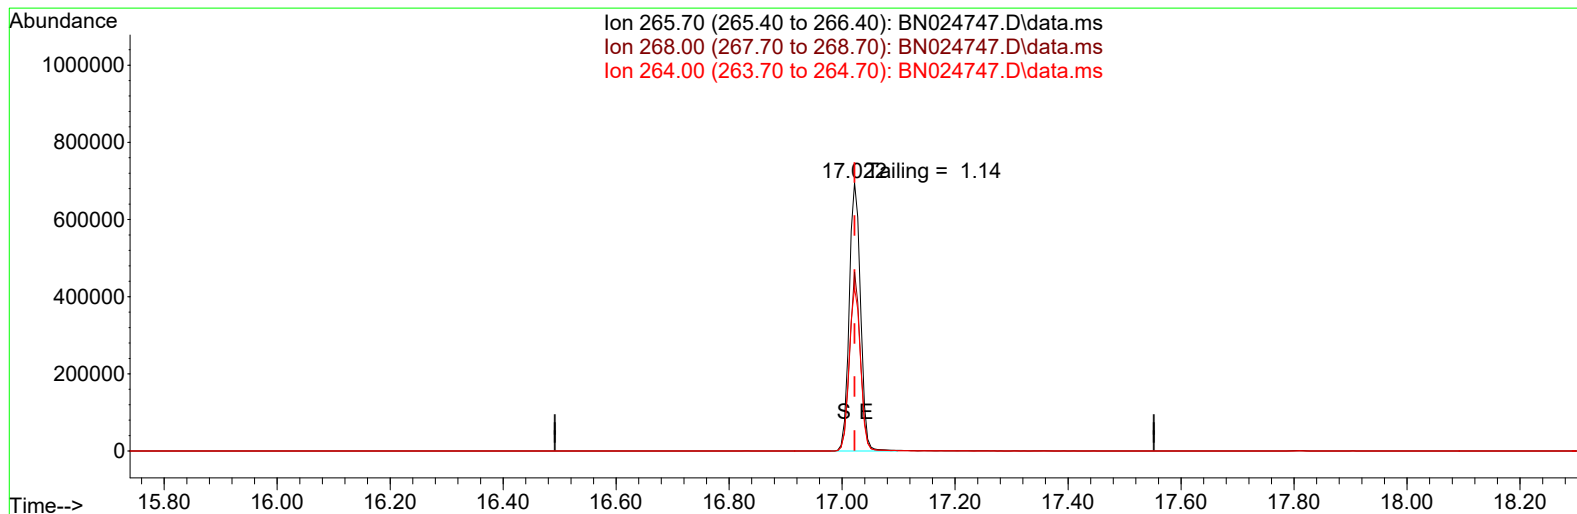

TIC: BN024747.D\data.ms

(70) Pentachlorophenol (C)




17.022min (0.000) 24935.87 ng

response 969059

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.66
264.00	61.60	60.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040423\
 Data File : BN024747.D
 Acq On : 04 Apr 2023 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 00:42:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 05 00:41:59 2023
 Response via : Initial Calibration

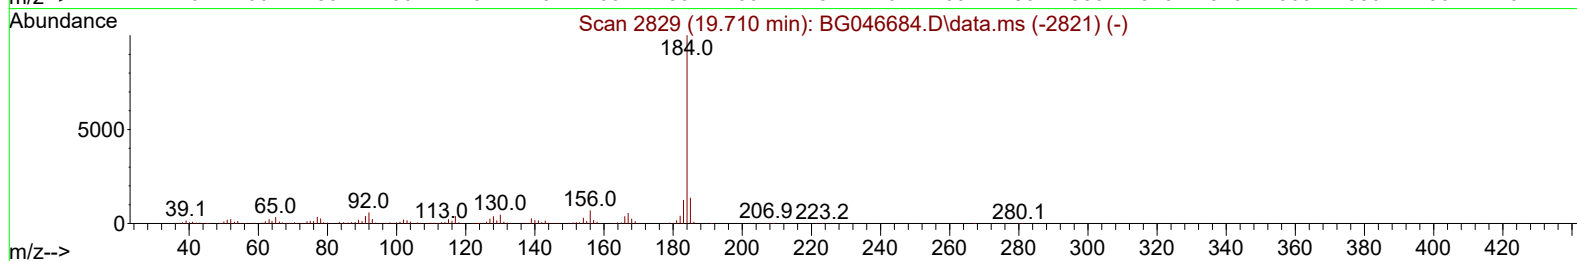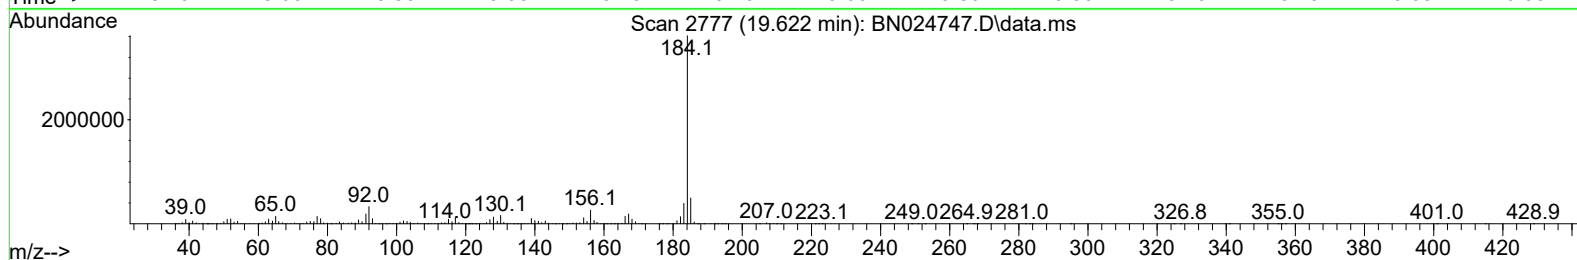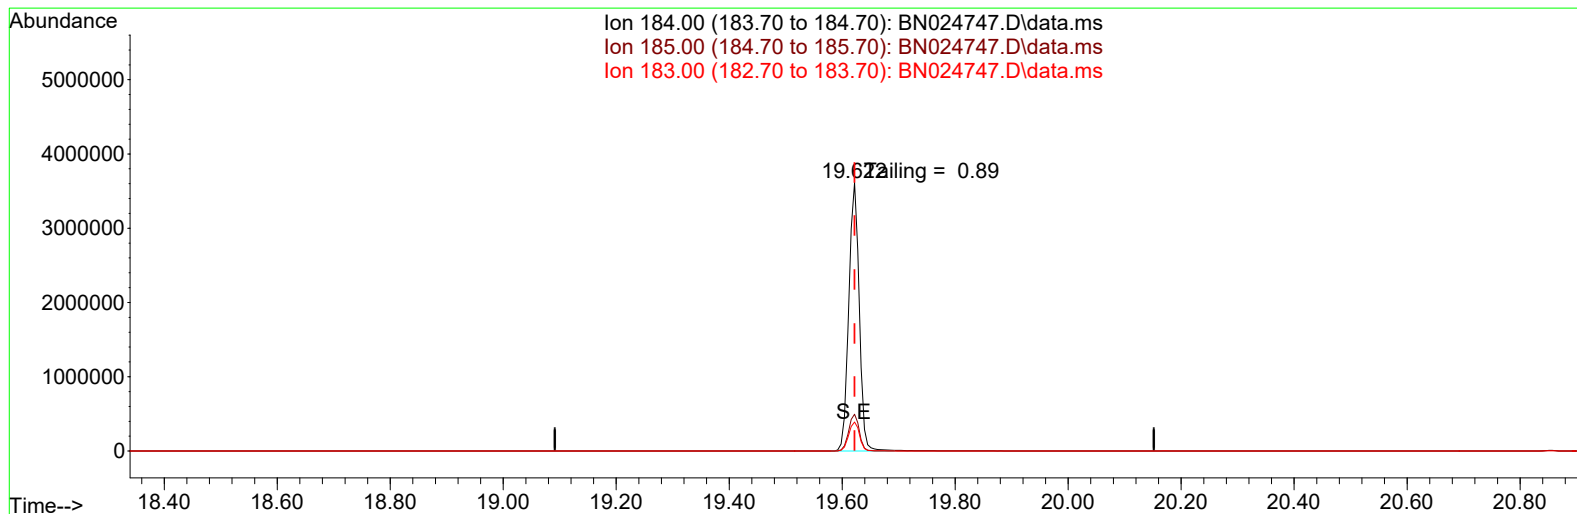

TIC: BN024747.D\data.ms

(77) Benzidine**19.622min (0.000) 139856.69 ng****response 4617225**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.73
183.00	13.20	10.81
0.00	0.00	0.00