
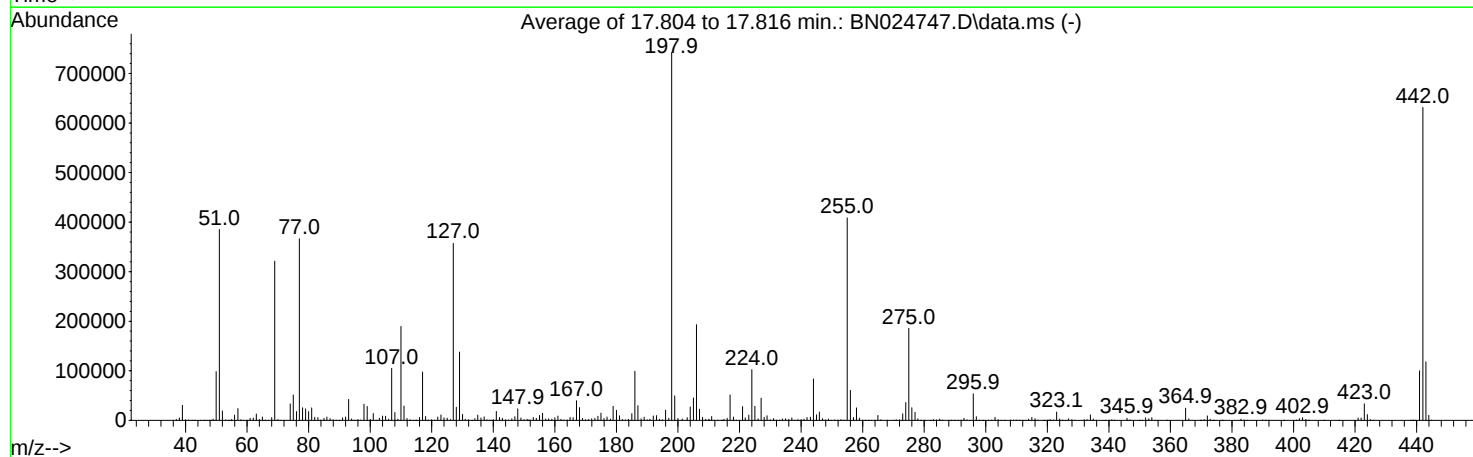


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040423\
 Data File : BN024747.D
 Acq On : 04 Apr 2023 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN040323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 05 00:51:08 2023

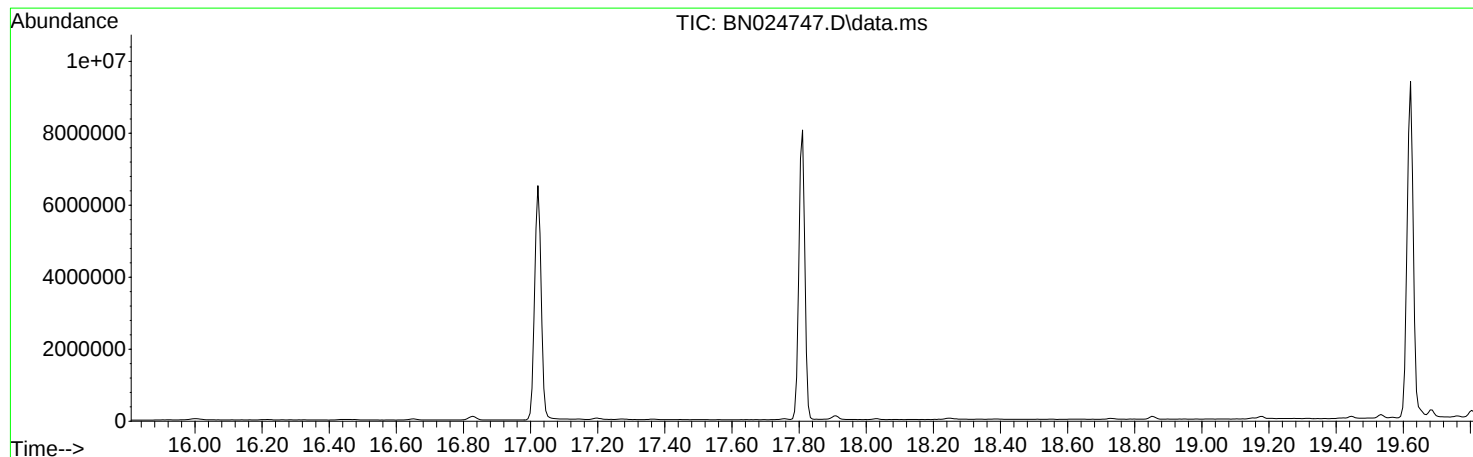




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.9	385182	PASS
68	69	0.00	2	1.7	5608	PASS
69	198	0.00	100	43.3	321169	PASS
70	69	0.00	2	0.5	1636	PASS
127	198	10	80	48.1	357163	PASS
197	198	0.00	2	0.5	4074	PASS
198	198	100	100	100.0	742251	PASS
199	198	5	9	6.7	49381	PASS
275	198	10	60	25.0	185579	PASS
365	198	1	100	3.3	24584	PASS
441	198	0.01	100	13.5	100077	PASS
442	442	50	100	100.0	631424	PASS
443	442	15	24	18.7	118208	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040423\
Data File : BN024747.D
Acq On : 04 Apr 2023 09:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 05 00:42:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 05 00:41:59 2023
Response via : Initial Calibration

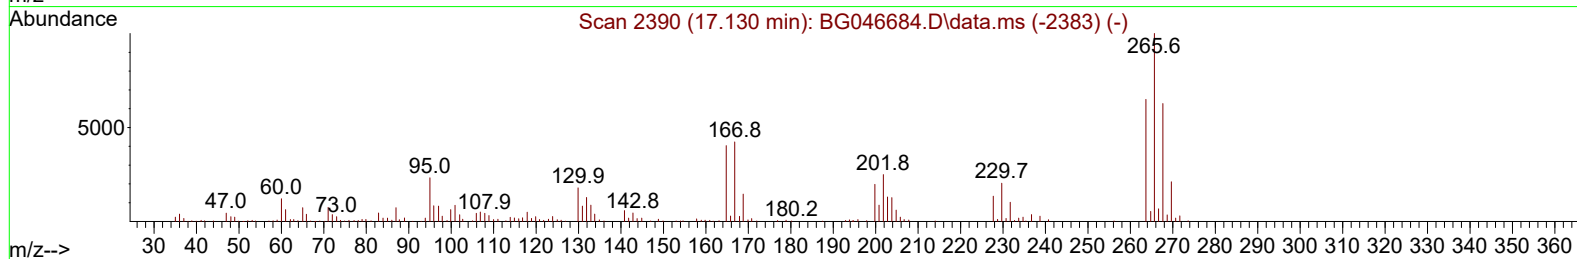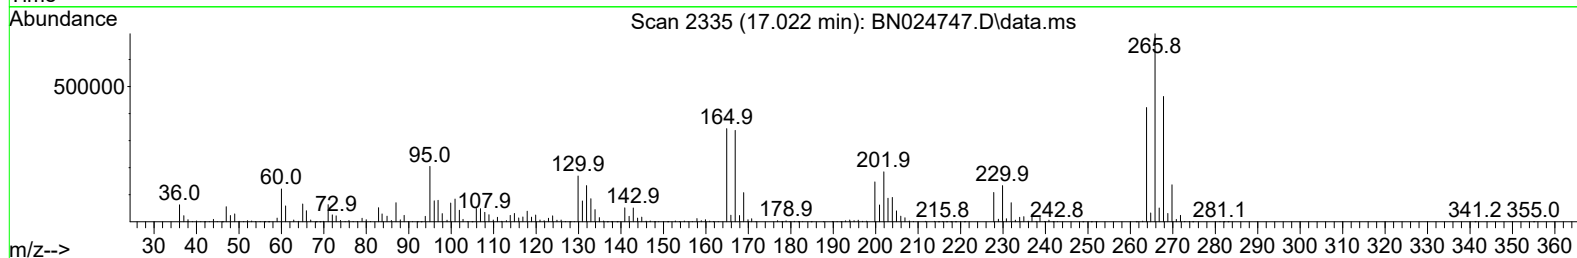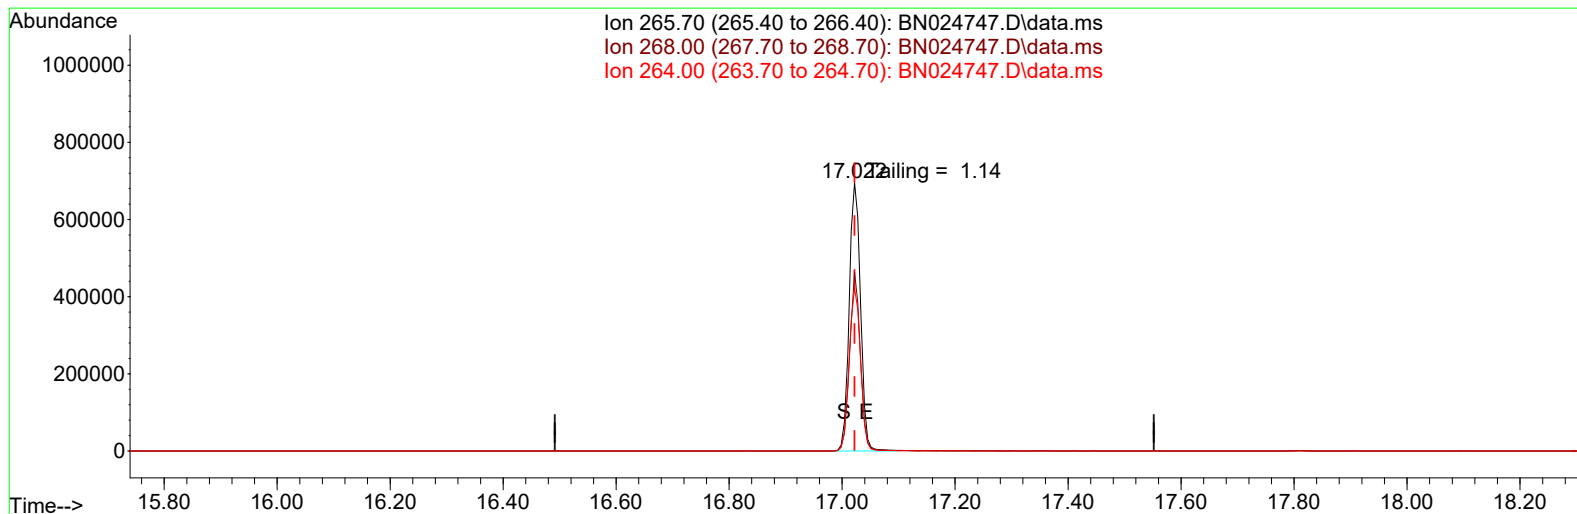

TIC: BN024747.D\data.ms

(70) Pentachlorophenol (C)

17.022min (0.000) 24935.87 ng




response 969059

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.66
264.00	61.60	60.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040423\
Data File : BN024747.D
Acq On : 04 Apr 2023 09:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 05 00:42:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 05 00:41:59 2023
Response via : Initial Calibration

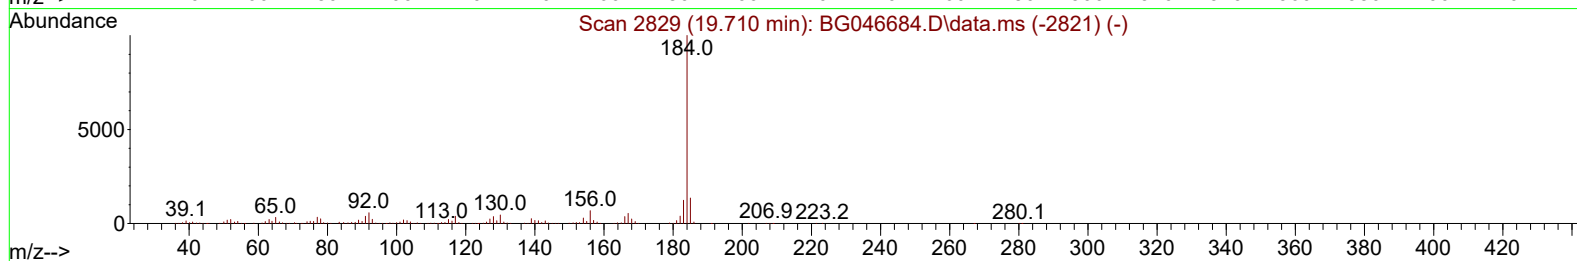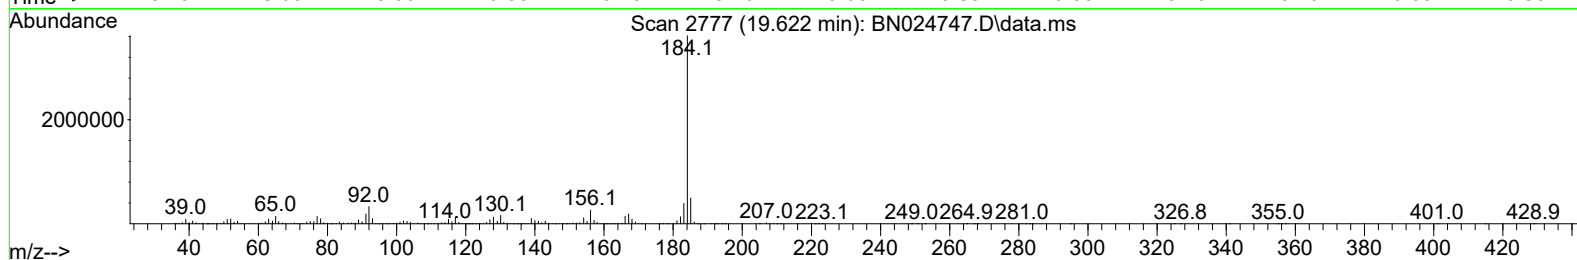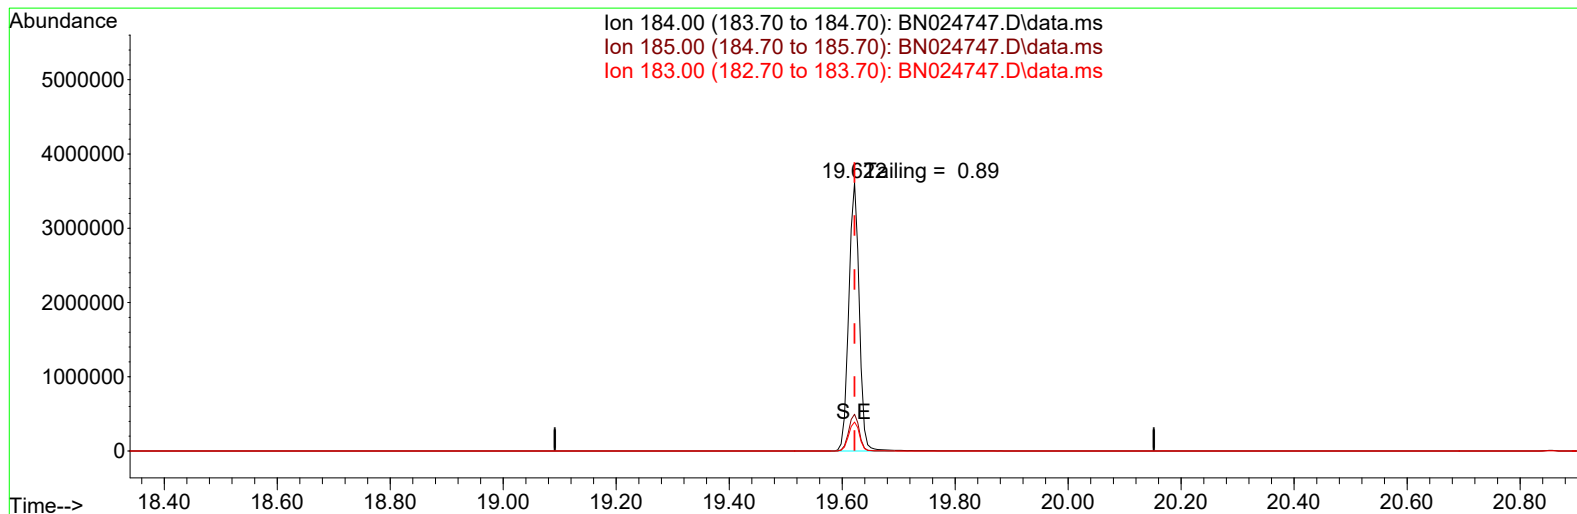

TIC: BN024747.D\data.ms

(77) Benzidine

19.622min (0.000) 139856.69 ng

response 4617225

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.73
183.00	13.20	10.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/3/2023	BNA_N	<u>BN024747.D</u>
Compound Name	Response	Retention Time
DDT	2404007	20.857
DDD	95379	20.41
DDE	5970	19.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
101349	2505356	4.05

Instrument :
BNA_N
ClientSampleId :
DFTPP