
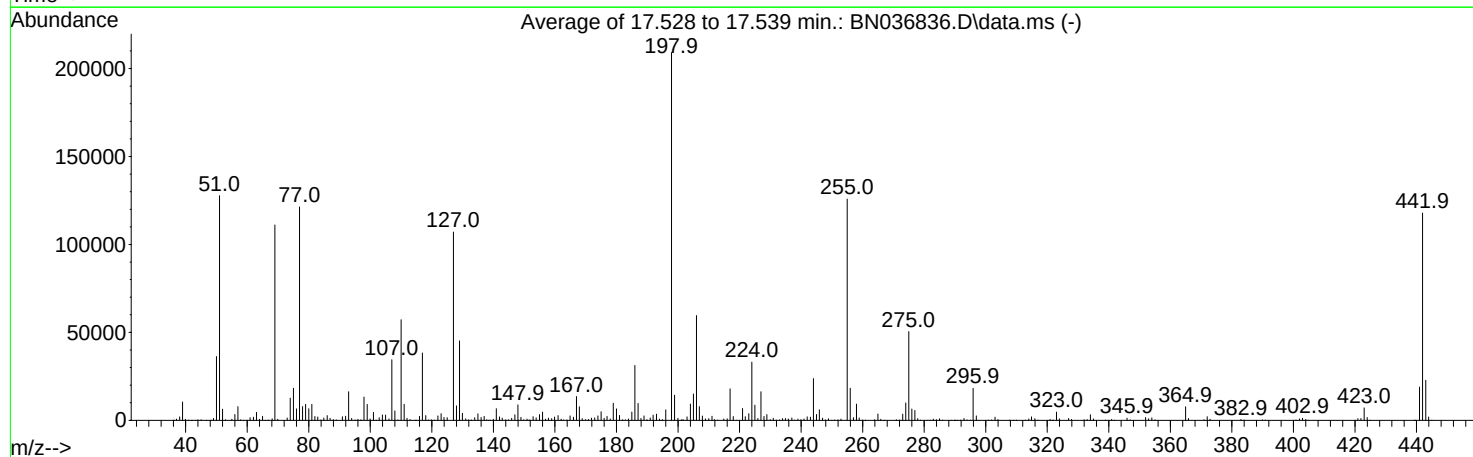


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040425\
Data File : BN036836.D
Acq On : 04 Apr 2025 13:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 04 17:30:43 2025

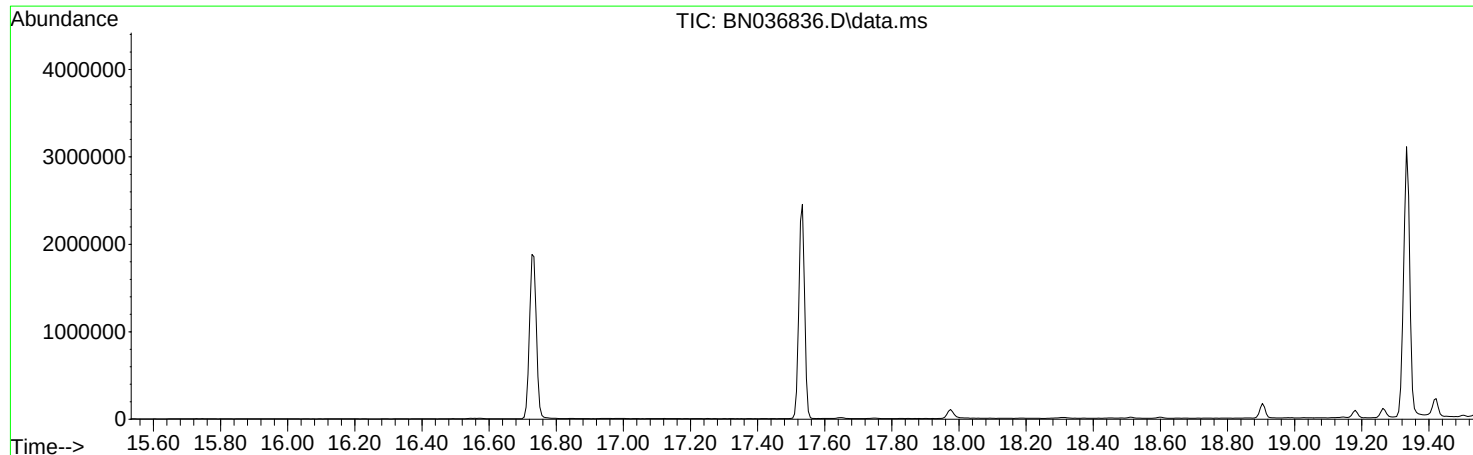




AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.1	127701	PASS
68	69	0.00	2	0.8	926	PASS
69	198	0.00	100	53.1	111072	PASS
70	69	0.00	2	0.6	654	PASS
127	198	10	80	51.2	107067	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	209109	PASS
199	198	5	9	6.8	14277	PASS
275	198	10	60	24.1	50483	PASS
365	198	1	100	3.7	7782	PASS
441	198	0.01	100	9.1	18954	PASS
442	442	50	100	100.0	117920	PASS
443	442	15	24	19.3	22803	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040425\
Data File : BN036836.D
Acq On : 04 Apr 2025 13:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 04 17:15:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

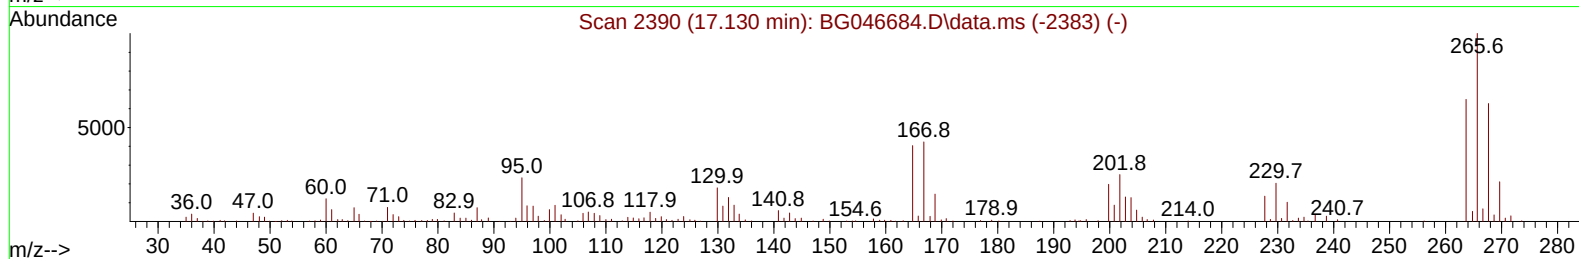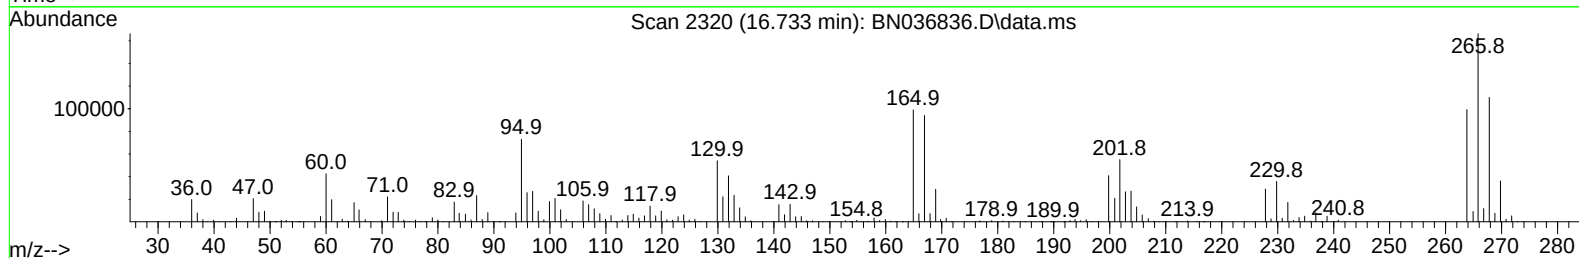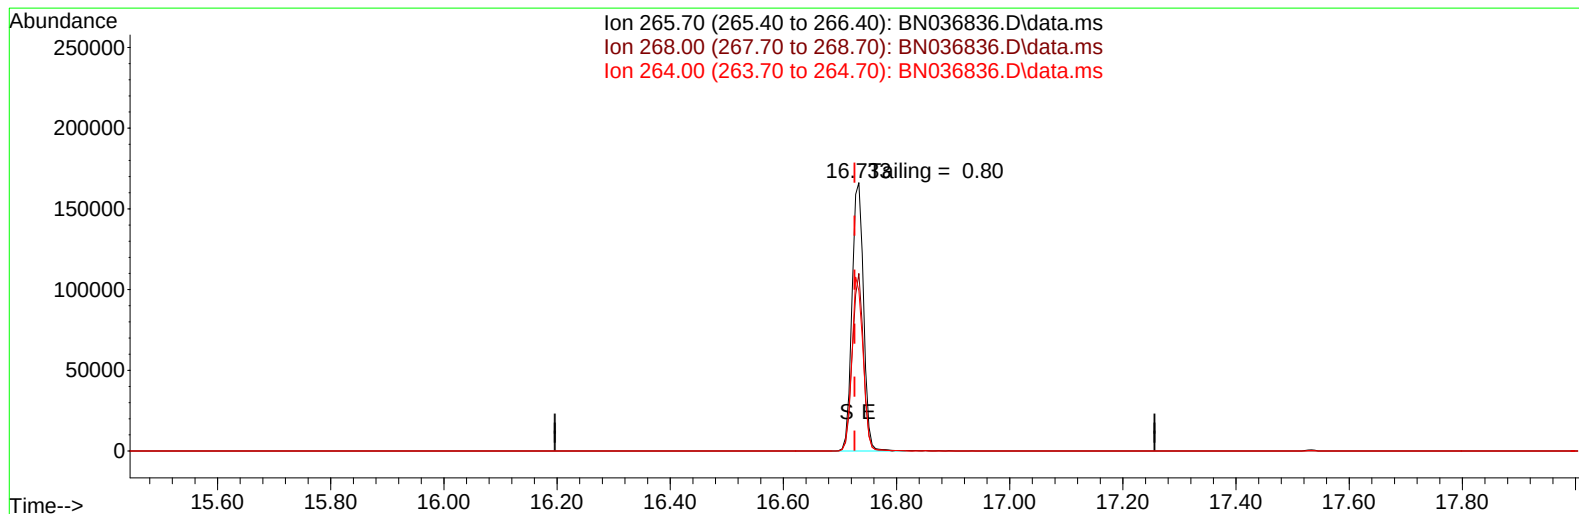

TIC: BN036836.D\data.ms

(70) Pentachlorophenol (C)

16.733min (+ 0.008) 19292.53 ng




response 236340

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.13
264.00	61.60	59.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040425\
Data File : BN036836.D
Acq On : 04 Apr 2025 13:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 04 17:18:00 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

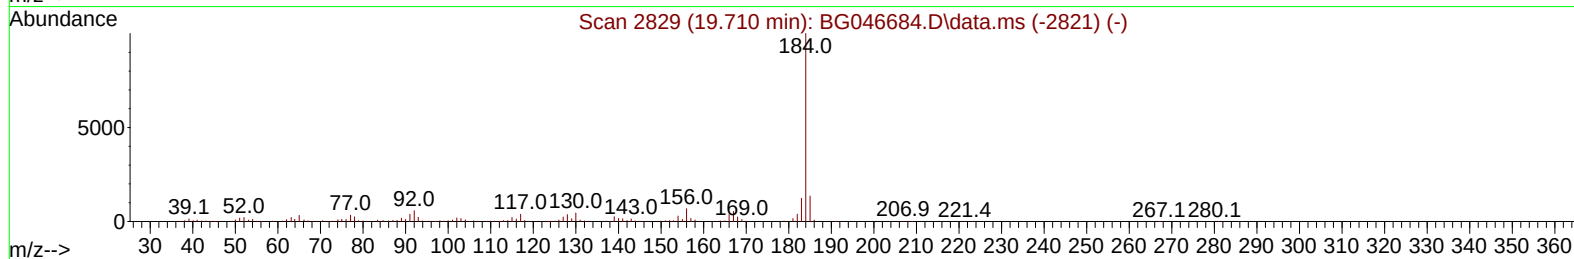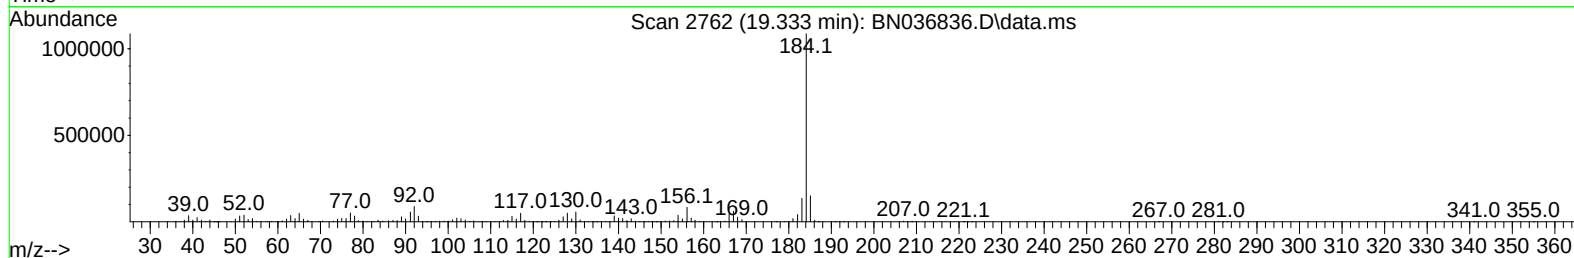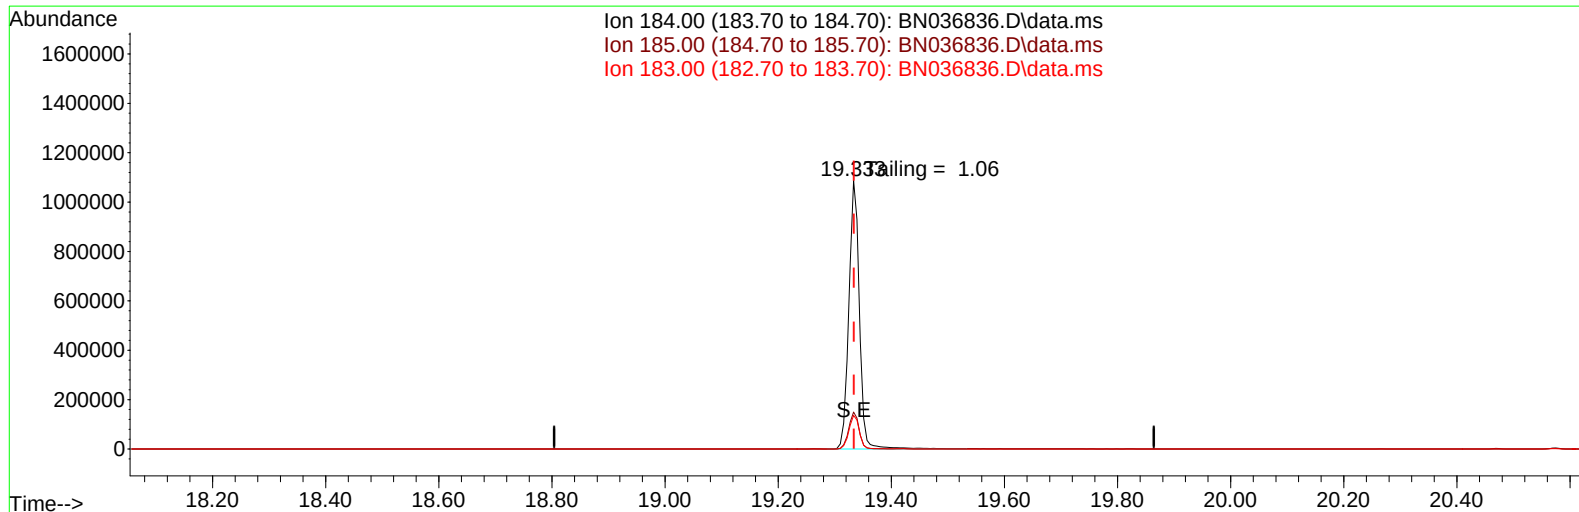

TIC: BN036836.D\data.ms

(77) Benzidine

19.333min (-0.001) 0.00 ng

response 1395649

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	12.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/4/2025	BNA_N	<u>BN036836.D</u>
Compound Name	Response	Retention Time
DDT	793119	20.574
DDD	11889	20.133
DDE	312	19.622
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12201	805320	1.52

Instrument :
BNA_N
ClientSampleId :
DFTPP