
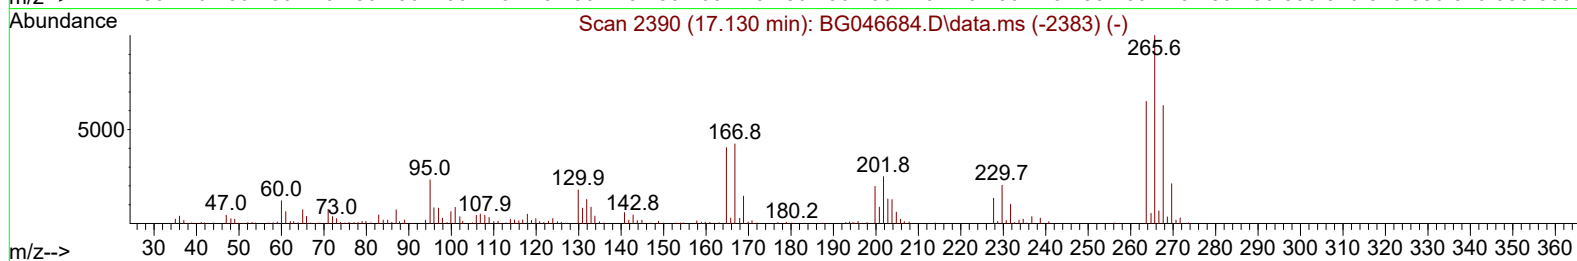
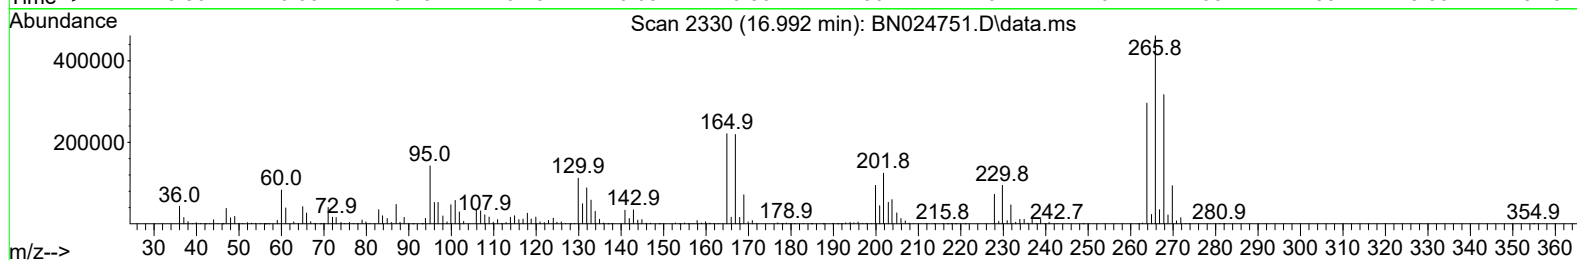


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040523\
Data File : BN024751.D
Acq On : 04 Apr 2023 17:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 06:18:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 05 06:18:03 2023
Response via : Initial Calibration

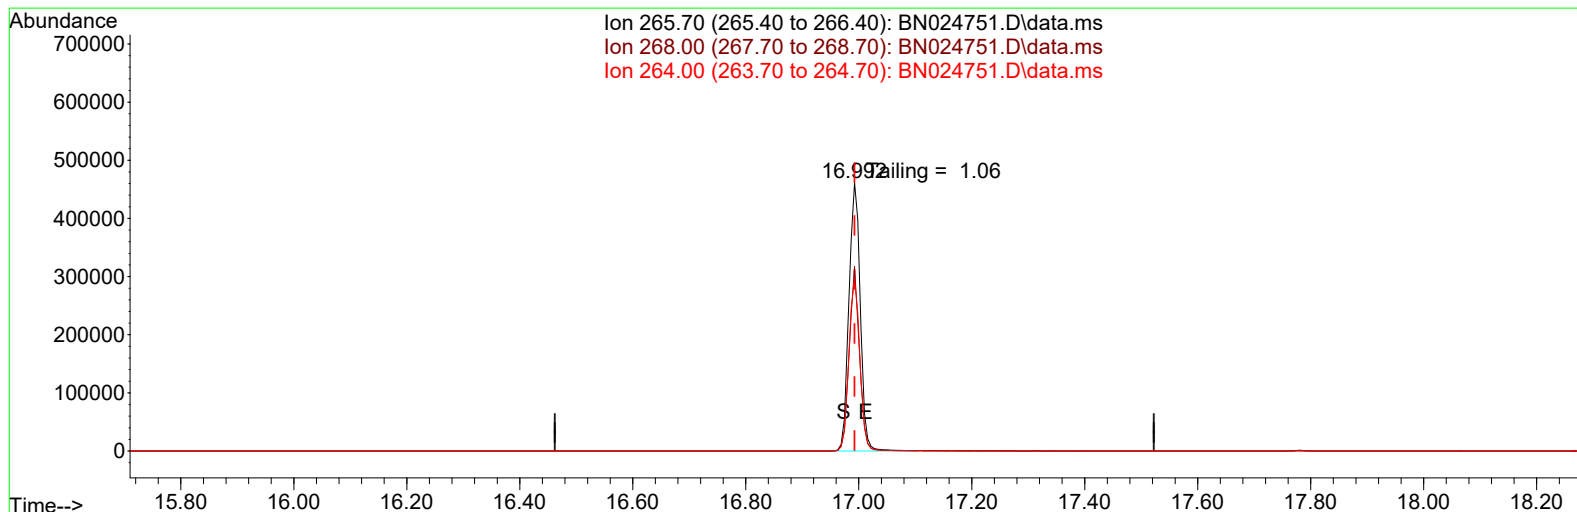

TIC: BN024751.D\data.ms

(70) Pentachlorophenol (C)




16.992min (0.000) 21217.10 ng

response 645379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.66
264.00	61.60	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040523\
Data File : BN024751.D
Acq On : 04 Apr 2023 17:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 06:18:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 05 06:18:03 2023
Response via : Initial Calibration

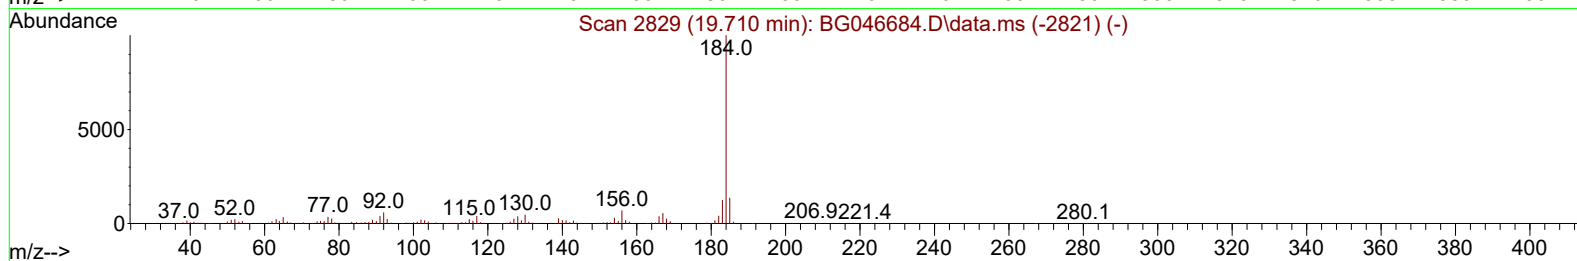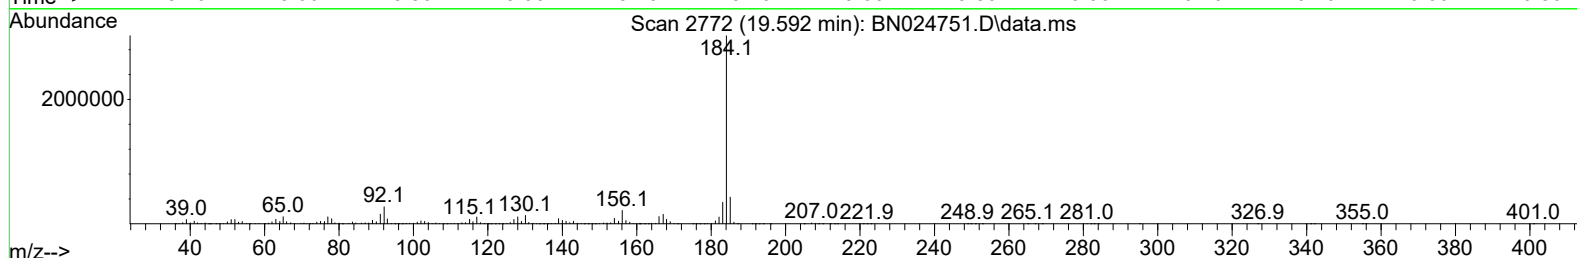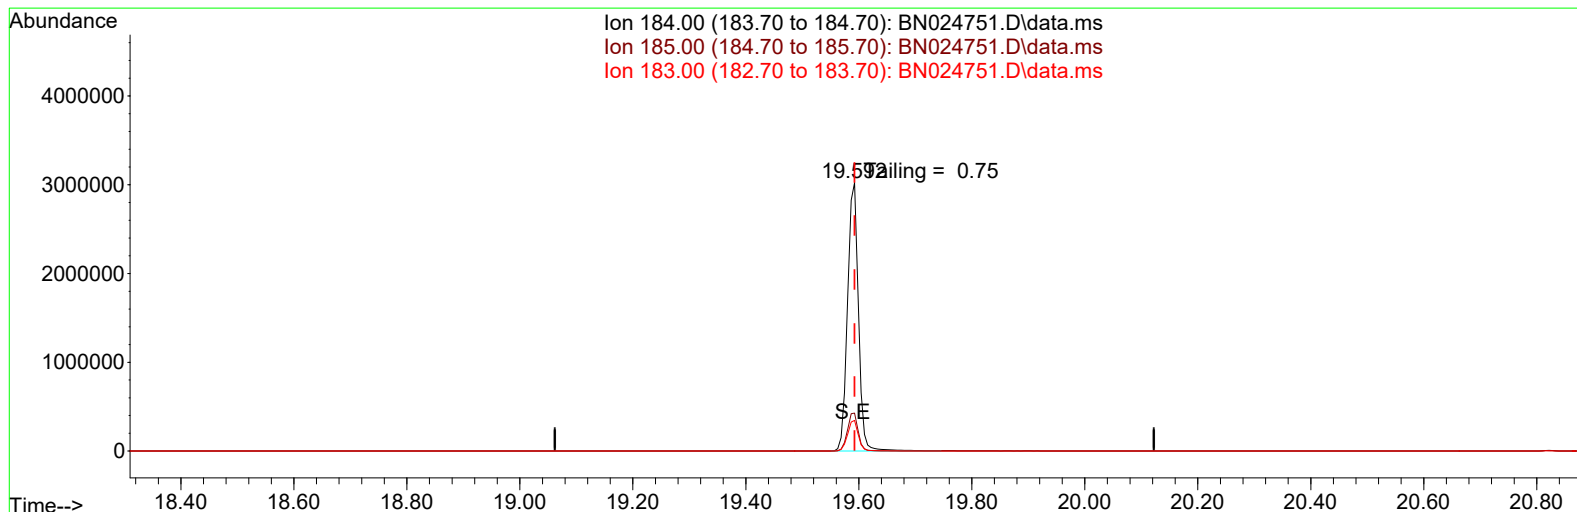

TIC: BN024751.D\data.ms

(77) Benzidine

19.592min (0.000) 0.00 ng

response 4056365

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.14
183.00	13.20	11.40
0.00	0.00	0.00