
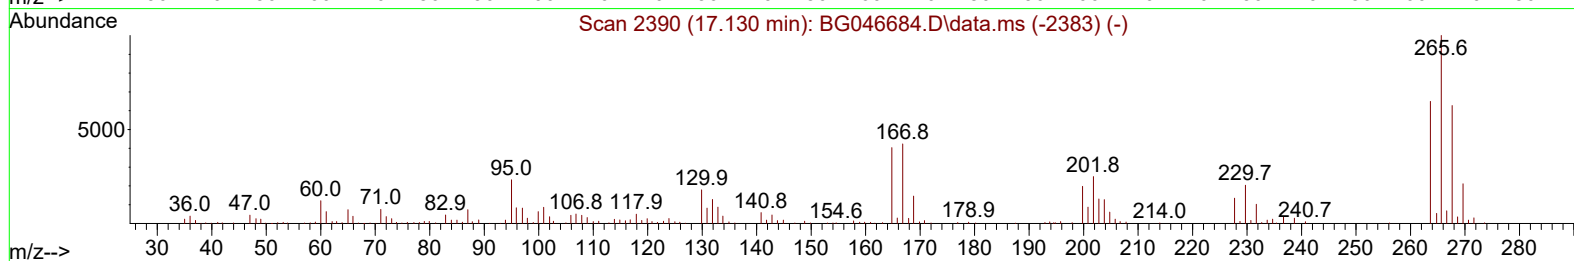
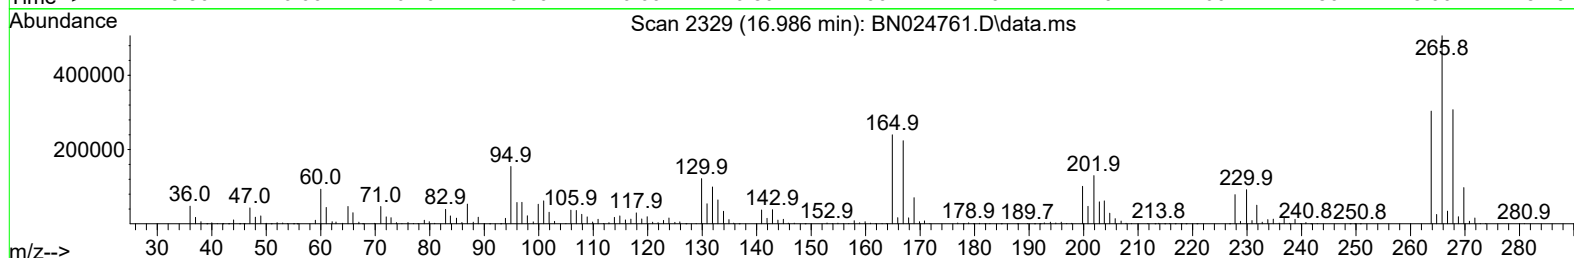


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040523\
Data File : BN024761.D
Acq On : 05 Apr 2023 08:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 07:19:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 07:19:36 2023
Response via : Initial Calibration

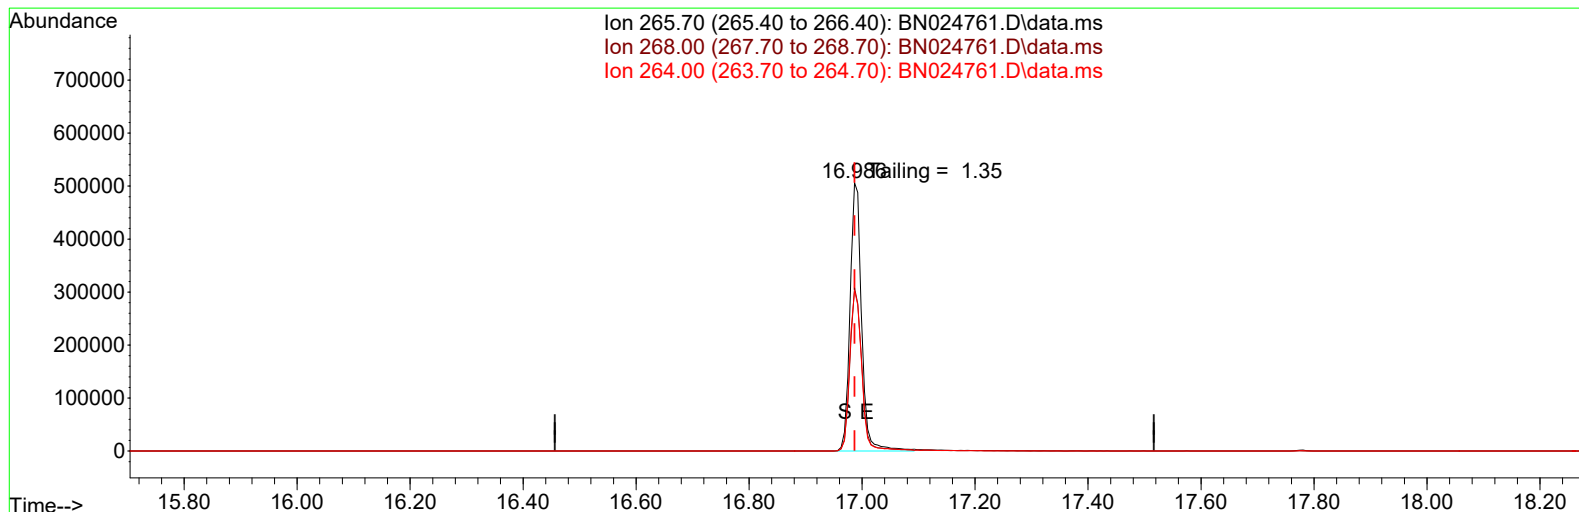

TIC: BN024761.D\data.ms

(70) Pentachlorophenol (C)




16.986min (0.000) 20885.50 ng

response 731832

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.73
264.00	61.60	59.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040523\
 Data File : BN024761.D
 Acq On : 05 Apr 2023 08:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 07:19:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 07:19:36 2023
 Response via : Initial Calibration

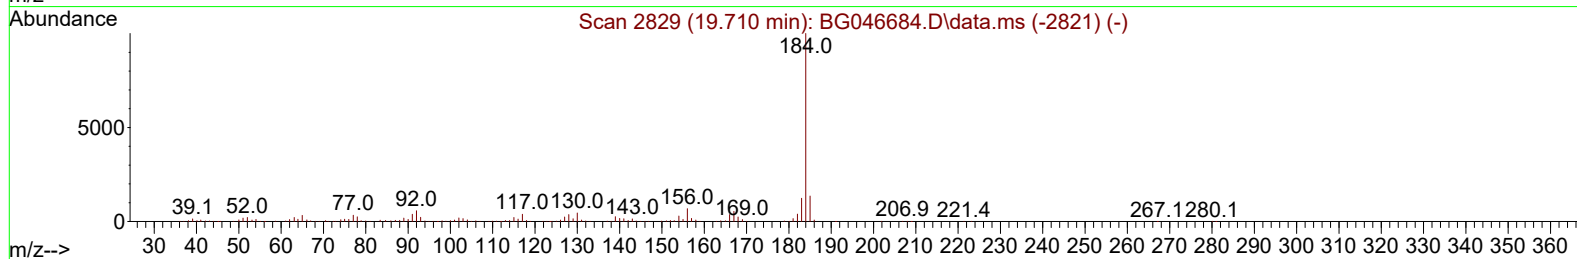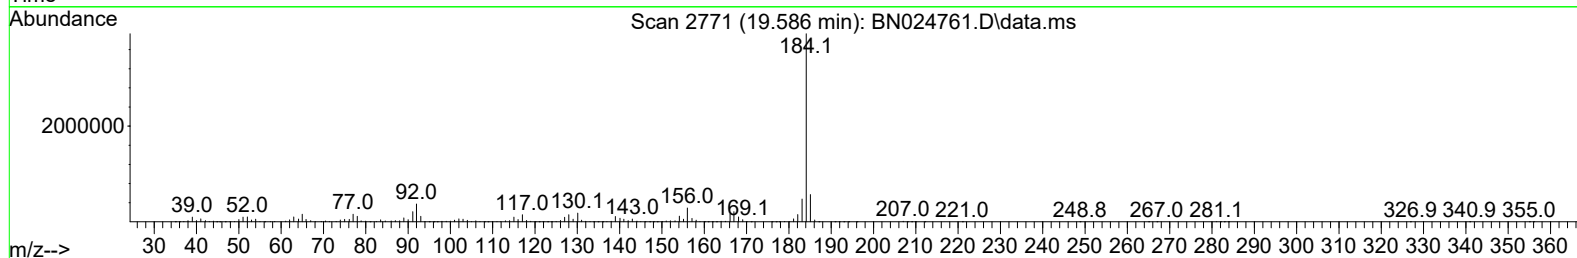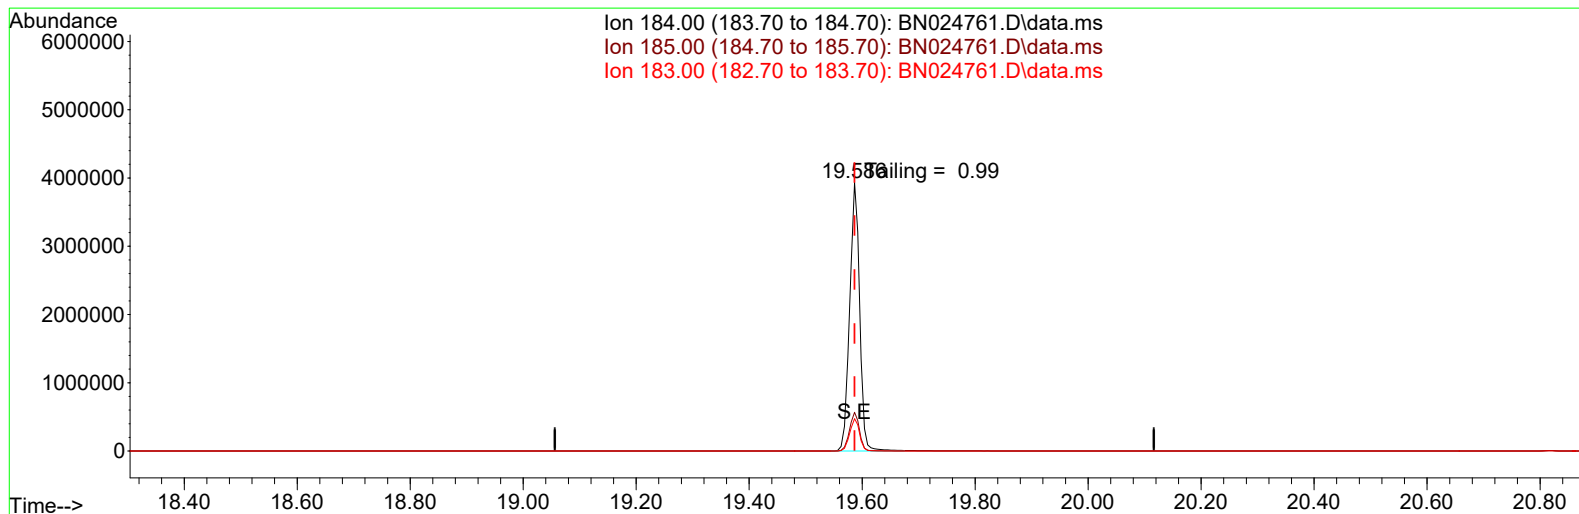

TIC: BN024761.D\data.ms

(77) Benzidine

19.586min (0.000) 0.00 ng

response 4849990

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.45
183.00	13.20	12.07
0.00	0.00	0.00