
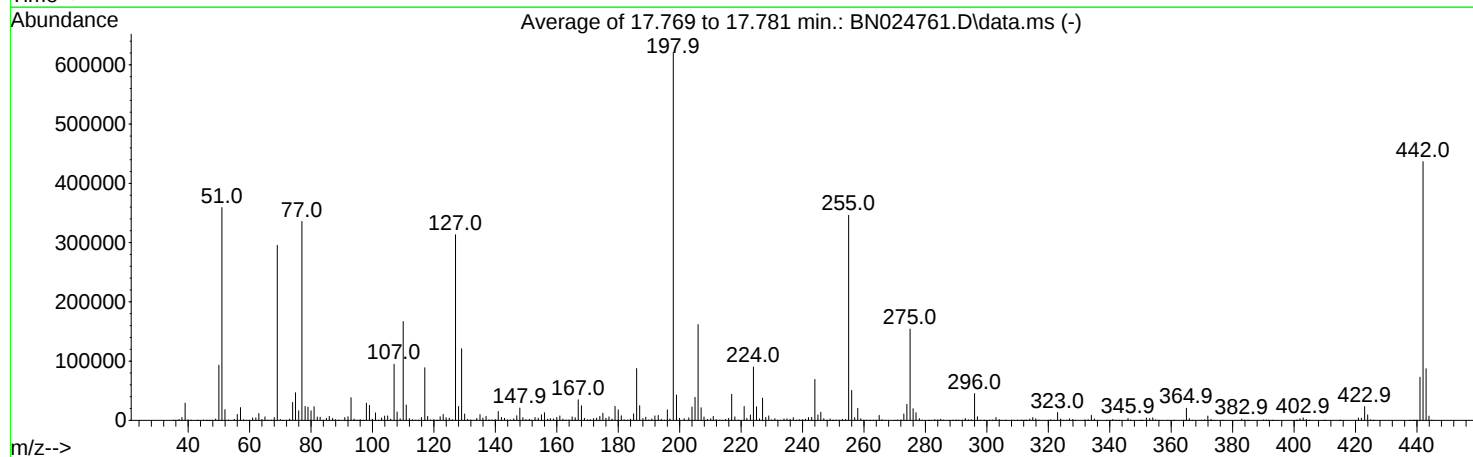


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040523\
 Data File : BN024761.D
 Acq On : 05 Apr 2023 08:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN040523.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 05 11:04:25 2023

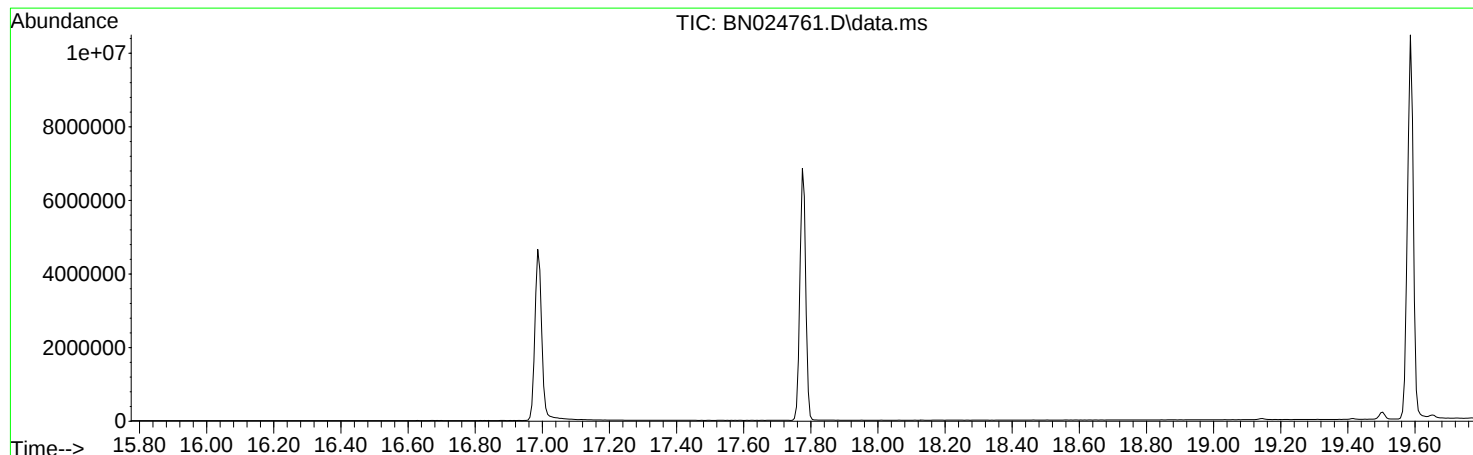




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.9	359279	PASS
68	69	0.00	2	1.7	4928	PASS
69	198	0.00	100	47.6	295403	PASS
70	69	0.00	2	0.6	1667	PASS
127	198	10	80	50.5	313259	PASS
197	198	0.00	2	0.4	2448	PASS
198	198	100	100	100.0	620843	PASS
199	198	5	9	6.9	42997	PASS
275	198	10	60	24.8	154264	PASS
365	198	1	100	3.3	20419	PASS
441	198	0.01	100	11.8	73051	PASS
442	442	50	100	100.0	436672	PASS
443	442	15	24	20.0	87376	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040523\
Data File : BN024761.D
Acq On : 05 Apr 2023 08:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 06 07:19:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 07:19:36 2023
Response via : Initial Calibration

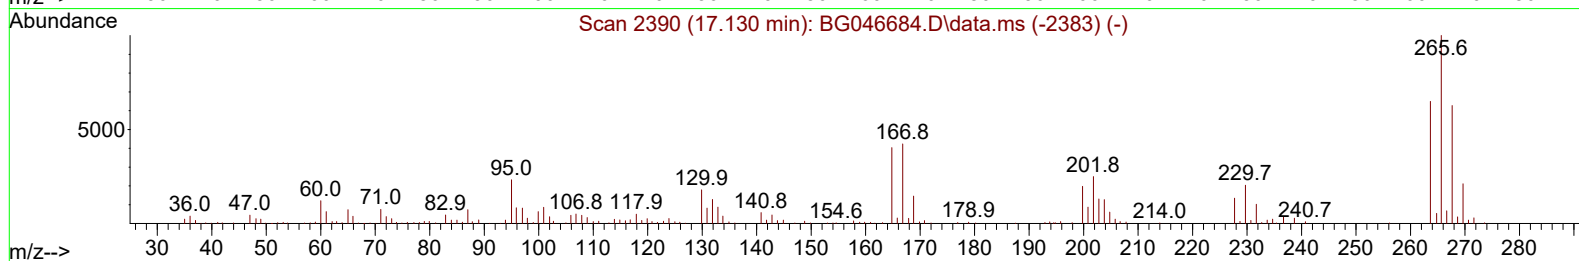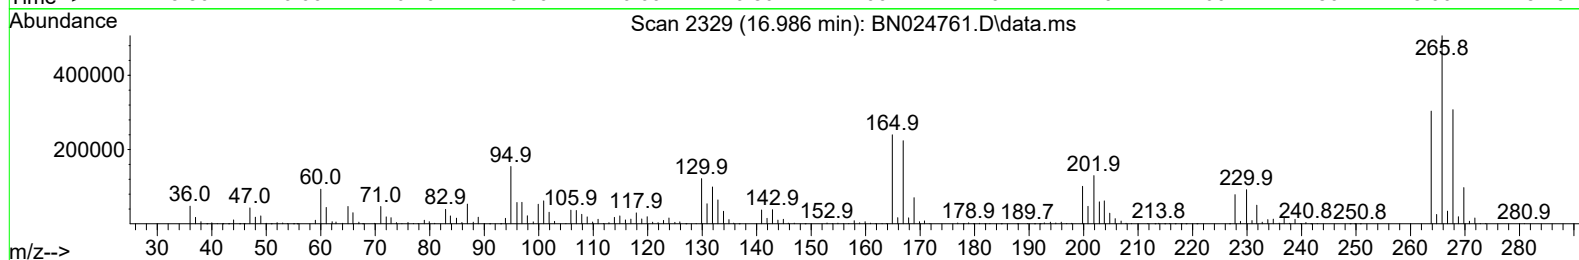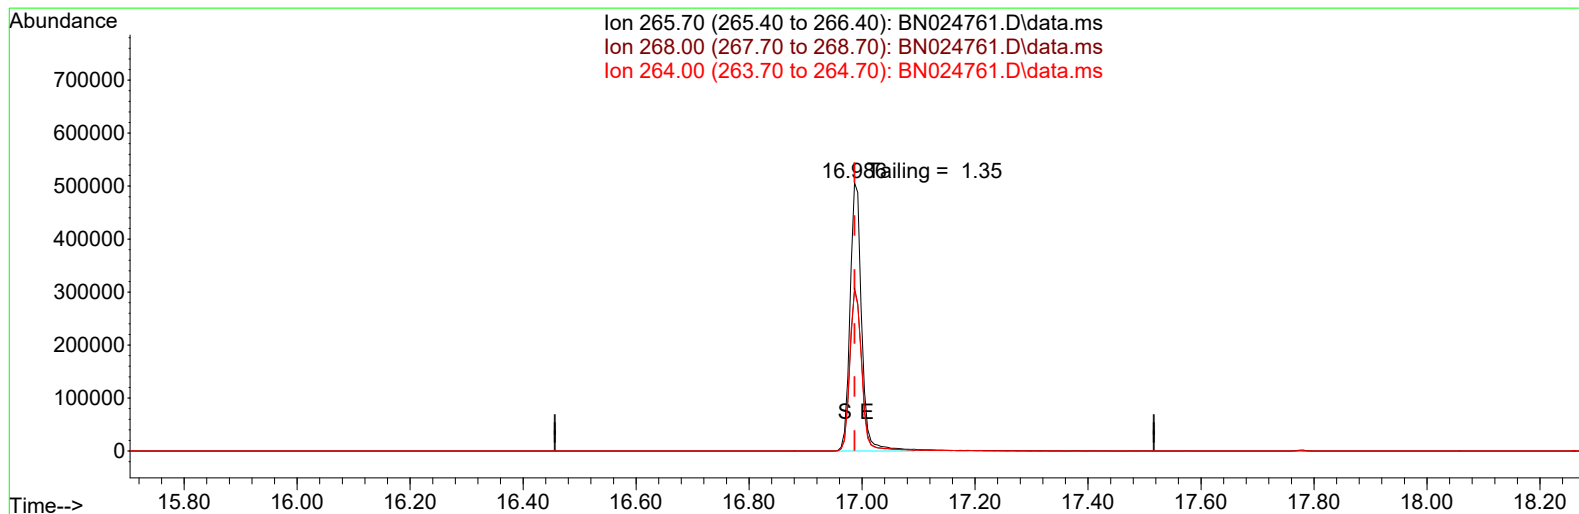

TIC: BN024761.D\data.ms

(70) Pentachlorophenol (C)

16.986min (0.000) 20885.50 ng




response 731832

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.73
264.00	61.60	59.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040523\
 Data File : BN024761.D
 Acq On : 05 Apr 2023 08:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 06 07:19:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 07:19:36 2023
 Response via : Initial Calibration

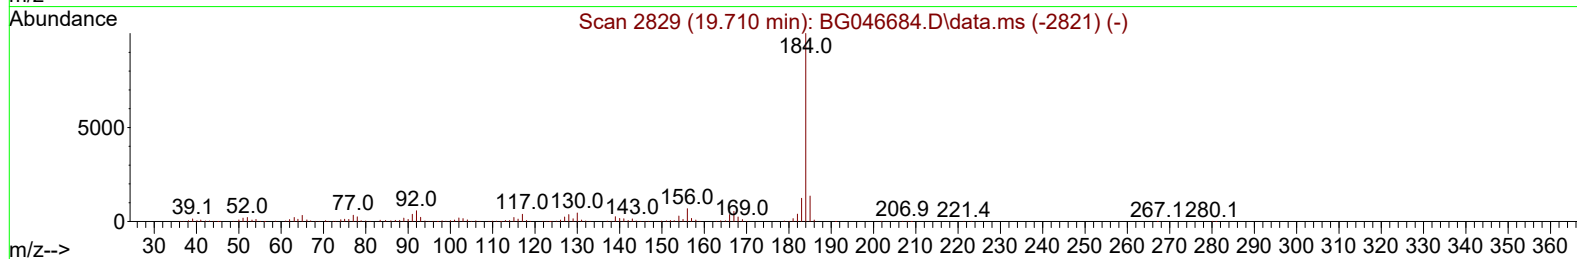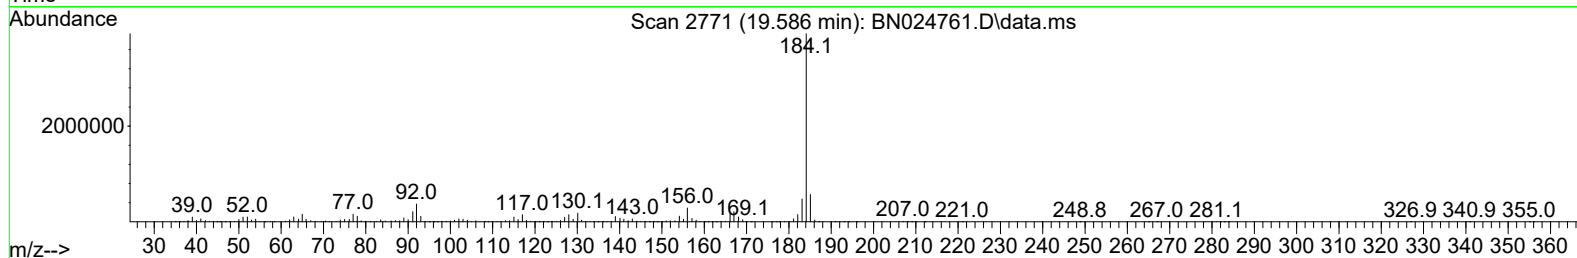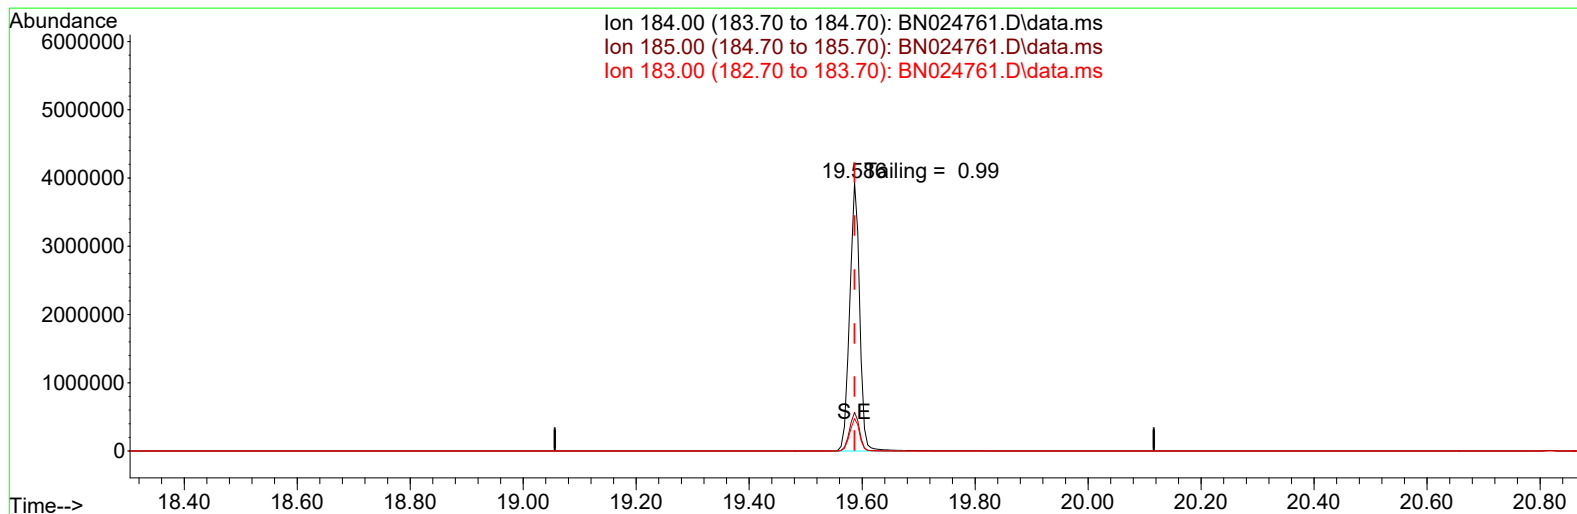

TIC: BN024761.D\data.ms

(77) Benzidine

19.586min (0.000) 0.00 ng

response 4849990

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.45
183.00	13.20	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/5/2023	BNA_N	<u>BN024761.D</u>
Compound Name	Response	Retention Time
DDT	2042127	20.816
DDD	32360	20.427
DDE	304	19.875
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32664	2074791	1.57

Instrument :
BNA_N
ClientSampleId :
DFTPP