

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
 Data File : BN024786.D
 Acq On : 06 Apr 2023 18:42
 Operator : CG/JU
 Sample : PB151755BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK755

Quant Time: Apr 06 23:08:03 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 22:57:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.954	152	8953	0.400	ng/ul	0.00
4) Naphthalene-d8	10.769	136	28131	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	16350	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.342	188	35165	0.400	ng/ul	0.00
17) Chrysene-d12	21.534	240	27070	0.400	ng/ul	0.00
23) Perylene-d12	23.986	264	30170	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.318	96	71175	7.745	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.358	152	14892	0.429	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	33741	0.509	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.592	166	5052	0.088	ng/ul#	11
20) Pyrene	19.739	202	5241	0.054	ng/ul#	1
26) Benzo(a)pyrene	23.837	252	11978	0.122	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
Data File : BN024786.D
Acq On : 06 Apr 2023 18:42
Operator : CG/JU
Sample : PB151755BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK755

Quant Time: Apr 06 23:08:03 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 22:57:45 2023
Response via : Initial Calibration




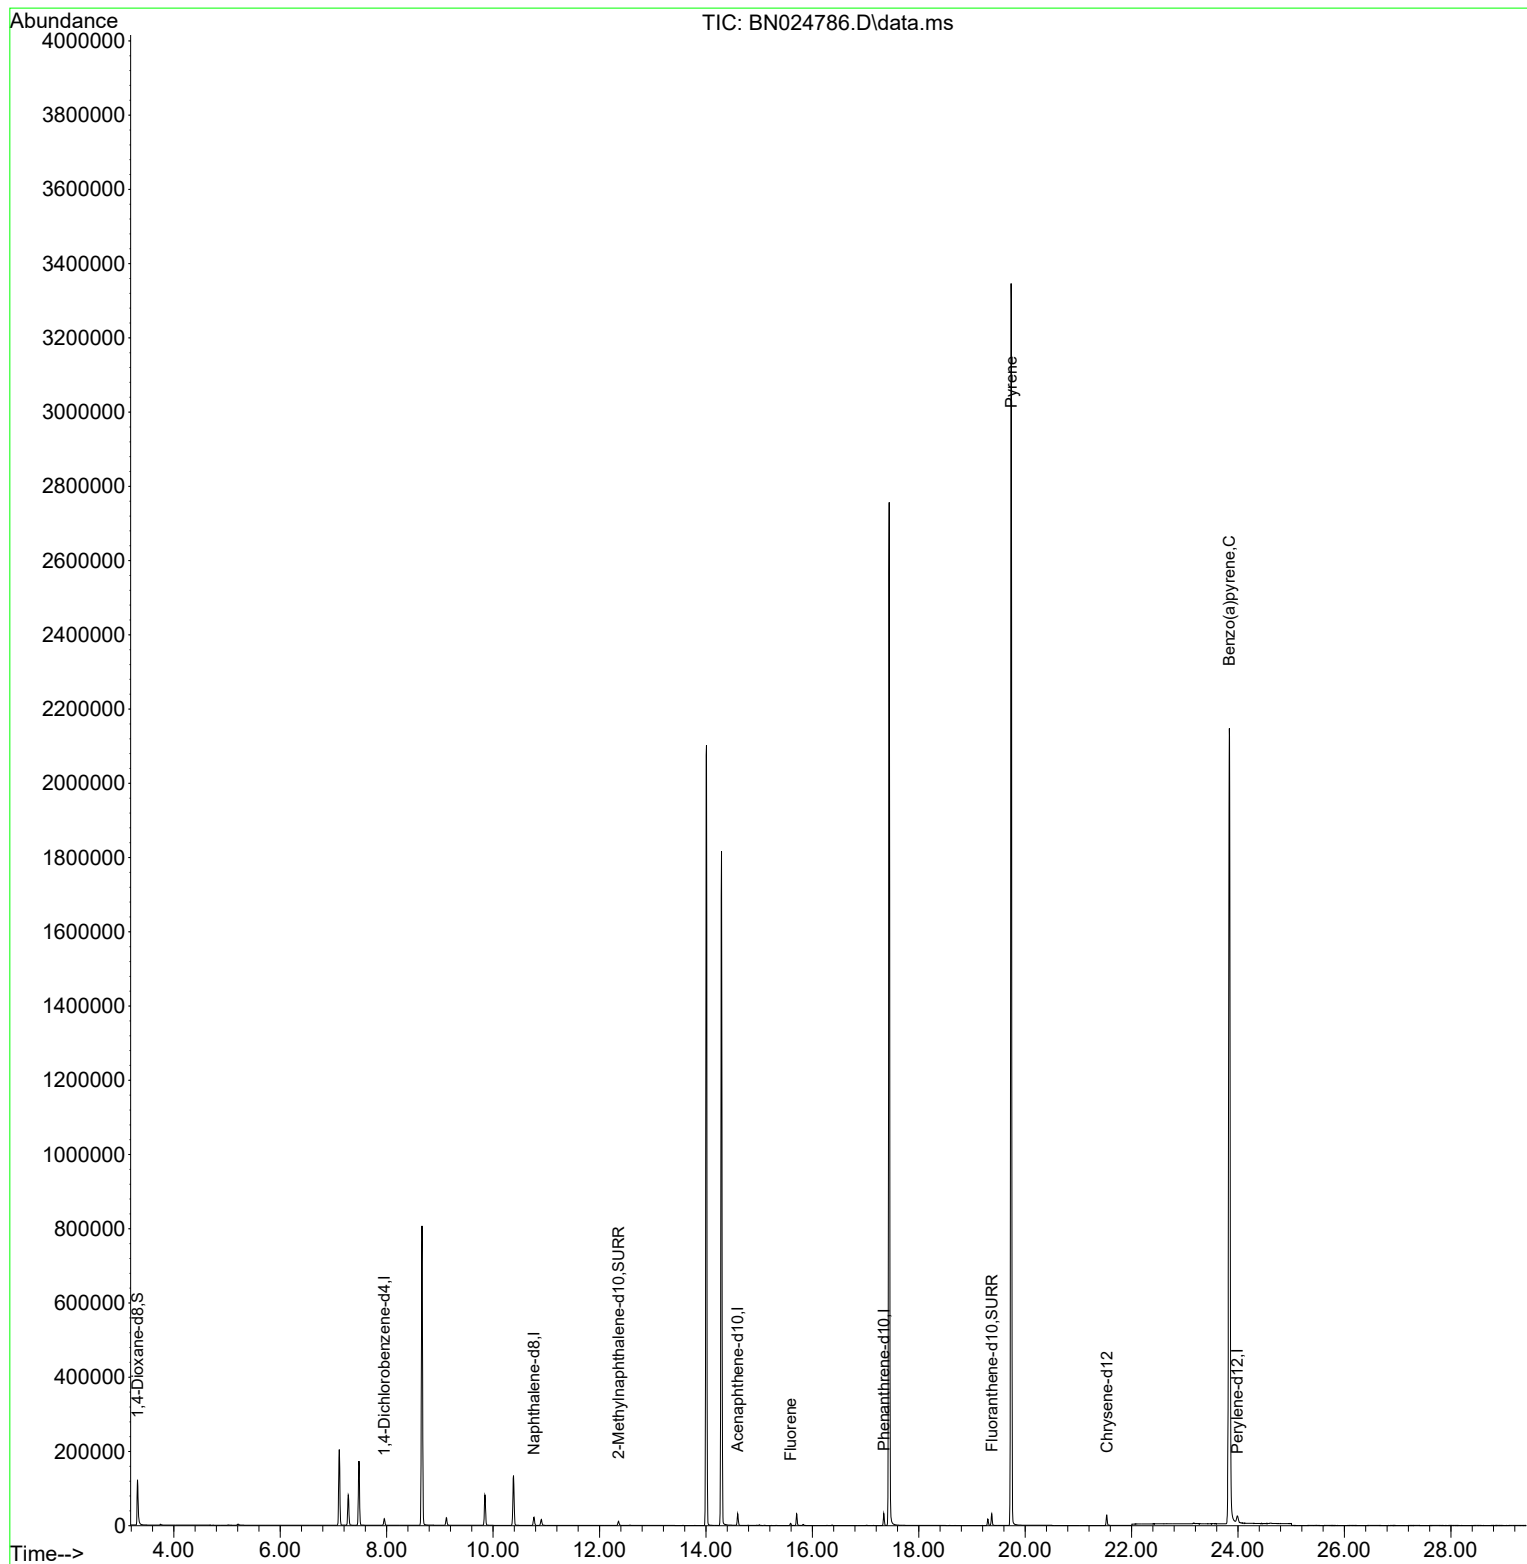


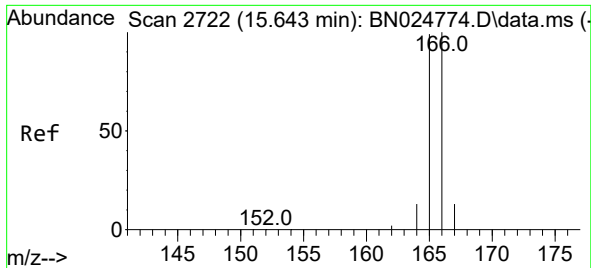

#12
Fluorene
Concen: 0.088 ng/ul
RT: 15.592 min Scan# 21
Delta R.T. -0.052 min
Lab File: BN024786.D
Acq: 06 Apr 2023 18:42




Instrument :
BNA_N
ClientSampleId :
SBLK755


Tgt Ion:166 Resp: 5052
Ion Ratio Lower Upper
166 100
165 5.9 80.0 120.0#
167 34.9 10.8 16.2#

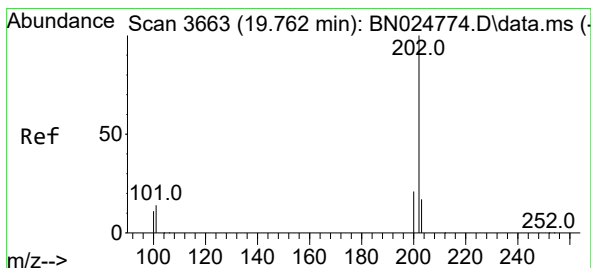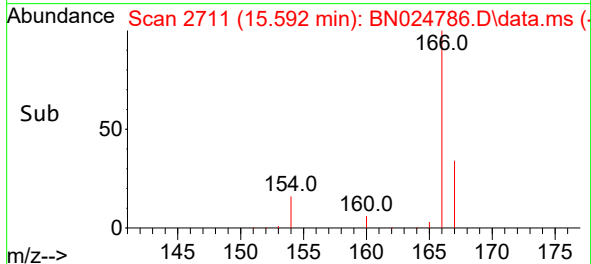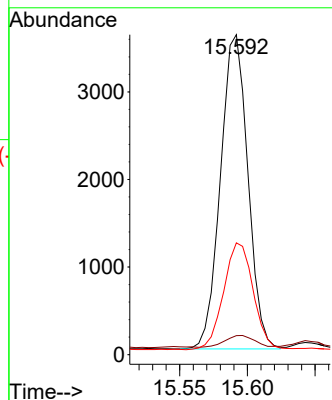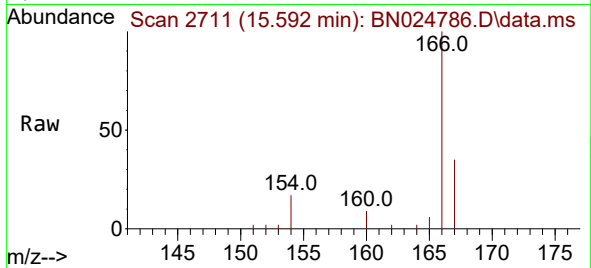

#20
Pyrene
Concen: 0.054 ng/ul
RT: 19.739 min Scan# 3658
Delta R.T. -0.024 min
Lab File: BN024786.D
Acq: 06 Apr 2023 18:42

Tgt Ion:202 Resp: 5241
Ion Ratio Lower Upper
202 100
101 168.2 10.9 16.3#
100 1204.8 8.7 13.1#

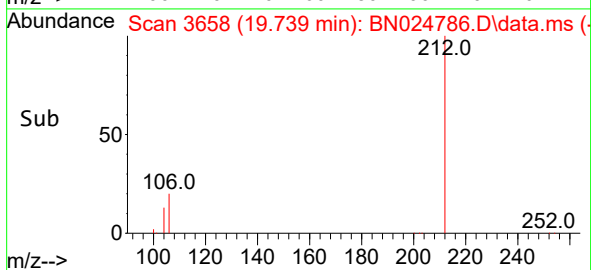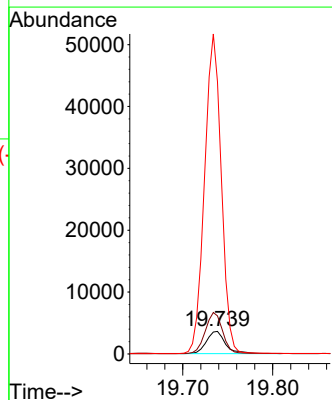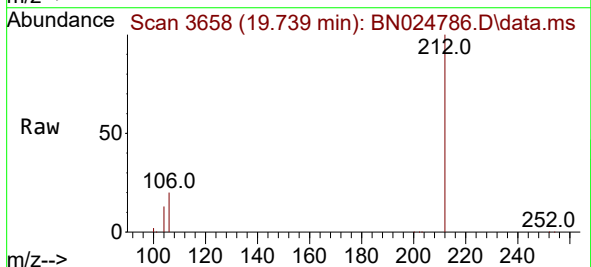

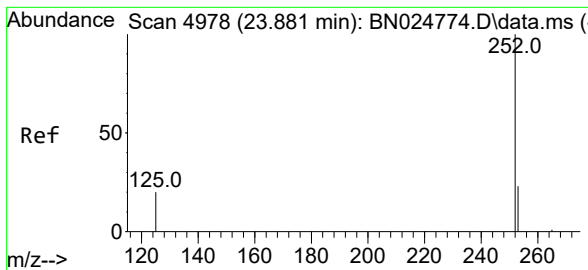

#26

Benzo(a)pyrene

Concen: 0.122 ng/ul

RT: 23.837 min Scan# 49

Delta R.T. -0.036 min

Lab File: BN024786.D


Acq: 06 Apr 2023 18:42

Instrument :

BNA_N

ClientSampleId :

SBLK755

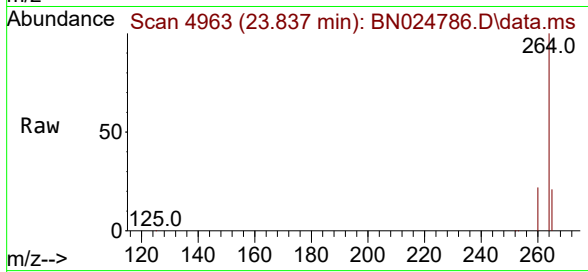

Tgt Ion:252 Resp: 11978

Ion Ratio Lower Upper

252 100

253 40.8 21.8 32.8#

125 36.1 15.4 23.0#

